
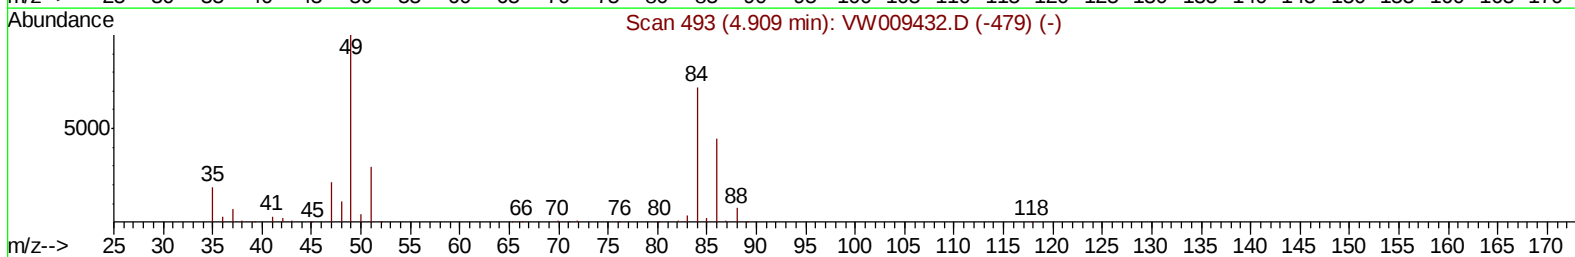
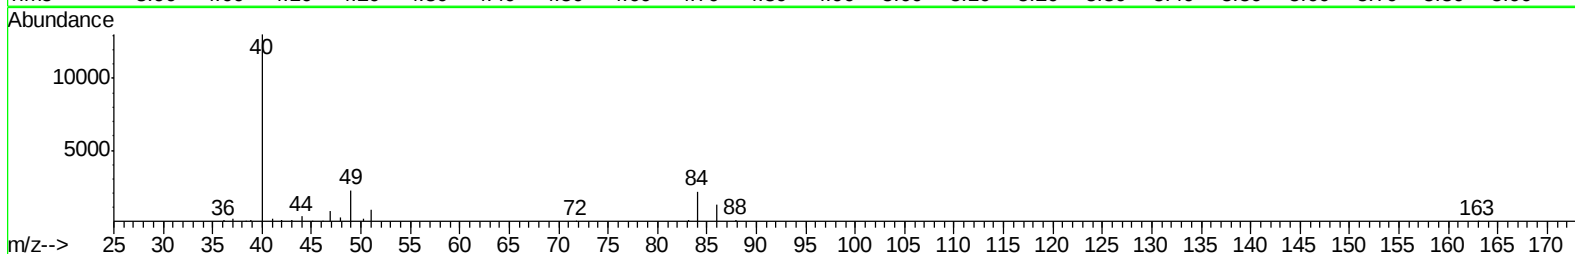


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032519\
Data File : VW009433.D
Acq On : 25 Mar 2019 17:51
Operator : SY/VA
Sample : VW0325SBL02
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 09:04:49 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 26 07:46:05 2019
Response via : Initial Calibration

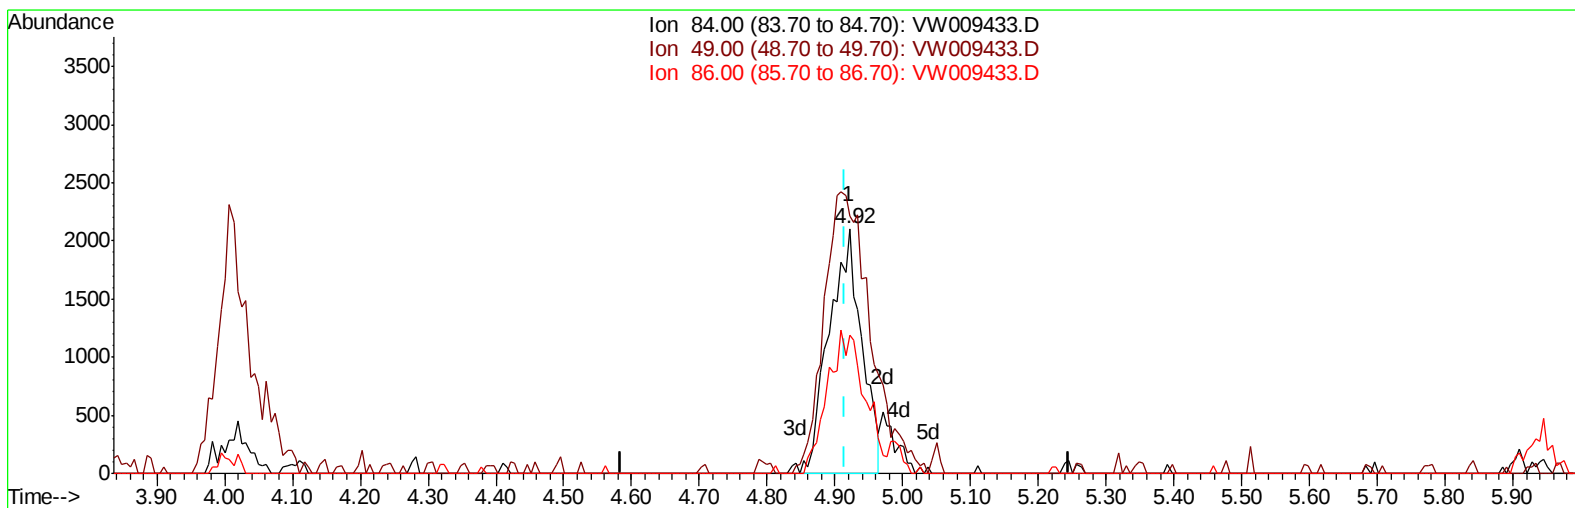

TIC: VW009433.D

(16) Methylene chloride (T)

4.922min (+0.006) 1.17ug/L

response 7020

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	105.42
86.00	63.50	56.65
0.00	0.00	0.00