

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032519\

Quantitation Report (LSC Reviewed)

Data File : VW009428.D

Acq On : 25 Mar 2019 15:14

Operator : SY/VA

Sample : K2031-16RE

Misc : 5.97G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 08:15:15 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Tue Mar 26 07:46:05 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :


BF5S6RE

Manual Integrations

APPROVED

MMDadoda

3/27/2019 12:13:13 PM

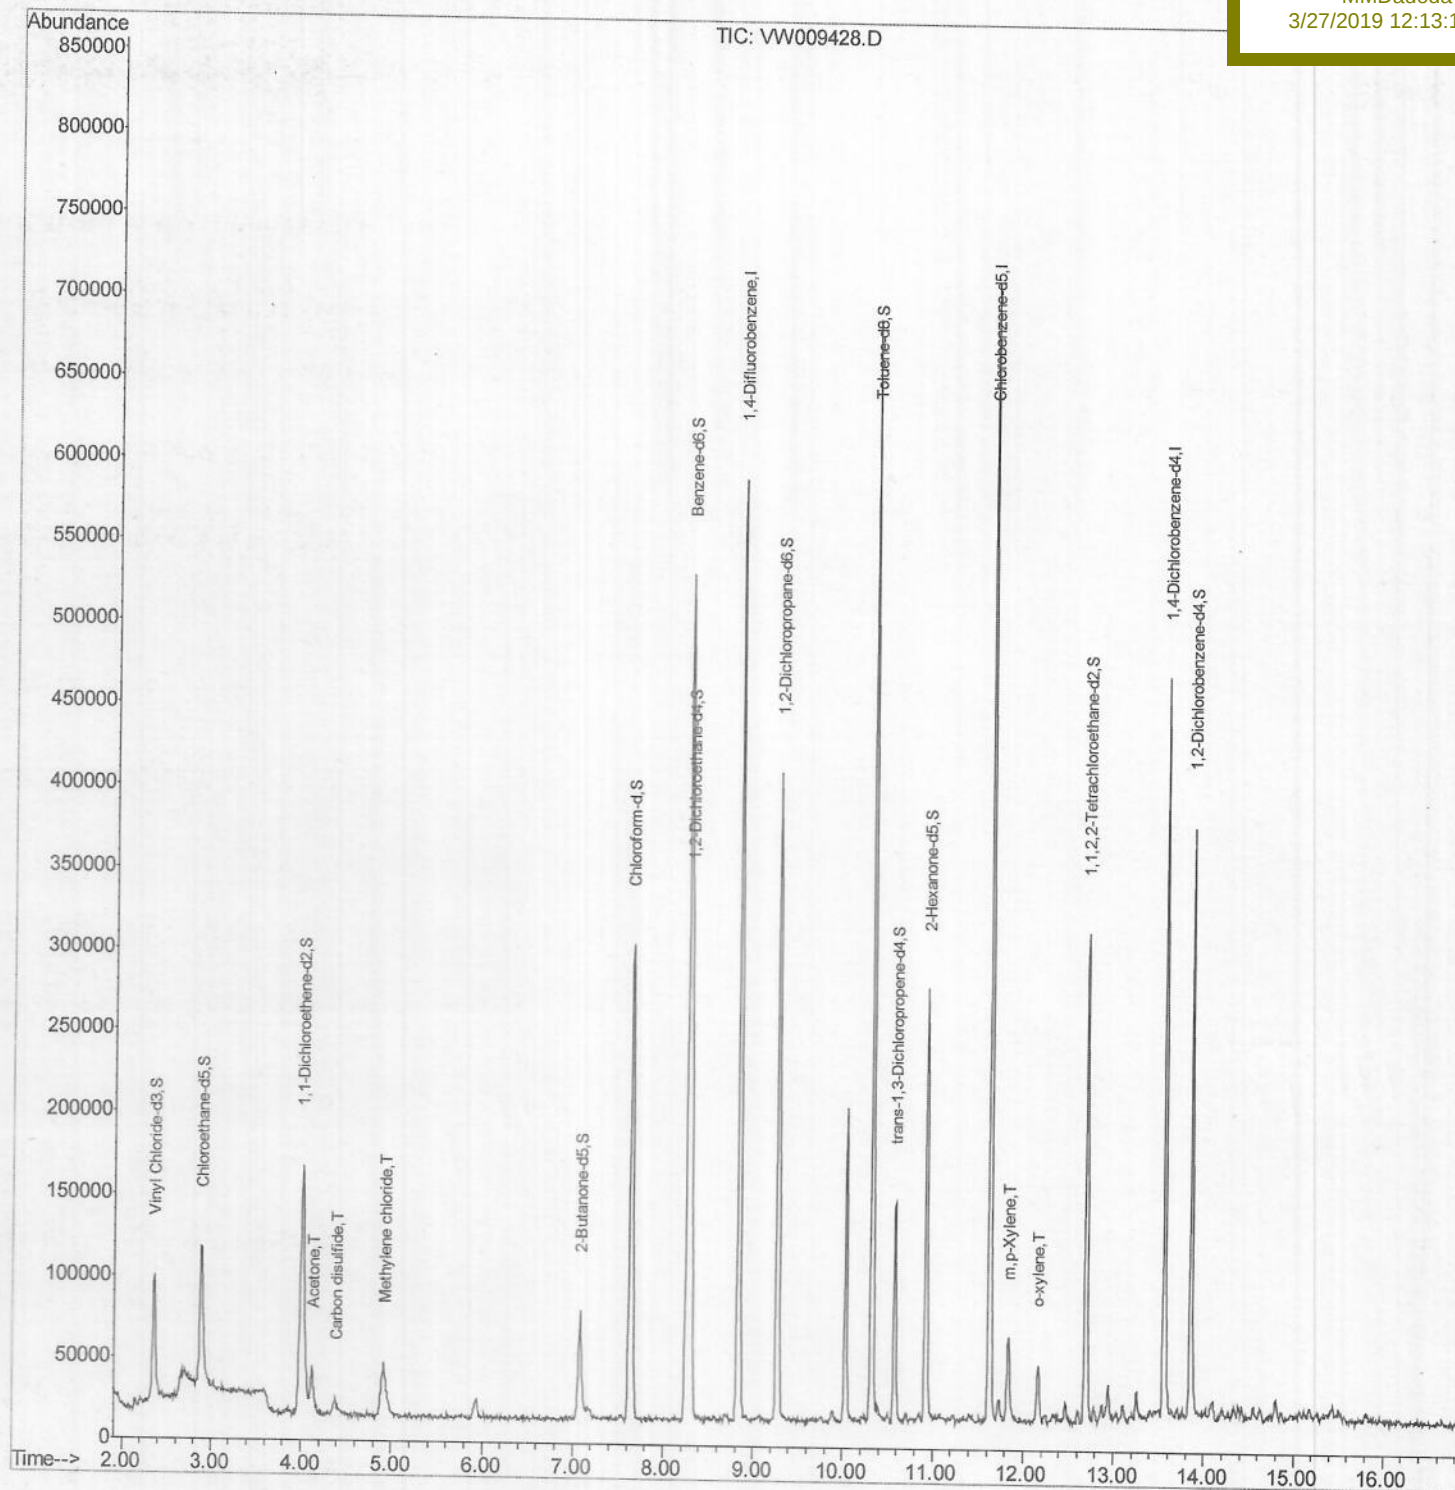

SOM2WLM031419S.M Mon Apr 08 08:14:23 2019

Page: 2

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\

Data File : VW009428.D

Acq On : 25 Mar 2019 15:14

Operator : SY/VA

Sample : K2031-16RE

Misc : 5.97G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:51:40 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Tue Mar 26 07:46:05 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :




BF5S6RE

Manual Integrations

APPROVED

MMDadoda

3/27/2019 12:13:13 PM

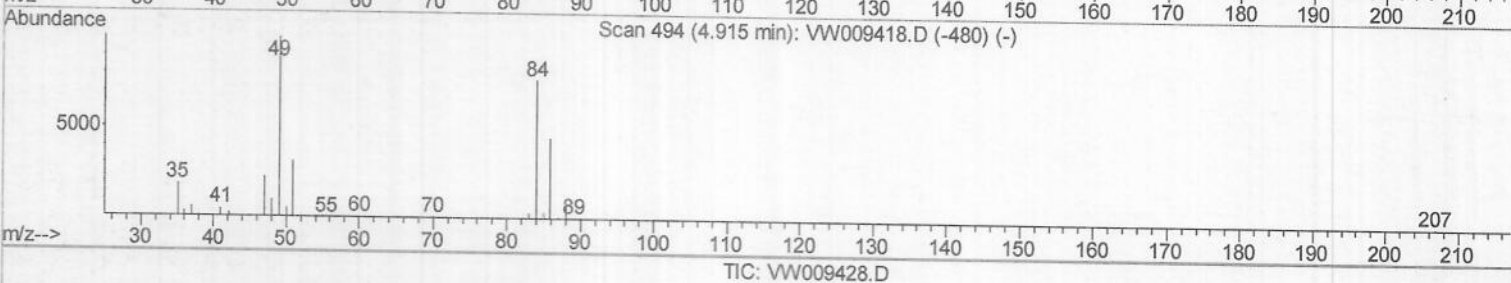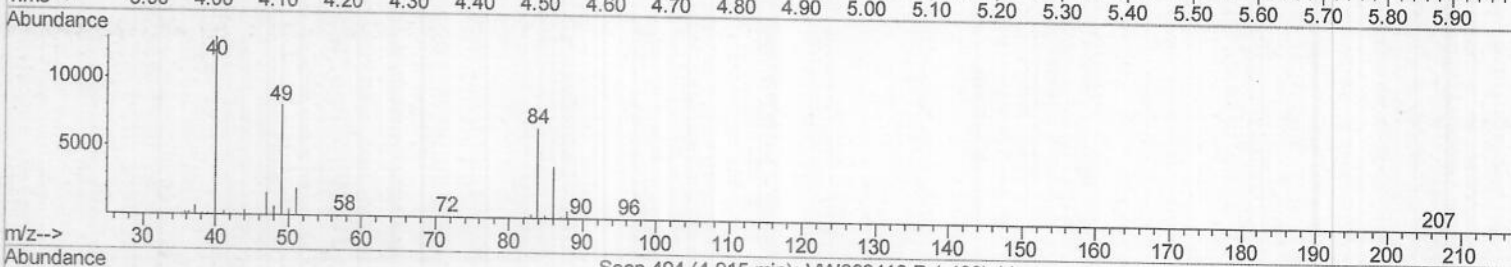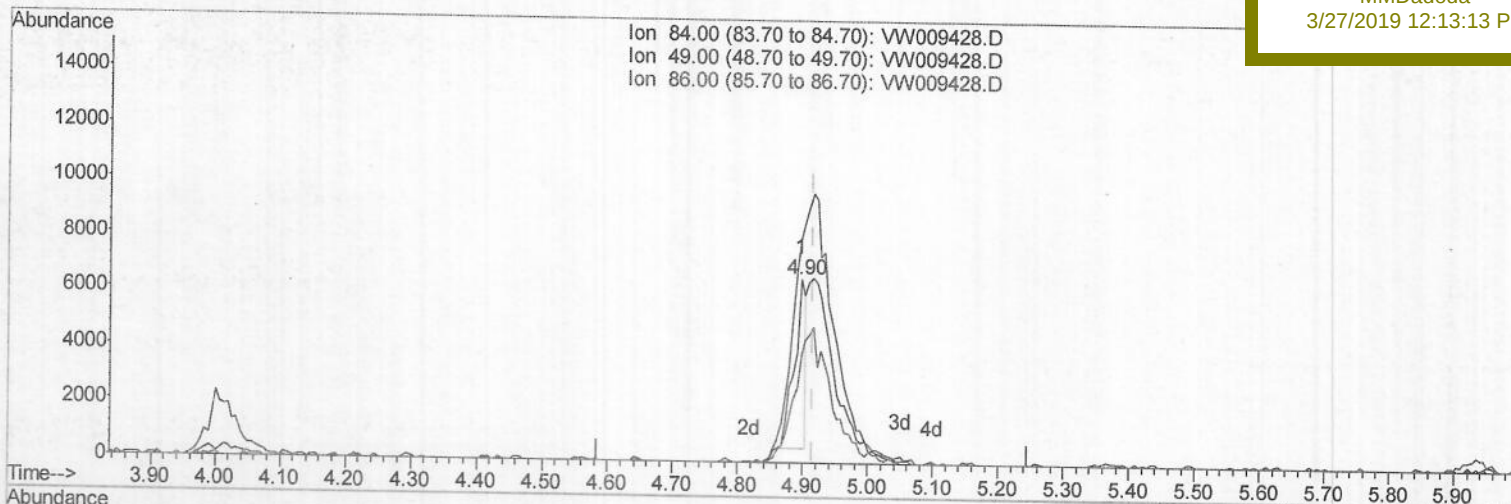

TIC: VW009428.D

(16) Methylene chloride (T)

4.897min (-0.018) 1.15ug/L

response 7568

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	122.96
86.00	63.50	58.17
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\

Data File : VW009428.D

Acq On : 25 Mar 2019 15:14

Operator : SY/VA

Sample : K2031-16RE

Misc : 5.97G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:51:40 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Tue Mar 26 07:46:05 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :




BF5S6RE

Manual Integrations

APPROVED

MMDadoda

3/27/2019 12:13:13 PM

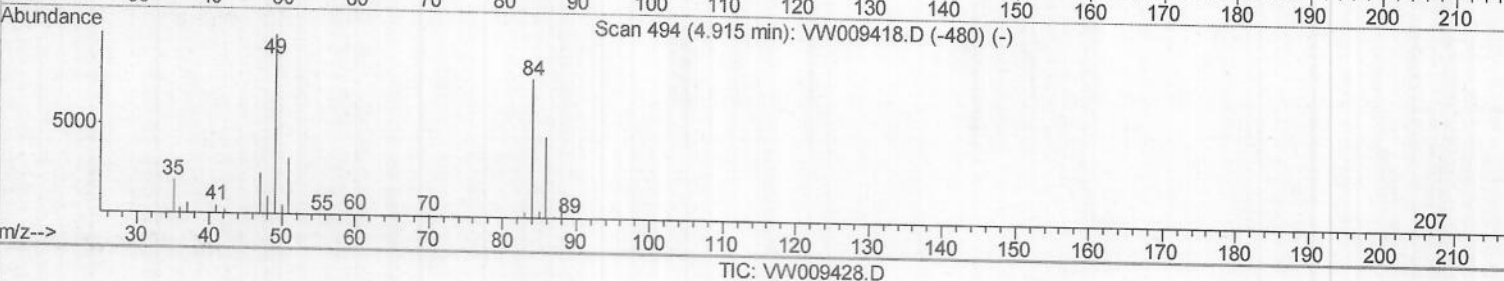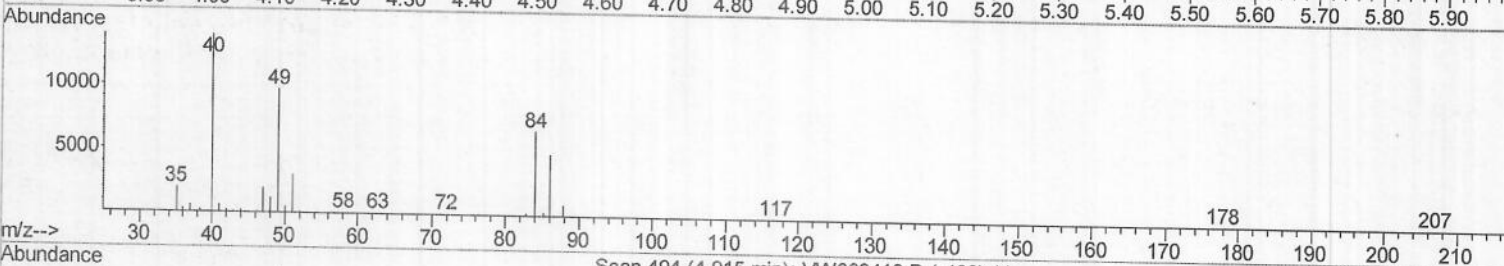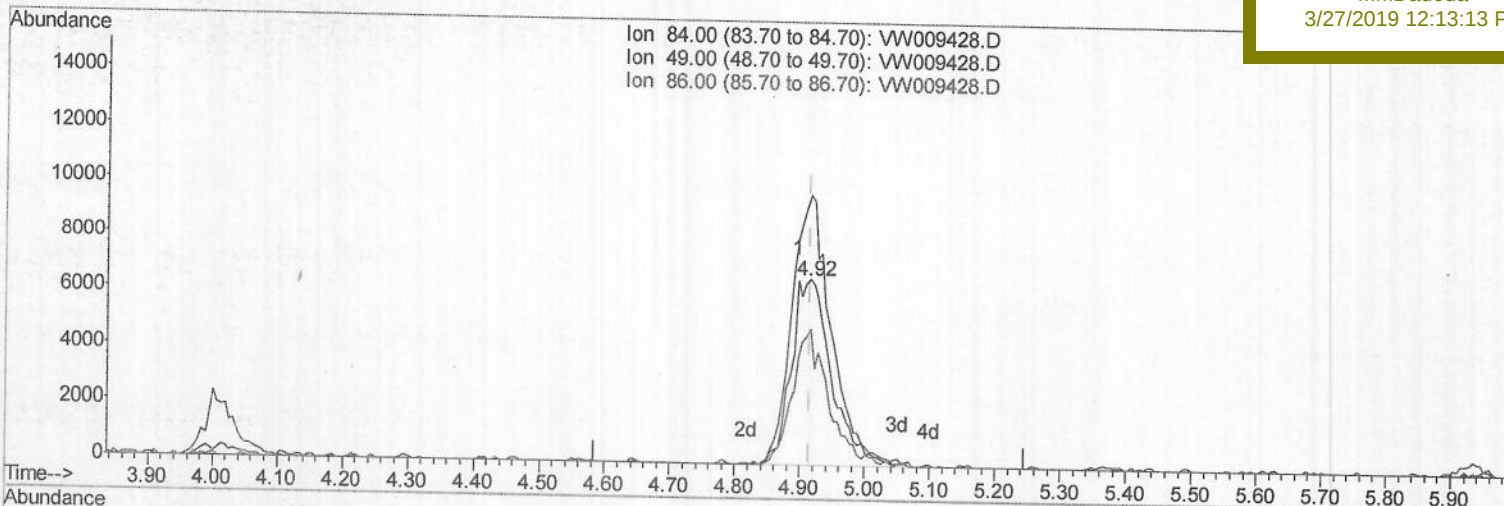

(16) Methylene chloride (T)

4.915min (-0.000) 4.38ug/L m

response 28707

Ion Exp% Act%

84.00 100 100

49.00 137.10 146.84

86.00 63.50 73.16

0.00 0.00 0.00

MD
4/5/19

TIC: VW009428.D

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032519\

Quantitation Report (LSC Reviewed)

Data File : VW009428.D

Acq On : 25 Mar 2019 15:14

Operator : SY/VA

Sample : K2031-16RE

Misc : 5.97G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 08:15:15 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Tue Mar 26 07:46:05 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

Client Sampled :

BF5S6RE

Manual Integrations

APPROVED

MMDadoda

3/27/2019 12:13:13 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	449547	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	367233	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	109638	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	108221	20.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.60%
7) Chloroethane-d5	2.89	69	120792	19.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.88%
10) 1,1-Dichloroethene-d2	4.01	63	180163	15.52	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.08%
20) 2-Butanone-d5	7.08	46	109865	49.45	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.90%
24) Chloroform-d	7.64	84	283585	23.12	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.48%
26) 1,2-Dichloroethane-d4	8.30	65	176304	23.86	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.44%
29) Benzene-d6	8.27	84	501695	24.77	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.08%
33) 1,2-Dichloropropane-d6	9.27	67	161151	26.49	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.96%
37) Toluene-d8	10.32	98	419588	22.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.64%
38) trans-1,3-Dichloropropene-	10.58	79	67162	21.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.92%
39) 2-Hexanone-d5	10.93	63	79844	54.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.40%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	132158	22.06	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.24%
61) 1,2-Dichlorobenzene-d4	13.86	152	88950	21.16	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.64%

Target Compounds

						Qvalue
13) Acetone	4.12	43	43627	23.946	ug/L	99
14) Carbon disulfide	4.38	76	17514	1.176	ug/L	99
16) Methylene chloride	4.92	84	28707m	4.379	ug/L	
54) m,p-Xylene	11.83	106	15075	1.606	ug/L	95
55) o-xylene	12.16	106	7902	0.863	ug/L	95

M.D
4/5/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed