

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\

Data File : VW009430.D

Acq On : 25 Mar 2019 16:08

Operator : SY/VA

Sample : K2031-20

Misc : 6.31G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:58:26 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Tue Mar 26 07:46:05 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

Client Sampled :


BF5T0

Manual Integrations

APPROVED

MMDadoda

3/27/2019 12:13:19 PM

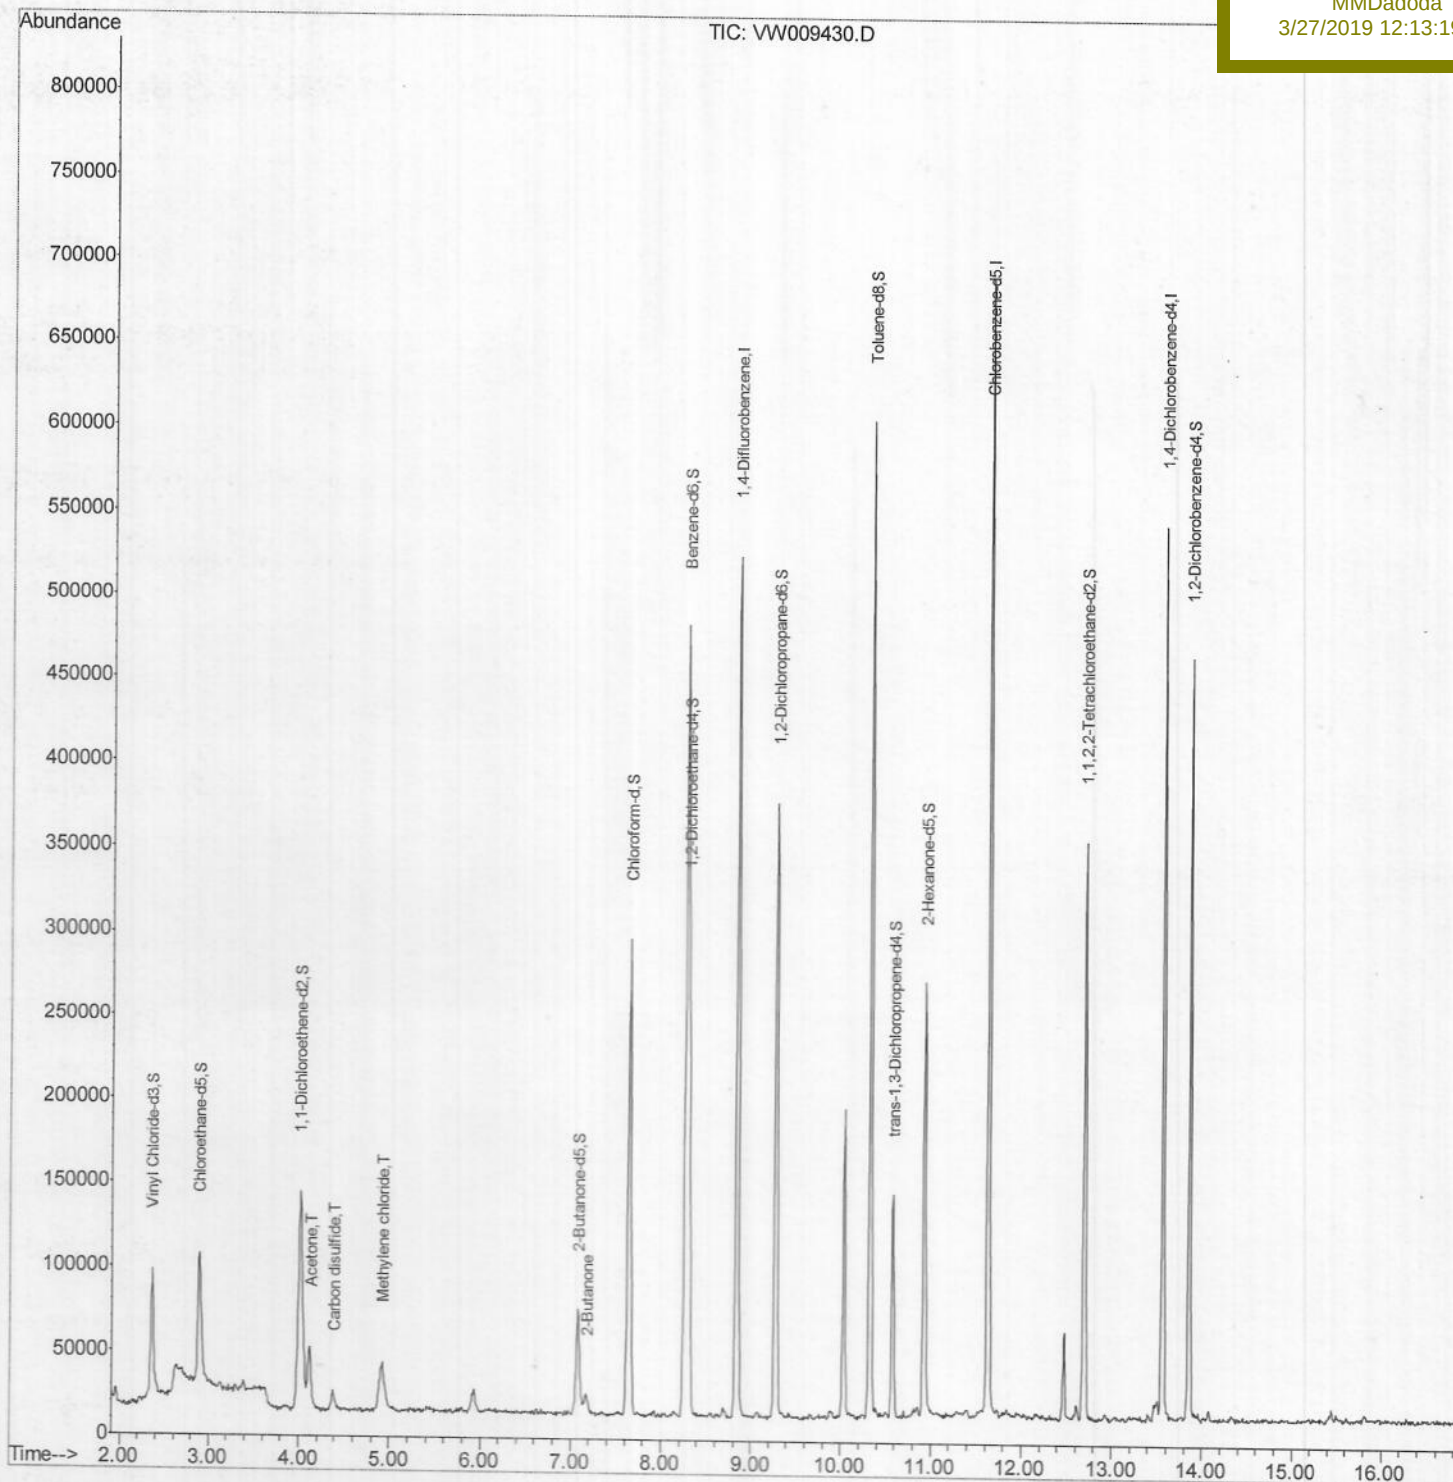

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009430.D
 Acq On : 25 Mar 2019 16:08
 Operator : SY/VA
 Sample : K2031-20
 Misc : 6.31G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5T0

Manual Integrations
 APPROVED

MMDadoda
 3/27/2019 12:13:19 PM

Quant Time: Mar 26 07:51:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 07:46:05 2019
 Response via : Initial Calibration

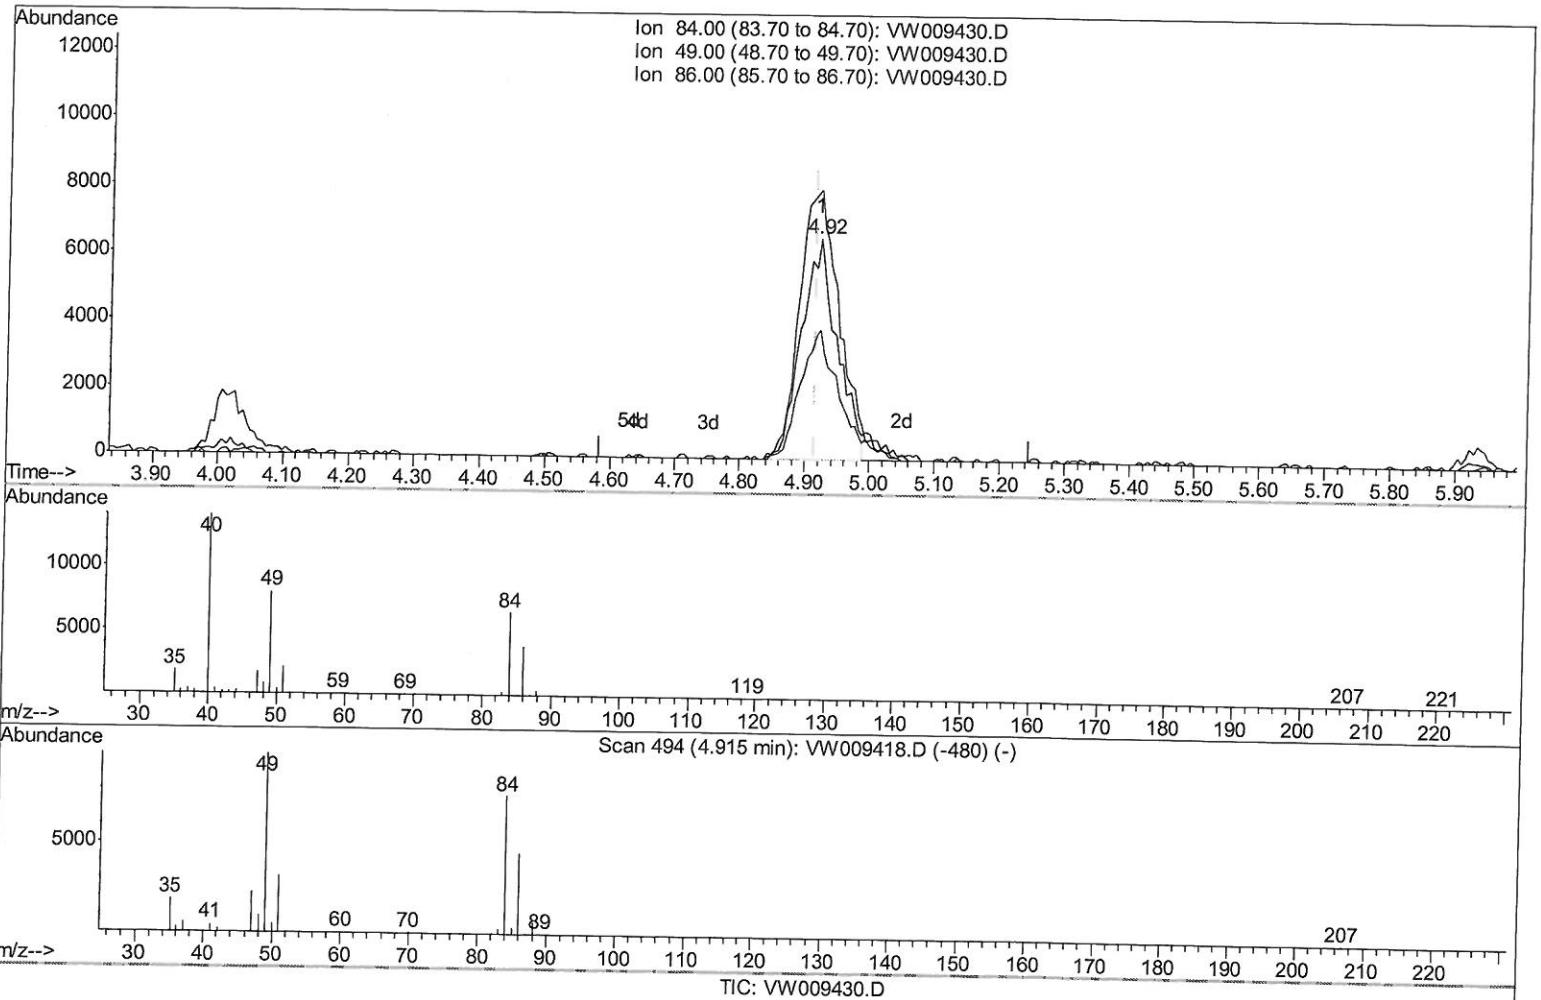

(16) Methylene chloride (T)

4.921min (+0.006) 4.34ug/L

response 25270

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	122.04
86.00	63.50	58.94
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009430.D
 Acq On : 25 Mar 2019 16:08
 Operator : SY/VA
 Sample : K2031-20
 Misc : 6.31G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BF5T0

Manual Integrations
APPROVED

MMDadoda
 3/27/2019 12:13:19 PM

Quant Time: Mar 26 07:51:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 07:46:05 2019
 Response via : Initial Calibration

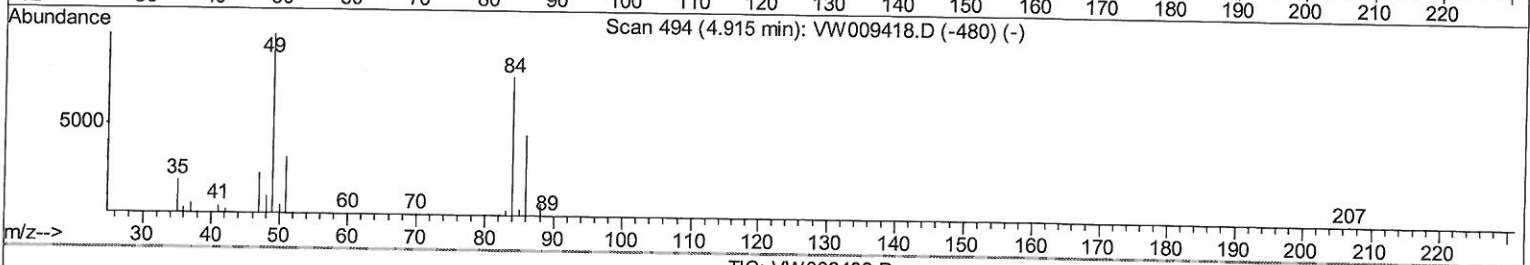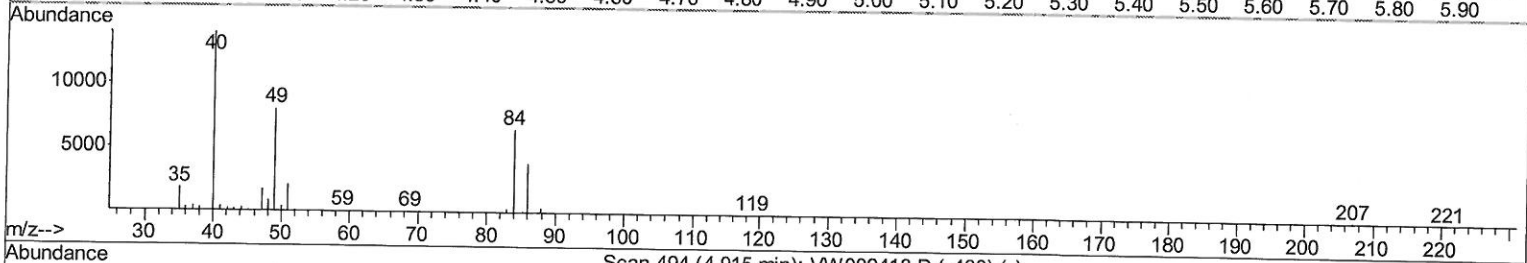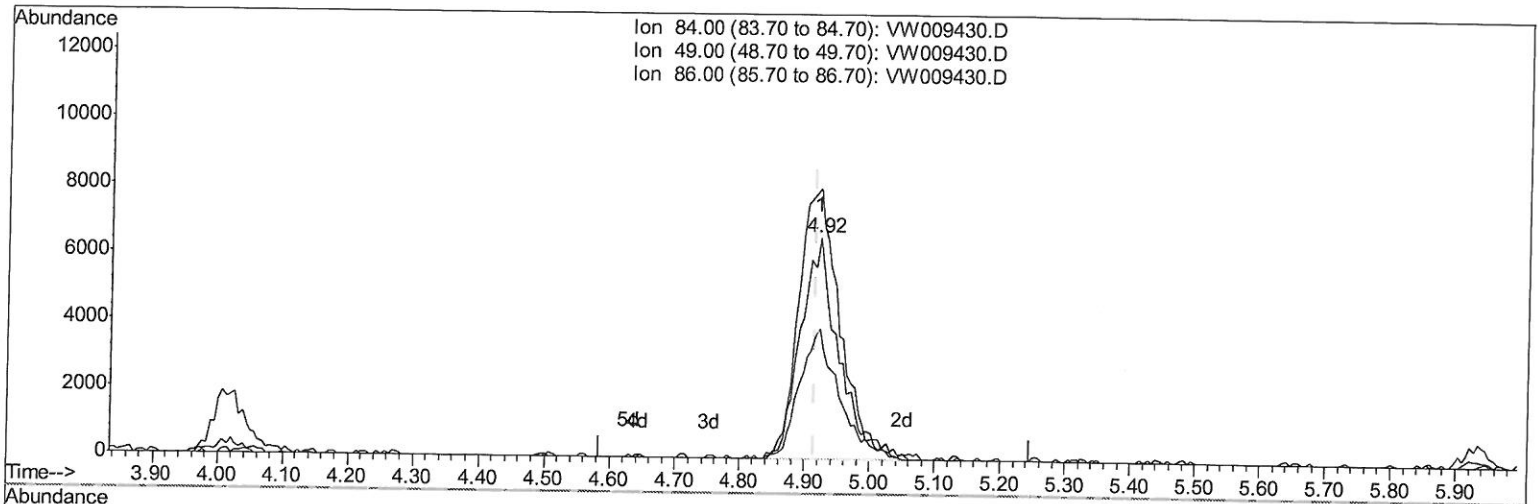

TIC: VW009430.D

(16) Methylene chloride (T)

4.921min (+0.006) 4.55ug/L m

response 26480

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	122.04
86.00	63.50	58.94
0.00	0.00	0.00

MO
4/6/19

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009430.D
 Acq On : 25 Mar 2019 16:08
 Operator : SY/VA
 Sample : K2031-20
 Misc : 6.31G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5T0

Manual Integrations
 APPROVED

MMDadoda
 3/27/2019 12:13:19 PM

Quant Time: Mar 26 07:51:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 07:46:05 2019
 Response via : Initial Calibration

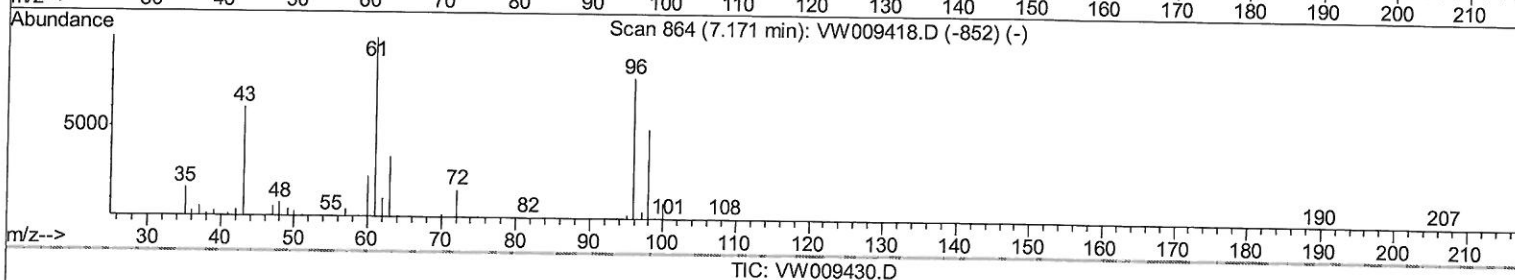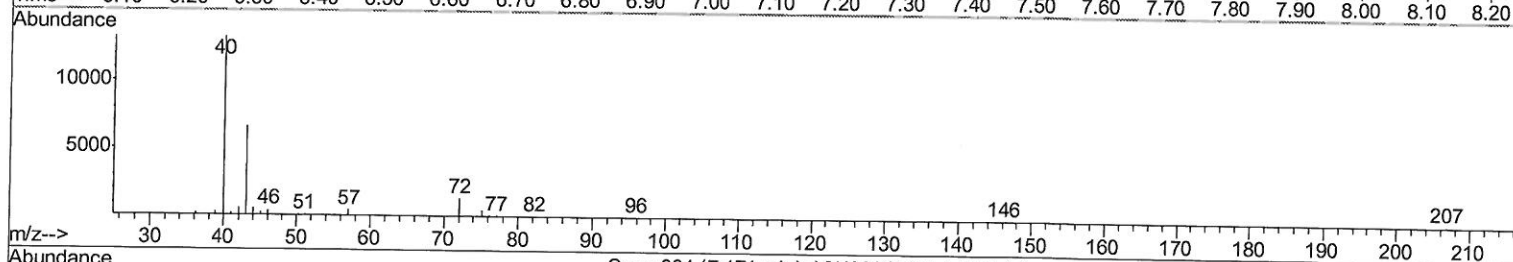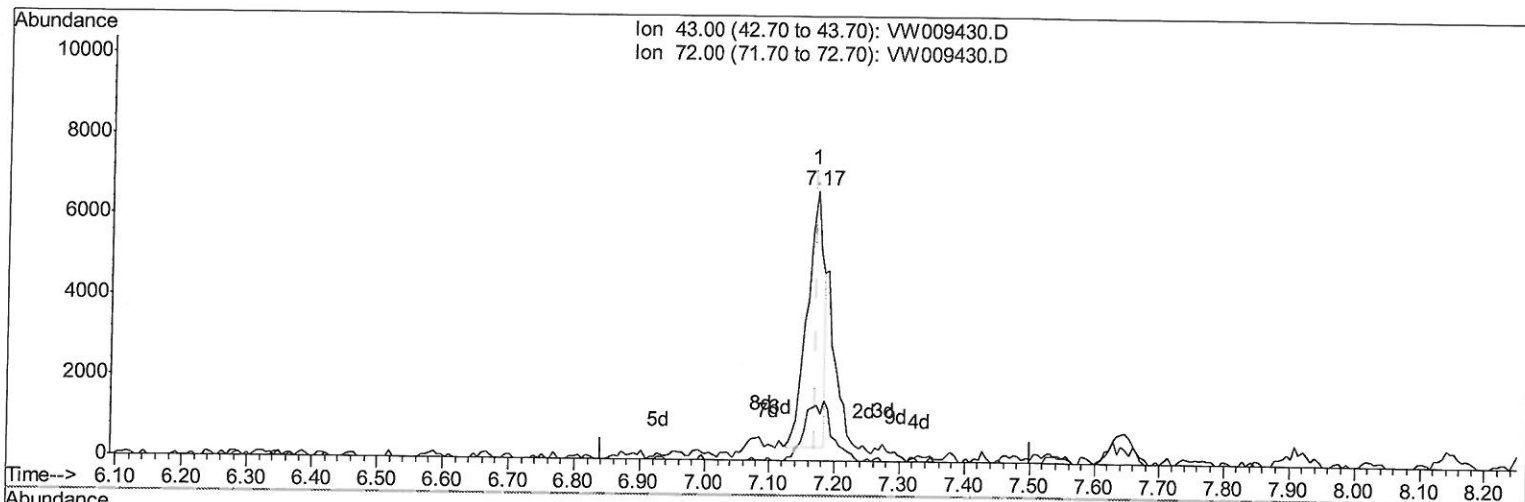

TIC: VW009430.D

(21) 2-Butanone

7.171min (-0.000) 4.99ug/L

response 11135

Ion	Exp%	Act%
43.00	100	100
72.00	26.10	22.17
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009430.D
 Acq On : 25 Mar 2019 16:08
 Operator : SY/VA
 Sample : K2031-20
 Misc : 6.31G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5T0

Manual Integrations
 APPROVED

MMDadoda
 3/27/2019 12:13:19 PM

Quant Time: Mar 26 07:51:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 07:46:05 2019
 Response via : Initial Calibration

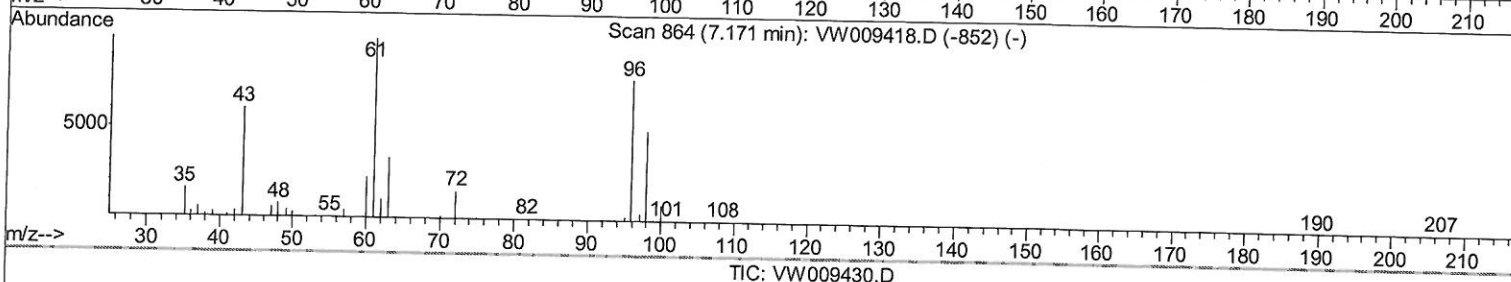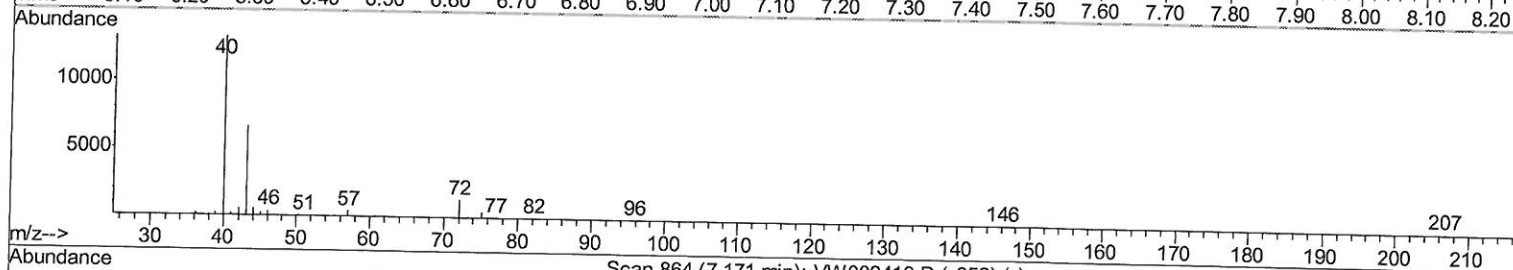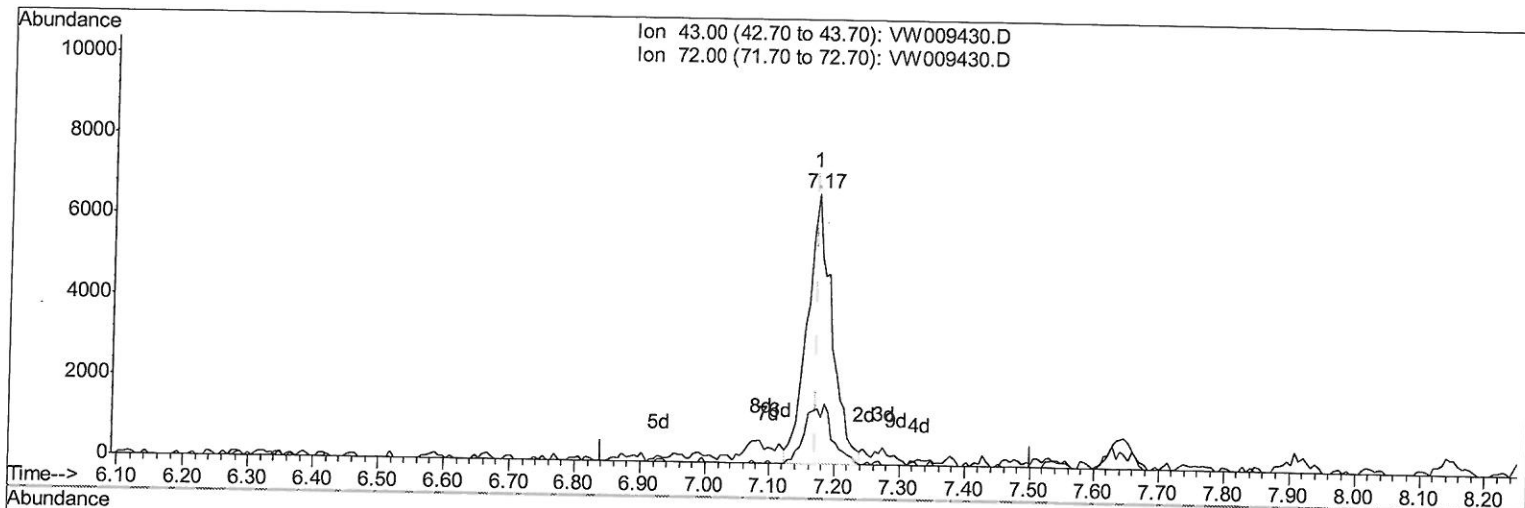

(21) 2-Butanone

7.171min (-0.000) 7.94ug/L m

response 17734

Ion	Exp%	Act%
43.00	100	100
72.00	26.10	13.92
0.00	0.00	0.00
0.00	0.00	0.00

> MO
4/6/19

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009430.D
 Acq On : 25 Mar 2019 16:08
 Operator : SY/VA
 Sample : K2031-20
 Misc : 6.31G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BF5T0

Manual Integrations
 APPROVED

MMDadoda
 3/27/2019 12:13:19 PM

Quant Time: Mar 26 07:51:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 07:46:05 2019
 Response via : Initial Calibration

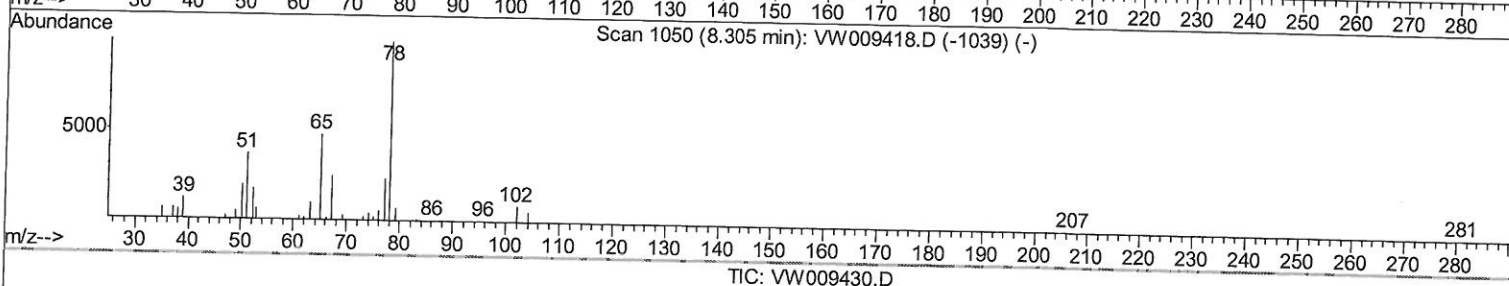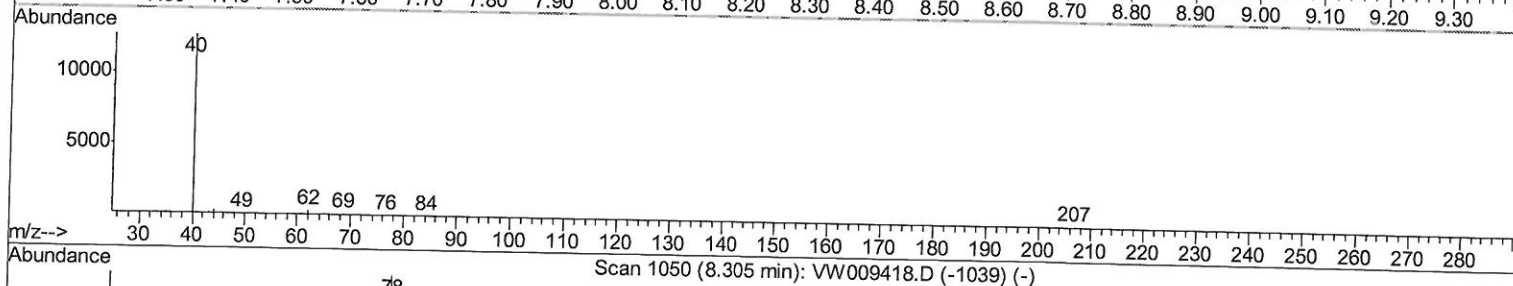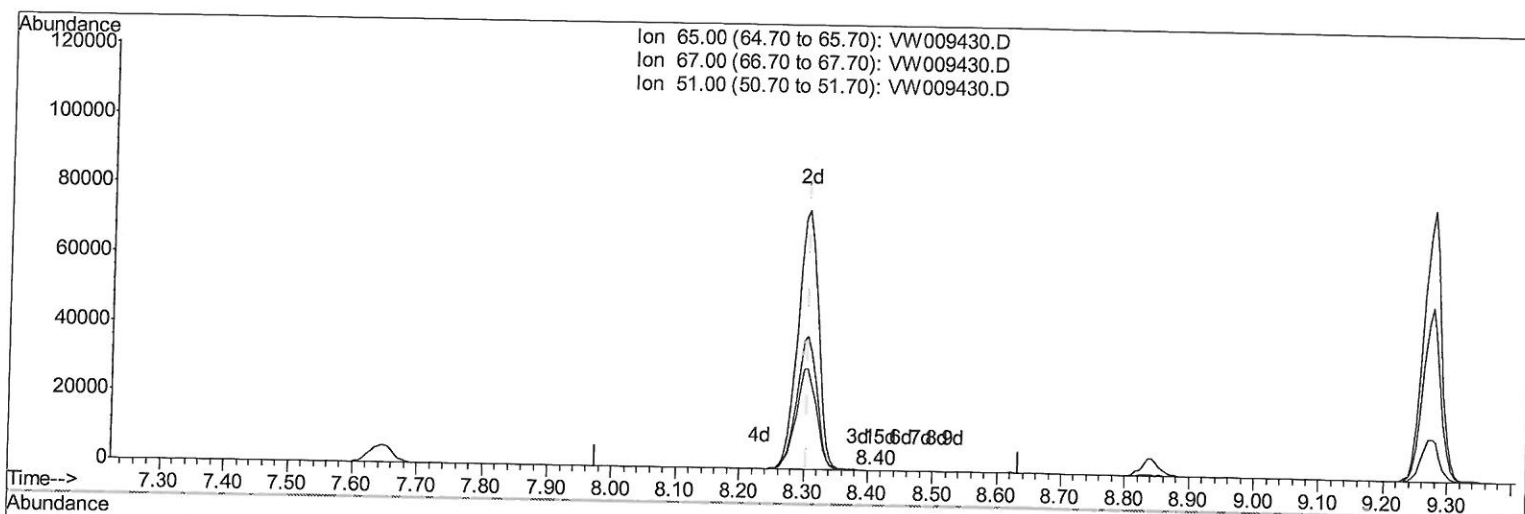

(26) 1,2-Dichloroethane-d4 (S)

8.403min (+0.098) 0.01ug/L

response 42

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	64.29
51.00	97.70	111.90
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009430.D
 Acq On : 25 Mar 2019 16:08
 Operator : SY/VA
 Sample : K2031-20
 Misc : 6.31G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5T0

Manual Integrations
 APPROVED

MMDadoda
 3/27/2019 12:13:19 PM

Quant Time: Mar 26 07:51:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 07:46:05 2019
 Response via : Initial Calibration

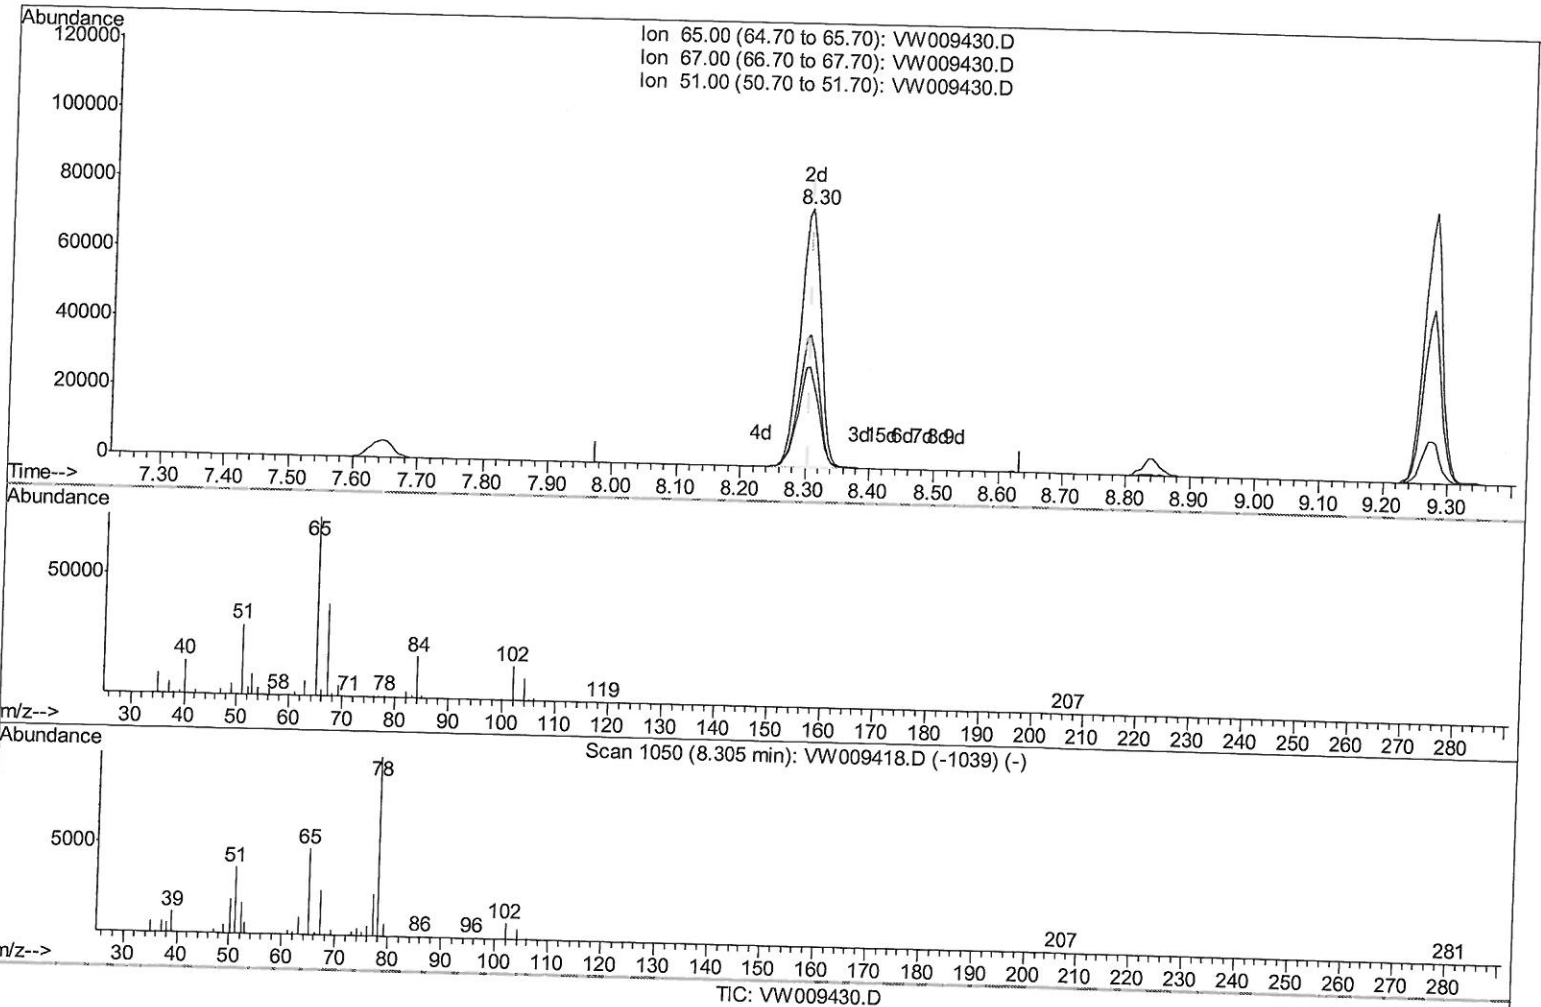

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 25.10ug/L m

response 164679

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	0.02#
51.00	97.70	0.03#
0.00	0.00	0.00

7 MO
 4/6/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\

Data File : VW009430.D

Acq On : 25 Mar 2019 16:08

Operator : SY/VA

Sample : K2031-20

Misc : 6.31G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:58:26 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Tue Mar 26 07:46:05 2019

Response via : Initial Calibration

Instrument :
MSVOA_W
Client Sampled :
BF5T0

Manual Integrations
APPROVED

MMDadoda
3/27/2019 12:13:19 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	399032	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	349408	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	127734	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	100901	21.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.64%
7) Chloroethane-d5	2.89	69	110572	19.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.28%
10) 1,1-Dichloroethene-d2	4.01	63	159285	15.46	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.84%
20) 2-Butanone-d5	7.08	46	105422	53.46	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.92%
24) Chloroform-d	7.65	84	253707	23.30	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.20%
26) 1,2-Dichloroethane-d4	8.30	65	164679m	25.10	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.40%
29) Benzene-d6	8.27	84	449803	23.34	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.36%
33) 1,2-Dichloropropane-d6	9.27	67	150079	25.93	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.72%
37) Toluene-d8	10.32	98	365087	20.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.96%
38) trans-1,3-Dichloropropene-	10.58	79	65520	22.54	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.16%
39) 2-Hexanone-d5	10.93	63	75860	54.12	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.24%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	145113	25.46	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.84%
61) 1,2-Dichlorobenzene-d4	13.86	152	112359	22.94	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.76%

Target Compounds

					Ovalue
13) Acetone	4.12	43	63627	39.345	ug/L 100
14) Carbon disulfide	4.38	76	16248	1.229	ug/L 96
16) Methylene chloride	4.92	84	26480m	4.551	ug/L
21) 2-Butanone	7.17	43	17734m	7.942	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MD
4/6/19

MD
4/6/19