


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
Data File : VW009431.D
Acq On : 25 Mar 2019 16:35
Operator : SY/VA
Sample : K2031-21RE
Misc : 4.11G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 09:01:28 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 26 07:46:05 2019
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampled :
BF5X8RE

Manual Integrations
APPROVED

MMDadoda
3/27/2019 12:13:24 PM

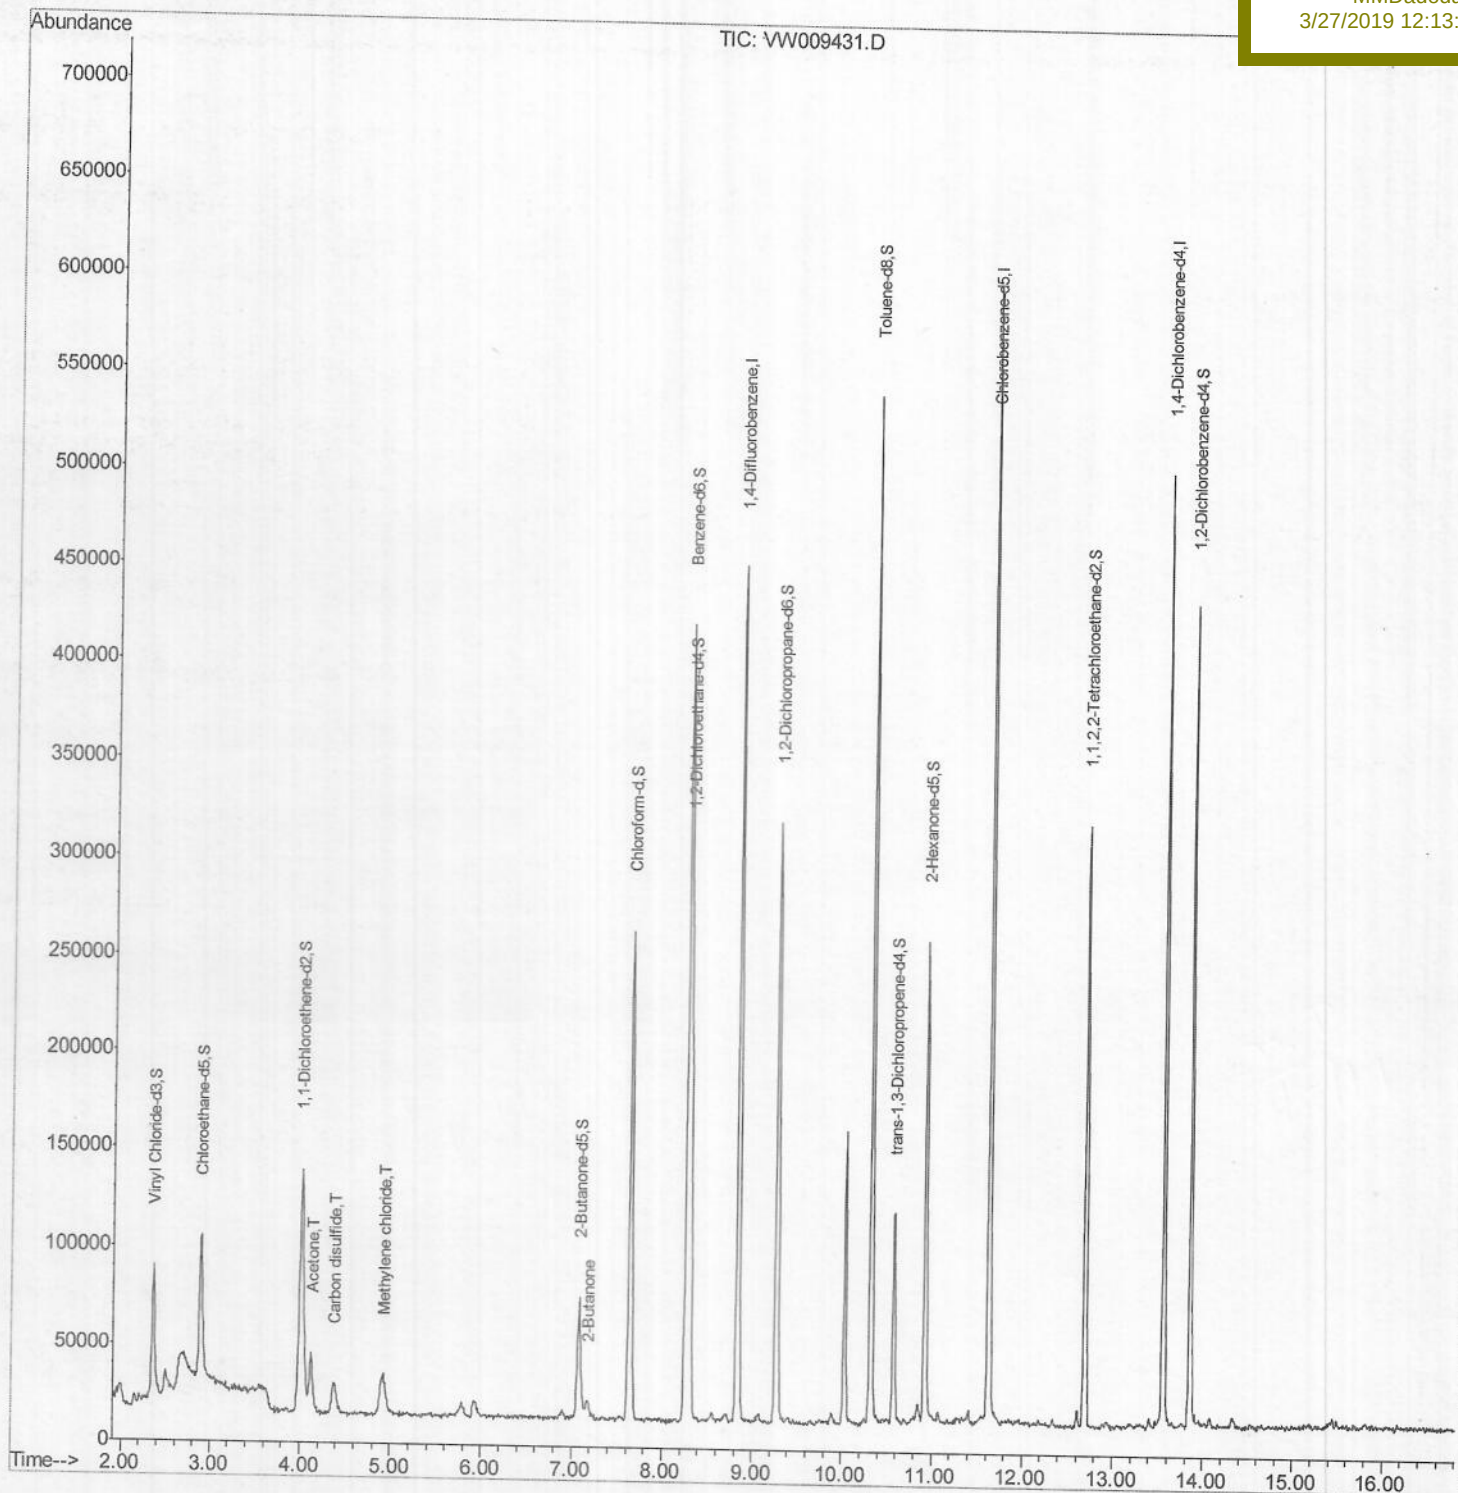

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009431.D
 Acq On : 25 Mar 2019 16:35
 Operator : SY/VA
 Sample : K2031-21RE
 Misc : 4.11G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:52:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 07:46:05 2019
 Response via : Initial Calibration

Instrument :
 MSVOA_W
 Client Sampled :
 BF5X8RE

Manual Integrations
 APPROVED

MMDadoda
 3/27/2019 12:13:24 PM

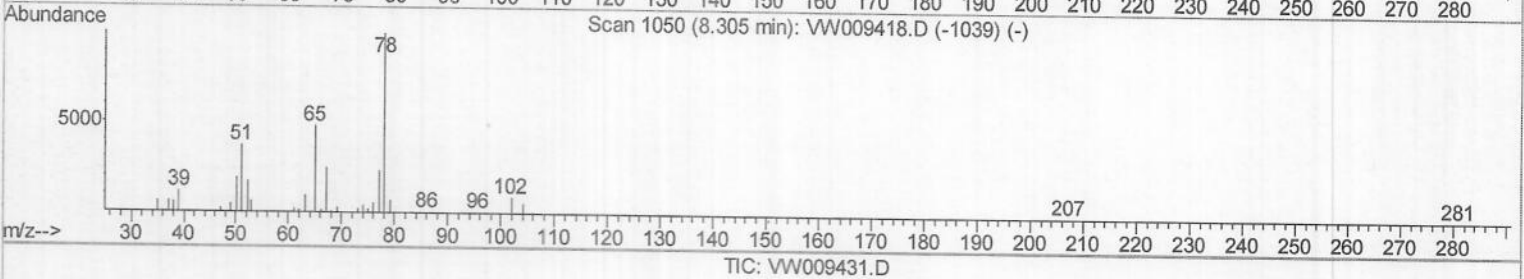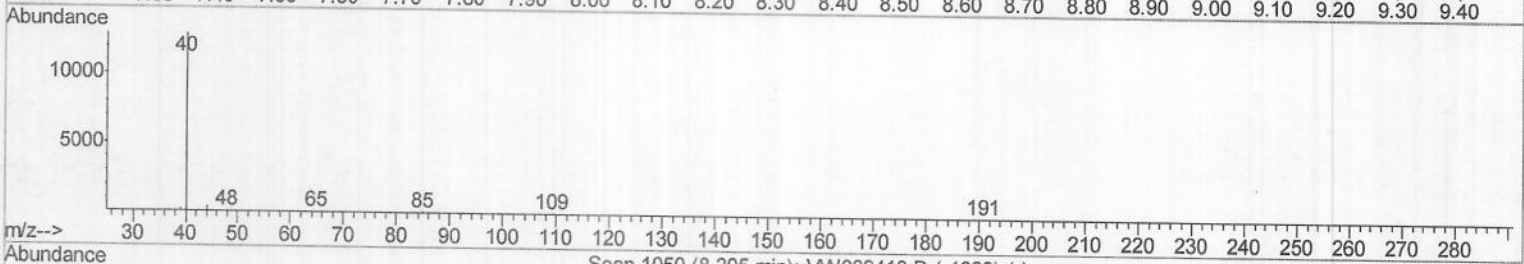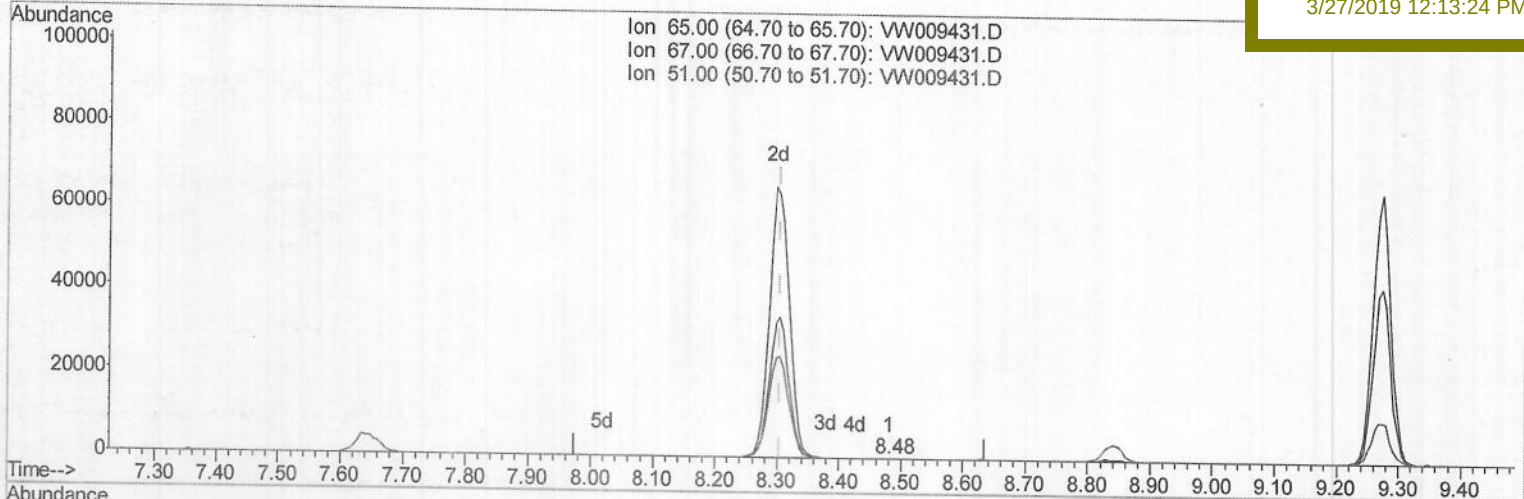

(26) 1,2-Dichloroethane-d4 (S)

8.482min (+0.177) 0.01ug/L

response 55

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	56.36
51.00	97.70	121.82
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009431.D
 Acq On : 25 Mar 2019 16:35
 Operator : SY/VA
 Sample : K2031-21RE
 Misc : 4.11G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 07:52:04 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 07:46:05 2019
 Response via : Initial Calibration

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5X8RE

Manual Integrations
 APPROVED

MMDadoda
 3/27/2019 12:13:24 PM

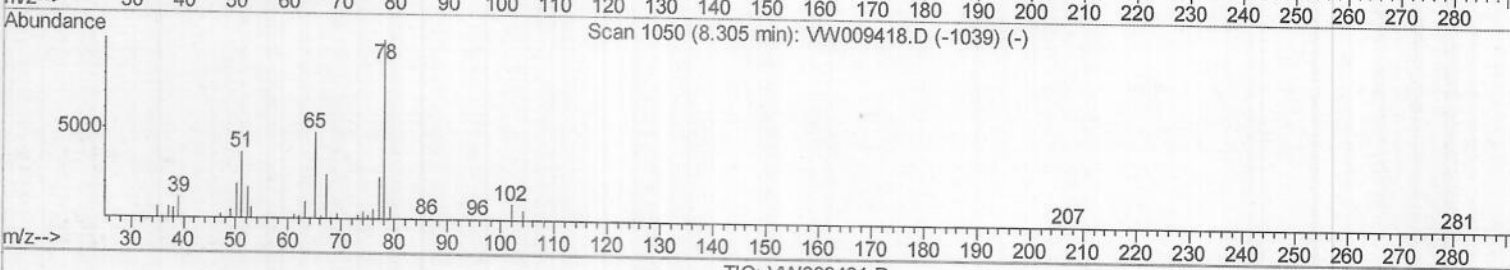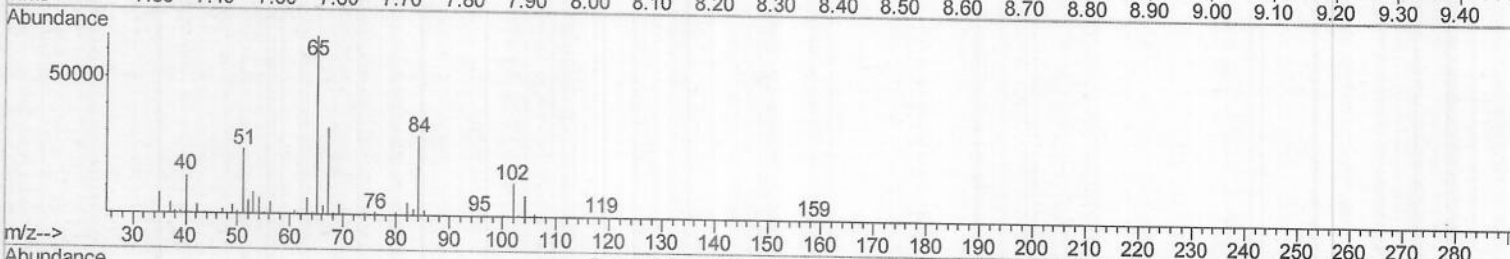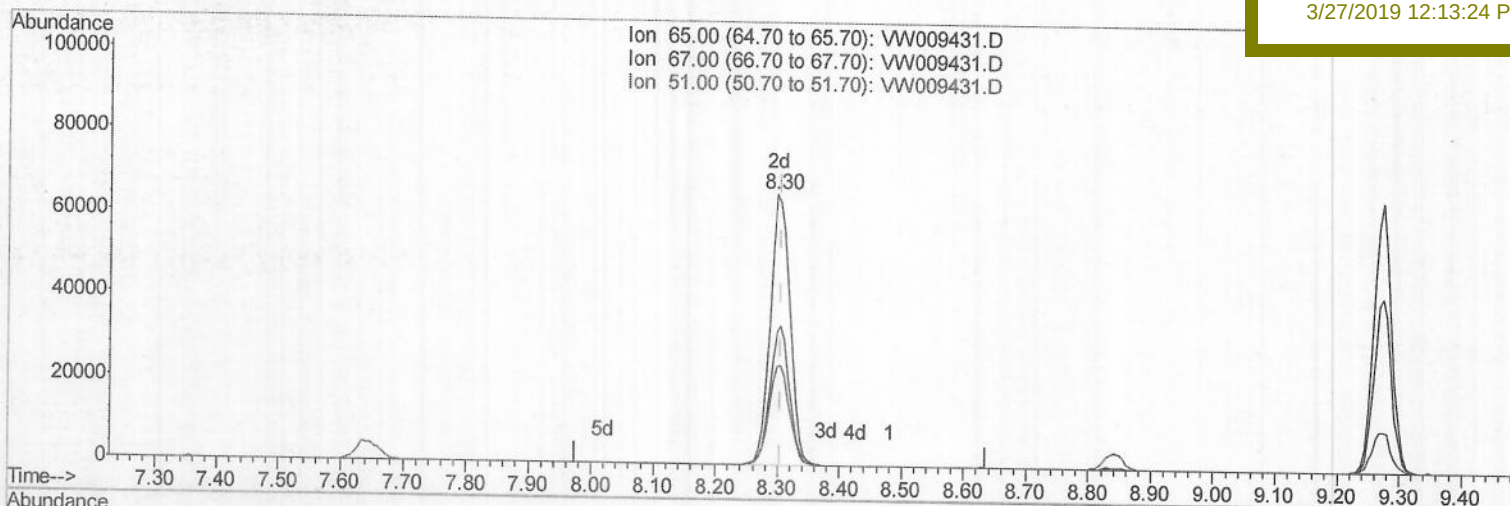

TIC: VW009431.D

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.006) 26.01ug/L m

response 145647

Ion Exp% Act%

65.00 100 100

67.00 50.80 0.02#

51.00 97.70 0.05#

0.00 0.00 0.00

m.d
4/5/14

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009431.D
 Acq On : 25 Mar 2019 16:35
 Operator : SY/VA
 Sample : K2031-21RE
 Misc : 4.11G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 09:01:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 07:46:05 2019
 Response via : Initial Calibration

Instrument :
 MSVOA_W
 Client Sampled :
 BF5X8RE

Manual Integrations
 APPROVED

MMDadoda
 3/27/2019 12:13:24 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	340559	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	303357	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	115166	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	88448	21.73	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	86.92%		
7) Chloroethane-d5	2.89	69	99365	20.87	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.48%		
10) 1,1-Dichloroethene-d2	4.01	63	142312	16.18	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	64.72%		
20) 2-Butanone-d5	7.08	46	103545	61.52	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	123.04%		
24) Chloroform-d	7.65	84	222752	23.97	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	95.88%		
26) 1,2-Dichloroethane-d4	8.30	65	145647m	26.01	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	104.04%		
29) Benzene-d6	8.27	84	400323	23.93	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	95.72%		
33) 1,2-Dichloropropane-d6	9.27	67	129690	25.81	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	103.24%		
37) Toluene-d8	10.32	98	328603	21.24	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	84.96%		
38) trans-1,3-Dichloropropene-	10.58	79	55319	21.92	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	87.68%		
39) 2-Hexanone-d5	10.93	63	72819	59.84	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	119.68%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	132531	26.78	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	107.12%		
61) 1,2-Dichlorobenzene-d4	13.86	152	104319	23.62	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	94.48%		

m.d
 4/5/19

Target Compounds

					Ovalue
13) Acetone	4.12	43	49924	36.172 ug/L	98
14) Carbon disulfide	4.38	76	38526	3.413 ug/L	97
16) Methylene chloride	4.92	84	19443	3.915 ug/L	95
21) 2-Butanone	7.17	43	13725	7.202 ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed