

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032519\
 Data File : VW009453.D
 Acq On : 26 Mar 2019 03:08
 Operator : SY/VA
 Sample : VIBLK16
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK16

Manual Integrations
 APPROVED

MMDadoda
 3/27/2019 12:15:34 PM

Quant Time: Mar 26 09:24:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 26 09:00:24 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	420598	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	424856	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	198753	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	80495	16.02	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.08%
7) Chloroethane-d5	2.89	69	94345	16.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.16%
10) 1,1-Dichloroethene-d2	4.01	63	135460	12.47	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.88%
20) 2-Butanone-d5	7.08	46	89964	43.28	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.56%
24) Chloroform-d	7.64	84	229290	19.98	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.92%
26) 1,2-Dichloroethane-d4	8.31	65	144142	20.85	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.40%
29) Benzene-d6	8.27	84	407261	17.38	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	69.52%
33) 1,2-Dichloropropane-d6	9.27	67	132681	18.85	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	75.40%
37) Toluene-d8	10.32	98	355791	16.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	65.68%
38) trans-1,3-Dichloropropene-	10.58	79	57249	16.20	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	64.80%
39) 2-Hexanone-d5	10.93	63	64727	37.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	141730	20.45	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.80%
61) 1,2-Dichlorobenzene-d4	13.86	152	148432	19.48	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	77.92%

Target Compounds				Ovalue
16) Methylene chloride	4.93	84	12571m	2.050 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032519\
Data File : VW009453.D
Acq On : 26 Mar 2019 03:08
Operator : SY/VA
Sample : VIBLK16
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK16

Manual Integrations
APPROVED

MMDadoda
3/27/2019 12:15:34 PM

Quant Time: Mar 26 09:24:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 26 09:00:24 2019
Response via : Initial Calibration

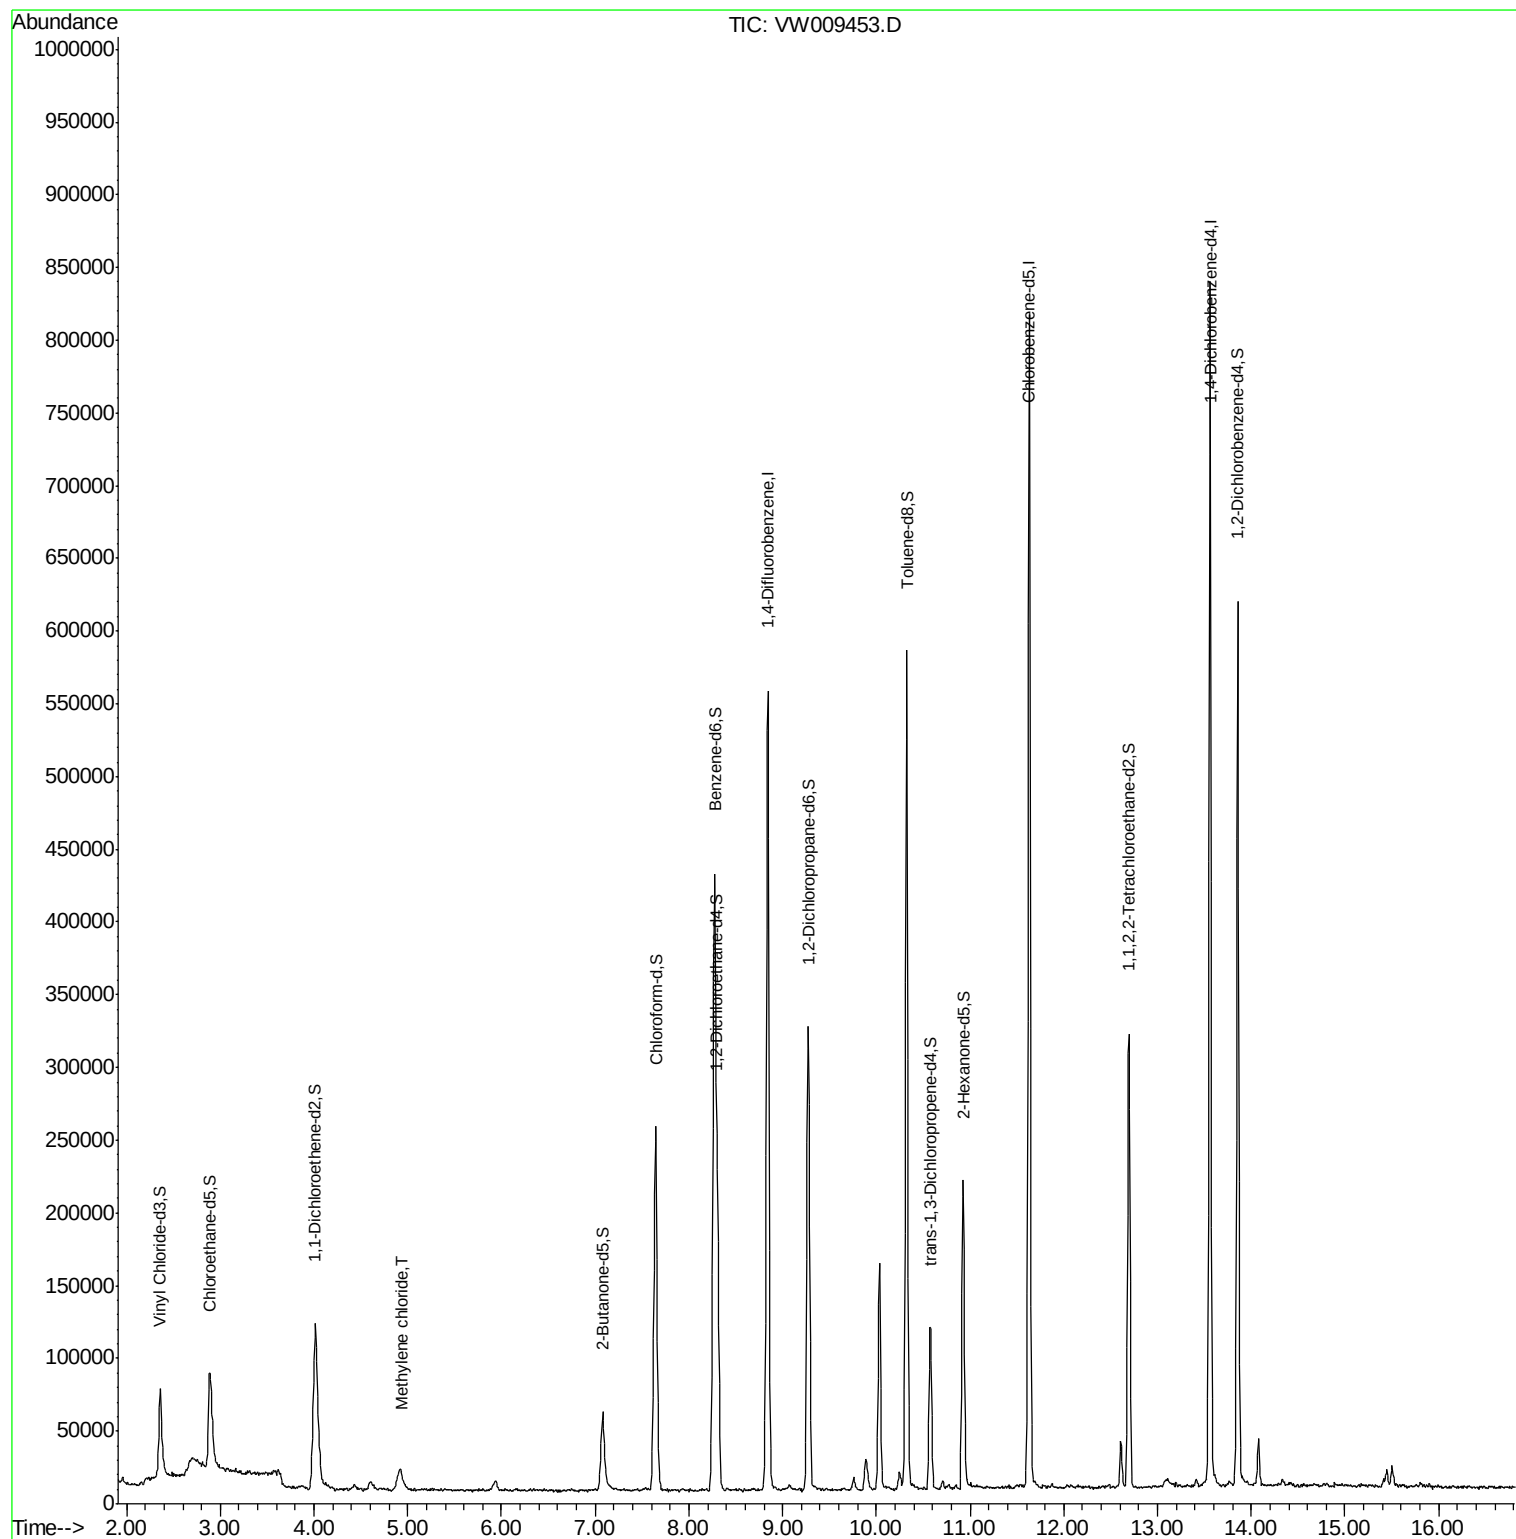

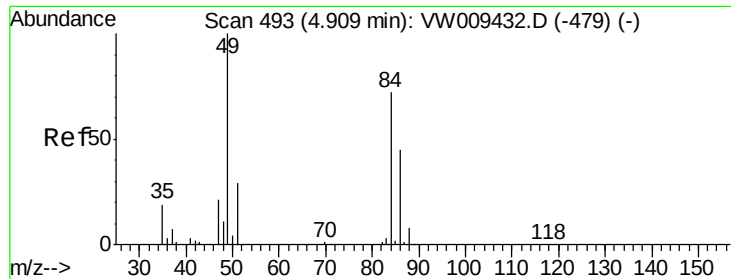

#16
Methylene chloride
Concen: 2.050 ug/L m
RT: 4.93 min Scan# 497
Delta R.T. 0.02 min
Lab File: VW009453.D
Acq: 26 Mar 2019 03:08

Instrument :
MSVOA_W
ClientSampleId :
VIBLK16

Tot Ion	Ratio	Lower	Upper
84	100		
49	93.4	96.0	178.2#
86	53.0	44.4	82.5

Manual Integrations
APPROVED

MMDadoda
3/27/2019 12:15:34 PM

