

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032520\
 Data File : VW015139.D
 Acq On : 25 Mar 2020 16:36
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Mar 26 05:17:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 26 05:02:00 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	549775	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	508523	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	183895	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	263185	27.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	110.88%
7) Chloroethane-d5	2.89	69	217833	27.82	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.28%
10) 1,1-Dichloroethene-d2	4.02	63	383276	20.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.32%
20) 2-Butanone-d5	7.07	46	121614	56.27	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.54%
24) Chloroform-d	7.65	84	434973	26.48	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	105.92%
26) 1,2-Dichloroethane-d4	8.49	65	117	0.01	ug/L	0.19
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.04%#
29) Benzene-d6	8.27	84	866621	26.63	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	106.52%
33) 1,2-Dichloropropane-d6	9.27	67	288523	26.69	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.76%
37) Toluene-d8	10.32	98	732085	26.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	105.56%
38) trans-1,3-Dichloropropene-	10.58	79	104623	25.28	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.12%
39) 2-Hexanone-d5	10.92	63	82484	51.65	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.30%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	190172	25.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.88%
61) 1,2-Dichlorobenzene-d4	13.85	152	184739	28.87	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	115.48%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	13.56	75	32063	5.616 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032520\
Data File : VW015139.D
Acq On : 25 Mar 2020 16:36
Operator : SY/VA
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Mar 26 05:17:31 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 26 05:02:00 2020
Response via : Initial Calibration

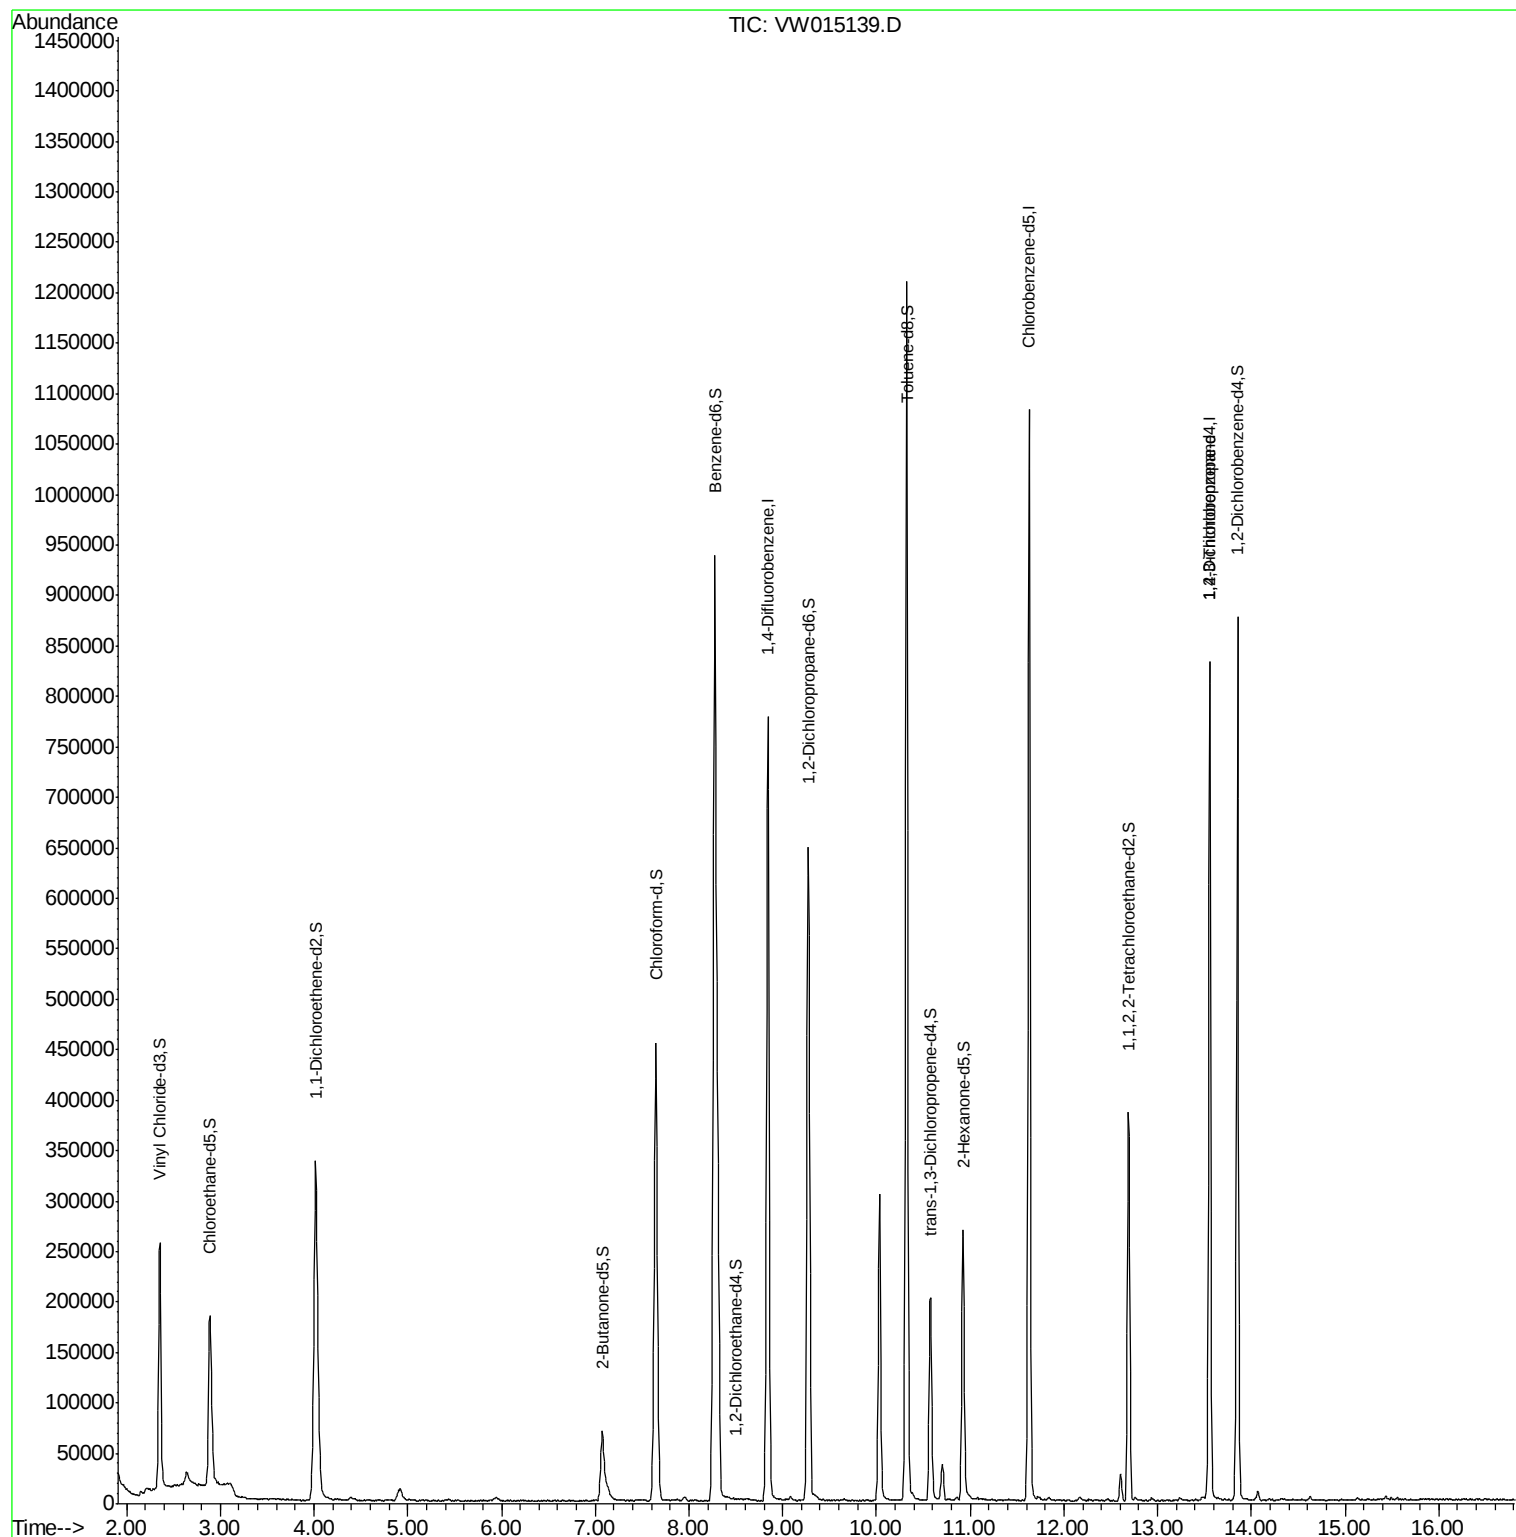

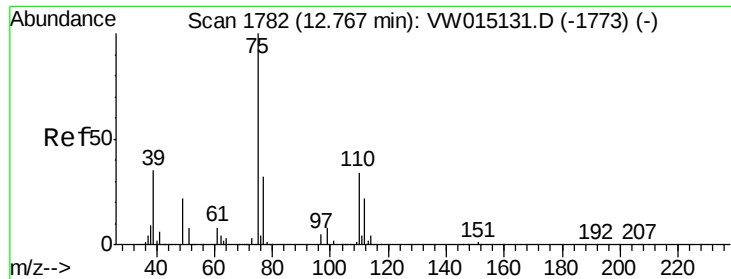

#59

1,2,3-Trichloropropane

Concen: 5.616 ug/L

RT: 13.56 min Scan# 1912

Delta R.T. 0.79 min

Lab File: VW015139.D

Acq: 25 Mar 2020 16:36

Instrument :

MSVOA_W

ClientSampleId :

Tot Ion: 75 Resp: 32063

Ion Ratio Lower Upper

75 100

77 36.2 25.8 38.6

