

(OT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032520\
Data File : VW015129.D
Acq On : 25 Mar 2020 09:37
Operator : SY/VA
Sample : VSTD2.503
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VSTD2.503

Manual Integrations APPROVED

apatel
4/15/2020 8:20:45 AM

Quant Time: Mar 25 14:03:45 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 25 13:57:31 2020
Response via : Initial Calibration

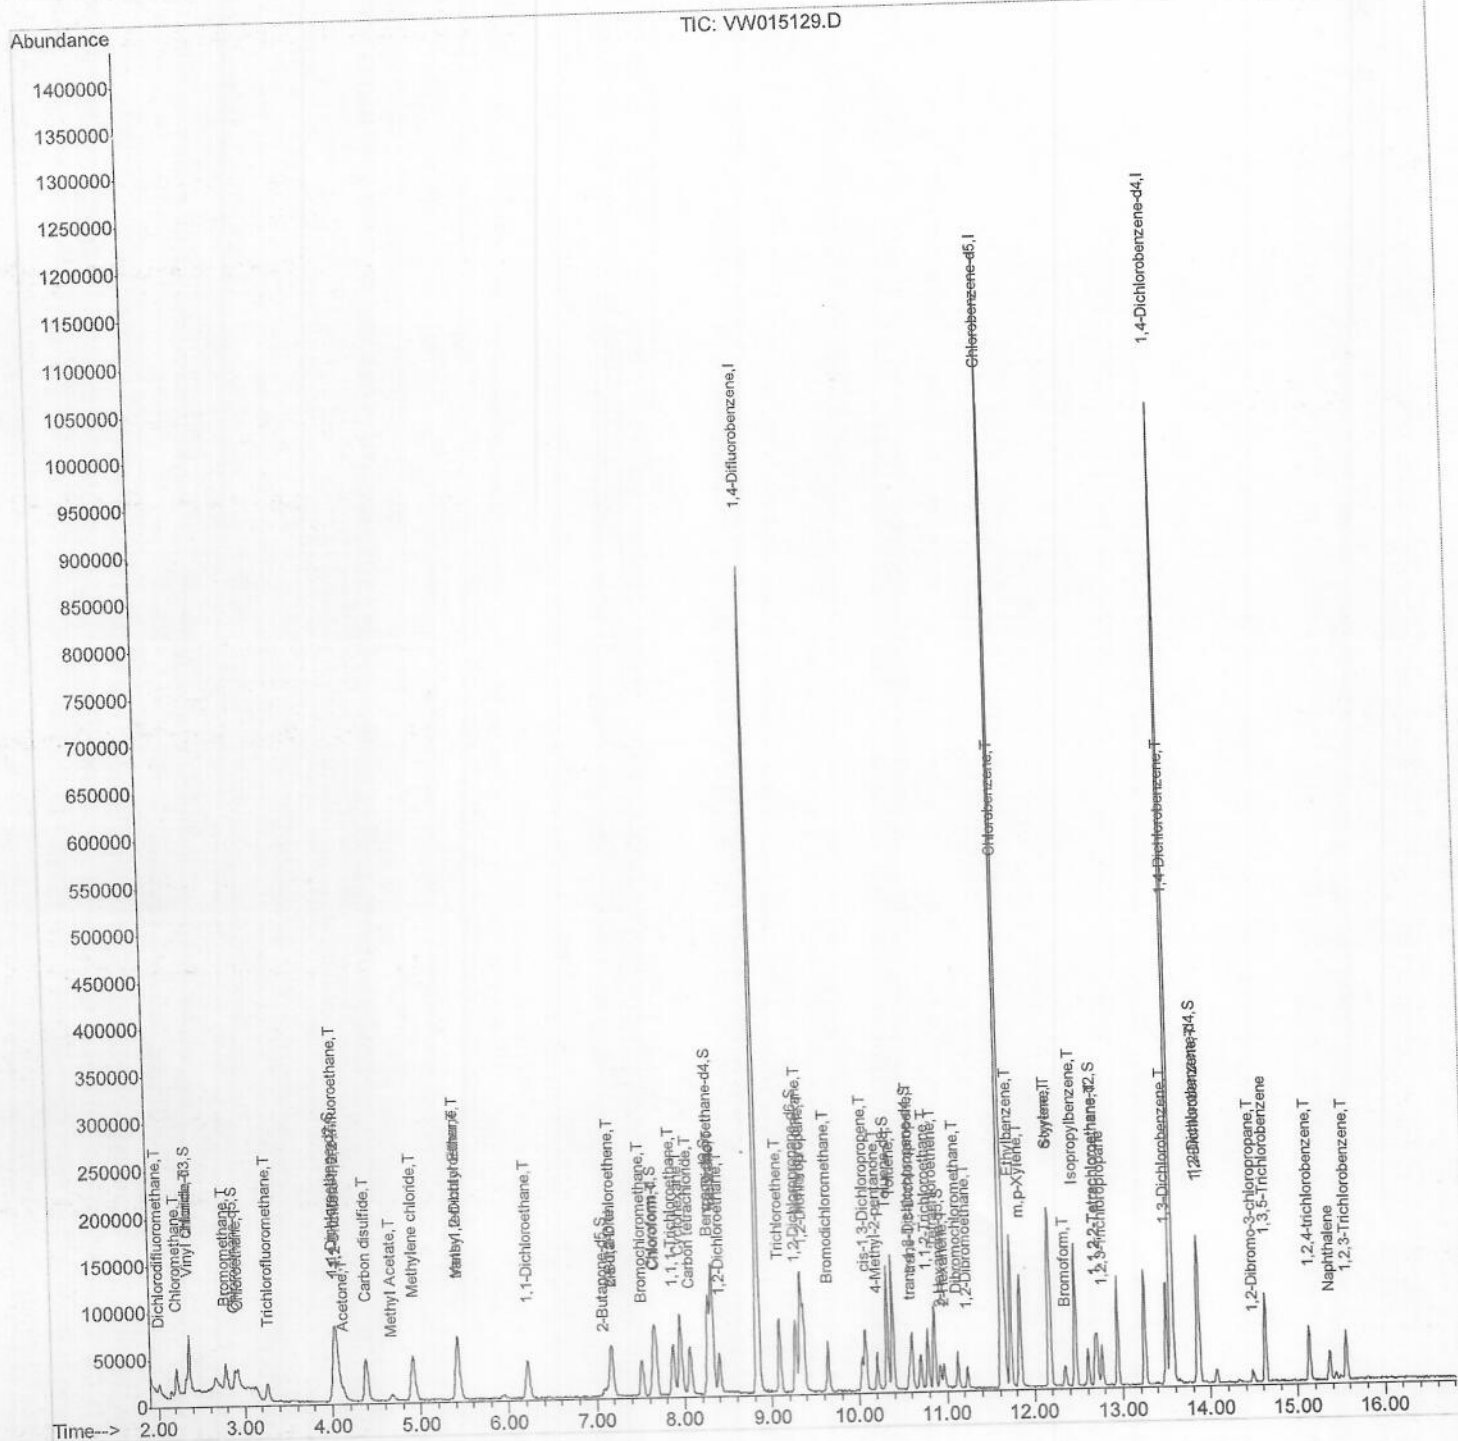

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032520\
 Data File : VW015129.D
 Acq On : 25 Mar 2020 09:37
 Operator : SY/VA
 Sample : VSTD2.503
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 VSTD2.503

Manual Integrations
 APPROVED

apatel
 4/15/2020 8:20:45 AM

Quant Time: Mar 25 13:59:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 25 13:57:31 2020
 Response via : Initial Calibration

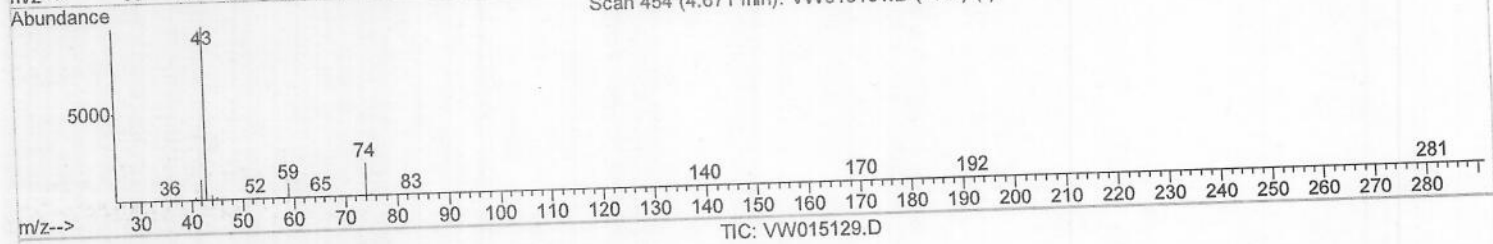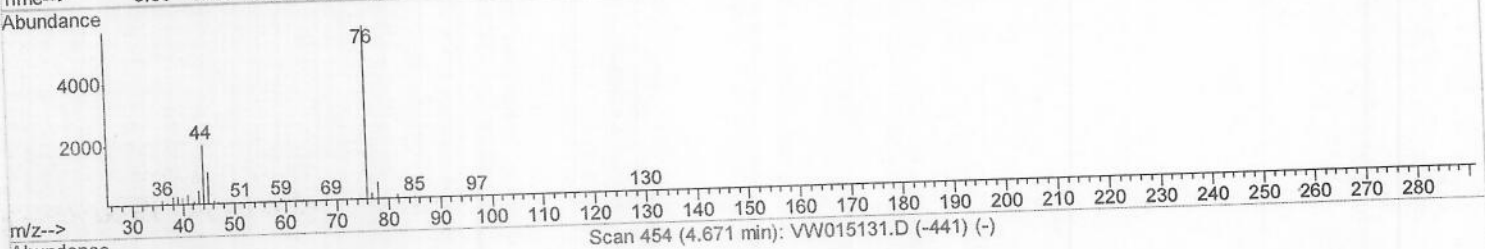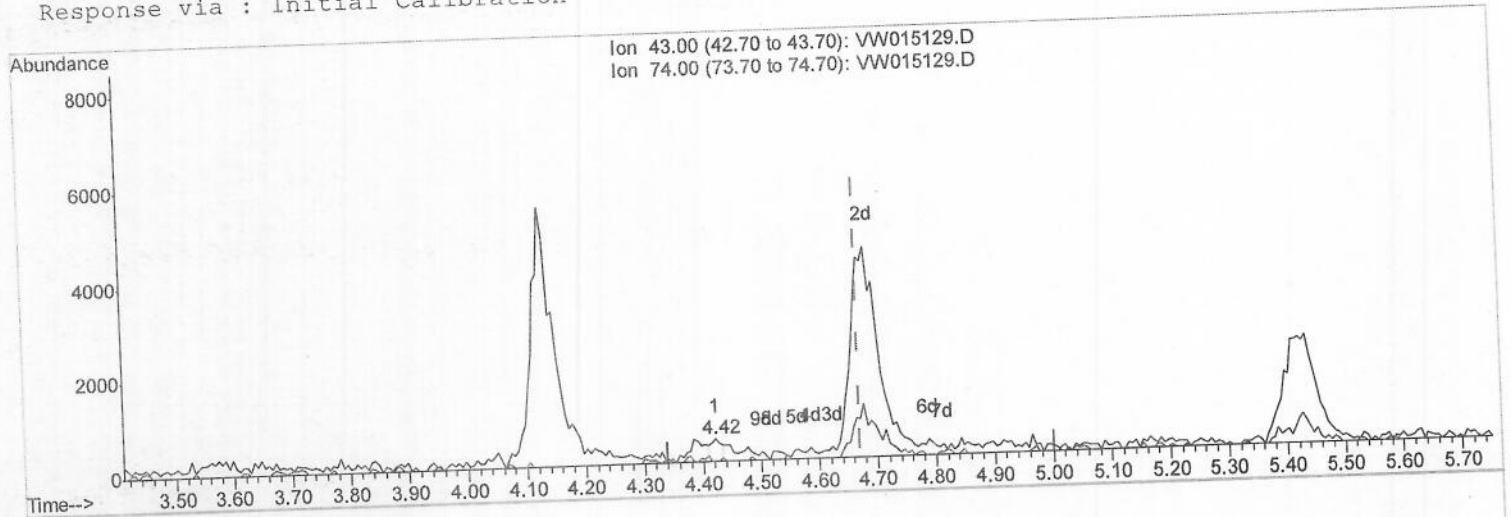

(15) Methyl Acetate (T)

4.422min (-0.250) 0.10ug/L

response 538

Ion	Exp%	Act%
43.00	100	100
74.00	19.40	18.22
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032520\
 Data File : VW015129.D
 Acq On : 25 Mar 2020 09:37
 Operator : SY/VA
 Sample : VSTD2.503
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 VSTD2.503

Manual Integrations
 APPROVED

apatel
 4/15/2020 8:20:45 AM

Quant Time: Mar 25 14:03:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 25 13:57:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	632159	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	565737	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	227483	25.00	ug/L	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) Vinyl Chloride-d3	2.35	65	31250	2.12	ug/L	0.00
7) Chloroethane-d5	2.89	69	24689	2.27	ug/L	0.00
10) 1,1-Dichloroethene-d2	4.02	63	59682	2.51	ug/L	0.00
20) 2-Butanone-d5	7.09	46	11607	4.52	ug/L	0.00
24) Chloroform-d	7.65	84	53939	2.69	ug/L	0.00
26) 1,2-Dichloroethane-d4	8.31	65	32128	2.85	ug/L	0.00
29) Benzene-d6	8.27	84	100781	2.70	ug/L	0.00
33) 1,2-Dichloropropane-d6	9.27	67	34043	2.72	ug/L	0.00
37) Toluene-d8	10.32	98	80181	2.57	ug/L	0.00
38) trans-1,3-Dichloropropene	10.58	79	12403	2.67	ug/L	0.00
39) 2-Hexanone-d5	10.92	63	7862	4.68	ug/L	0.00
48) 1,1,2,2-Tetrachloroethane	12.69	84	23436	2.86	ug/L	0.00
61) 1,2-Dichlorobenzene-d4	13.85	152	22574	2.80	ug/L	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	2.01	85	12897	2.428	ug/L	98
3) Chloromethane	2.21	50	27894	2.374	ug/L	99
5) Vinyl chloride	2.36	62	35814	2.340	ug/L	99
6) Bromomethane	2.78	94	19624	2.754	ug/L	96
8) Chloroethane	2.93	64	20982	2.464	ug/L	100
9) Trichlorofluoromethane	3.26	101	17840	2.499	ug/L	98
11) 1,1,2-Trichloro-1,2,2-trif	4.06	101	25833	2.622	ug/L #	73
12) 1,1-Dichloroethene	4.04	96	24689	2.641	ug/L	97
13) Acetone	4.13	43	11945	4.161	ug/L	88
14) Carbon disulfide	4.38	76	91861	2.603	ug/L	97
15) Methyl Acetate	4.68	43	14564m	2.788	ug/L	95
16) Methylene chloride	4.92	84	32562	2.811	ug/L	89
17) Methyl tert-butyl Ether	5.42	73	29140	2.528	ug/L #	98
18) trans-1,2-Dichloroethene	5.42	96	25830	2.664	ug/L	99
19) 1,1-Dichloroethane	6.21	63	55975	2.601	ug/L	95
21) 2-Butanone	7.18	43	15568	4.422	ug/L	97
22) cis-1,2-Dichloroethene	7.17	96	24009	2.448	ug/L	91
23) Bromochloromethane	7.51	128	11026	2.858	ug/L	100
25) Chloroform	7.68	83	50398	2.575	ug/L	100
27) 1,2-Dichloroethane	8.40	62	36380	2.693	ug/L	98
30) Cyclohexane	7.95	56	40114	2.153	ug/L	97
31) 1,1,1-Trichloroethane	7.87	97	39327	2.703	ug/L	100
32) Carbon tetrachloride	8.07	117	34110	2.629	ug/L	100
34) Benzene	8.32	78	106604	2.562	ug/L	98
35) Trichloroethene	9.09	95	26968	2.658	ug/L	96
36) Methylcyclohexane	9.34	83	40175	2.324	ug/L	98
40) 1,2-Dichloropropane	9.37	63	30734	2.660	ug/L	96
41) Bromodichloromethane	9.65	83	34911	2.678	ug/L	97
42) cis-1,3-Dichloropropene	10.07	75	35095	2.333	ug/L	95
43) 4-Methyl-2-pentanone	10.21	43	28512	4.394	ug/L	95

MD
 04/15/2020

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032520\
 Data File : VW015129.D
 Acq On : 25 Mar 2020 09:37
 Operator : SY/VA
 Sample : VSTD2.503
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VSTD2.503

Manual Integrations
 APPROVED

apatel
 4/15/2020 8:20:45 AM

Quant Time: Mar 25 13:59:23 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 25 13:57:31 2020
 Response via : Initial Calibration

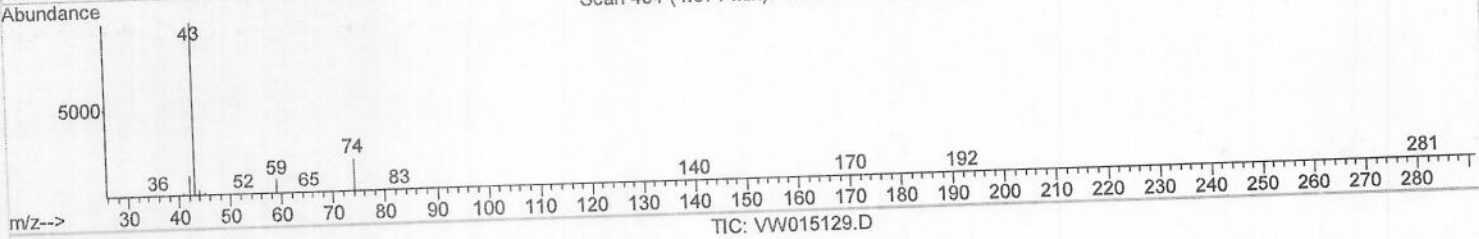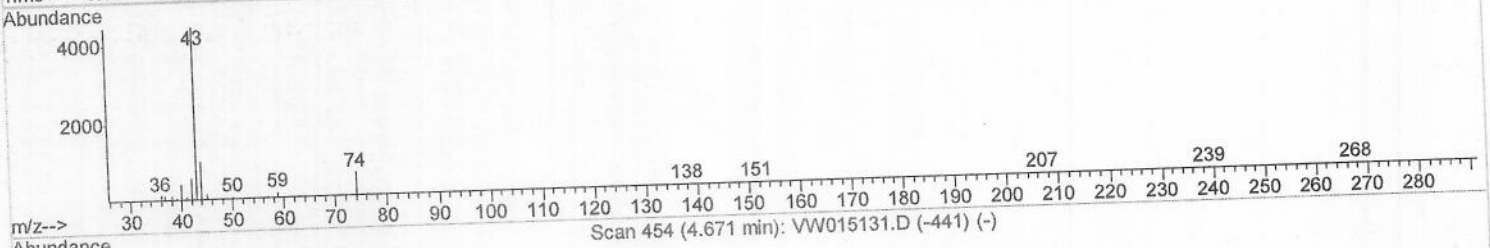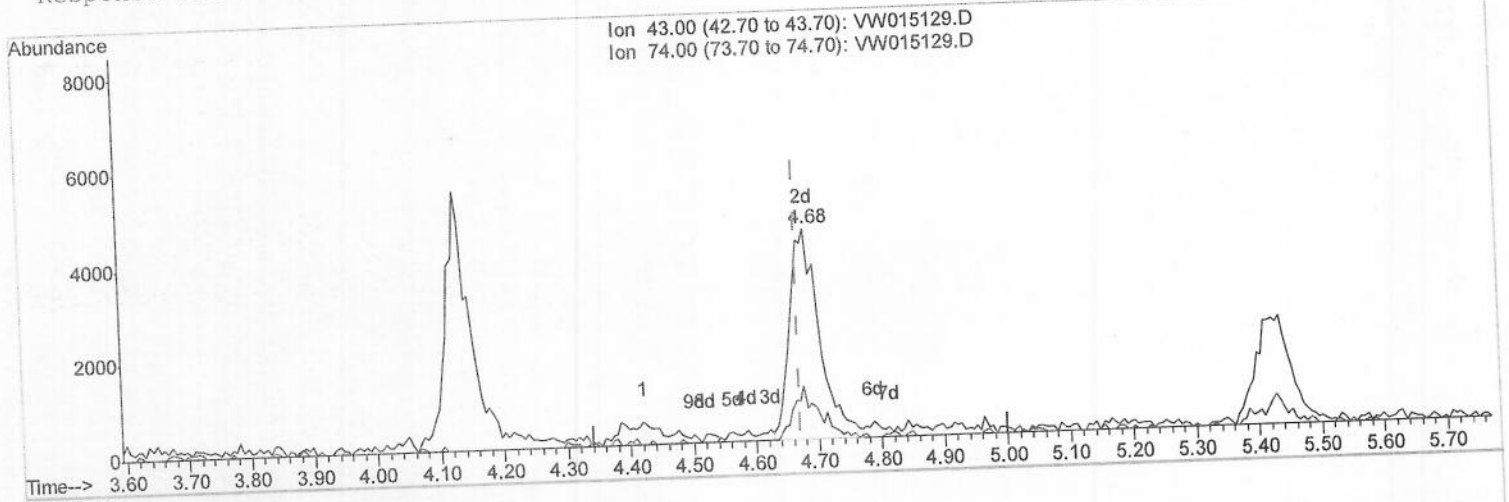

(15) Methyl Acetate (T)

4.684min (+0.013) 2.79ug/L m

response 14564

Ion	Exp%	Act%
43.00	100	100
74.00	19.40	0.67#
0.00	0.00	0.00
0.00	0.00	0.00

MD
 04/15/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032520\
 Data File : VW015129.D
 Acq On : 25 Mar 2020 09:37
 Operator : SY/VA
 Sample : VSTD2.503
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 VSTD2.503

Manual Integrations
 APPROVED

apatel
 4/15/2020 8:20:45 AM

Quant Time: Mar 25 14:03:45 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 25 13:57:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QI	Ion	Response	Conc	Units	Dev(Min)
44) Toluene	10.38	91		97843	2.415	ug/L	98
45) trans-1,3-Dichloropropene	10.60	75		31288	2.526	ug/L	99
46) 1,1,2-Trichloroethane	10.79	97		18339	2.785	ug/L	97
47) Tetrachloroethene	10.86	164		17693	2.714	ug/L	93
49) 2-Hexanone	10.97	43		16054	3.464	ug/L	96
50) Dibromochloromethane	11.13	129		17421	2.503	ug/L	92
51) 1,2-Dibromoethane	11.23	107		15703	2.733	ug/L	96
52) Chlorobenzene	11.65	112		64300	2.692	ug/L	98
53) Ethylbenzene	11.73	91		102468	2.310	ug/L	100
54) m,p-Xylene	11.83	106		34314	2.214	ug/L	98
55) o-xylene	12.16	106		31237	2.156	ug/L	88
56) Styrene	12.18	104		51619	2.086	ug/L	98
57) Isopropylbenzene	12.46	105		84391	2.137	ug/L	99
58) 1,1,2,2-Tetrachloroethane	12.71	83		21793	2.620	ug/L #	98
59) 1,2,3-Trichloropropane	12.77	75		16266	2.550	ug/L	91
62) Bromoform	12.35	173		8673	2.707	ug/L #	97
63) 1,3-Dichlorobenzene	13.50	146		37961	2.581	ug/L	95
64) 1,4-Dichlorobenzene	13.58	146		40461	2.664	ug/L	99
65) 1,2-Dichlorobenzene	13.87	146		35266	2.638	ug/L	98
66) 1,2-Dibromo-3-chloropropan	14.48	75		3579	3.004	ug/L	92
67) 1,3,5-Trichlorobenzene	14.63	180		24654	2.530	ug/L	96
68) 1,2,4-trichlorobenzene	15.13	180		15680	2.179	ug/L	98
69) Naphthalene	15.36	128		24065	2.960	ug/L	99
70) 1,2,3-Trichlorobenzene	15.55	180		15145	2.338	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed