


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
Data File : VW009475.D
Acq On : 26 Mar 2019 20:54
Operator : SY/VA
Sample : K2068-01
Misc : 5.36G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF5M0

Manual Integrations
APPROVED

apatel
4/12/2019 8:30:45 AM

Quant Time: Mar 27 08:30:32 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 08:01:36 2019
Response via : Initial Calibration

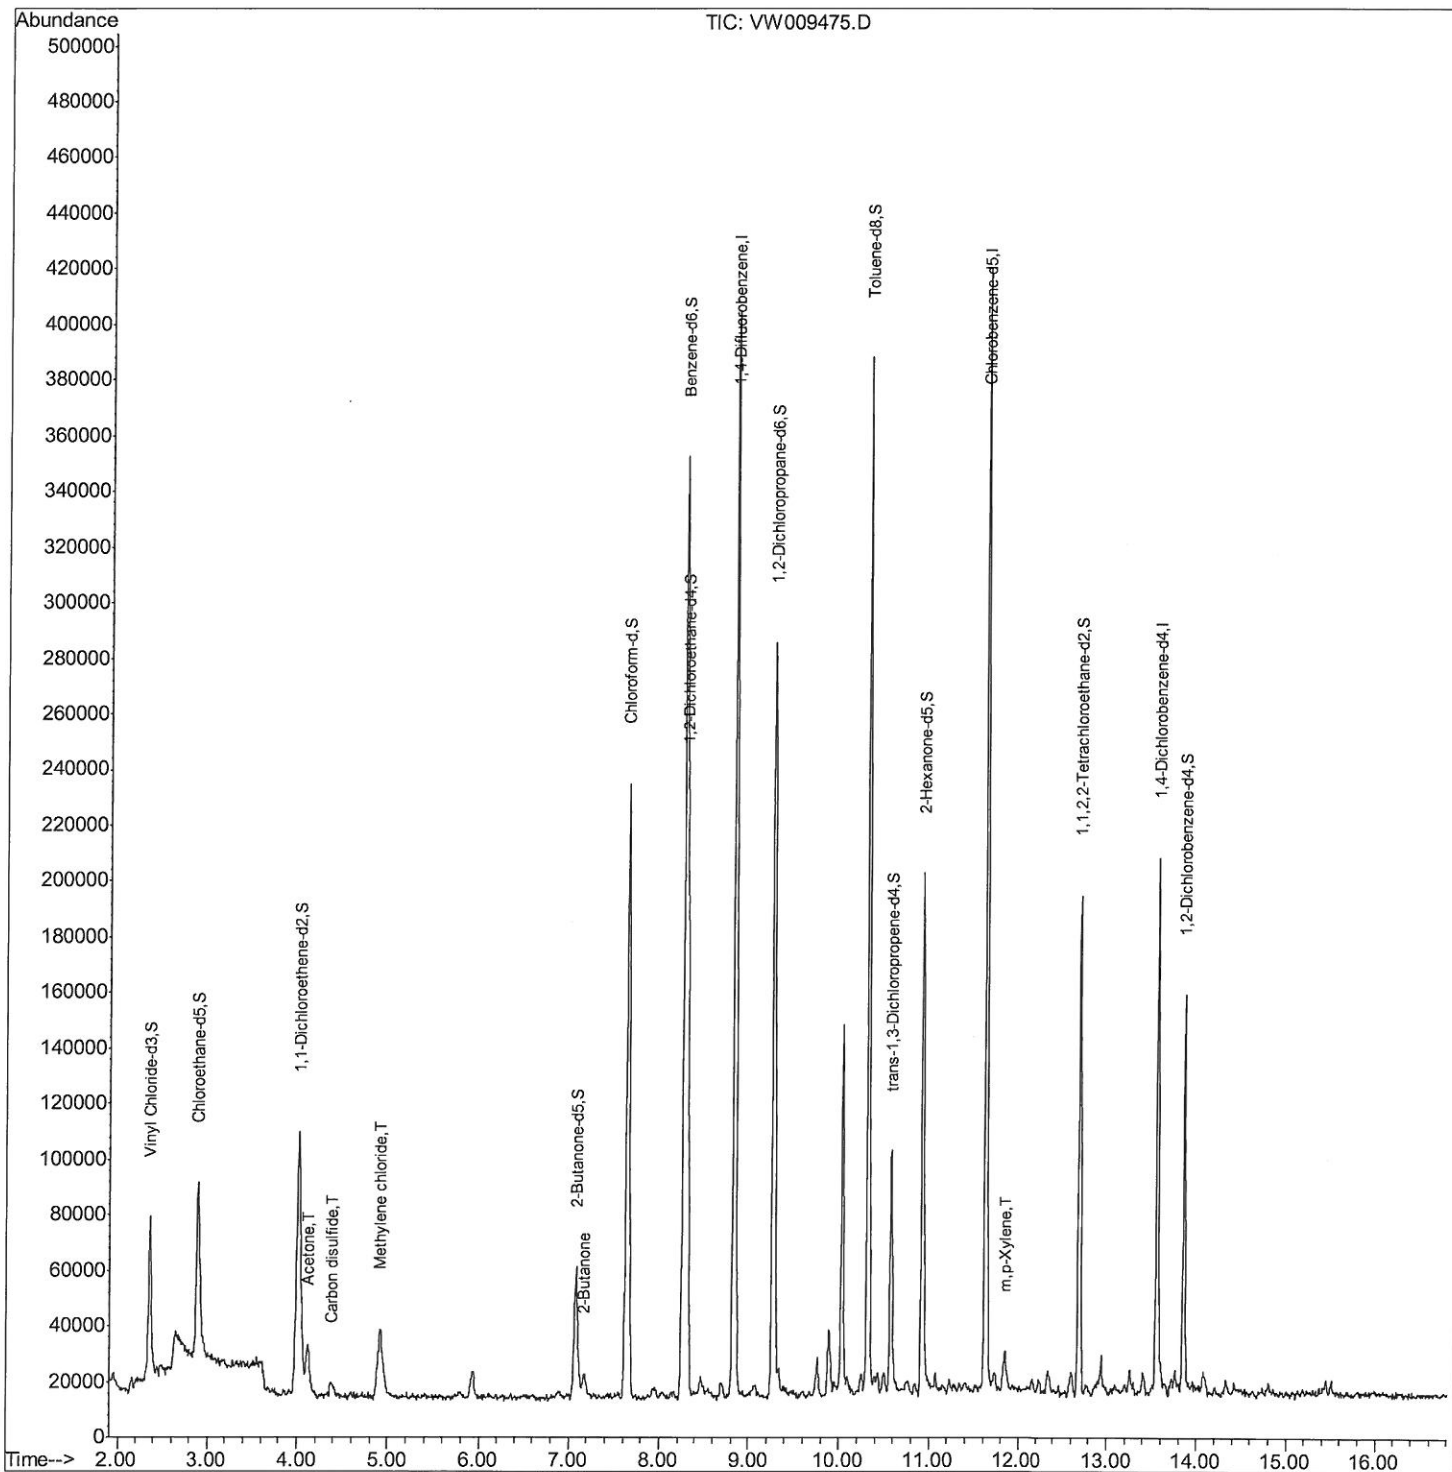

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009475.D
 Acq On : 26 Mar 2019 20:54
 Operator : SY/VA
 Sample : K2068-01
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 BF5M0

Manual Integrations
APPROVED

apatel
 4/12/2019 8:30:45 AM

Quant Time: Mar 27 08:07:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

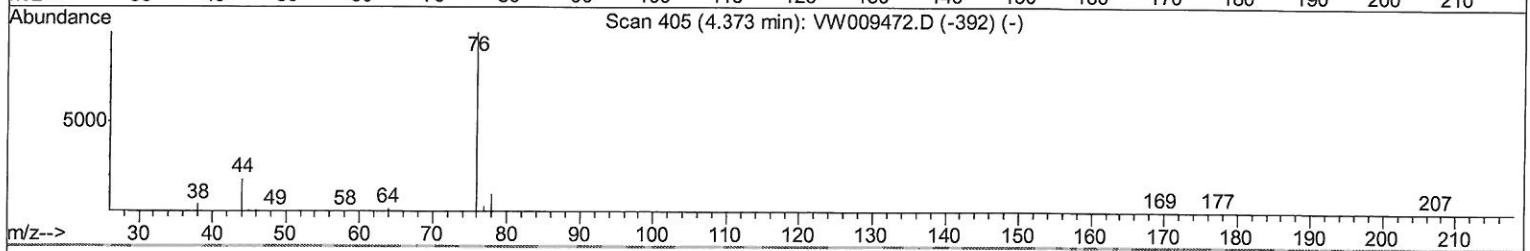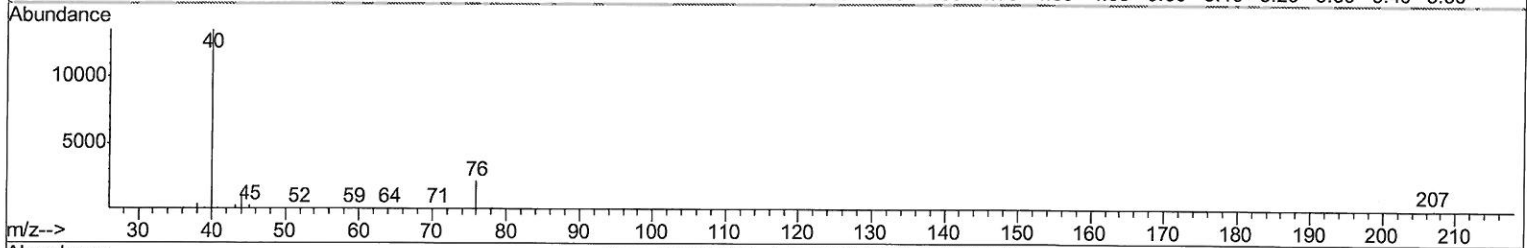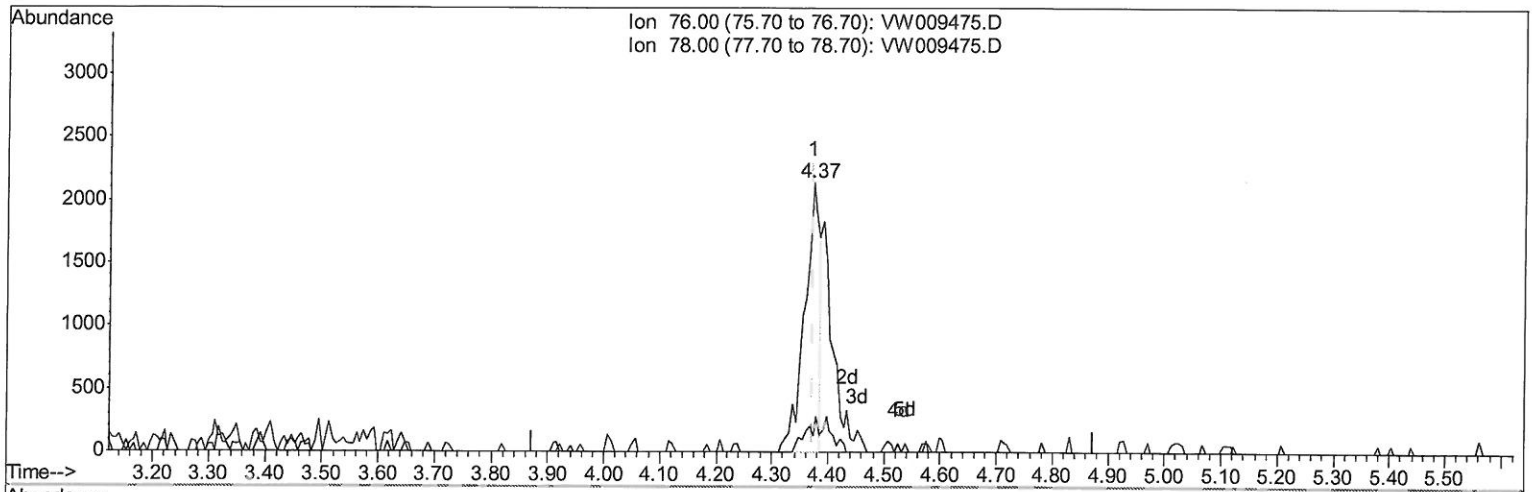

TIC: VW009475.D

(14) Carbon disulfide (T)

4.373min (0.000) 0.40ug/L

response 4093

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	5.84#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009475.D
 Acq On : 26 Mar 2019 20:54
 Operator : SY/VA
 Sample : K2068-01
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5M0

Manual Integrations
 APPROVED

apatel
 4/12/2019 8:30:45 AM

Quant Time: Mar 27 08:07:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

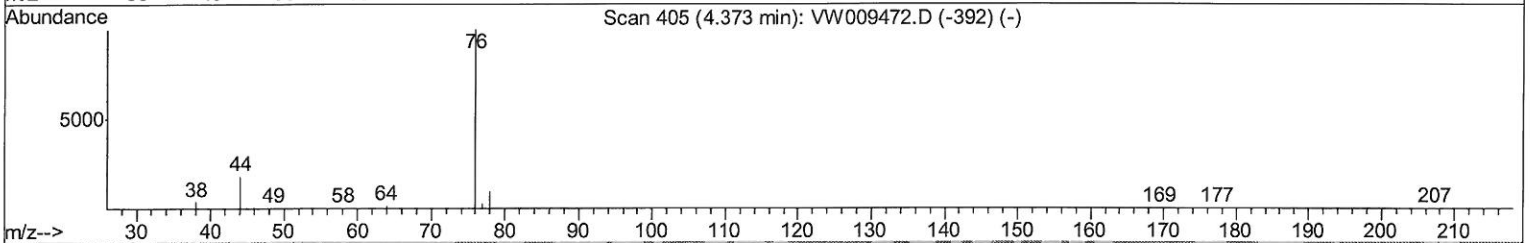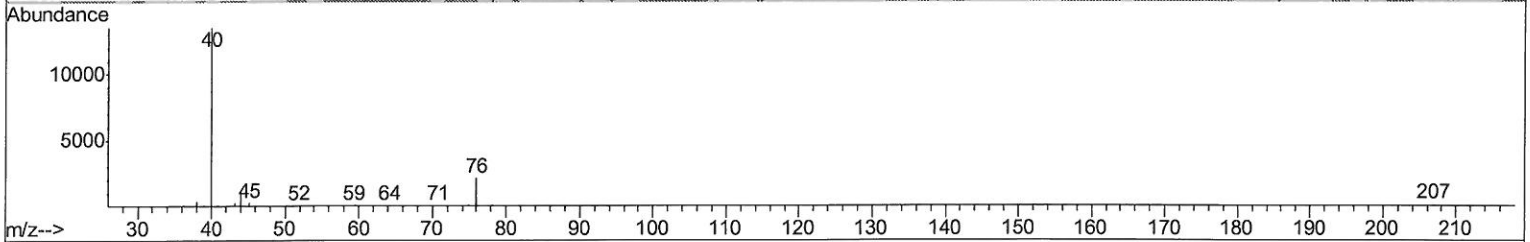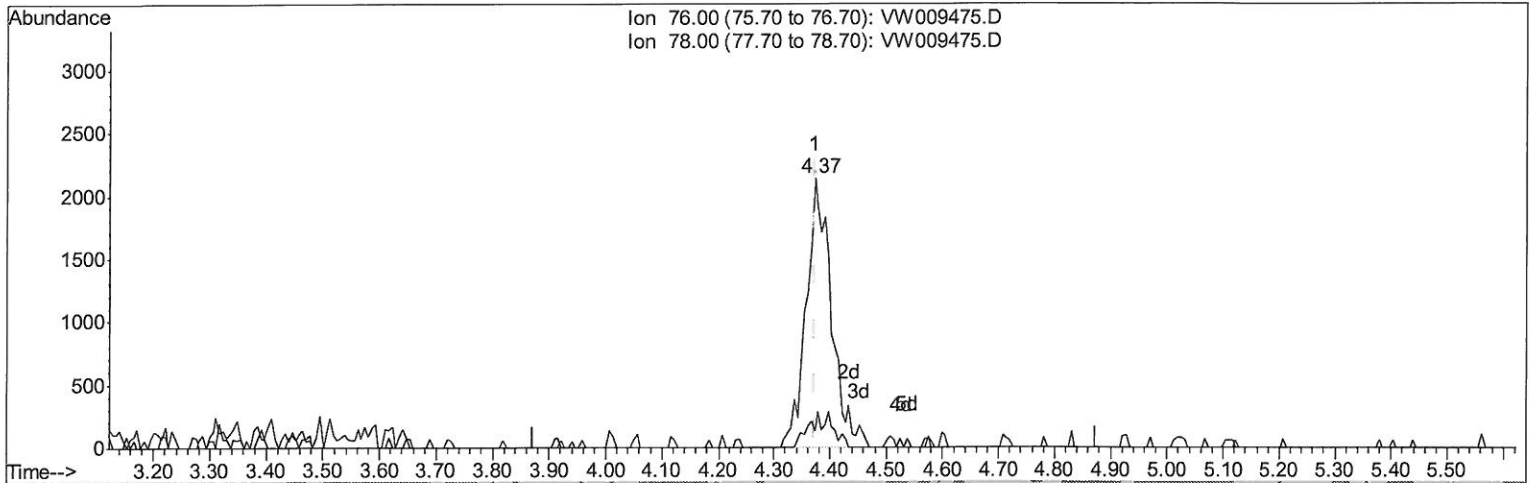

TIC: VW009475.D

(14) Carbon disulfide (T)

4.373min (0.000) 0.65ug/L m

response 6672

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	5.84#
0.00	0.00	0.00
0.00	0.00	0.00

> M/L
4/6/19

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009475.D
 Acq On : 26 Mar 2019 20:54
 Operator : SY/VA
 Sample : K2068-01
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BF5M0

Manual Integrations
APPROVED

apatel
 4/12/2019 8:30:45 AM

Quant Time: Mar 27 08:07:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

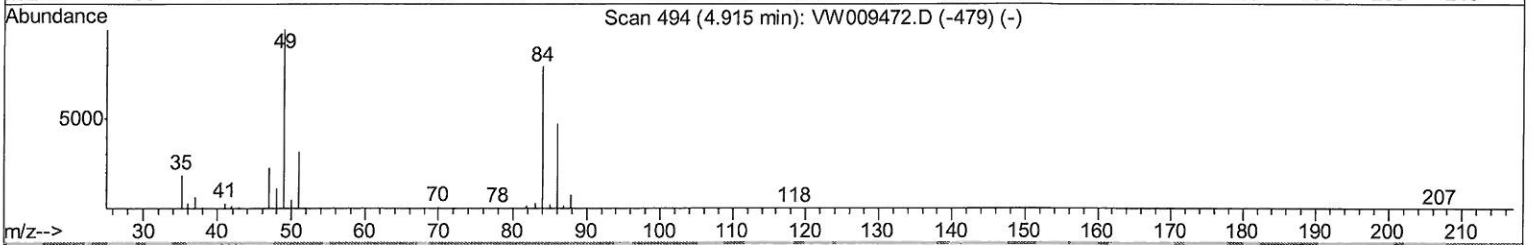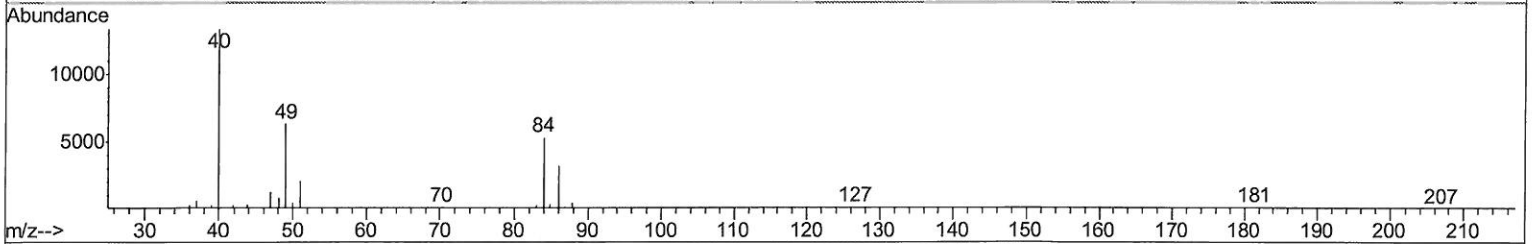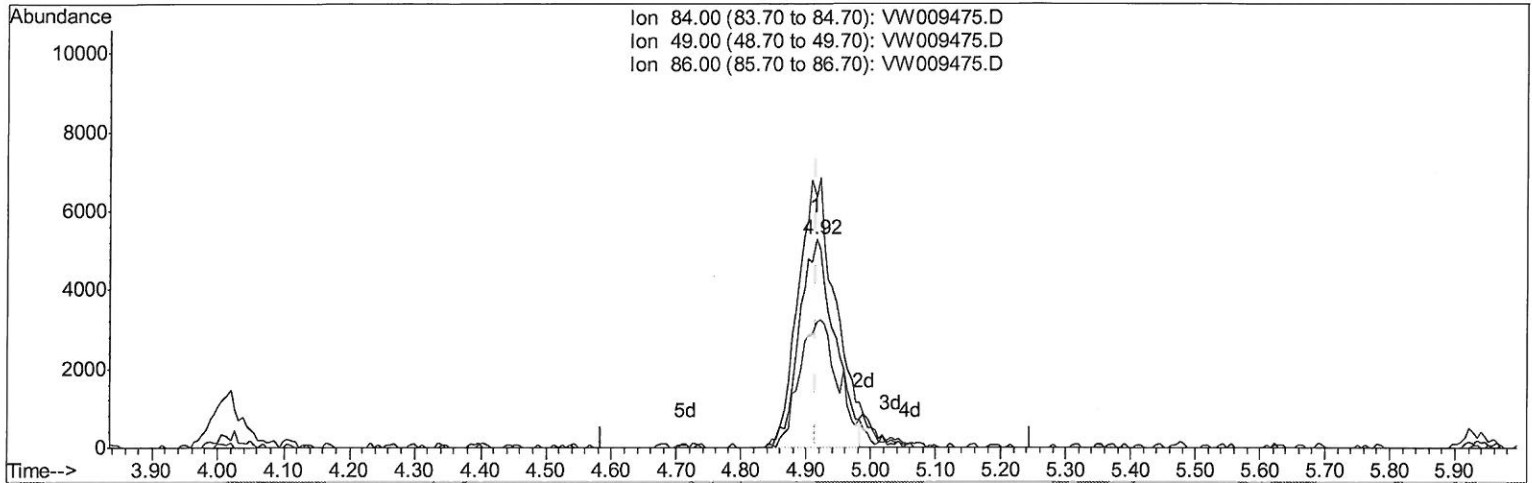

TIC: VW009475.D

(16) Methylene chloride (T)

4.915min (0.000) 4.49ug/L

response 20121

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	120.04
86.00	63.50	60.27
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009475.D
 Acq On : 26 Mar 2019 20:54
 Operator : SY/VA
 Sample : K2068-01
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5M0

Manual Integrations
 APPROVED

apatel
 4/12/2019 8:30:45 AM

Quant Time: Mar 27 08:07:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

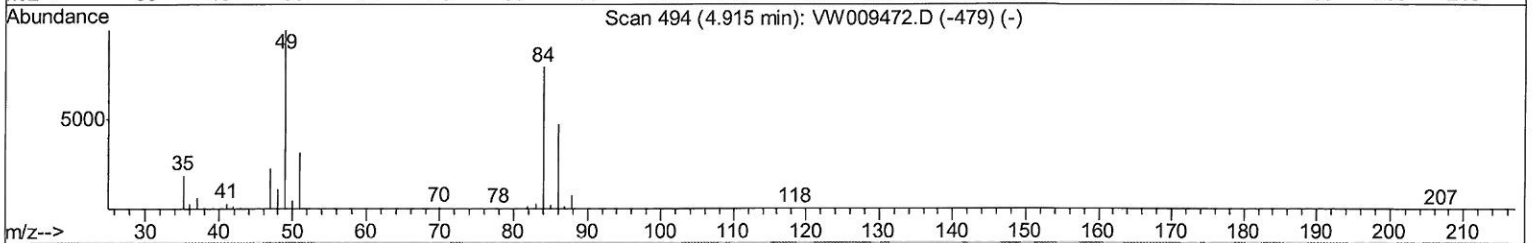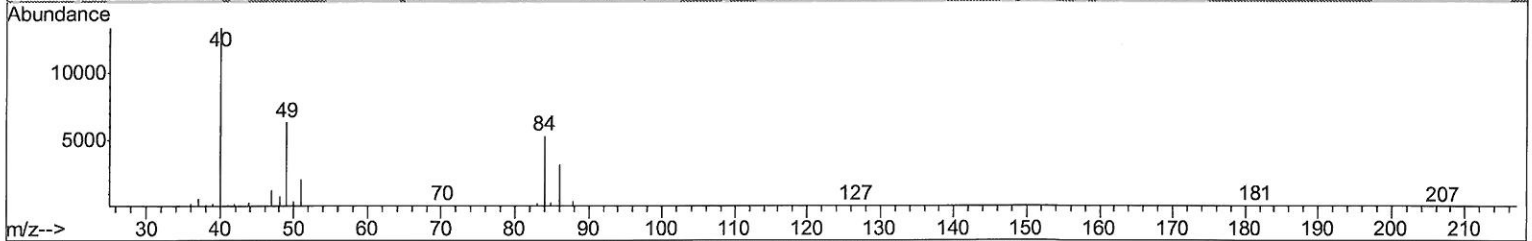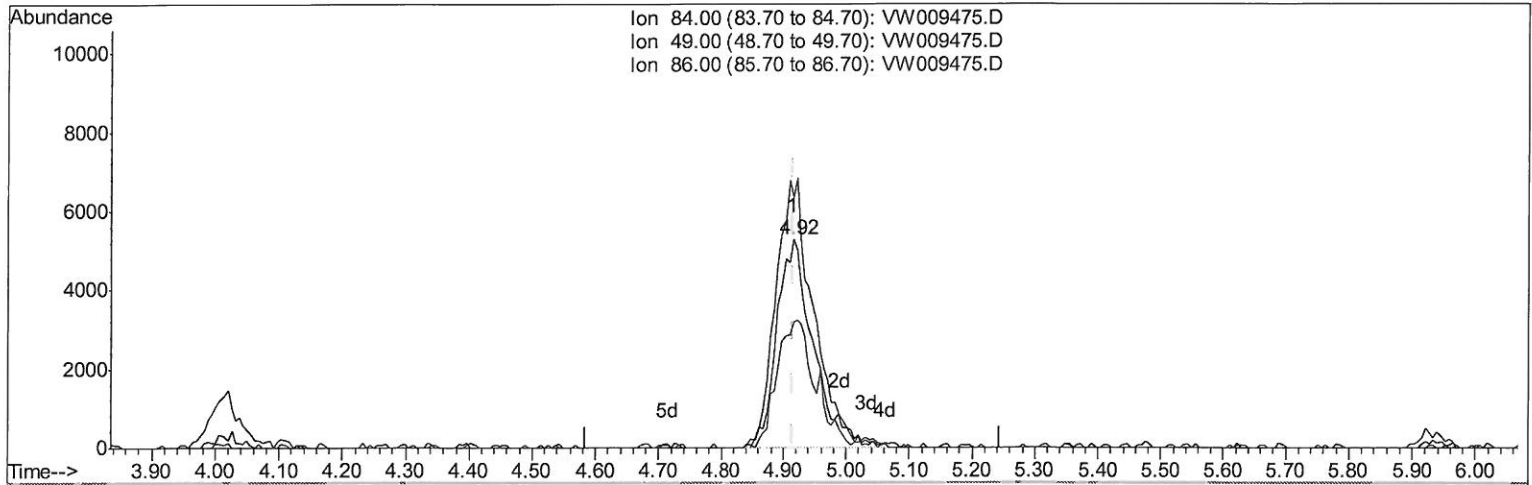

TIC: VW009475.D

(16) Methylene chloride (T)

4.915min (0.000) 4.78ug/L m

response 21432

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	120.04
86.00	63.50	60.27
0.00	0.00	0.00

Handwritten: > MO
 4/6/19

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009475.D
 Acq On : 26 Mar 2019 20:54
 Operator : SY/VA
 Sample : K2068-01
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BF5M0

Manual Integrations
 APPROVED

apatel
 4/12/2019 8:30:45 AM

Quant Time: Mar 27 08:07:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

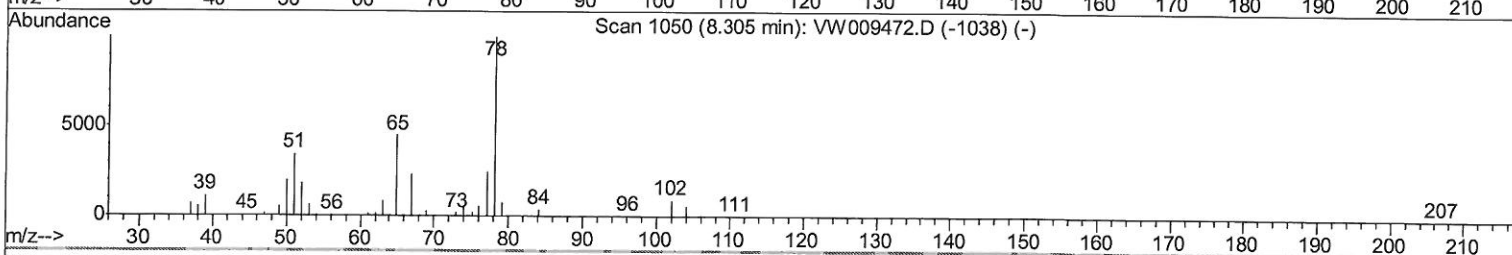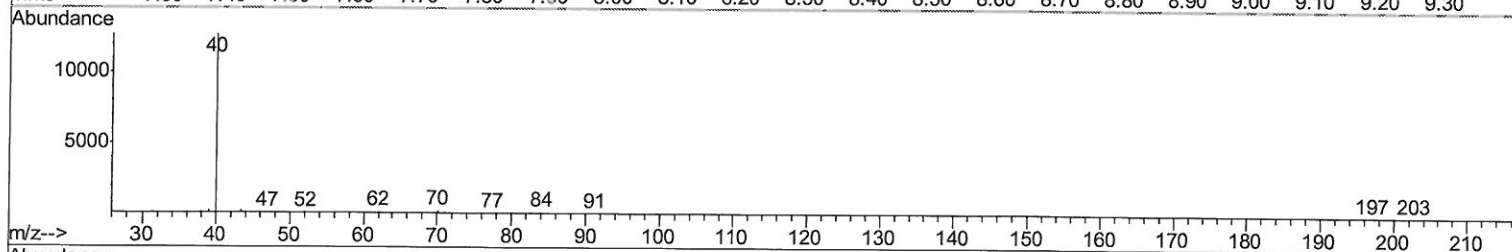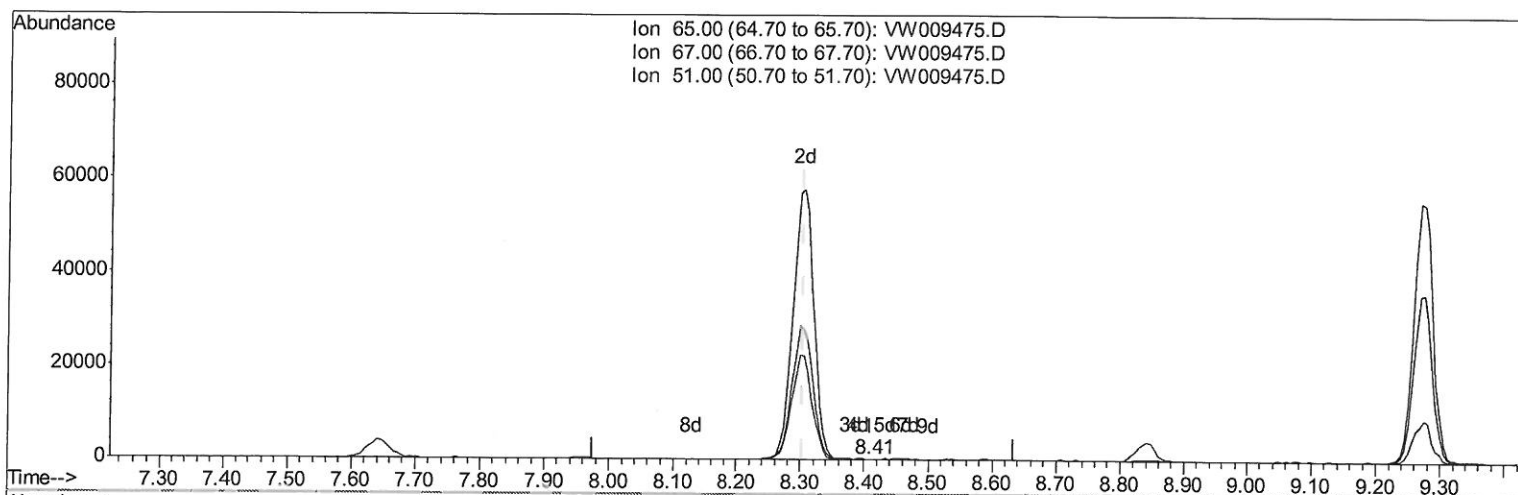

TIC: VW009475.D

(26) 1,2-Dichloroethane-d4 (S)

8.409min (+0.104) 0.01ug/L

response 74

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	48.65
51.00	97.70	93.24
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009475.D
 Acq On : 26 Mar 2019 20:54
 Operator : SY/VA
 Sample : K2068-01
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5M0

Manual Integrations
 APPROVED

apatel
 4/12/2019 8:30:45 AM

Quant Time: Mar 27 08:07:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

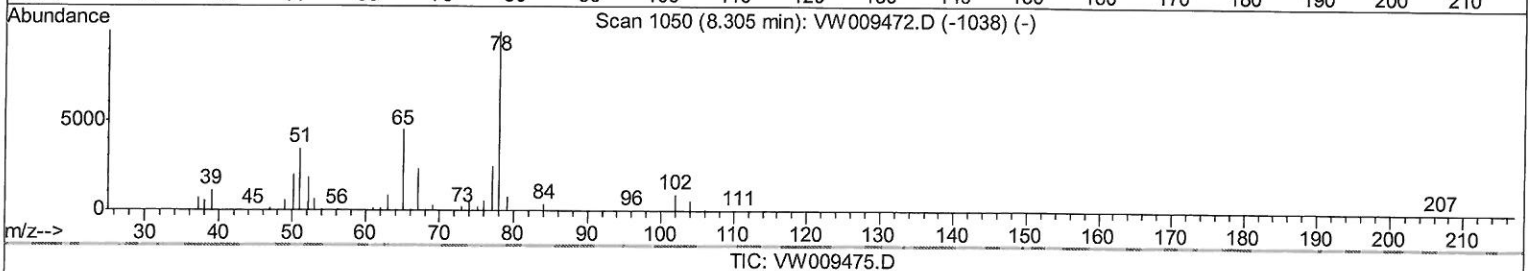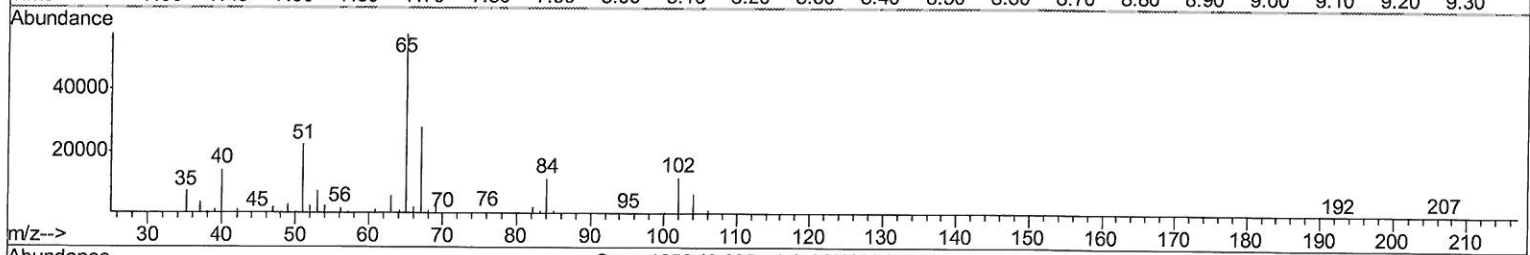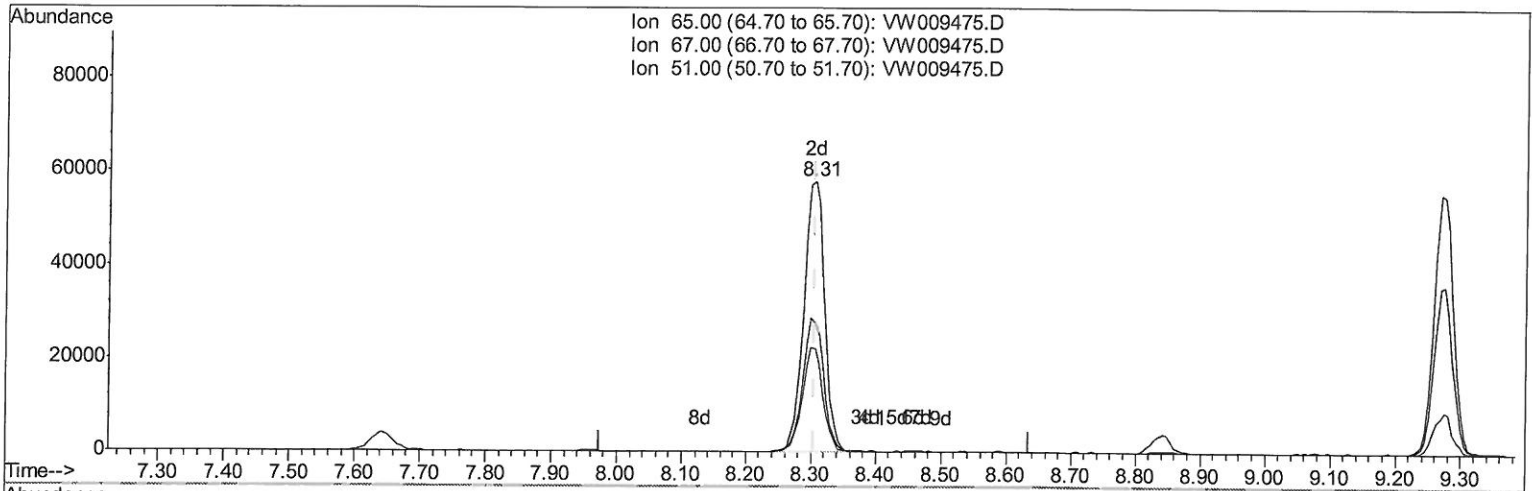

(26) 1,2-Dichloroethane-d4 (S)

8.305min (-0.000) 25.57ug/L m

response 129243

Ion	Exp%	Act%
65.00	100	100
67.00	50.80	0.03#
51.00	97.70	0.05#
0.00	0.00	0.00

Handwritten:
 7M0
 4/6/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009475.D
 Acq On : 26 Mar 2019 20:54
 Operator : SY/VA
 Sample : K2068-01
 Misc : 5.36G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5M0

Manual Integrations
 APPROVED

apatel
 4/12/2019 8:30:45 AM

Quant Time: Mar 27 08:30:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	307491	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	213515	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	45970	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	72629	19.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.08%
7) Chloroethane-d5	2.89	69	86895	20.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.84%
10) 1,1-Dichloroethene-d2	4.01	63	112119	14.12	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.48%
20) 2-Butanone-d5	7.07	46	79687	52.44	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.88%
24) Chloroform-d	7.65	84	198036	23.60	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.40%
26) 1,2-Dichloroethane-d4	8.31	65	129243m	25.57	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.28%
29) Benzene-d6	8.27	84	326705	27.75	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.00%
33) 1,2-Dichloropropane-d6	9.27	67	113952	32.22	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	128.88%#
37) Toluene-d8	10.32	98	232476	21.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.40%
38) trans-1,3-Dichloropropene-	10.58	79	44041	24.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.16%
39) 2-Hexanone-d5	10.93	63	54525	63.65	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	127.30%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	78280	22.47	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.88%
61) 1,2-Dichlorobenzene-d4	13.85	152	35049	19.88	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.52%

Target Compounds

					Ovalue
13) Acetone	4.12	43	28797	23.108	ug/L 96
14) Carbon disulfide	4.37	76	6672m	0.655	ug/L
16) Methylene chloride	4.92	84	21432m	4.780	ug/L
21) 2-Butanone	7.17	43	11071	6.434	ug/L 99
54) m,p-Xylene	11.84	106	3591	0.658	ug/L 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

MO
 4/6/19