


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
Data File : VW009479.D
Acq On : 26 Mar 2019 22:43
Operator : SY/VA
Sample : K2065-13
Misc : 5.79G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF5L6

Manual Integrations
APPROVED

MMDadoda
4/10/2019 9:56:58 AM

Quant Time: Mar 27 08:45:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 08:01:36 2019
Response via : Initial Calibration

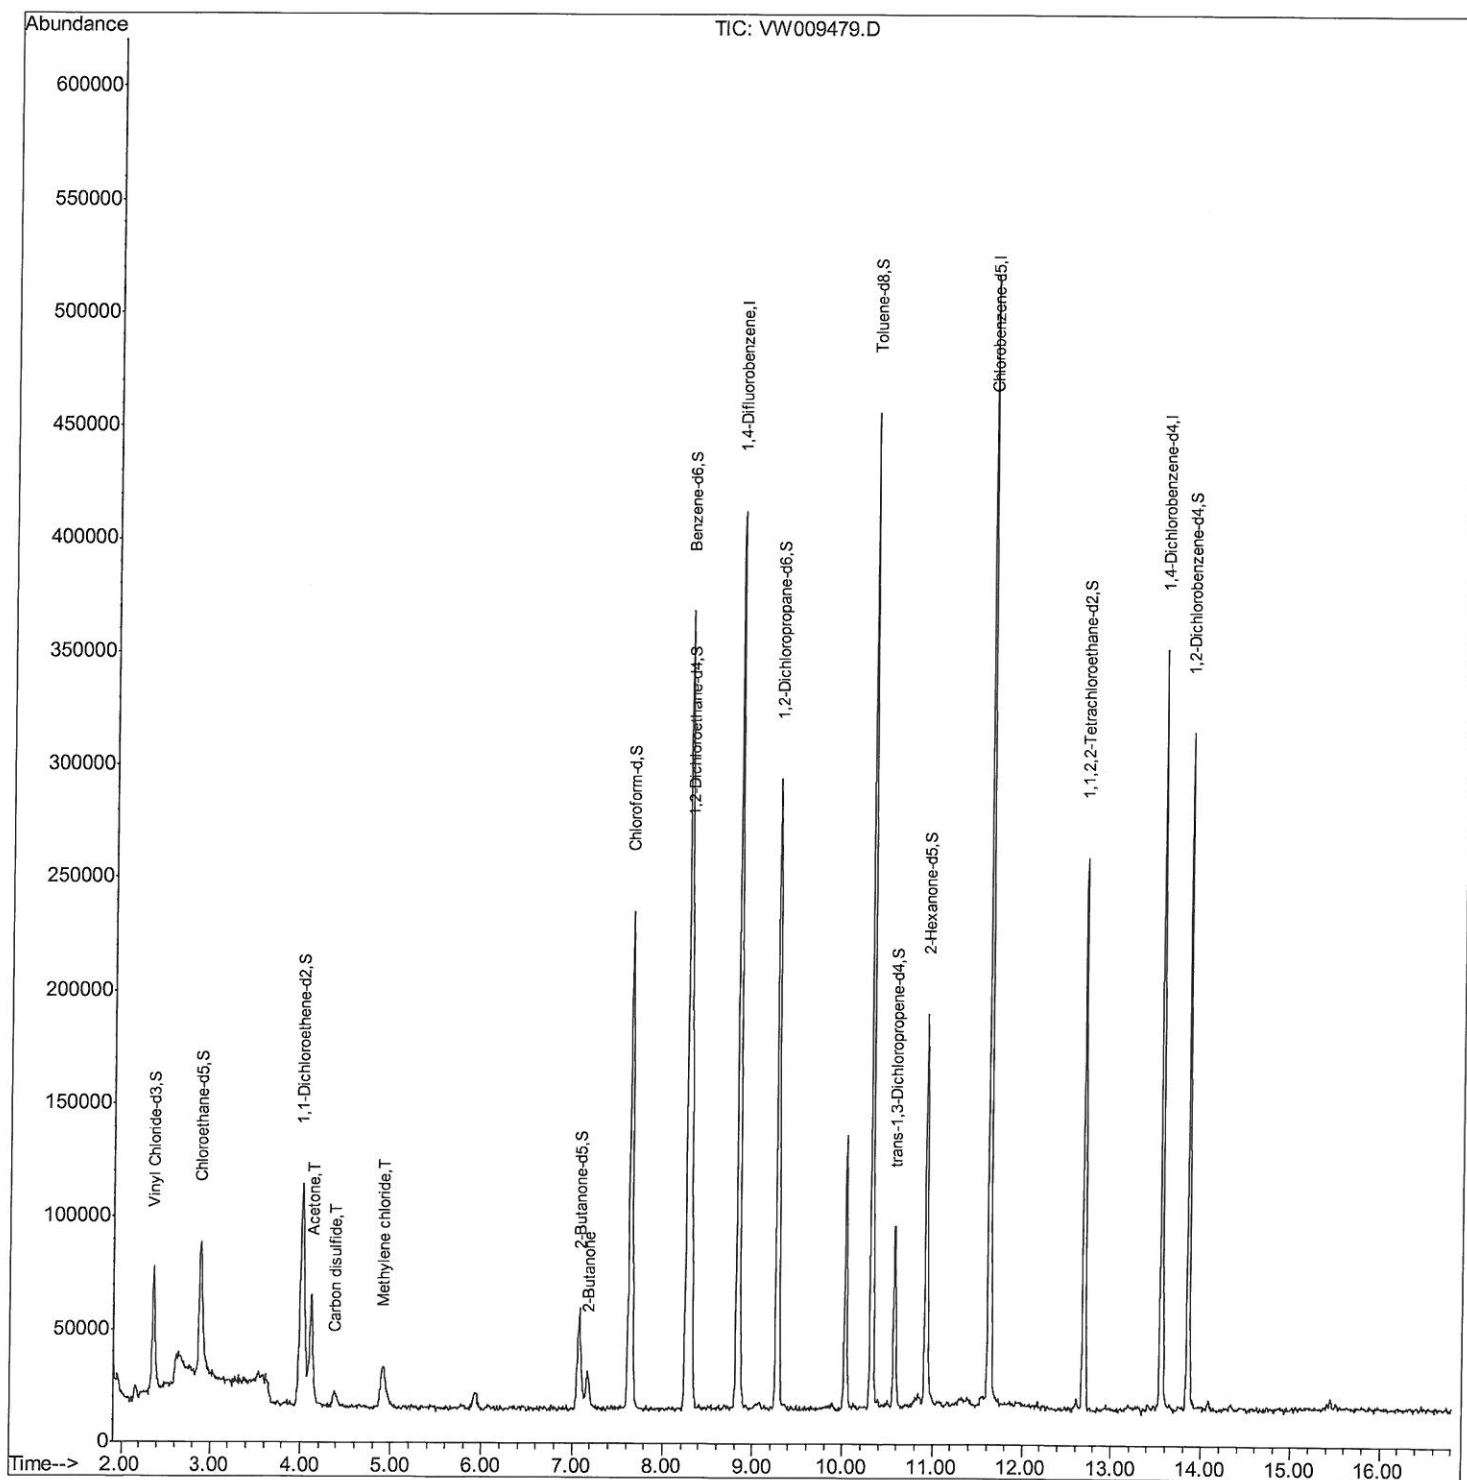

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009479.D
 Acq On : 26 Mar 2019 22:43
 Operator : SY/VA
 Sample : K2065-13
 Misc : 5.79G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5L6

Manual Integrations
 APPROVED

MMDadoda
 4/10/2019 9:56:58 AM

Quant Time: Mar 27 08:07:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

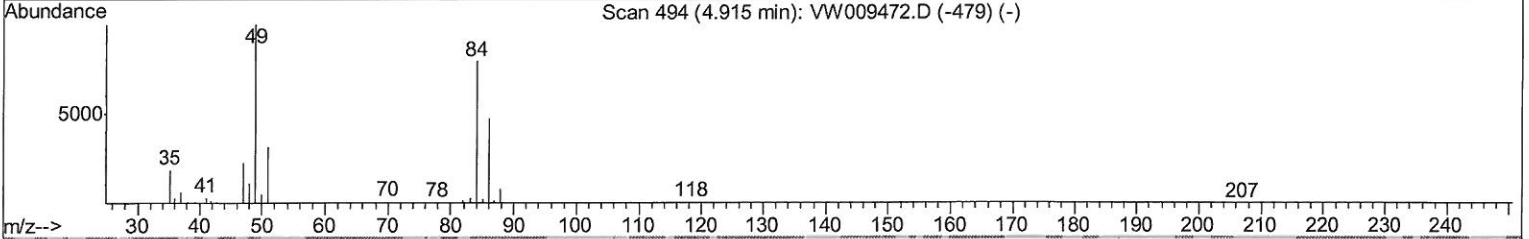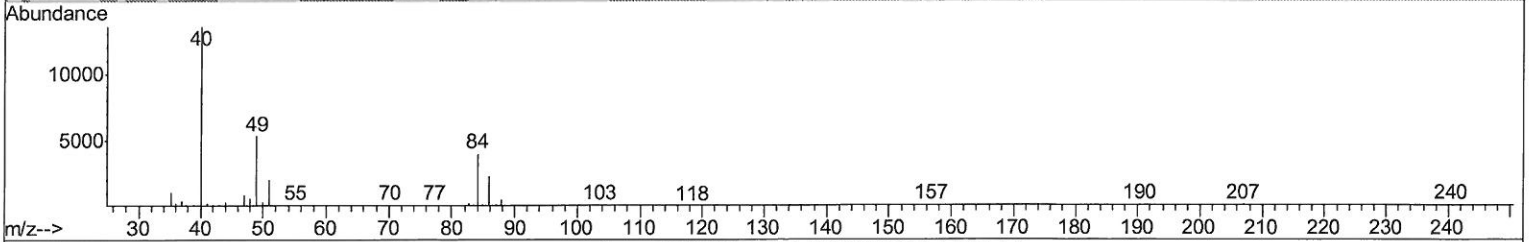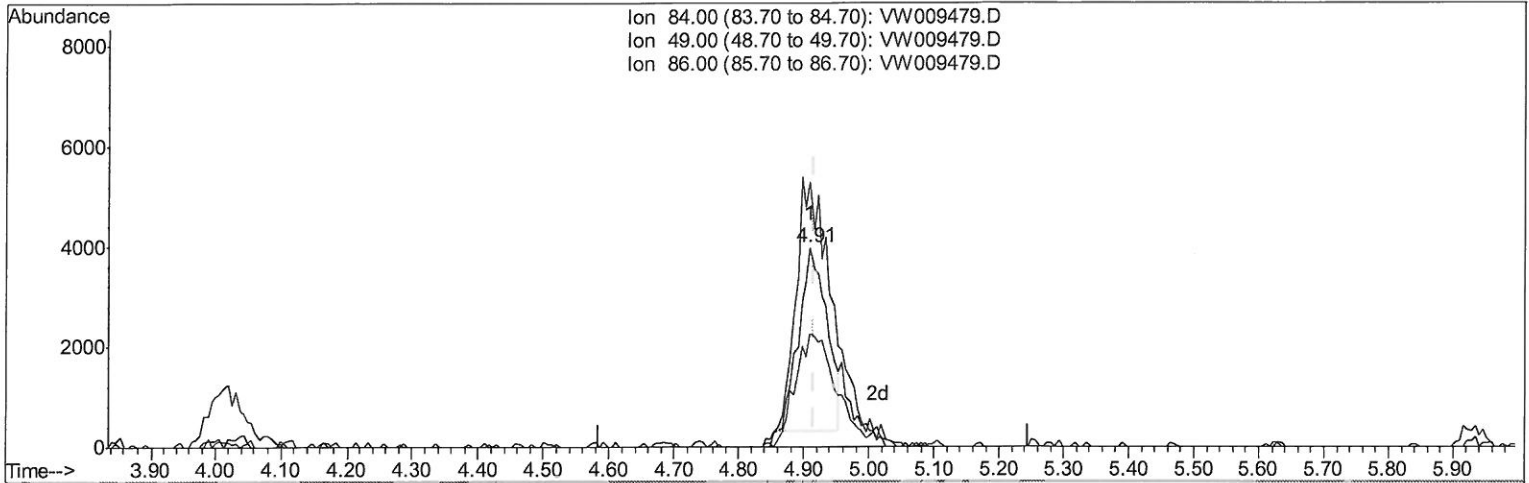

TIC: VW009479.D

(16) Methylene chloride (T)

4.909min (-0.006) 2.45ug/L

response 11003

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	133.25
86.00	63.50	56.57
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009479.D
 Acq On : 26 Mar 2019 22:43
 Operator : SY/VA
 Sample : K2065-13
 Misc : 5.79G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5L6

Manual Integrations
 APPROVED

MMDadoda
 4/10/2019 9:56:58 AM

Quant Time: Mar 27 08:07:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

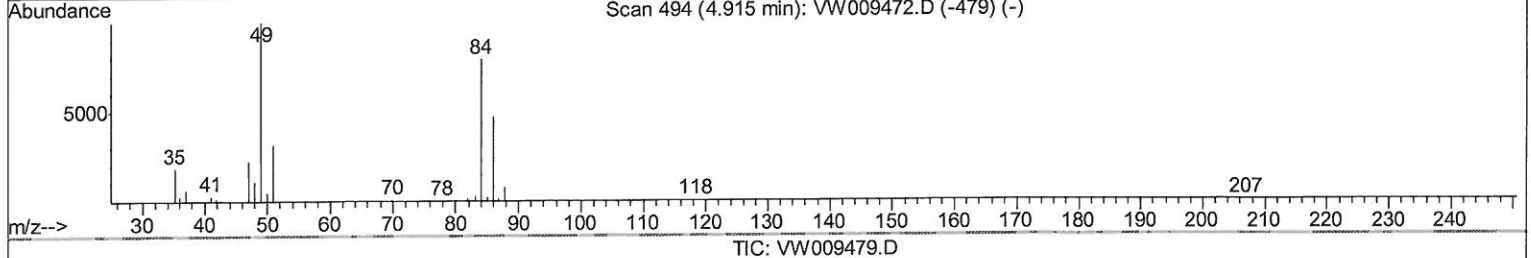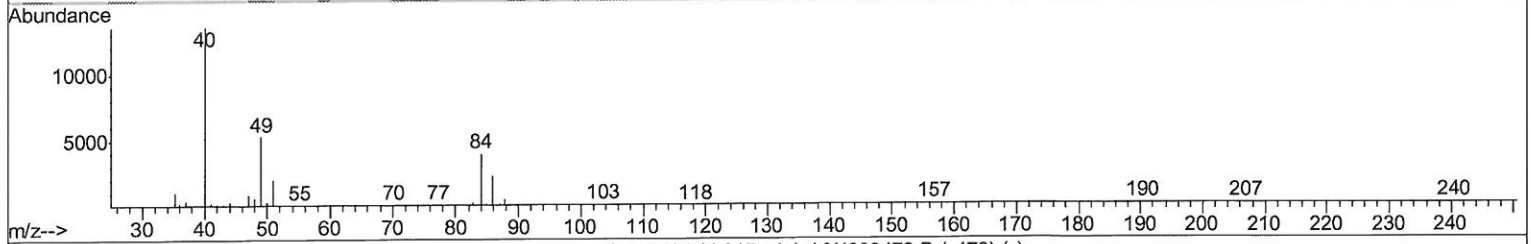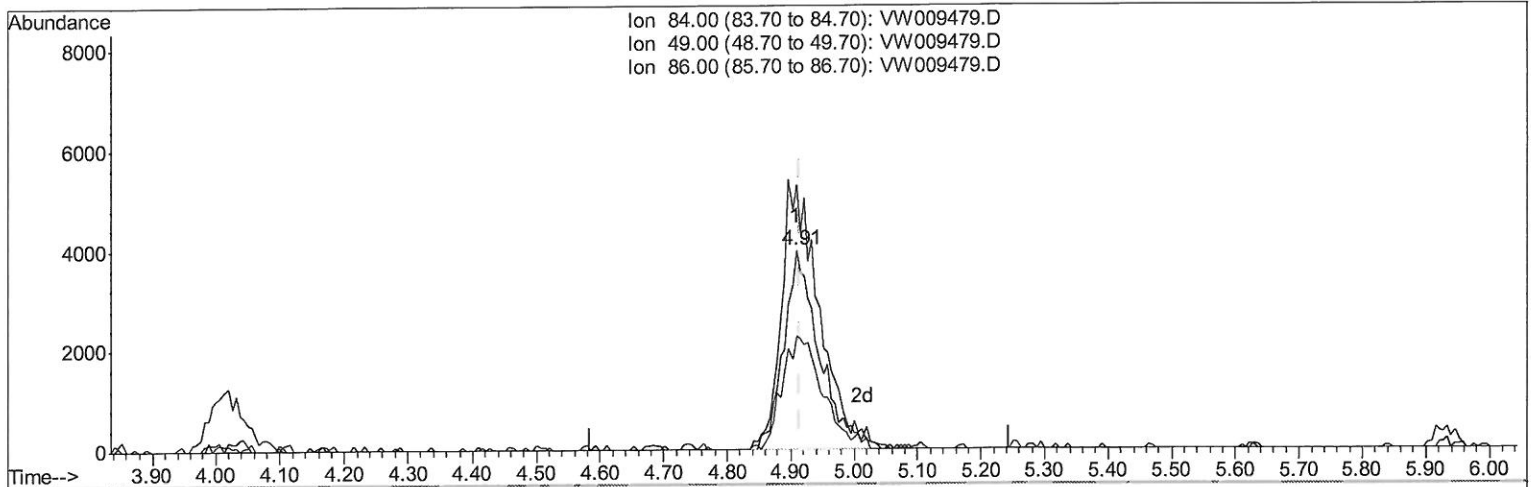

(16) Methylene chloride (T)

4.909min (-0.006) 3.46ug/L m

response 15523

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	133.25
86.00	63.50	56.57
0.00	0.00	0.00

>MO
4/6/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009479.D
 Acq On : 26 Mar 2019 22:43
 Operator : SY/VA
 Sample : K2065-13
 Misc : 5.79G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5L6

Manual Integrations
 APPROVED

MMDadoda
 4/10/2019 9:56:58 AM

Quant Time: Mar 27 08:45:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	307362	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	261027	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	80305	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	73576	20.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.12%
7) Chloroethane-d5	2.89	69	84644	19.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.80%
10) 1,1-Dichloroethene-d2	4.01	63	119151	15.01	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.04%
20) 2-Butanone-d5	7.08	46	74815	49.25	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.50%
24) Chloroform-d	7.65	84	202304	24.12	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.48%
26) 1,2-Dichloroethane-d4	8.30	65	123952	24.53	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.12%
29) Benzene-d6	8.27	84	339984	23.62	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.48%
33) 1,2-Dichloropropane-d6	9.27	67	115098	26.62	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.48%
37) Toluene-d8	10.32	98	269031	20.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.84%
38) trans-1,3-Dichloropropene-	10.58	79	40526	18.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.64%
39) 2-Hexanone-d5	10.93	63	46981	44.86	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.72%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	106313	24.97	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.88%
61) 1,2-Dichlorobenzene-d4	13.85	152	72961	23.69	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.76%

Target Compounds

					Ovalue
13) Acetone	4.12	43	84040	67.466	ug/L 99
14) Carbon disulfide	4.38	76	9822	0.964	ug/L # 94
16) Methylene chloride	4.91	84	15523m	3.463	ug/L
21) 2-Butanone	7.17	43	24029	13.971	ug/L

MO
78 4/6/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed