


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
Data File : VW009482.D
Acq On : 27 Mar 2019 00:05
Operator : SY/VA
Sample : K2065-17
Misc : 5.38G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1




Quant Time: Mar 27 08:56:53 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 08:01:36 2019
Response via : Initial Calibration

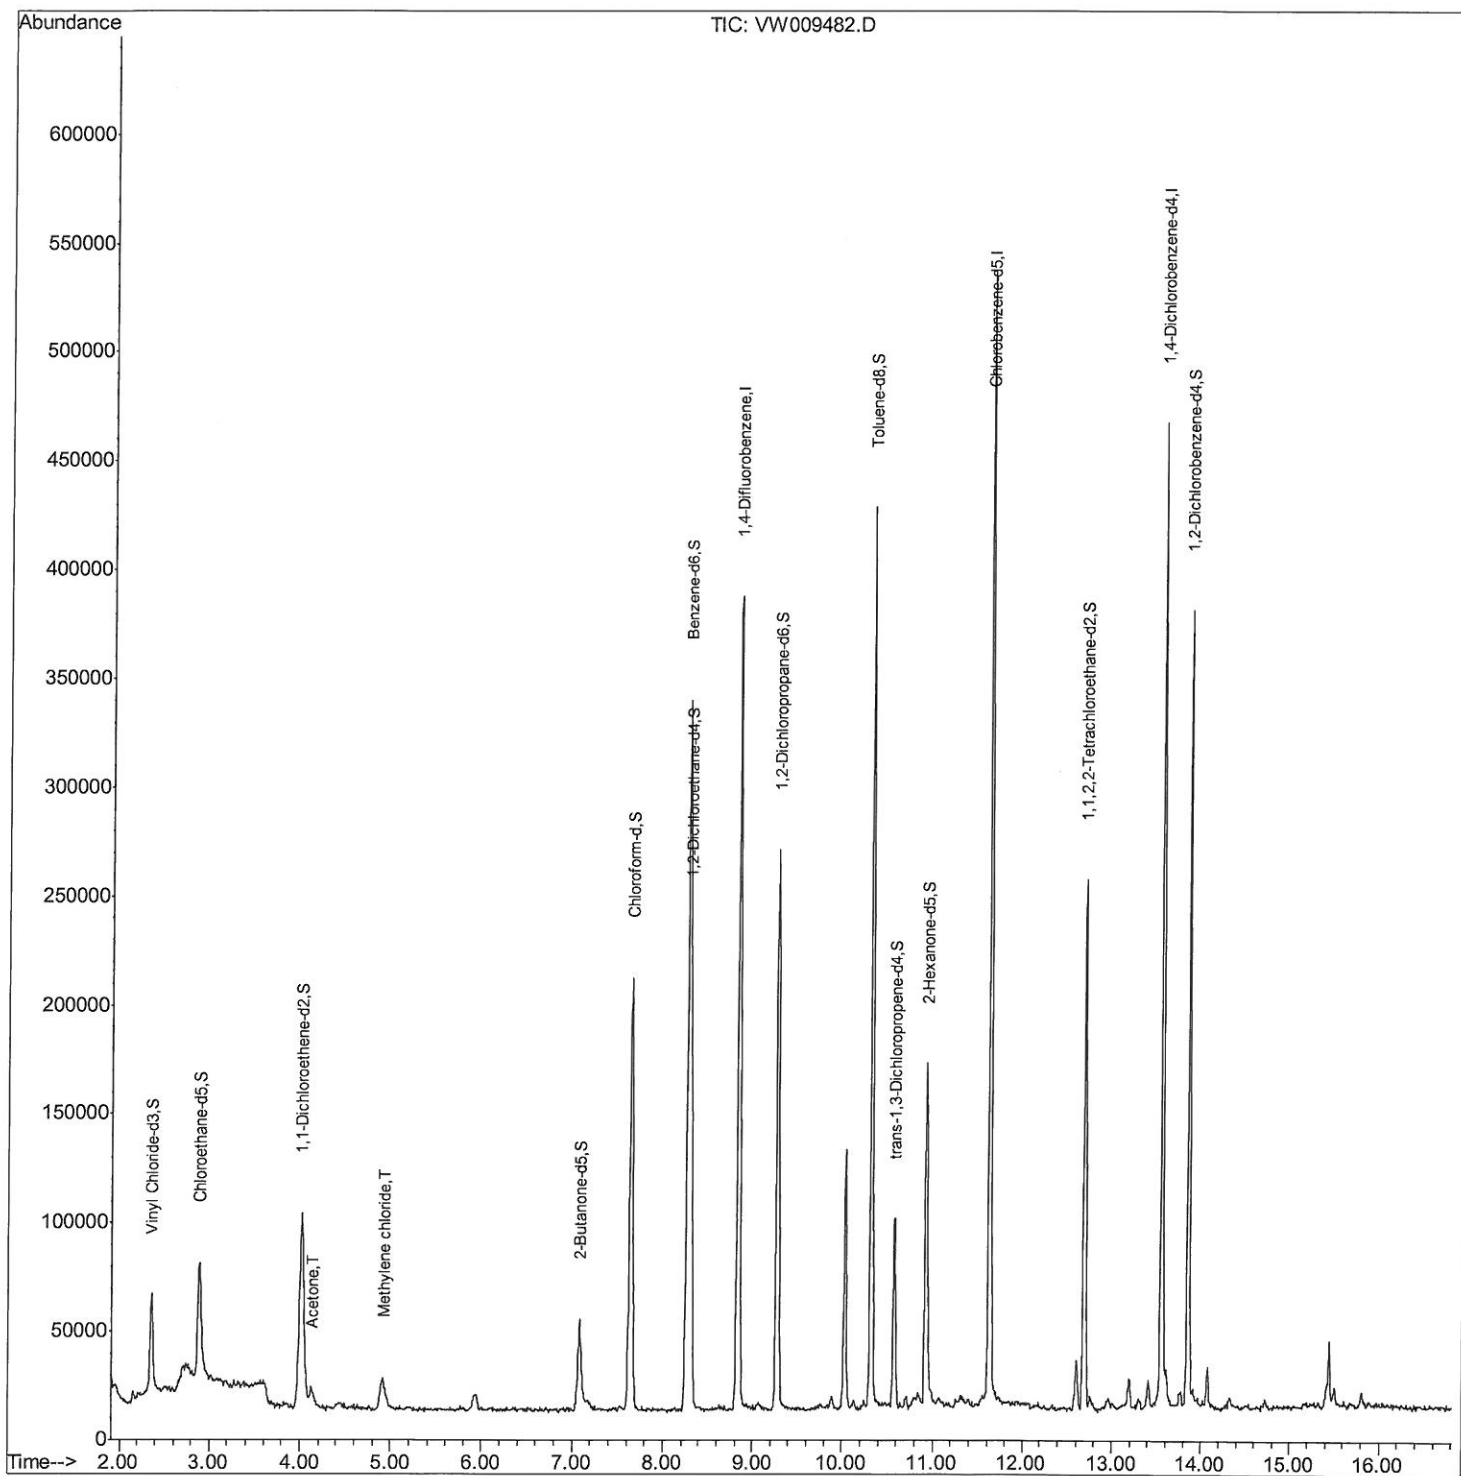

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009482.D
 Acq On : 27 Mar 2019 00:05
 Operator : SY/VA
 Sample : K2065-17
 Misc : 5.38G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 08:08:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

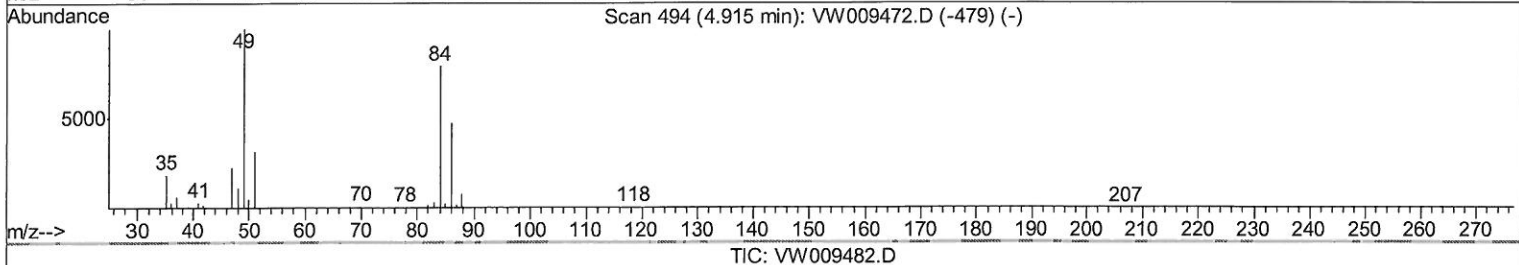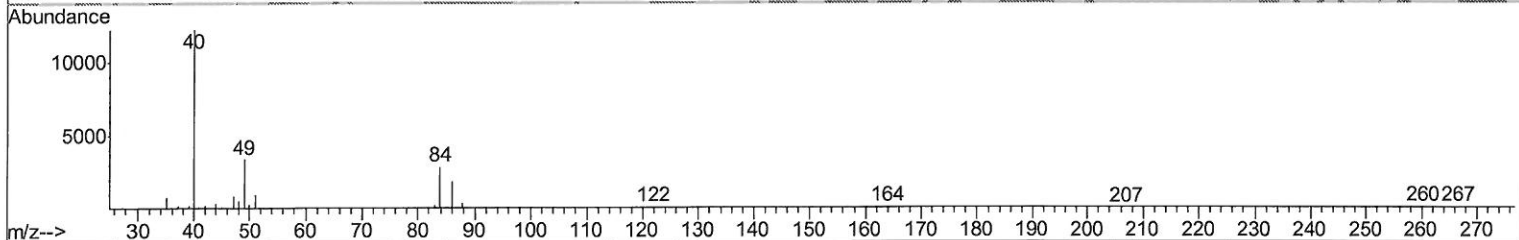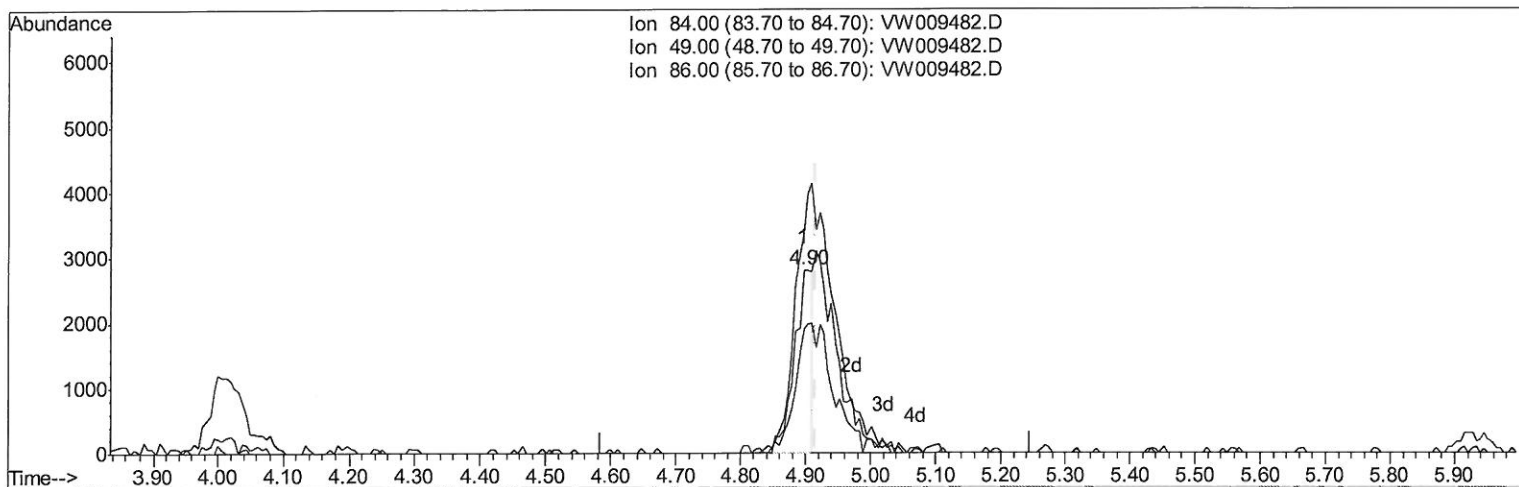

(16) Methylene chloride (T)

4.897min (-0.018) 1.29ug/L




response 5437

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	120.61
86.00	63.50	67.34
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009482.D
 Acq On : 27 Mar 2019 00:05
 Operator : SY/VA
 Sample : K2065-17
 Misc : 5.38G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 08:08:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

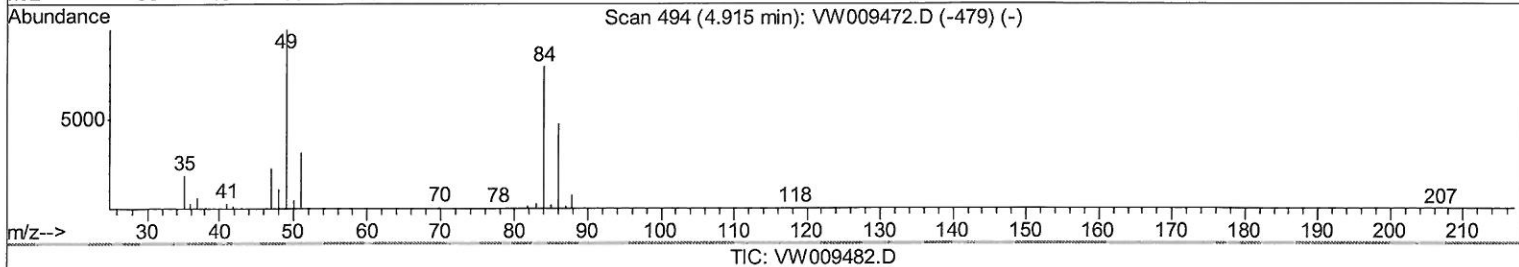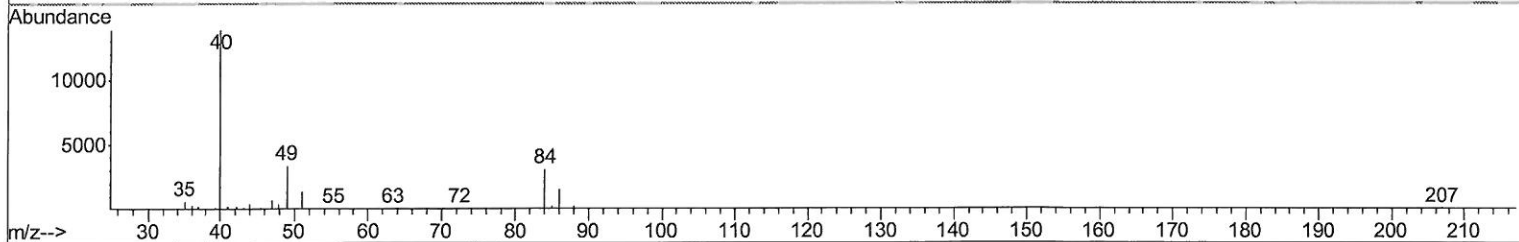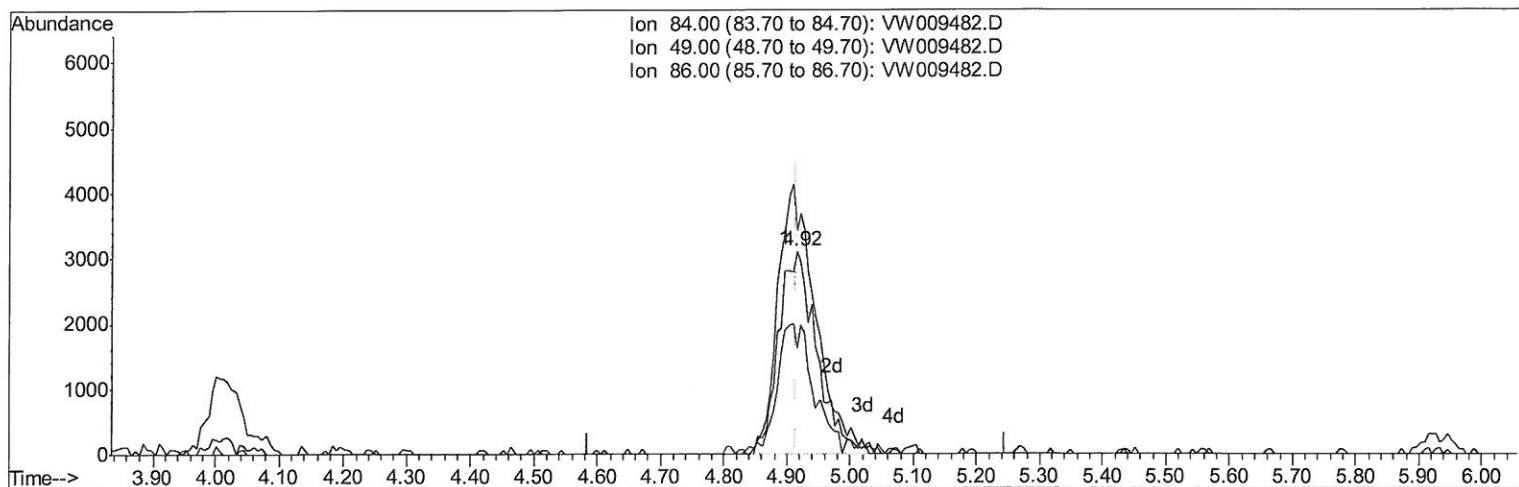

(16) Methylene chloride (T)

4.916min (+0.000) 3.09ug/L m

response 13027

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	110.08
86.00	63.50	52.06
0.00	0.00	0.00

Handwritten: > MG
4/6/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009482.D
 Acq On : 27 Mar 2019 00:05
 Operator : SY/VA
 Sample : K2065-17
 Misc : 5.38G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 08:56:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	289009	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	272365	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	107408	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	62699	18.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.60%
7) Chloroethane-d5	2.89	69	71588	17.71	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.84%
10) 1,1-Dichloroethene-d2	4.01	63	107798	14.44	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.76%
20) 2-Butanone-d5	7.09	46	67115	46.99	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.98%
24) Chloroform-d	7.64	84	182376	23.12	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.48%
26) 1,2-Dichloroethane-d4	8.30	65	114200	24.04	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.16%
29) Benzene-d6	8.27	84	311020	20.71	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.84%
33) 1,2-Dichloropropane-d6	9.27	67	106017	23.50	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.00%
37) Toluene-d8	10.32	98	255878	18.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.68%
38) trans-1,3-Dichloropropene-	10.58	79	42733	18.86	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.44%
39) 2-Hexanone-d5	10.93	63	45425	41.57	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.14%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	104730	23.57	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.28%
61) 1,2-Dichlorobenzene-d4	13.85	152	89902	21.83	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.32%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.13	43	16547	14.127	ug/L	73
16) Methylene chloride	4.92	84	13027m	3.091	ug/L	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

73
4/6/19