

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\

Data File : VW009486.D

Acq On : 27 Mar 2019 01:54

Operator : SY/VA

Sample : K2068-06

Misc : 5.02G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 11:59:50 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Wed Mar 27 08:01:36 2019

Response via : Initial Calibration

Instrument :

MSVOA_W


Client Sampled :

BF5M8

Manual Integrations
APPROVED

apatel

4/12/2019 8:30:48 AM

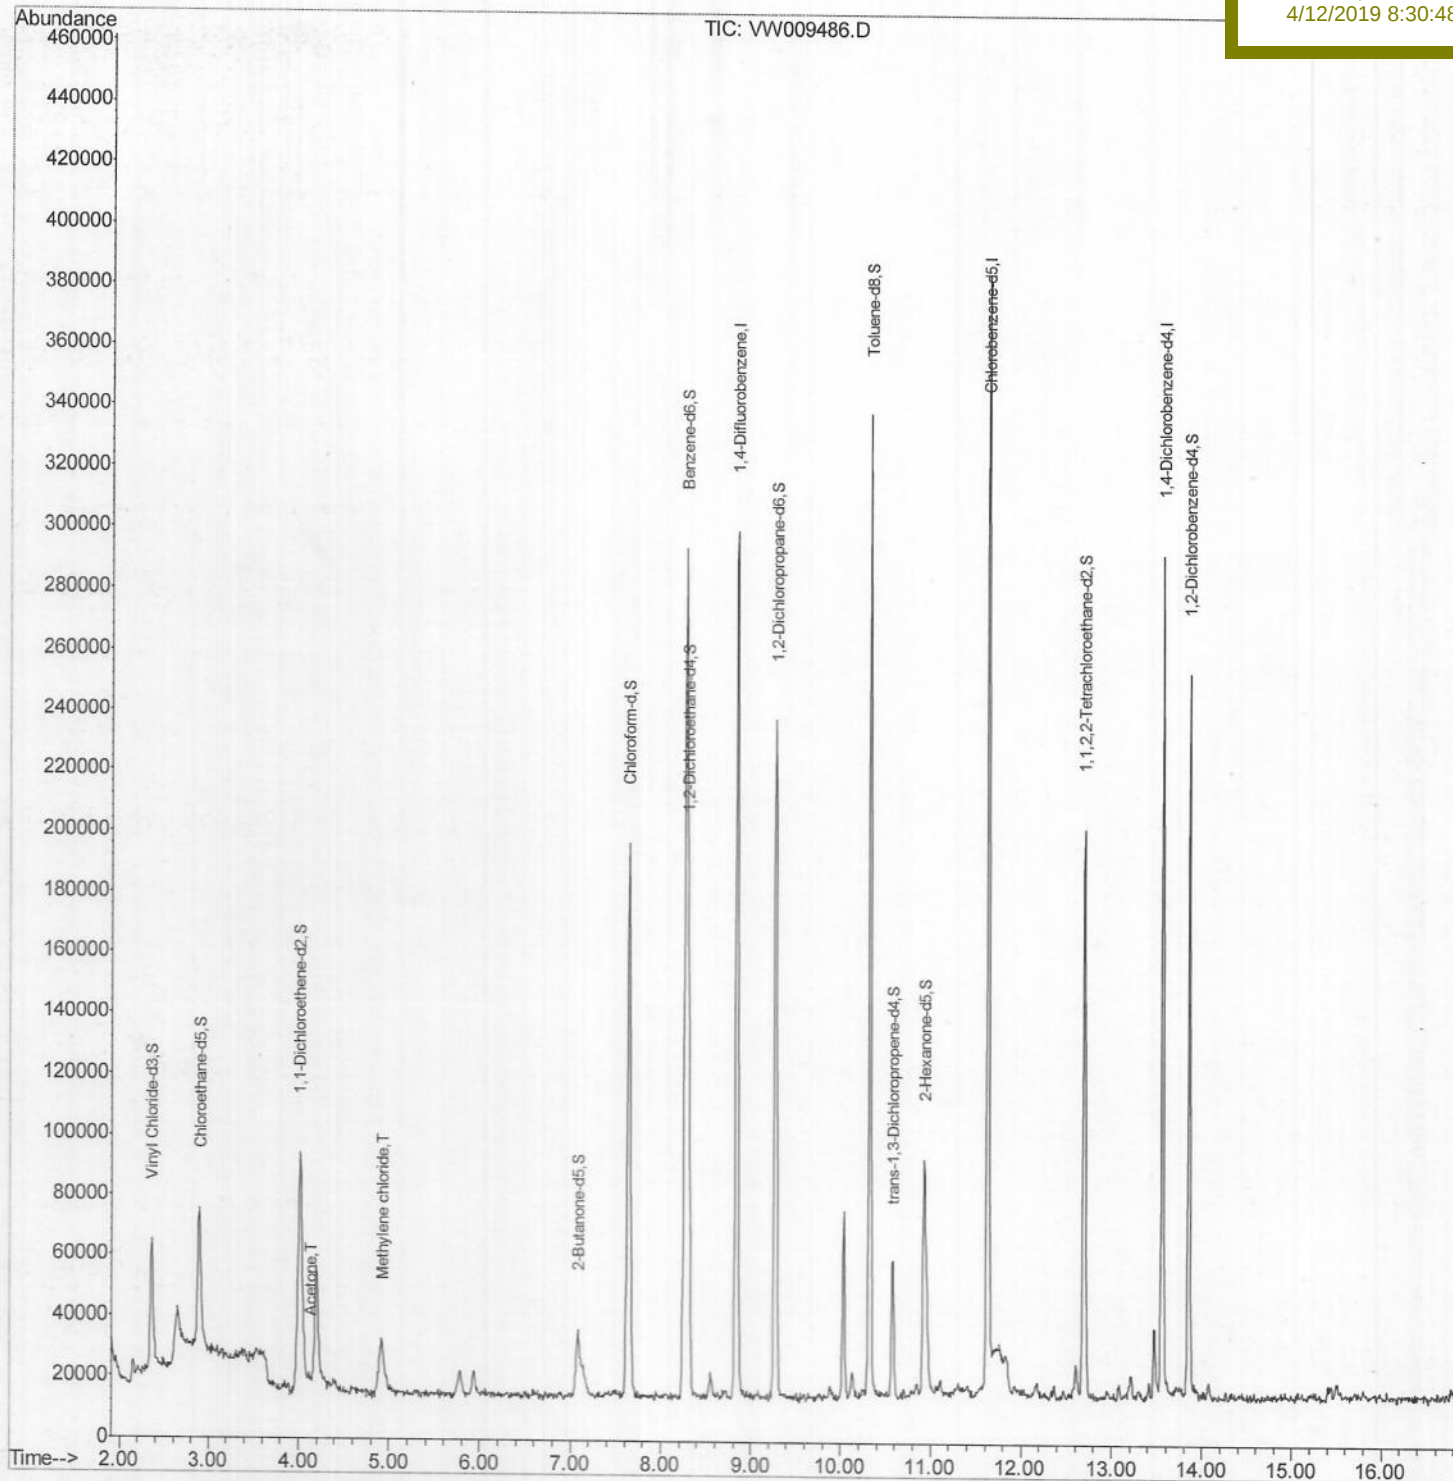

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\

Data File : VW009486.D

Acq On : 27 Mar 2019 01:54

Operator : SY/VA

Sample : K2068-06

Misc : 5.02G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 08:08:46 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Wed Mar 27 08:01:36 2019

Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :




BF5M8

Manual Integrations

APPROVED

apatel

4/12/2019 8:30:48 AM

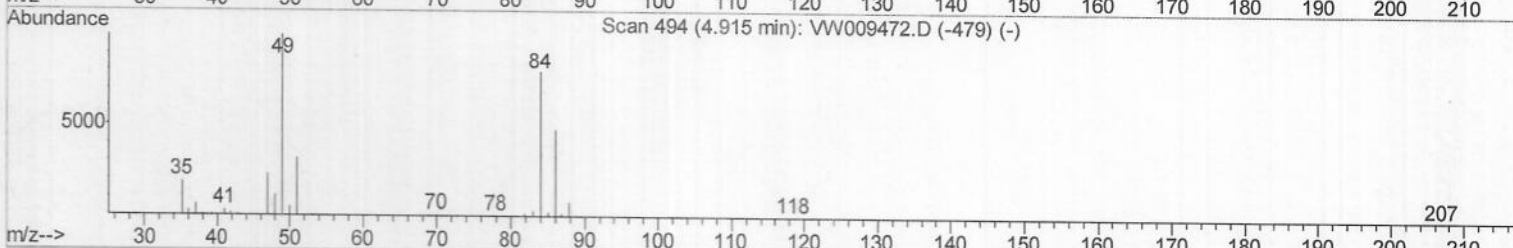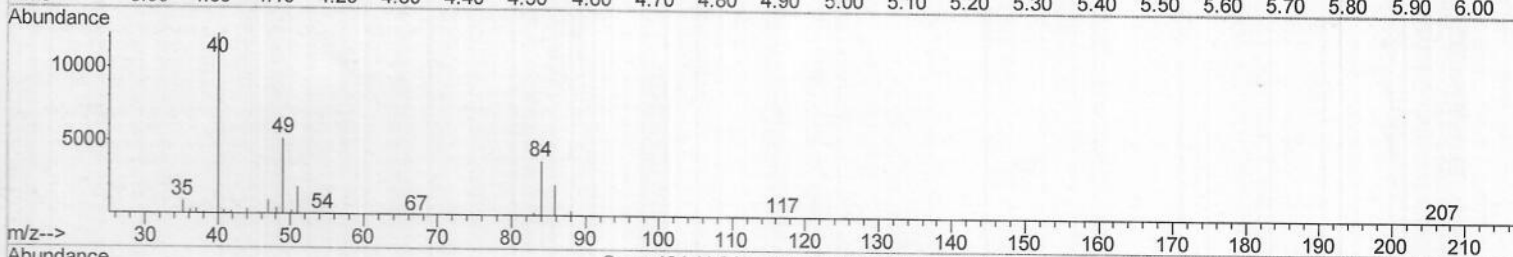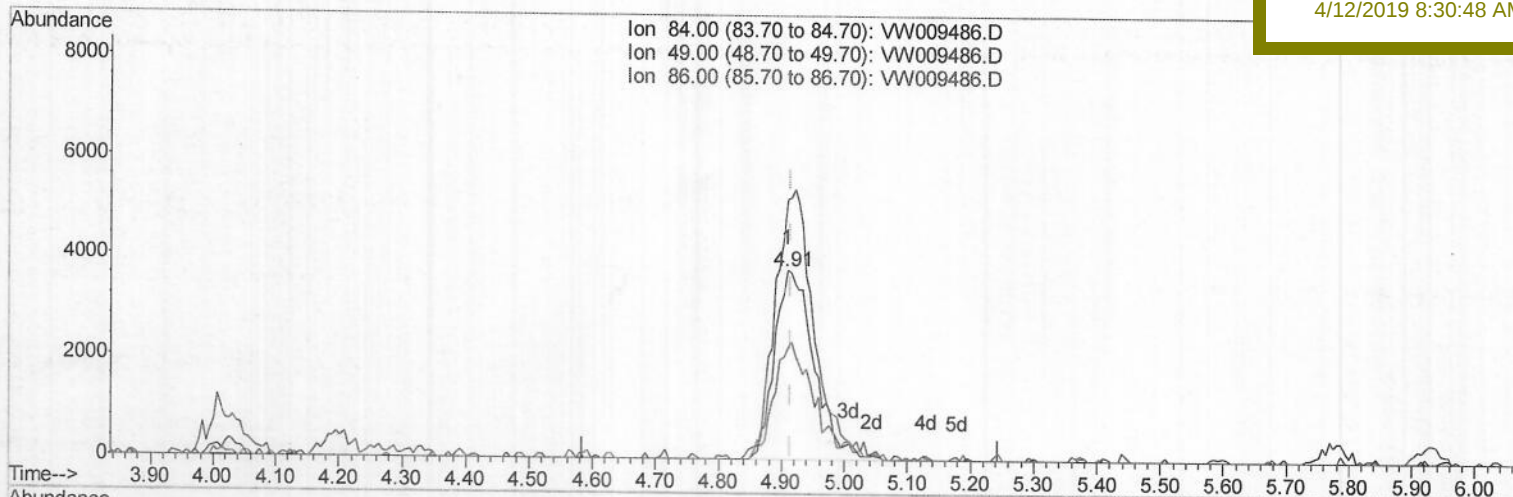

TIC: VW009486.D

(16) Methylene chloride (T)

4.909min (-0.006) 5.01ug/L m

response 16473

M.D
3/27/19

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	138.99
86.00	63.50	58.62
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\

Data File : VW009486.D

Acq On : 27 Mar 2019 01:54

Operator : SY/VA

Sample : K2068-06

Misc : 5.02G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 08:08:46 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Wed Mar 27 08:01:36 2019




Response via : Initial Calibration

Instrument :

MSVOA_W

ClientSampleId :

BF5M8

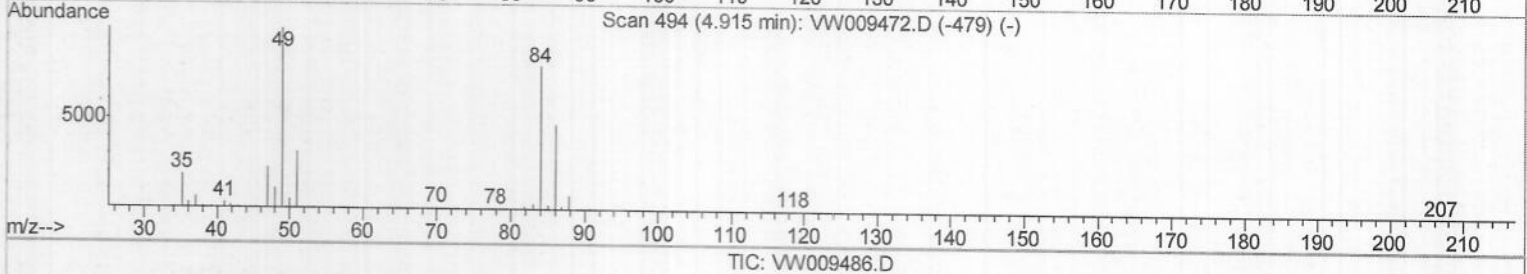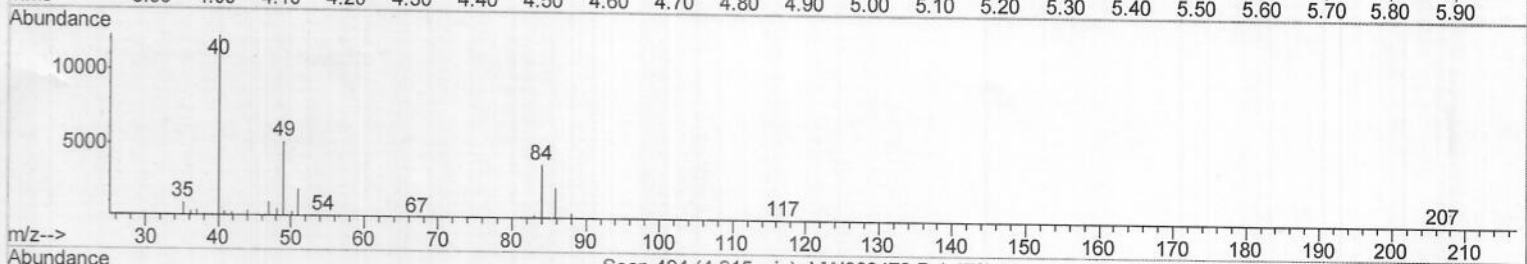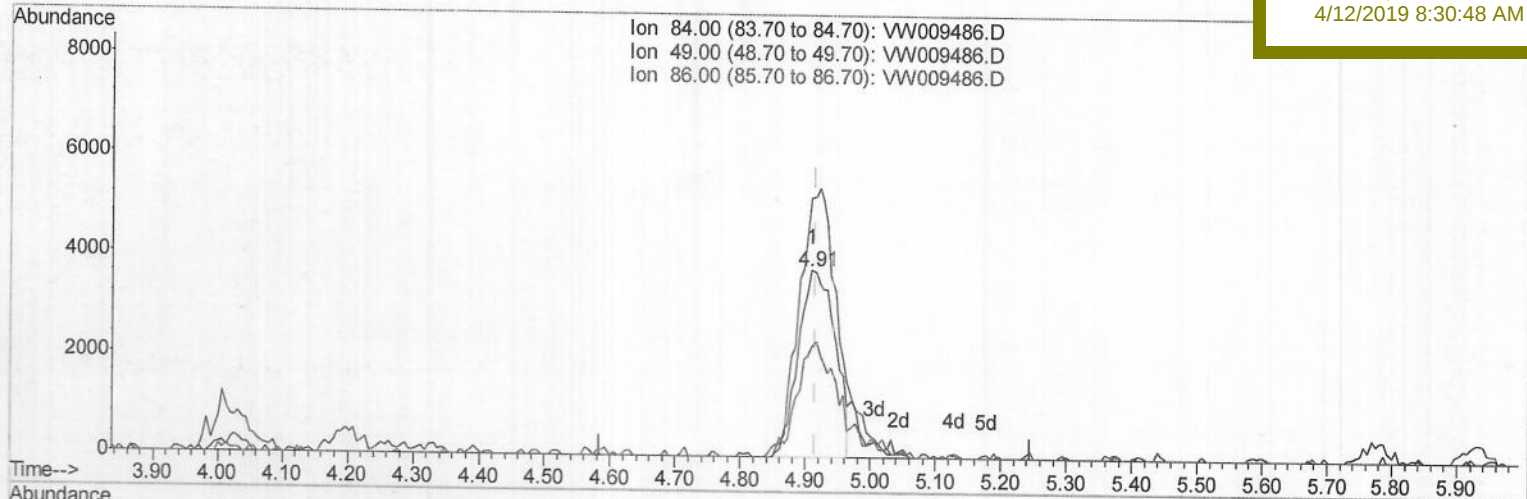Manual Integrations
APPROVEDapatel
4/12/2019 8:30:48 AM

(16) Methylene chloride (T)

4.909min (-0.006) 4.47ug/L

response 14706

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	138.99
86.00	63.50	58.62
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009486.D
 Acq On : 27 Mar 2019 01:54
 Operator : SY/VA
 Sample : K2068-06
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 BF5M8

Quant Time: Mar 30 11:59:50 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

apatel
 4/12/2019 8:30:48 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	225657	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	189696	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	63062	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.35	65	61457	22.79	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.16%		
7) Chloroethane-d5	2.90	69	64083	20.31	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.24%		
10) 1,1-Dichloroethene-d2	4.01	63	94745	16.26	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	65.04%		
20) 2-Butanone-d5	7.07	46	32786	29.40	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	58.80%		
24) Chloroform-d	7.65	84	161190	26.17	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	104.68%		
26) 1,2-Dichloroethane-d4	8.31	65	104283	28.11	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	112.44%		
29) Benzene-d6	8.27	84	265387	25.37	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	101.48%		
33) 1,2-Dichloropropane-d6	9.27	67	93512	29.76	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	119.04%		
37) Toluene-d8	10.32	98	200767	20.76	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	83.04%		
38) trans-1,3-Dichloropropene-	10.58	79	22035	13.96	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	55.84%		
39) 2-Hexanone-d5	10.93	63	19518	25.65	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	51.30%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	84092	27.17	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	108.68%		
61) 1,2-Dichlorobenzene-d4	13.86	152	60305	24.94	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.76%		

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.12	43	6094	6.664	ug/L	55
16) Methylene chloride	4.91	84	16473m	5.006	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

m
 3/27/19