


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
Data File : VW009489.D
Acq On : 27 Mar 2019 03:16
Operator : SY/VA
Sample : K2065-16
Misc : 5.56G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF5P8

Manual Integrations
APPROVED

MMDadoda
3/30/2019 12:37:44 PM

Quant Time: Mar 27 09:23:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 08:01:36 2019
Response via : Initial Calibration

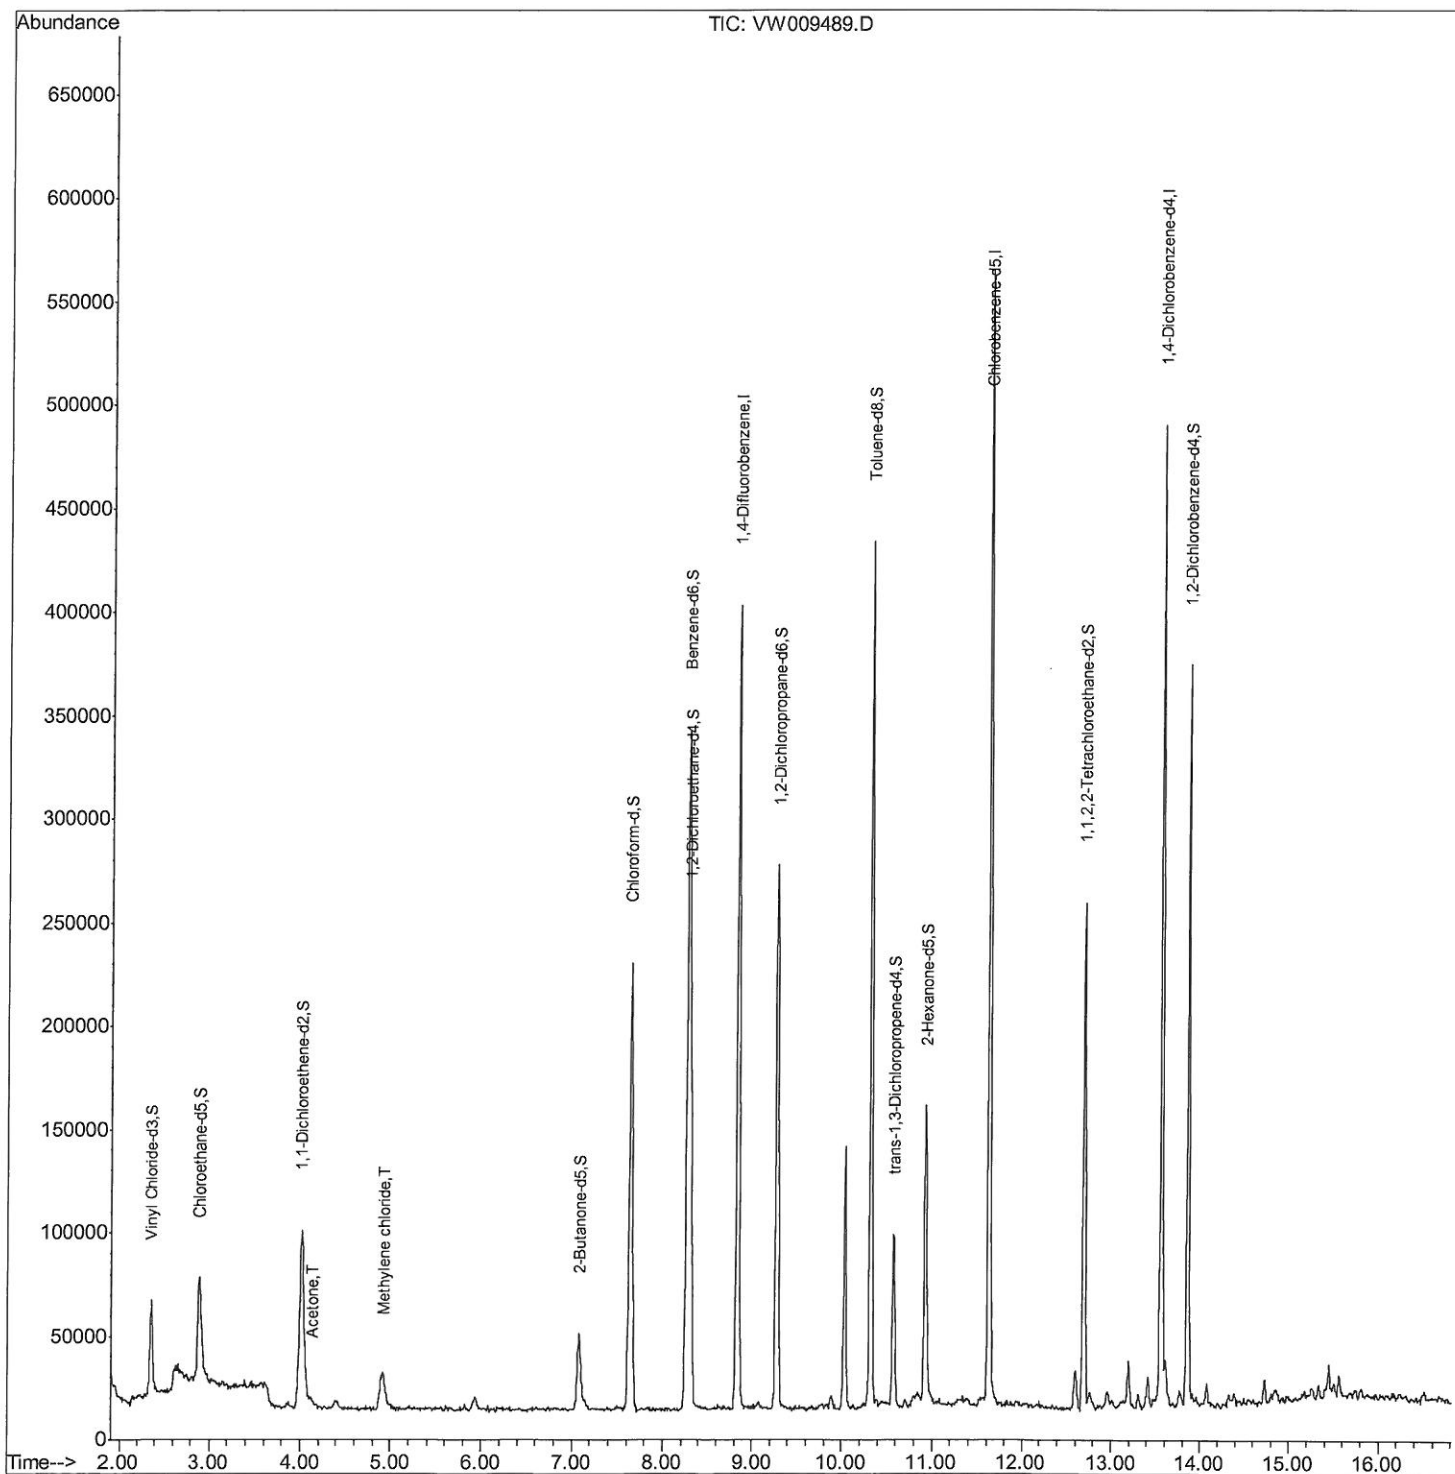

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
Data File : VW009489.D
Acq On : 27 Mar 2019 03:16
Operator : SY/VA
Sample : K2065-16
Misc : 5.56G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF5P8

Manual Integrations
APPROVED

MMDadoda
3/30/2019 12:37:44 PM

Quant Time: Mar 27 08:09:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 08:01:36 2019
Response via : Initial Calibration

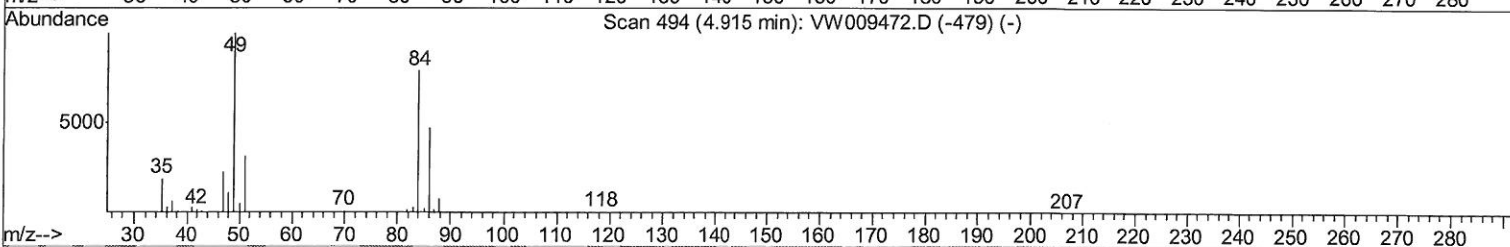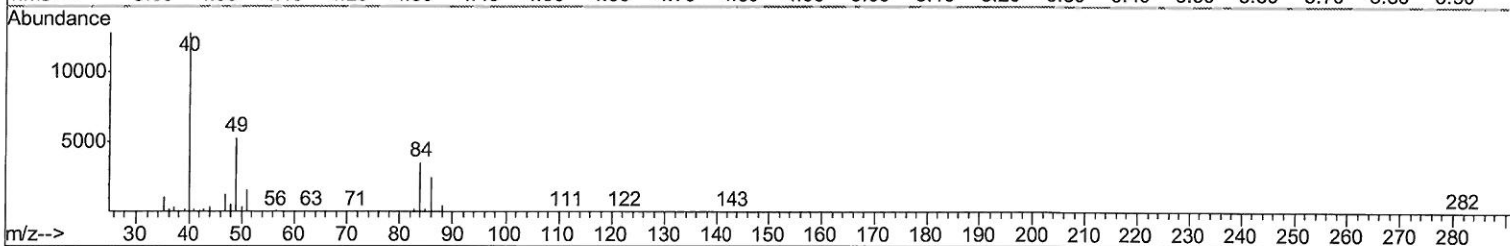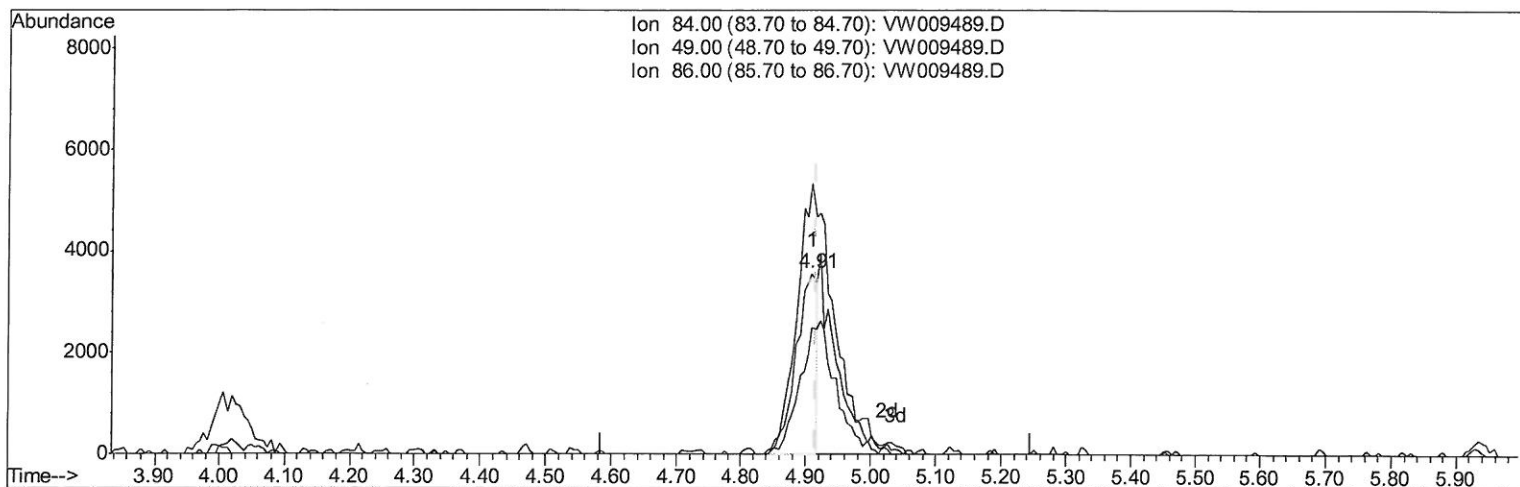

TIC: VW009489.D

(16) Methylene chloride (T)

4.910min (-0.006) 1.77ug/L

response 7779

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	149.52
86.00	63.50	70.16
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009489.D
 Acq On : 27 Mar 2019 03:16
 Operator : SY/VA
 Sample : K2065-16
 Misc : 5.56G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5P8

Manual Integrations
 APPROVED

MMDadoda
 3/30/2019 12:37:44 PM

Quant Time: Mar 27 08:09:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

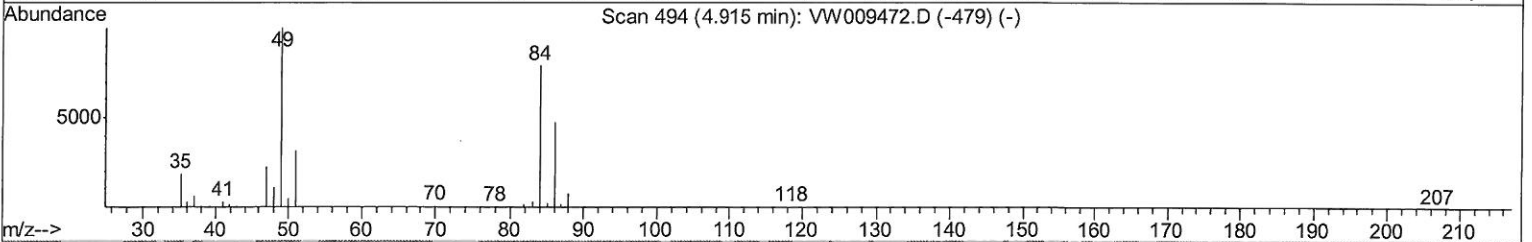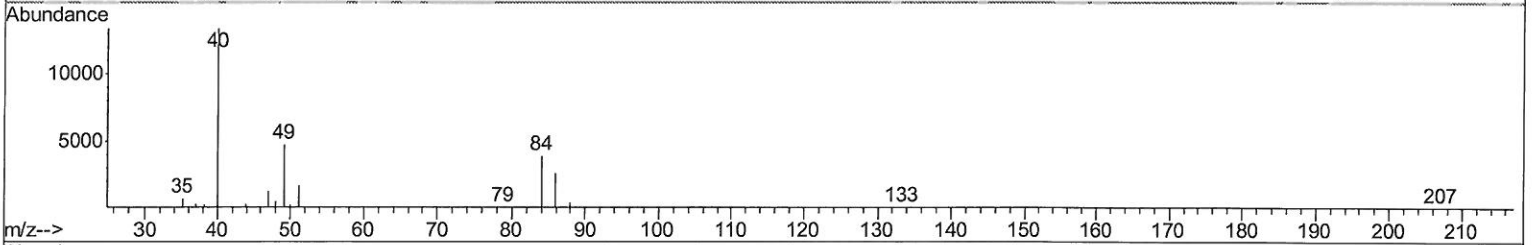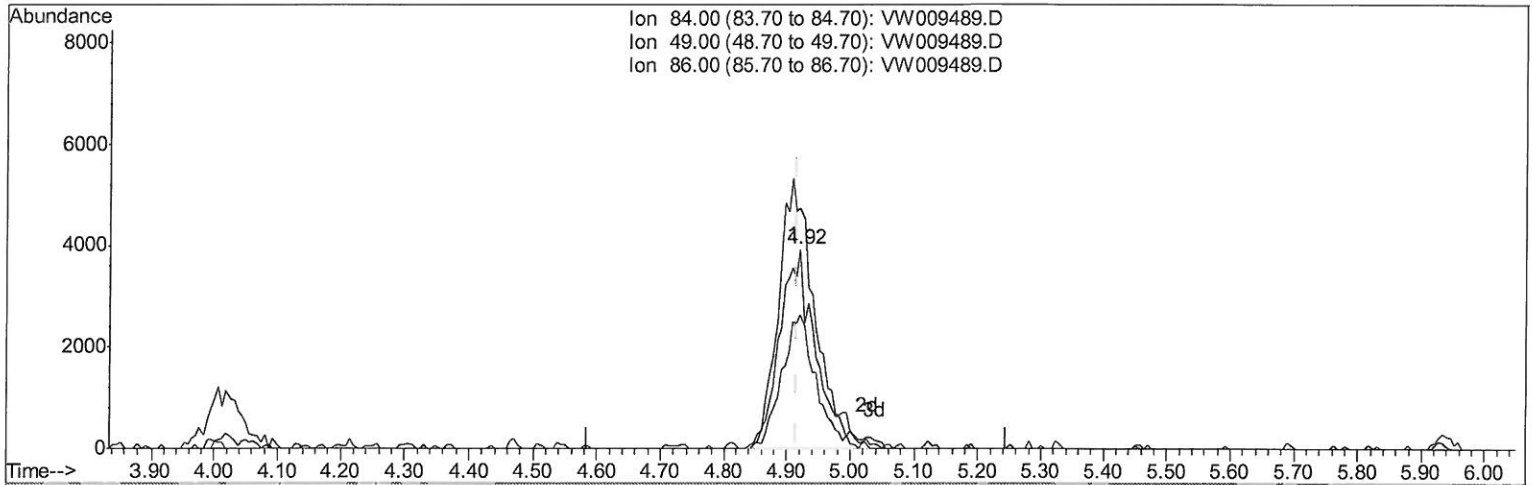

TIC: VW009489.D

(16) Methylene chloride (T)
 4.922min (+0.006) 3.52ug/L m
 response 15495

>MD
4/6/19

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	120.87
86.00	63.50	67.02
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
Data File : VW009489.D
Acq On : 27 Mar 2019 03:16
Operator : SY/VA
Sample : K2065-16
Misc : 5.56G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BF5P8

Manual Integrations
APPROVED

MMDadoda
3/30/2019 12:37:44 PM

Quant Time: Mar 27 08:09:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 08:01:36 2019
Response via : Initial Calibration

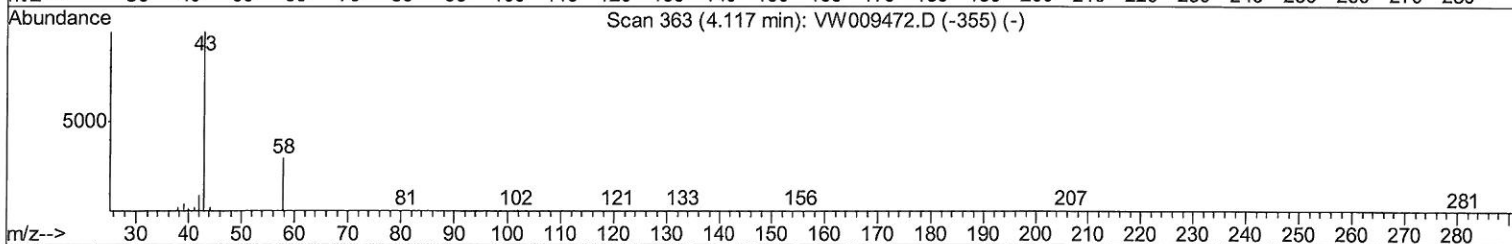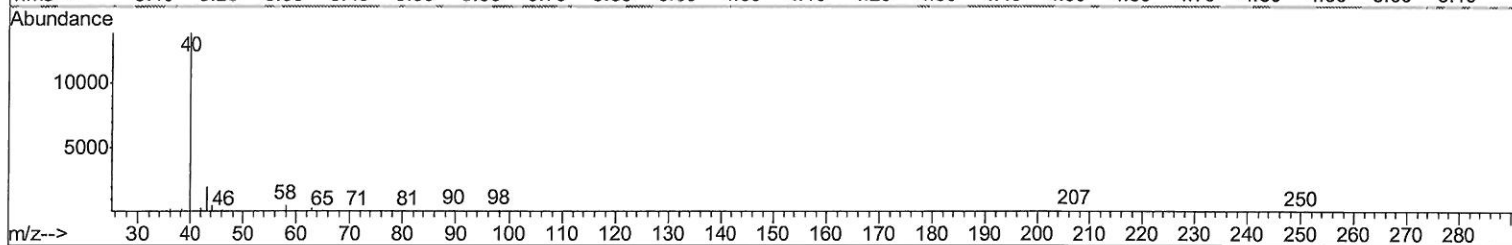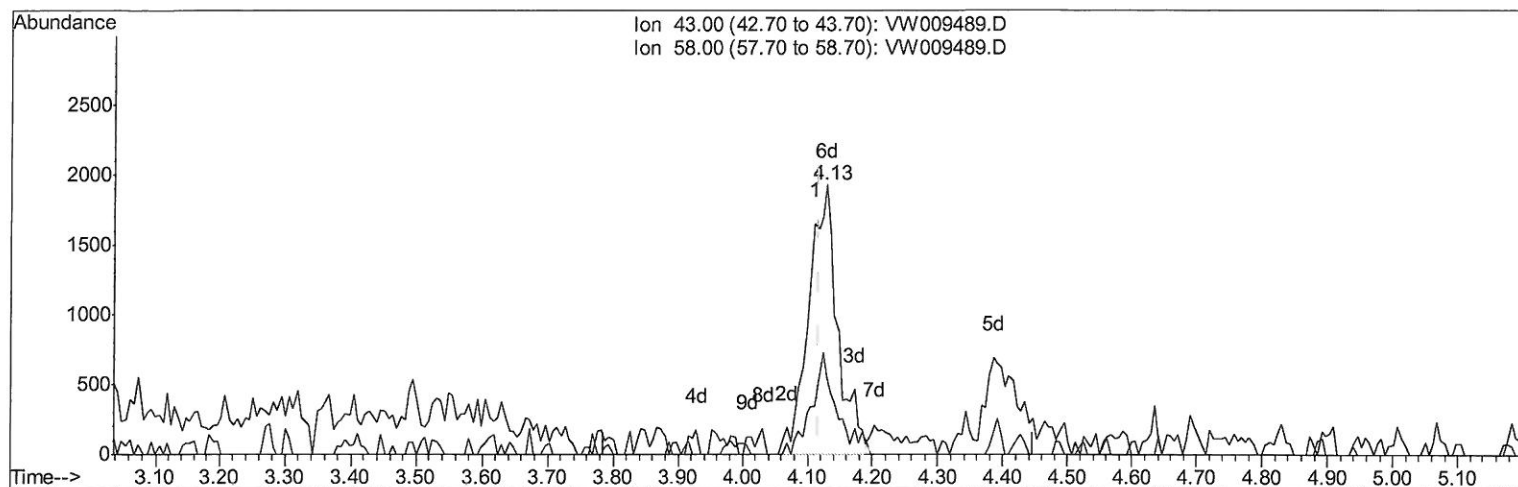

TIC: VW009489.D

(13) Acetone (T)

4.129min (+0.012) 4.87ug/L m

response 5964

Ion	Exp%	Act%
43.00	100	100
58.00	28.10	2.41
0.00	0.00	0.00
0.00	0.00	0.00

> MD
4/6/19

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
Data File : VW009489.D
Acq On : 27 Mar 2019 03:16
Operator : SY/VA
Sample : K2065-16
Misc : 5.56G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF5P8

Manual Integrations
APPROVED

MMDadoda
3/30/2019 12:37:44 PM

Quant Time: Mar 27 08:09:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 27 08:01:36 2019
Response via : Initial Calibration

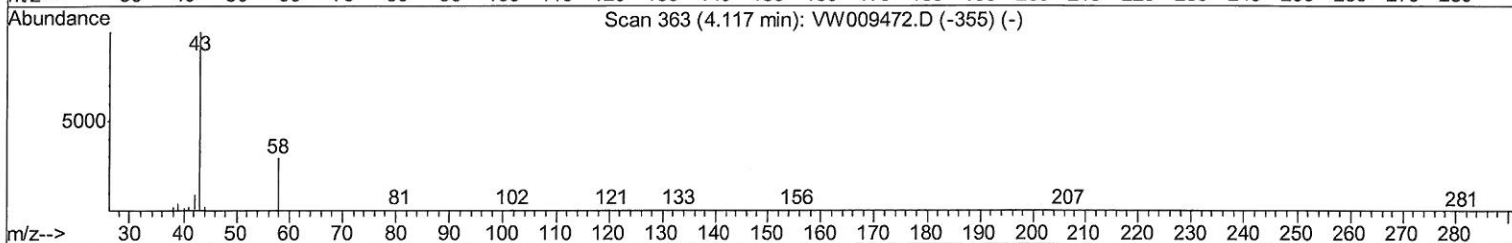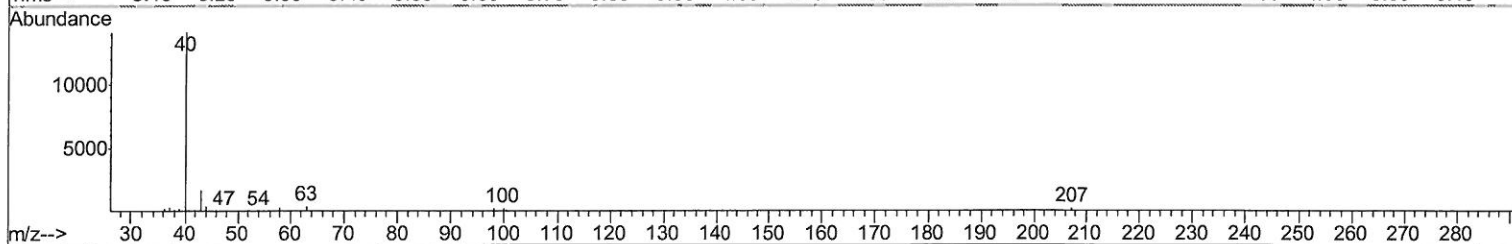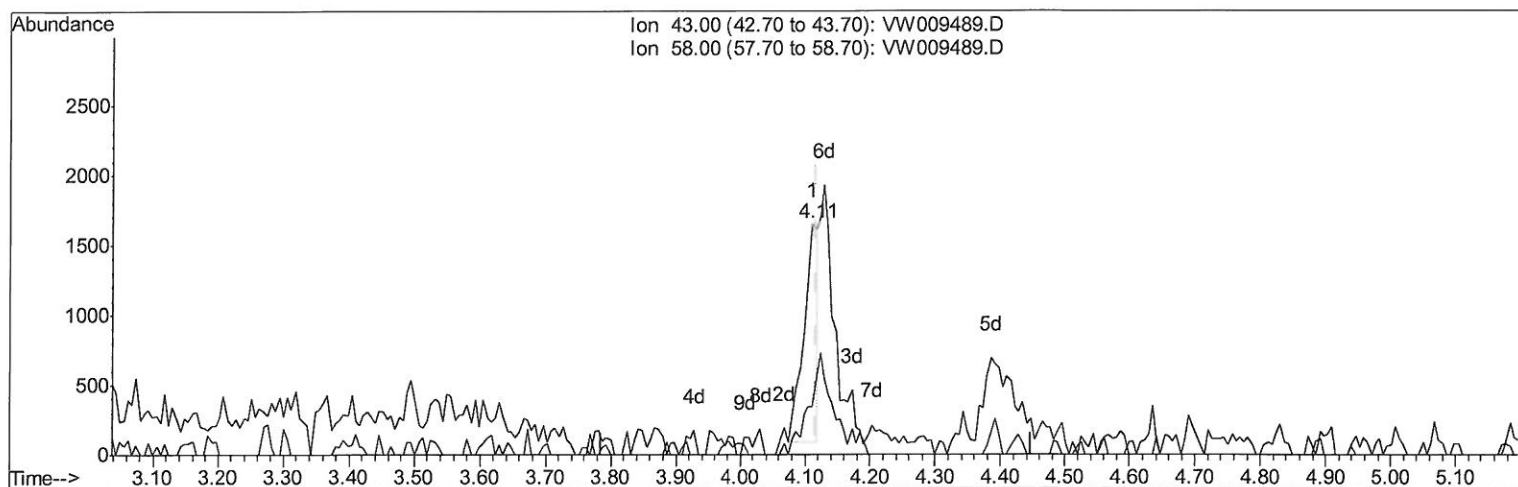

TIC: VW009489.D

(13) Acetone (T)

4.111min (-0.006) 1.84ug/L

response 2251

Ion	Exp%	Act%
43.00	100	100
58.00	28.10	6.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032619\
 Data File : VW009489.D
 Acq On : 27 Mar 2019 03:16
 Operator : SY/VA
 Sample : K2065-16
 Misc : 5.56G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5P8

Manual Integrations
 APPROVED

MMDadoda
 3/30/2019 12:37:44 PM

Quant Time: Mar 27 09:23:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 27 08:01:36 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	302167	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	285257	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	110722	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	60095	16.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.56%
7) Chloroethane-d5	2.89	69	71283	16.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.48%
10) 1,1-Dichloroethene-d2	4.01	63	103484	13.26	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.04%
20) 2-Butanone-d5	7.07	46	62269	41.70	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.40%
24) Chloroform-d	7.64	84	190592	23.11	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.44%
26) 1,2-Dichloroethane-d4	8.30	65	120360	24.23	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.92%
29) Benzene-d6	8.27	84	320384	20.37	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.48%
33) 1,2-Dichloropropane-d6	9.27	67	112726	23.86	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.44%
37) Toluene-d8	10.32	98	263343	18.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.40%
38) trans-1,3-Dichloropropene-	10.57	79	42748	18.01	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.04%
39) 2-Hexanone-d5	10.93	63	42324	36.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	105445	22.66	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.64%
61) 1,2-Dichlorobenzene-d4	13.85	152	91539	21.56	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.24%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.13	43	5964m	4.870	ug/L	
16) Methylene chloride	4.92	84	15495m	3.516	ug/L	

7 MD
 4/6/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed