
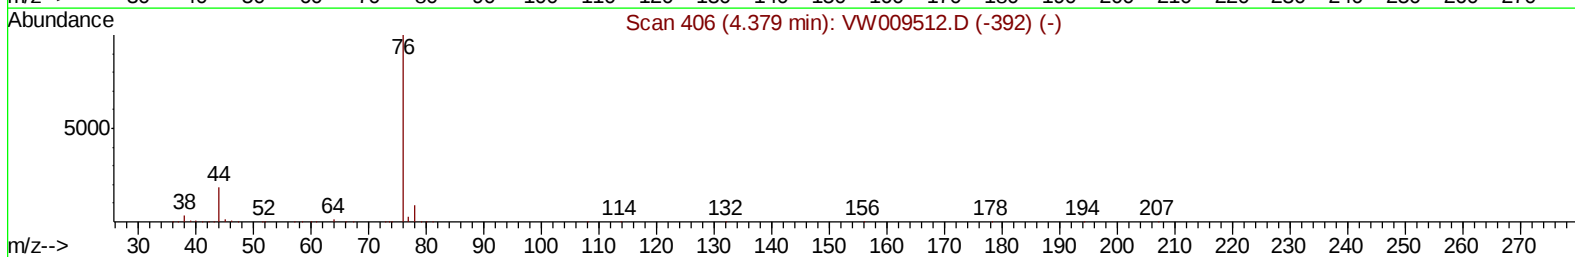
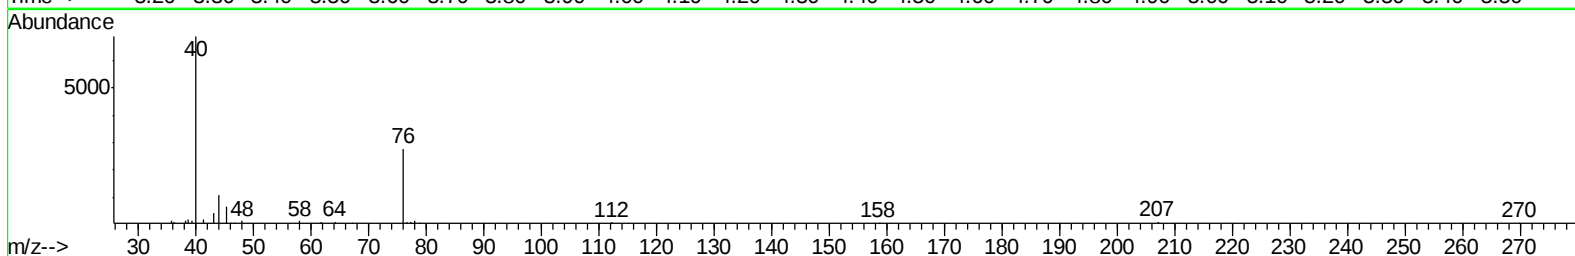


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032719\
Data File : VW009518.D
Acq On : 28 Mar 2019 00:05
Operator : SY/VA
Sample : K2068-12
Misc : 5.50G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:46:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 07:41:43 2019
Response via : Initial Calibration

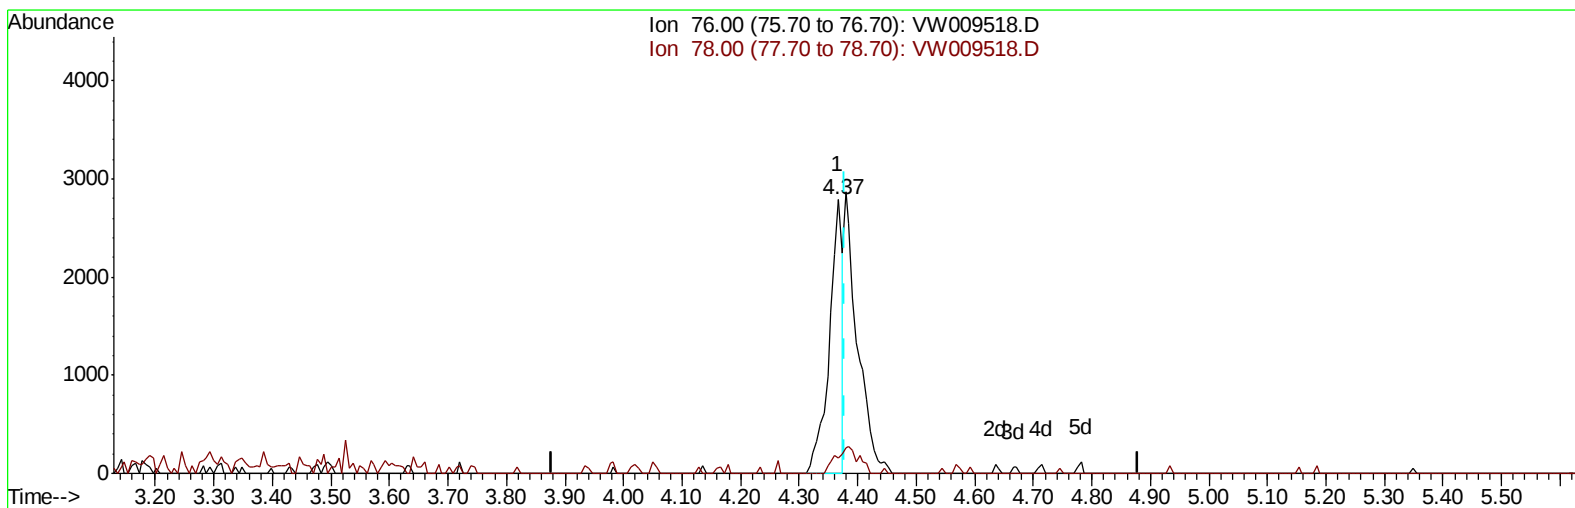

TIC: VW009518.D

(14) Carbon disulfide (T)




4.367min (-0.012) 0.42ug/L

response 4254

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	5.44#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032719\
Data File : VW009518.D
Acq On : 28 Mar 2019 00:05
Operator : SY/VA
Sample : K2068-12
Misc : 5.50G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:46:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 07:41:43 2019
Response via : Initial Calibration

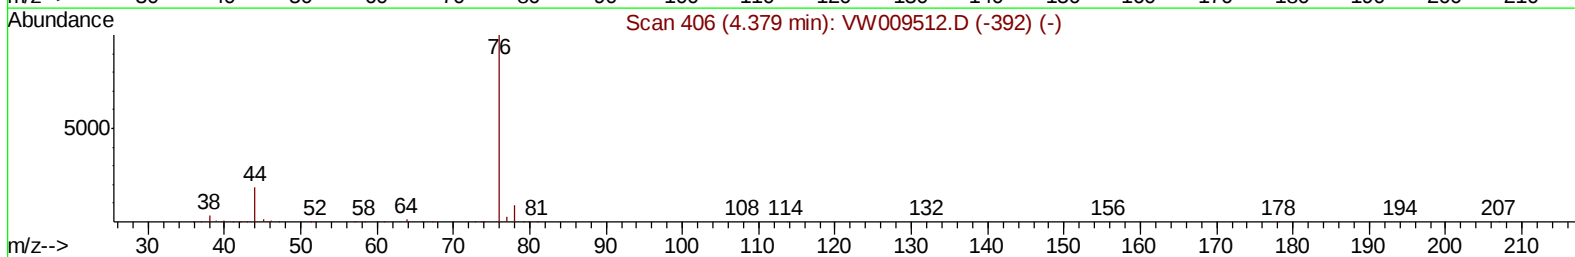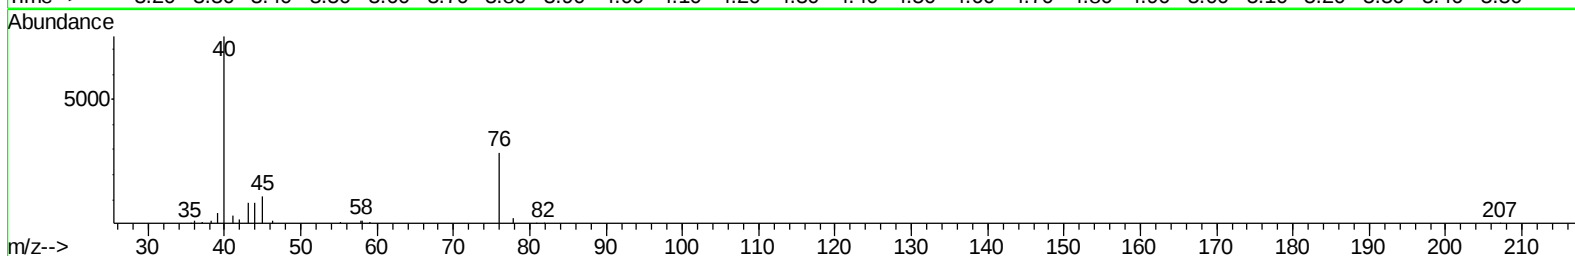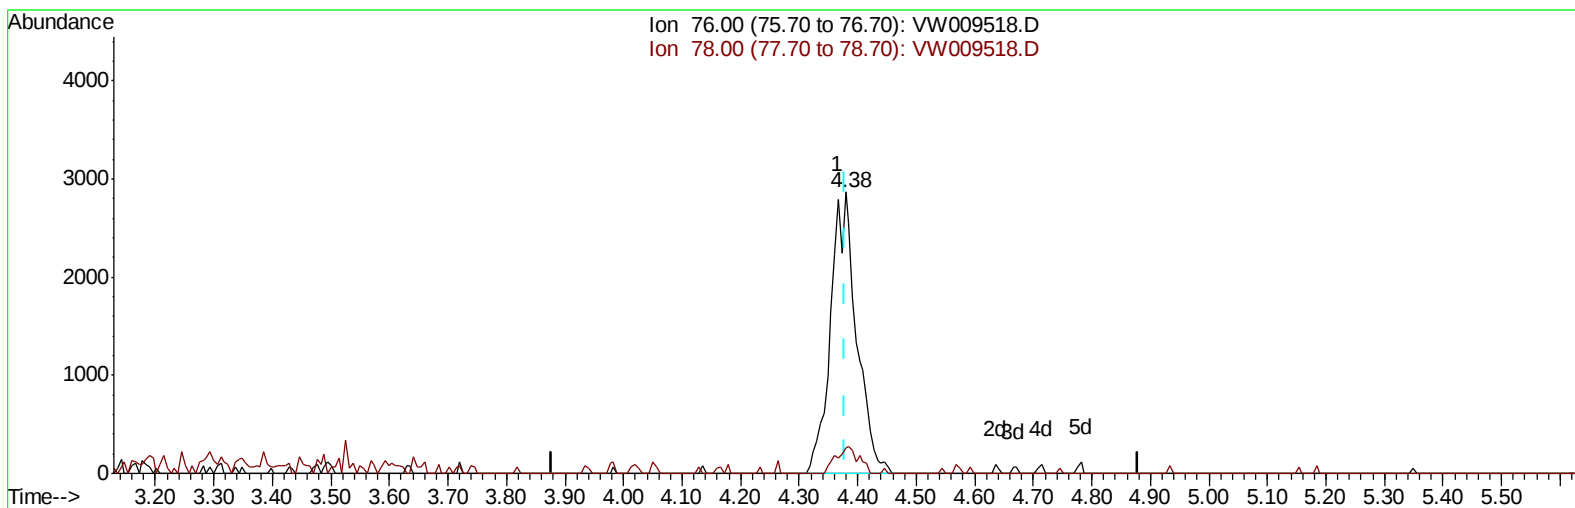

TIC: VW009518.D

(14) Carbon disulfide (T)

4.379min (-0.000) 0.88ug/L m

response 8852

Ion	Exp%	Act%
76.00	100	100
78.00	9.10	8.89
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
 Data File : VW009518.D
 Acq On : 28 Mar 2019 00:05
 Operator : SY/VA
 Sample : K2068-12
 Misc : 5.50G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 08:16:15 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 07:41:43 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	303008	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	255043	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	83183	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	61907	17.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.40%
7) Chloroethane-d5	2.89	69	78923m	18.63	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.52%
10) 1,1-Dichloroethene-d2	4.01	63	104416	13.34	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	53.36%
20) 2-Butanone-d5	7.07	46	82321	54.97	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.94%
24) Chloroform-d	7.65	84	184711	22.34	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.36%
26) 1,2-Dichloroethane-d4	8.30	65	115093	23.10	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.40%
29) Benzene-d6	8.27	84	304225	21.63	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	86.52%
33) 1,2-Dichloropropane-d6	9.27	67	102846	24.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.36%
37) Toluene-d8	10.32	98	238915	18.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.48%
38) trans-1,3-Dichloropropene-	10.57	79	31142	14.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	58.72%
39) 2-Hexanone-d5	10.93	63	47974	46.89	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.78%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	104348	25.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.32%
61) 1,2-Dichlorobenzene-d4	13.85	152	69954	21.93	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.72%


Target Compounds

					Ovalue
13) Acetone	4.12	43	74687	60.819 ug/L	98
14) Carbon disulfide	4.38	76	8852m	0.881 ug/L	
16) Methylene chloride	4.91	84	18718	4.236 ug/L	97
21) 2-Butanone	7.18	43	23610	13.924 ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032719\
Data File : VW009518.D
Acq On : 28 Mar 2019 00:05
Operator : SY/VA
Sample : K2068-12
Misc : 5.50G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 08:16:15 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 07:41:43 2019
Response via : Initial Calibration

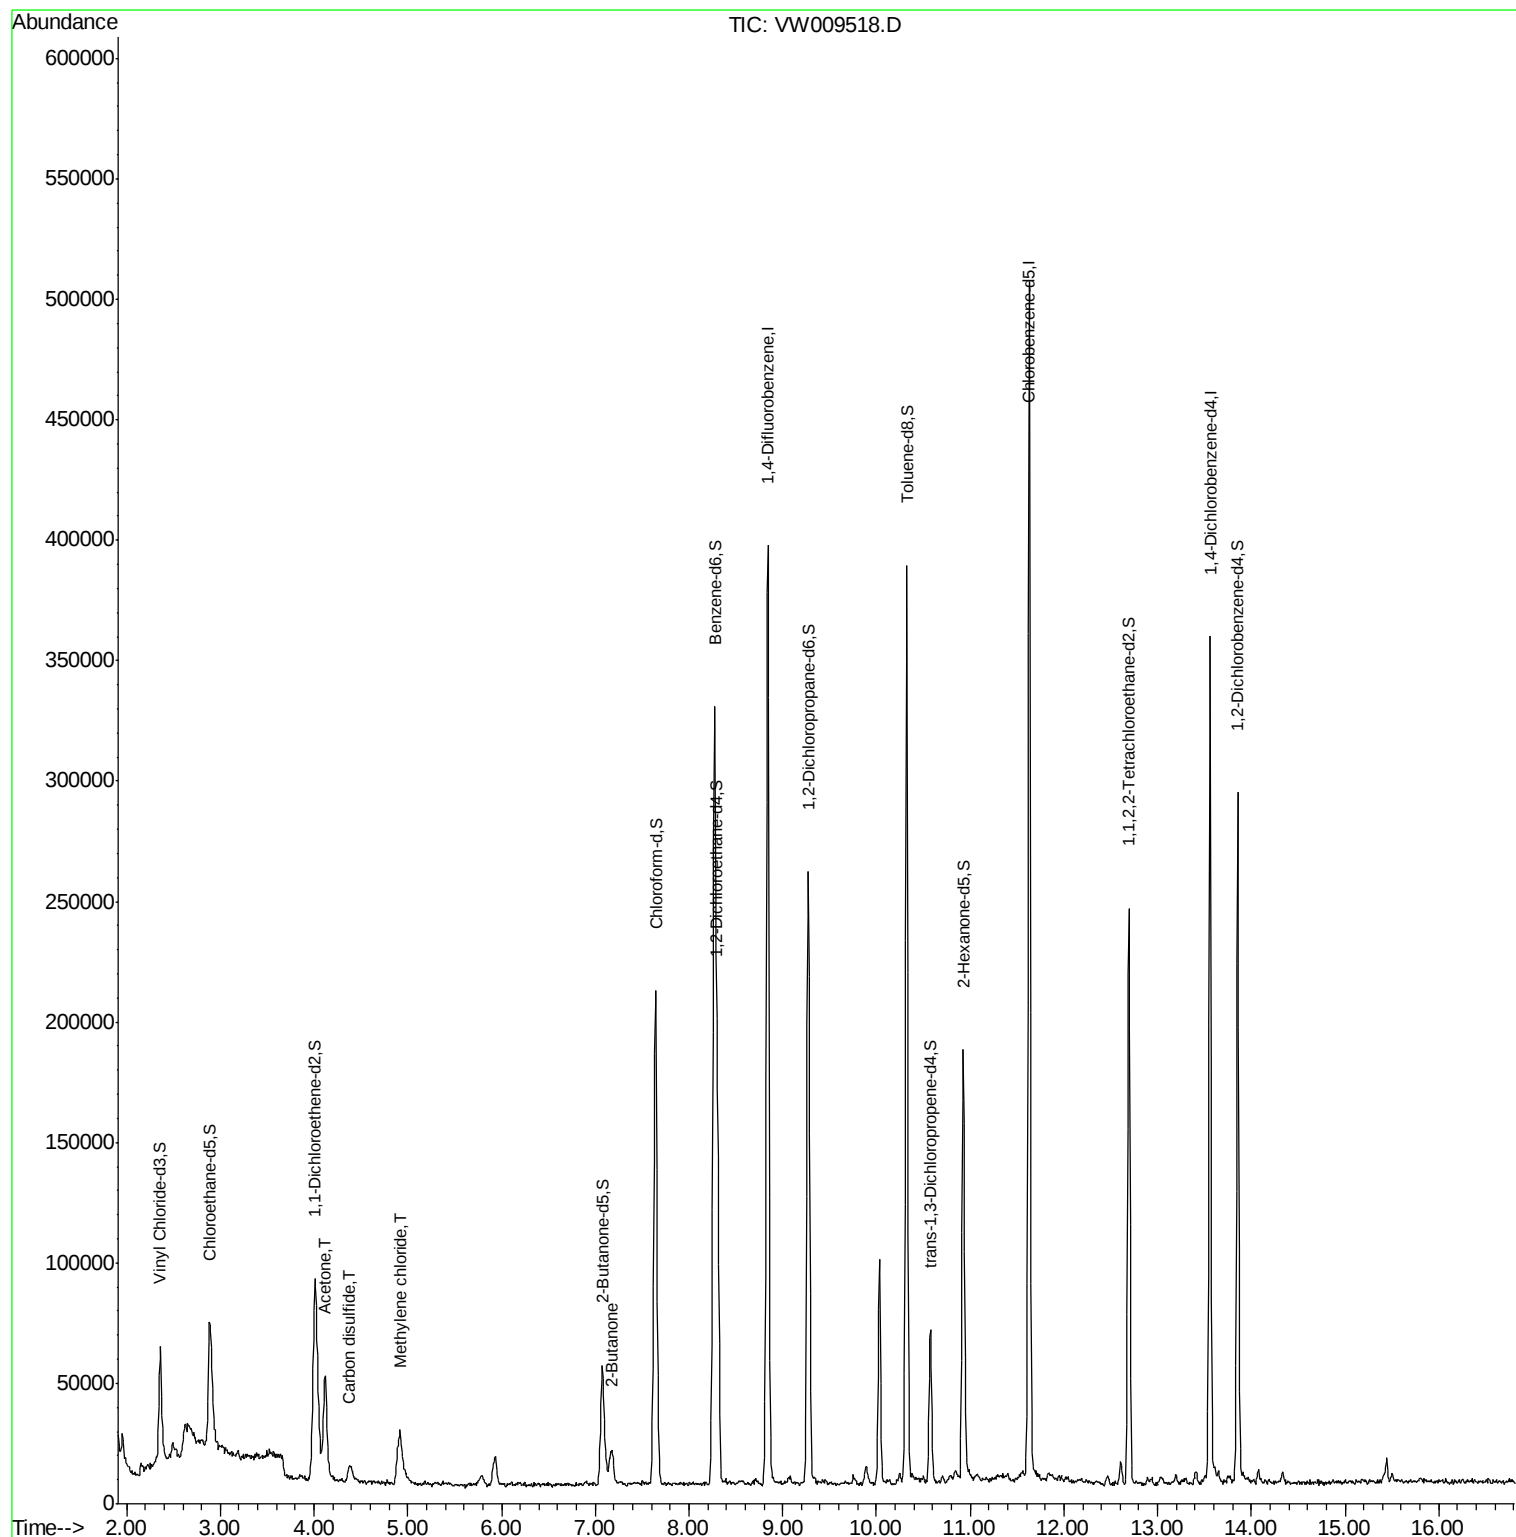

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
 Data File : VW009518.D
 Acq On : 28 Mar 2019 00:05
 Operator : SY/VA
 Sample : K2068-12
 Misc : 5.50G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:46:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 07:41:43 2019
 Response via : Initial Calibration

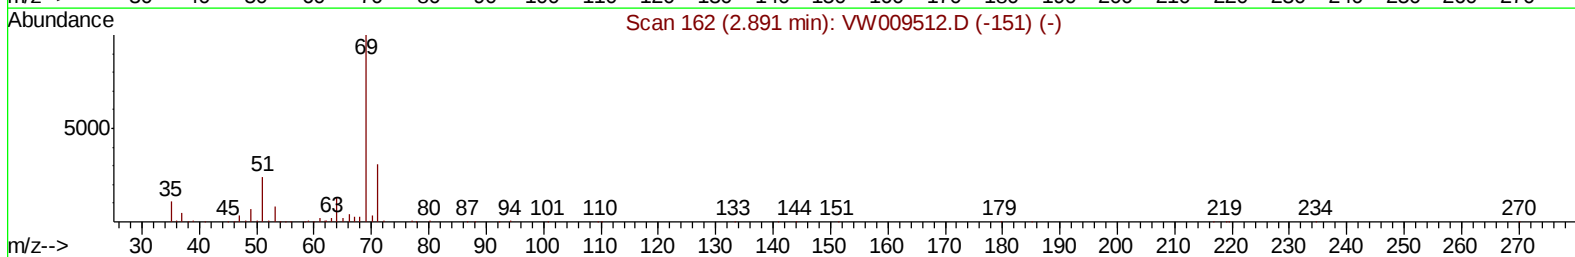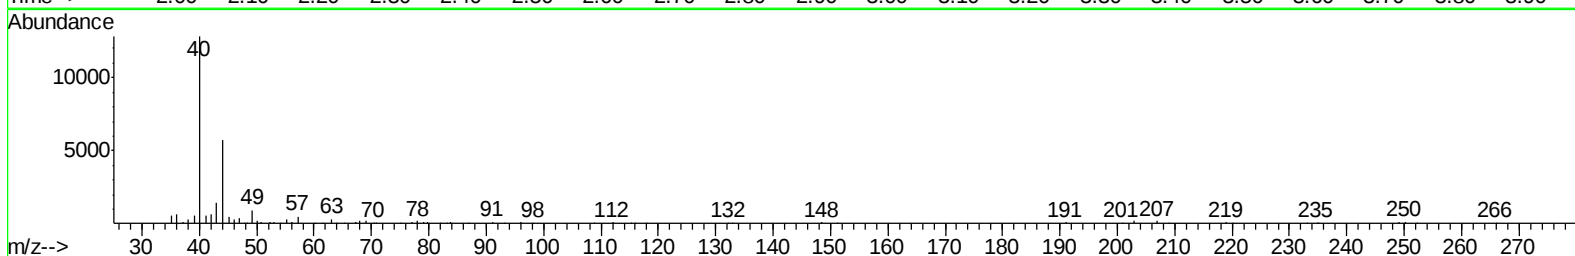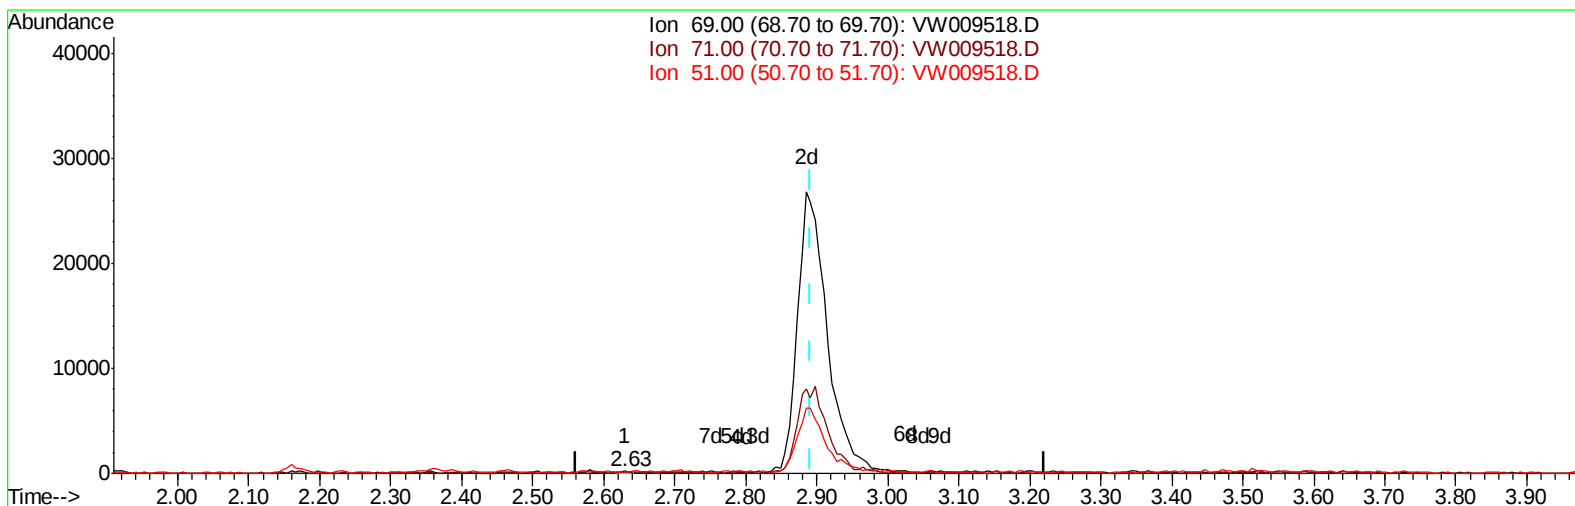

TIC: VW009518.D

(7) Chloroethane-d5 (S)




2.629min (-0.262) 0.08ug/L

response 319

Ion	Exp%	Act%
69.00	100	100
71.00	32.80	31.35
51.00	30.40	25.71
0.00	0.00	0.00

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW032719\
Data File : VW009518.D
Acq On : 28 Mar 2019 00:05
Operator : SY/VA
Sample : K2068-12
Misc : 5.50G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:46:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 07:41:43 2019
Response via : Initial Calibration

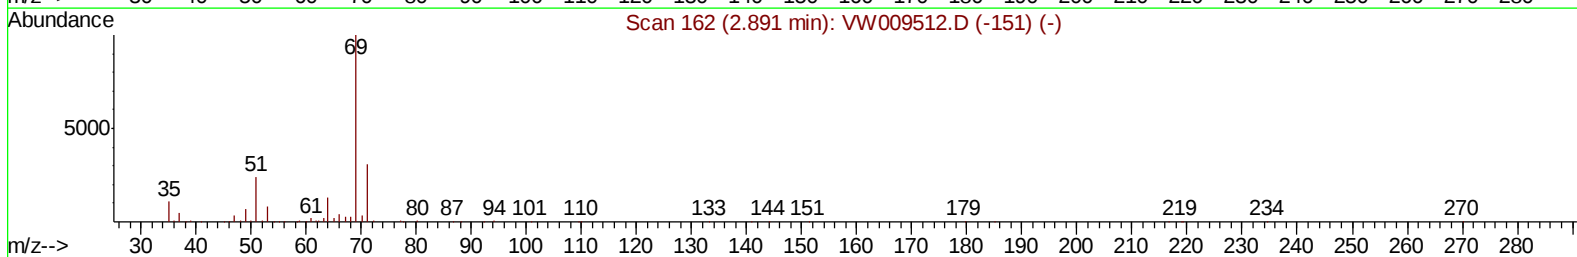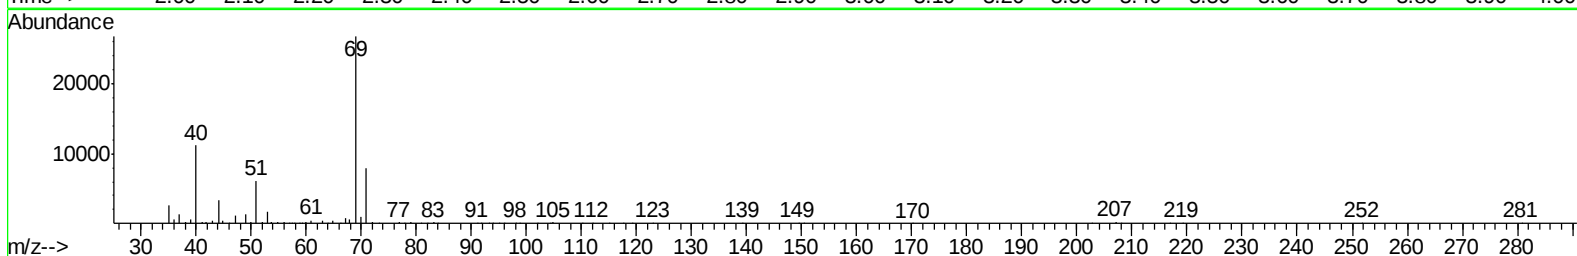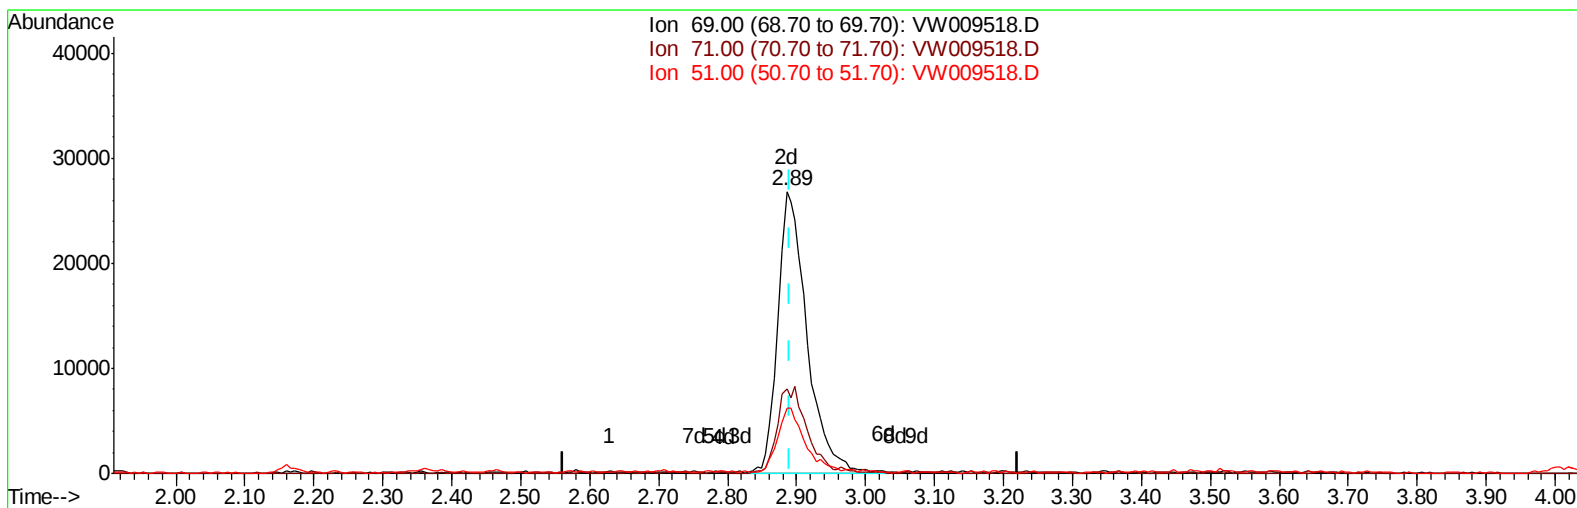

TIC: VW009518.D

(7) Chloroethane-d5 (S)

2.885min (-0.006) 18.63ug/L m

response 78923

Ion	Exp%	Act%
69.00	100	100
71.00	32.80	0.13#
51.00	30.40	0.10#
0.00	0.00	0.00