


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
Data File : VW009507.D
Acq On : 27 Mar 2019 17:07
Operator : SY/VA
Sample : K2065-13
Misc : 6.09G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF5L6RE

Manual Integrations
APPROVED

MMDadoda
3/28/2019 2:47:55 PM

Quant Time: Mar 28 07:11:06 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 04:55:04 2019
Response via : Initial Calibration

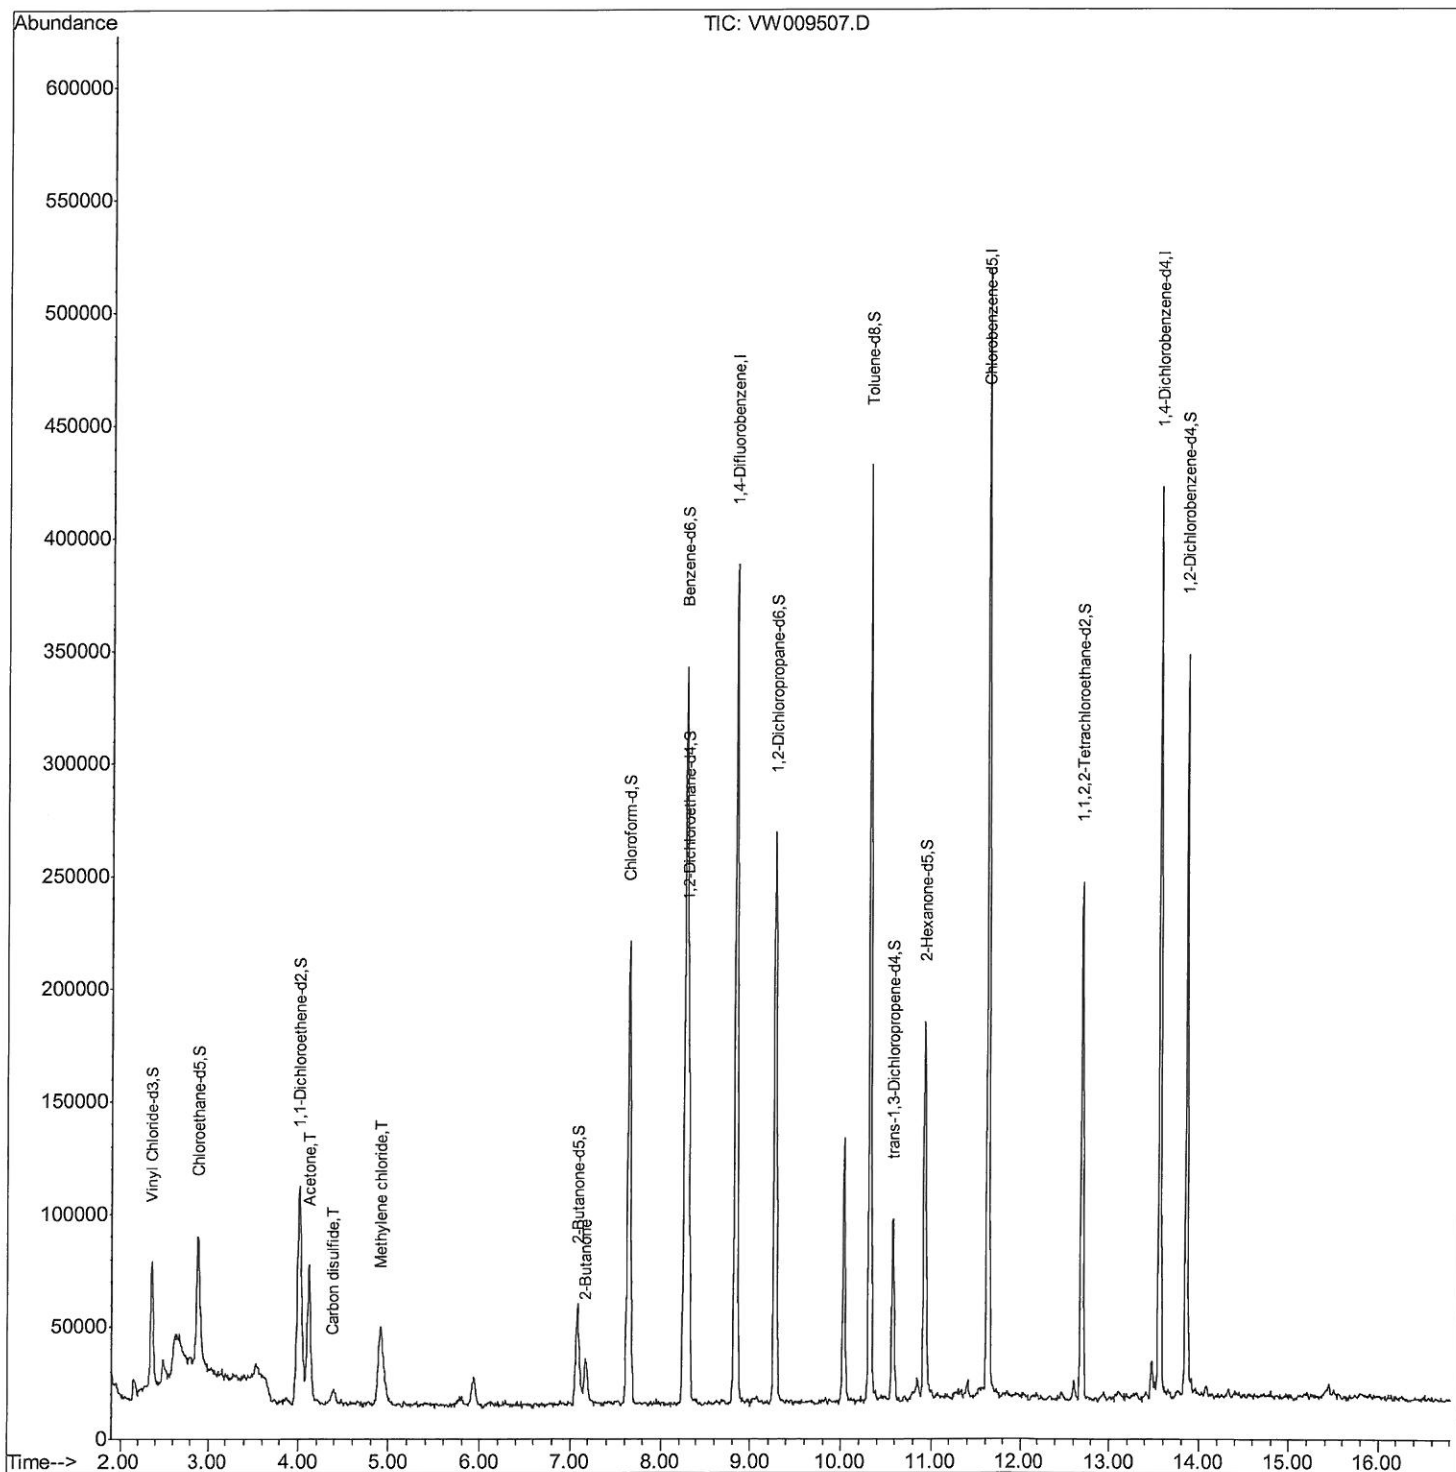

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
 Data File : VW009507.D
 Acq On : 27 Mar 2019 17:07
 Operator : SY/VA
 Sample : K2065-13
 Misc : 6.09G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BF5L6RE

Manual Integrations
APPROVED

MMDadoda
 3/28/2019 2:47:55 PM

Quant Time: Mar 28 05:01:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 04:55:04 2019
 Response via : Initial Calibration

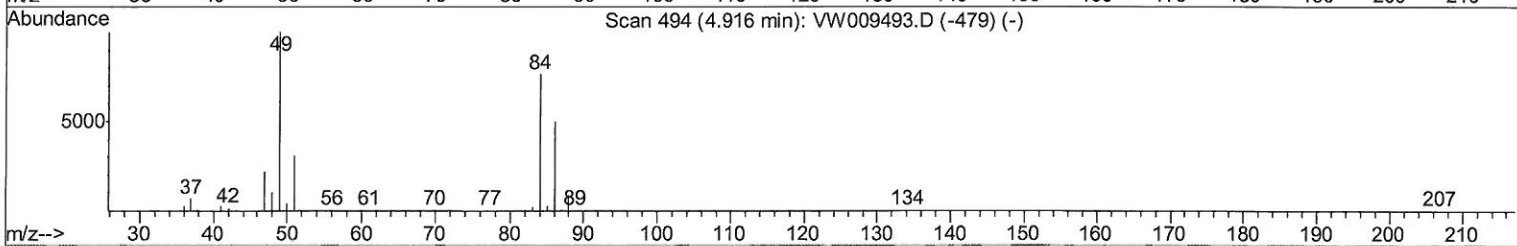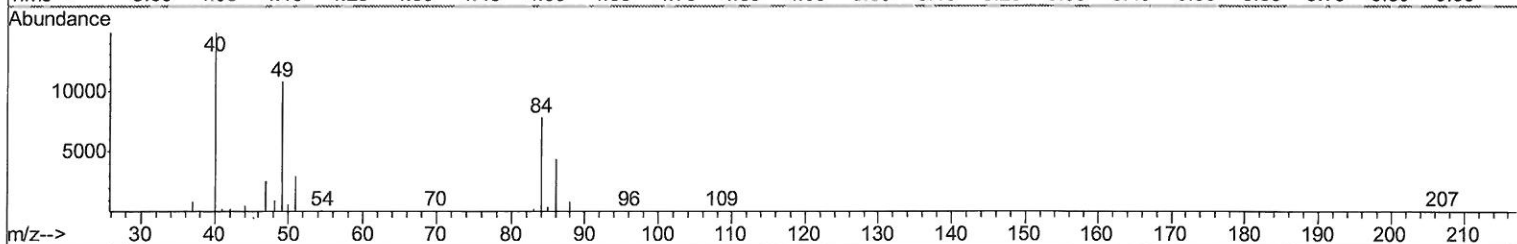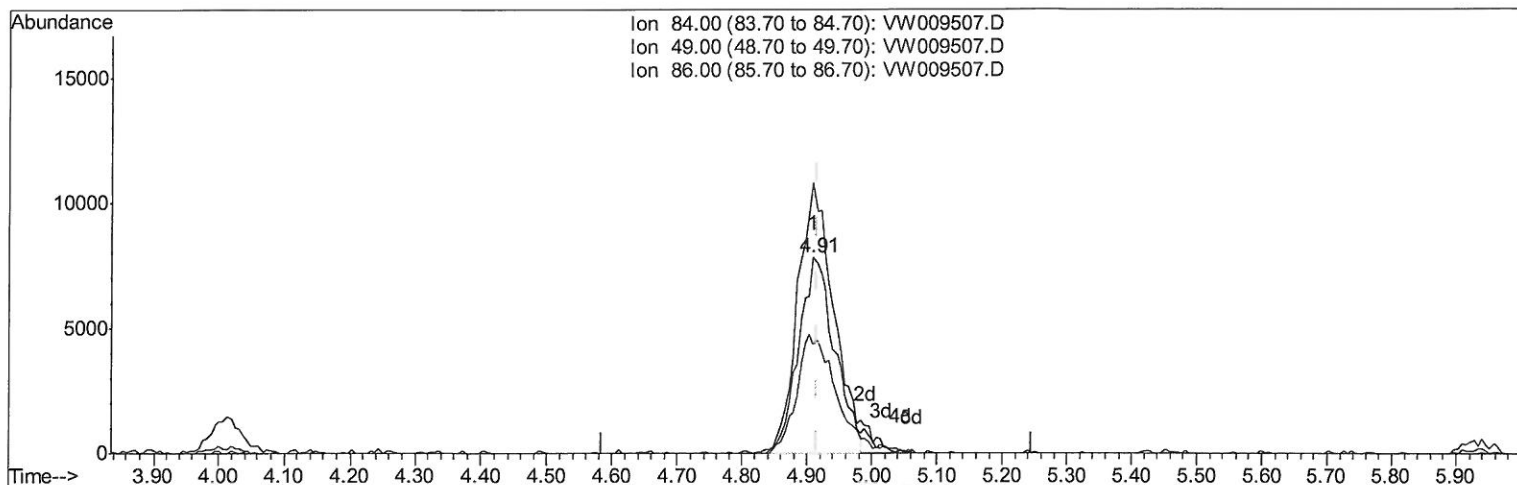

TIC: VW009507.D

(16) Methylene chloride (T)

4.909min (-0.006) 7.09ug/L

response 30237

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	137.66
86.00	63.50	55.99
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
 Data File : VW009507.D
 Acq On : 27 Mar 2019 17:07
 Operator : SY/VA
 Sample : K2065-13
 Misc : 6.09G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5L6RE

Manual Integrations
 APPROVED

MMDadoda
 3/28/2019 2:47:55 PM

Quant Time: Mar 28 05:01:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 04:55:04 2019
 Response via : Initial Calibration

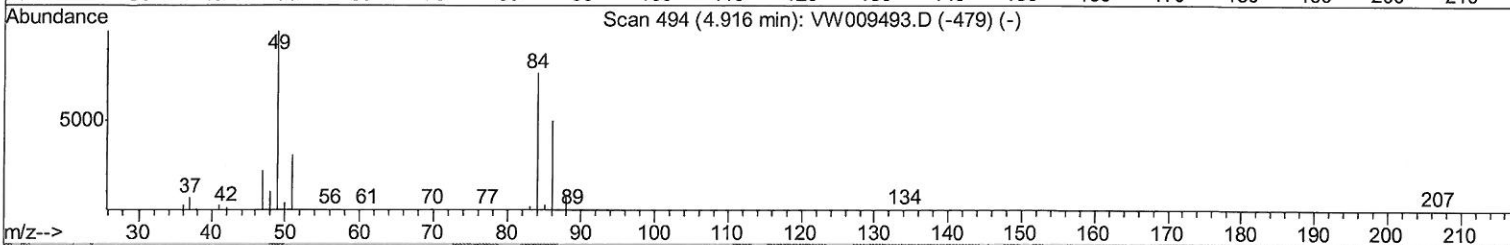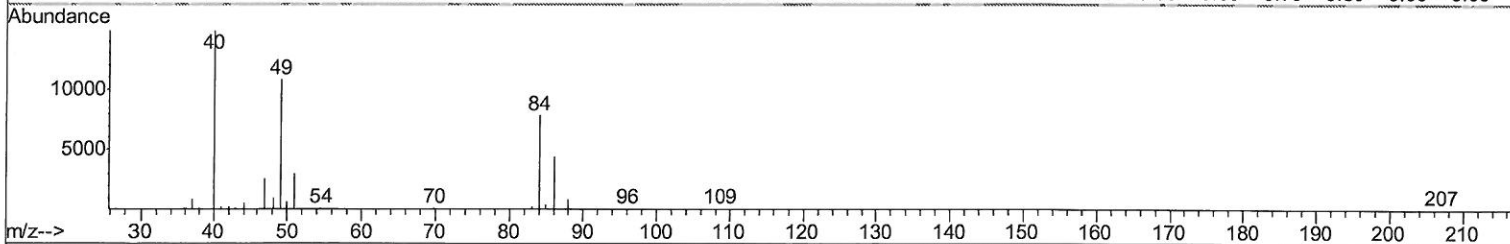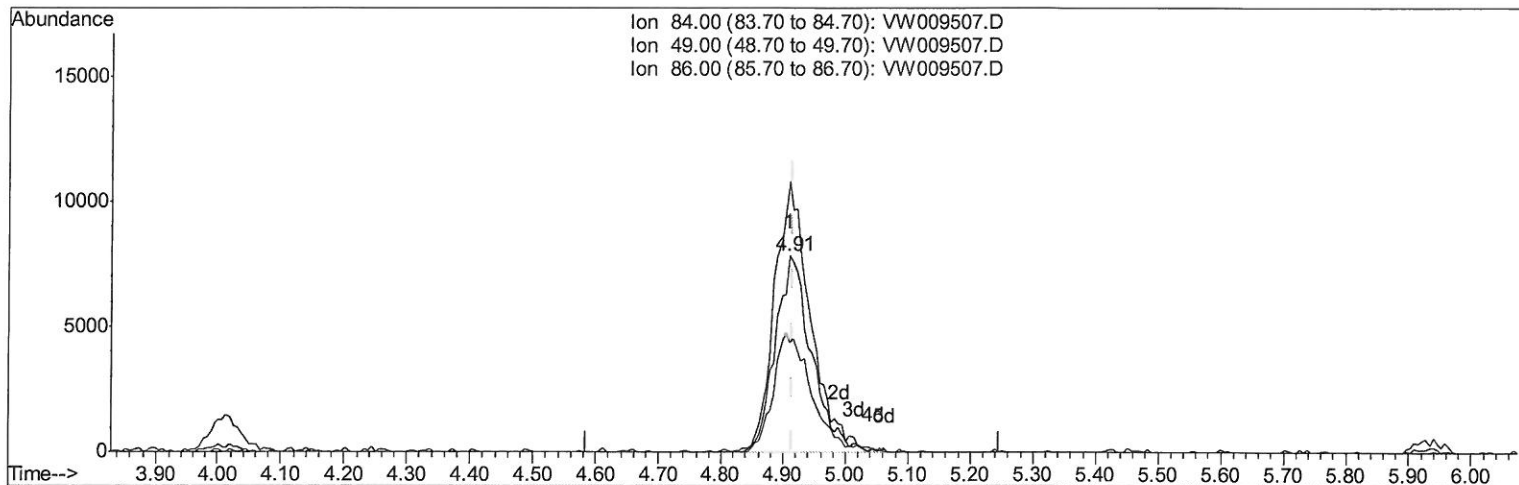

(16) Methylene chloride (T)
 4.909min (-0.006) 7.40ug/L m
 response 31559

MD
 4/6/19

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	137.66
86.00	63.50	55.99
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
 Data File : VW009507.D
 Acq On : 27 Mar 2019 17:07
 Operator : SY/VA
 Sample : K2065-13
 Misc : 6.09G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5L6RE

Manual Integrations
 APPROVED

MMDadoda
 3/28/2019 2:47:55 PM

Quant Time: Mar 28 07:11:06 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 04:55:04 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	292396	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	255091	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	97163	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	71124	20.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.44%
7) Chloroethane-d5	2.89	69	81943	20.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.16%
10) 1,1-Dichloroethene-d2	4.01	63	114793	15.20	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.80%
20) 2-Butanone-d5	7.08	46	74679	51.68	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.36%
24) Chloroform-d	7.64	84	187108	23.45	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.80%
26) 1,2-Dichloroethane-d4	8.31	65	112456	23.39	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.56%
29) Benzene-d6	8.27	84	316131	22.47	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.88%
33) 1,2-Dichloropropane-d6	9.27	67	102806	24.33	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.32%
37) Toluene-d8	10.32	98	252968	19.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.80%
38) trans-1,3-Dichloropropene-	10.58	79	39643	18.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.72%
39) 2-Hexanone-d5	10.93	63	47950	46.86	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.72%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	101745	24.45	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.80%
61) 1,2-Dichlorobenzene-d4	13.86	152	80860	21.70	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.80%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	4.12	43	103140	87.038	ug/L	98
14) Carbon disulfide	4.37	76	7484	0.772	ug/L	96
16) Methylene chloride	4.91	84	31559m	7.401	ug/L	93
21) 2-Butanone	7.17	43	30369	18.561	ug/L	93

7 ml
 4/6/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed