


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
Data File : VW009513.D
Acq On : 27 Mar 2019 21:37
Operator : SY/VA
Sample : VW0327SBL02
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK15

Manual Integrations
APPROVED

MMDadoda
3/28/2019 2:48:01 PM

Quant Time: Mar 28 07:56:36 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 07:41:43 2019
Response via : Initial Calibration

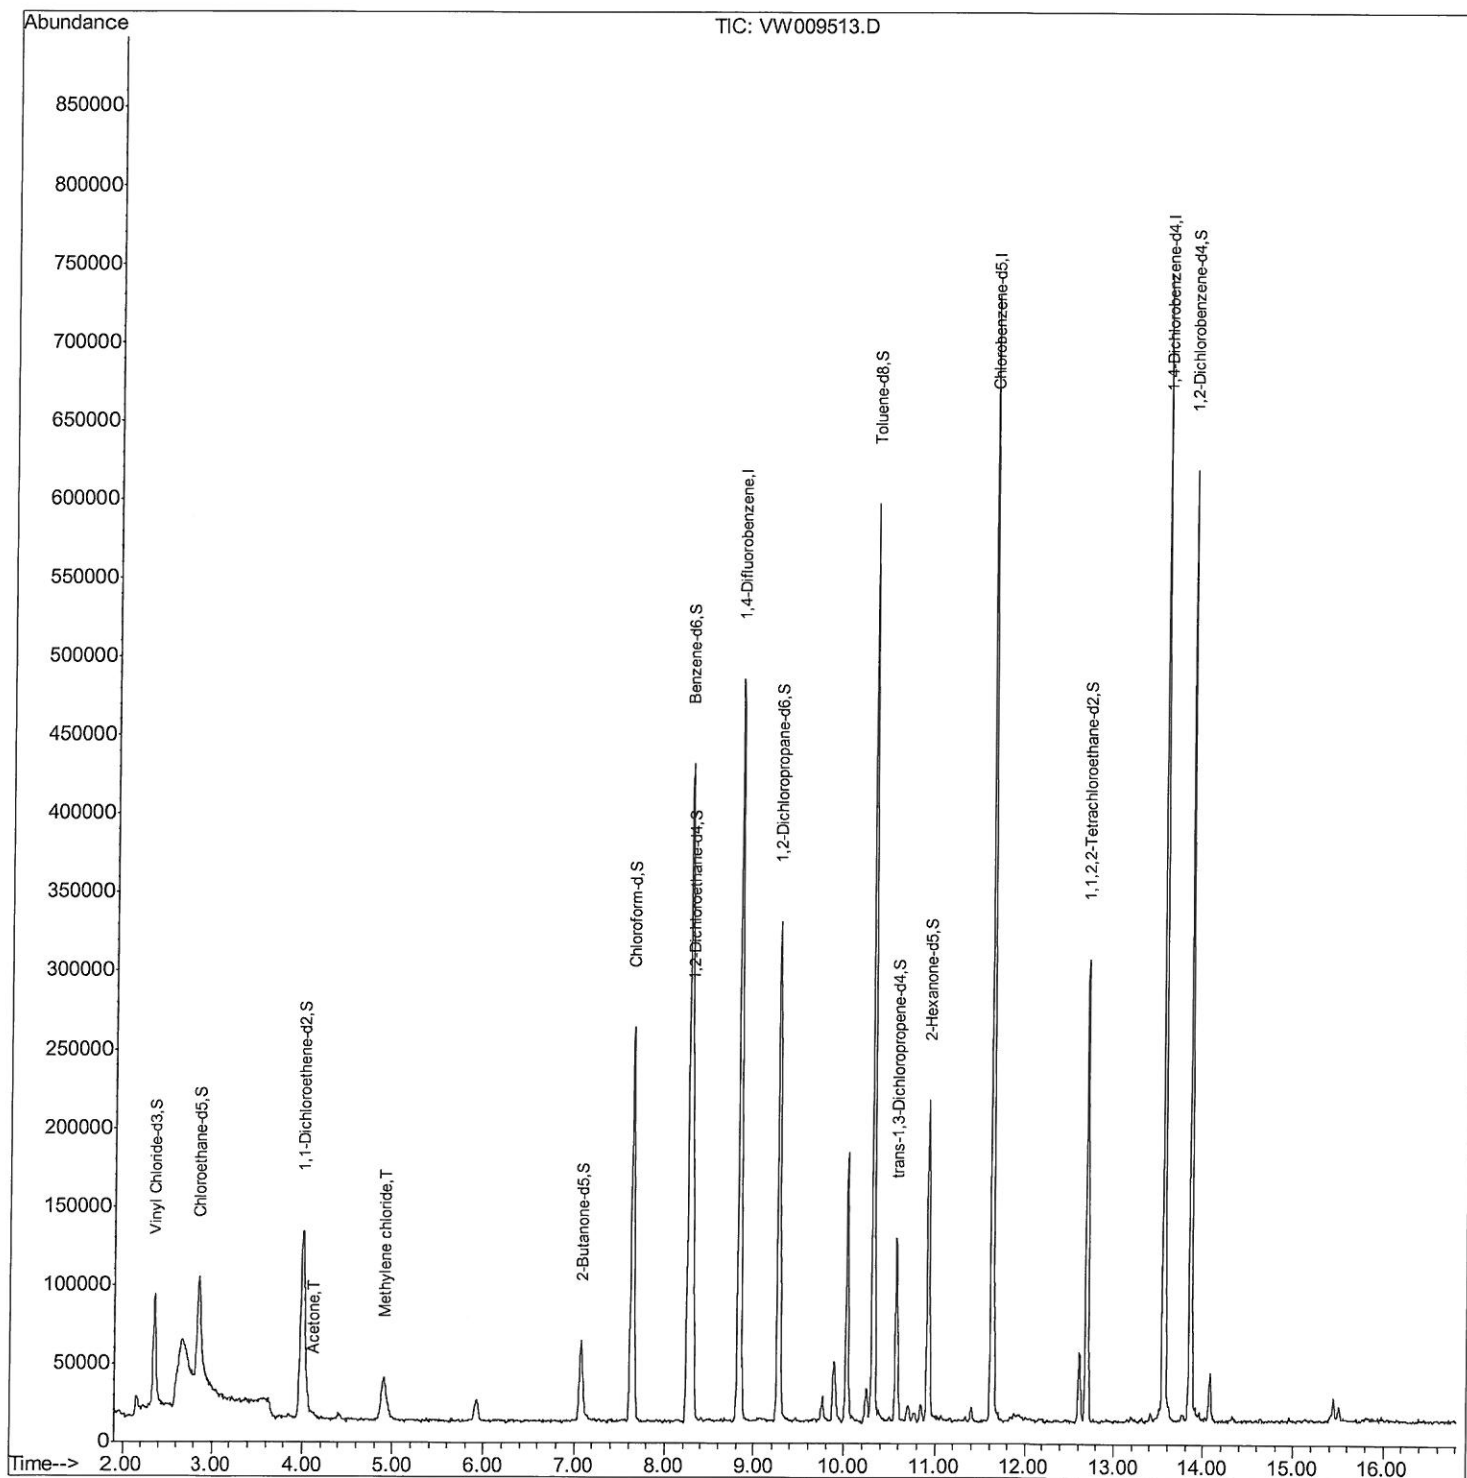

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
Data File : VW009513.D
Acq On : 27 Mar 2019 21:37
Operator : SY/VA
Sample : VW0327SBL02
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK15

Manual Integrations
APPROVED

MMDadoda
3/28/2019 2:48:01 PM

Quant Time: Mar 28 07:46:22 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Thu Mar 28 07:41:43 2019
Response via : Initial Calibration

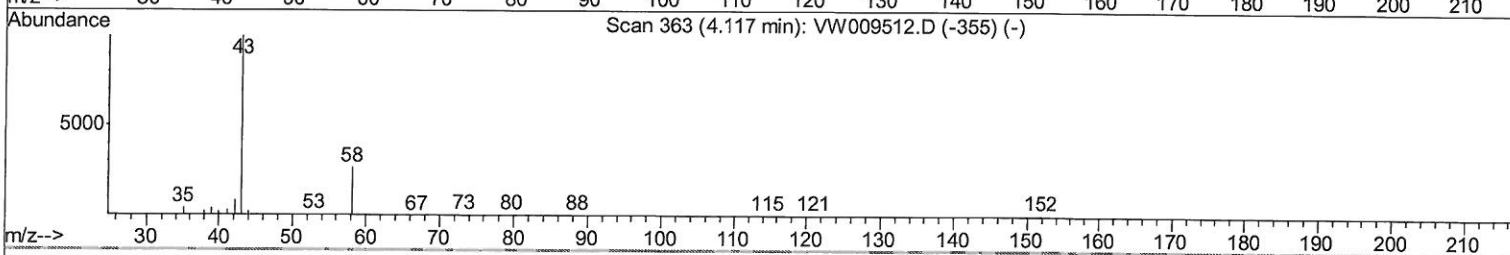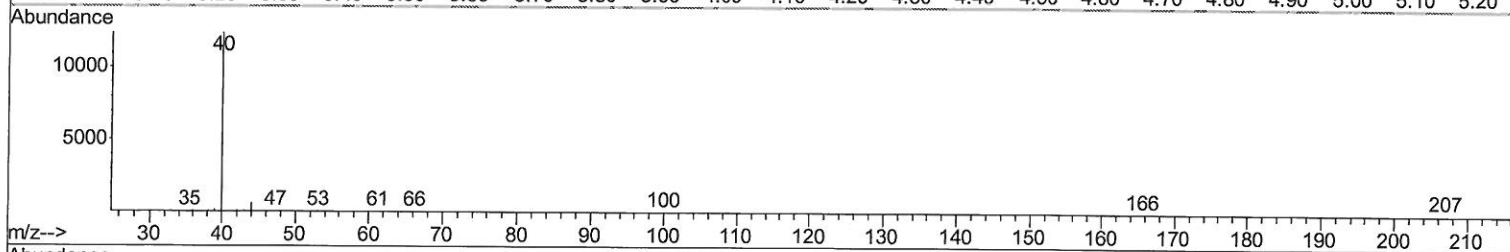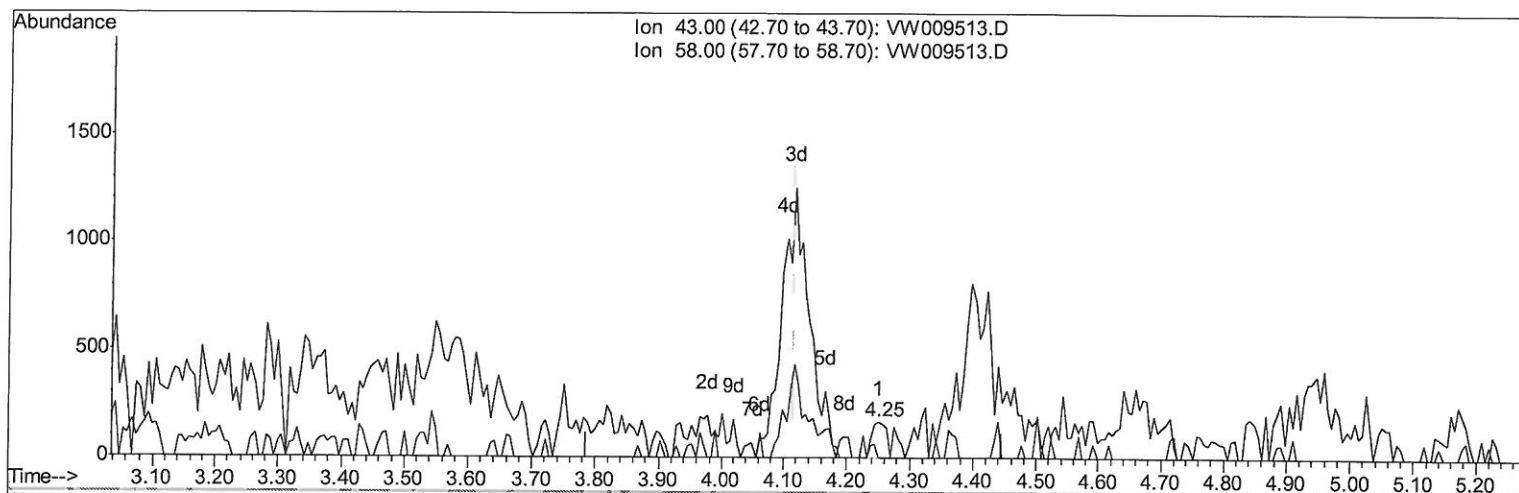

TIC: VW009513.D

(13) Acetone (T)

4.251min (+0.134) 0.17ug/L

response 254

Ion	Exp%	Act%
43.00	100	100
58.00	28.10	17.72
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
 Data File : VW009513.D
 Acq On : 27 Mar 2019 21:37
 Operator : SY/VA
 Sample : VW0327SBL02
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK15

Manual Integrations
 APPROVED

MMDadoda
 3/28/2019 2:48:01 PM

Quant Time: Mar 28 07:46:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 07:41:43 2019
 Response via : Initial Calibration

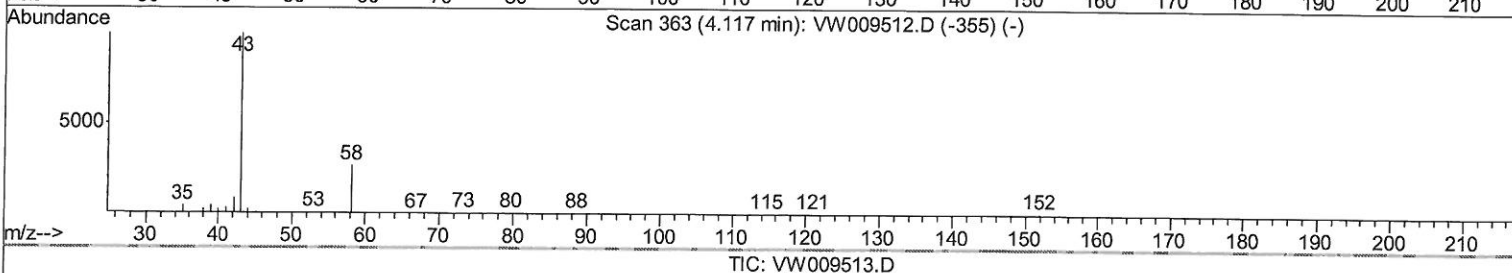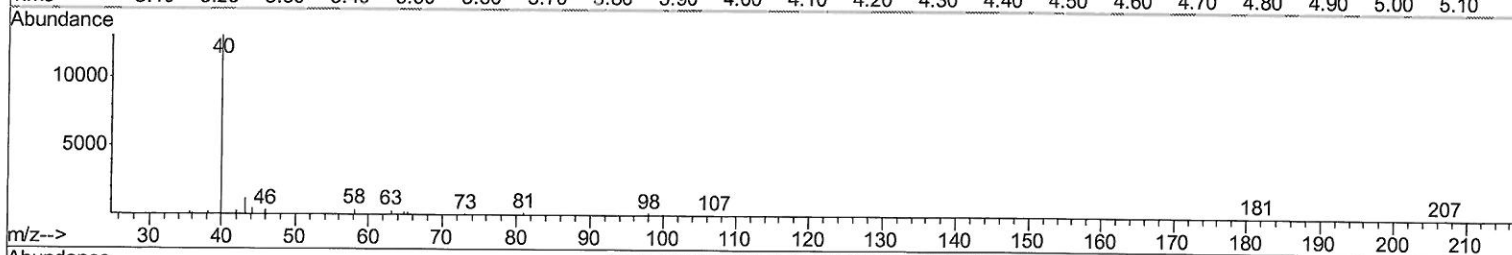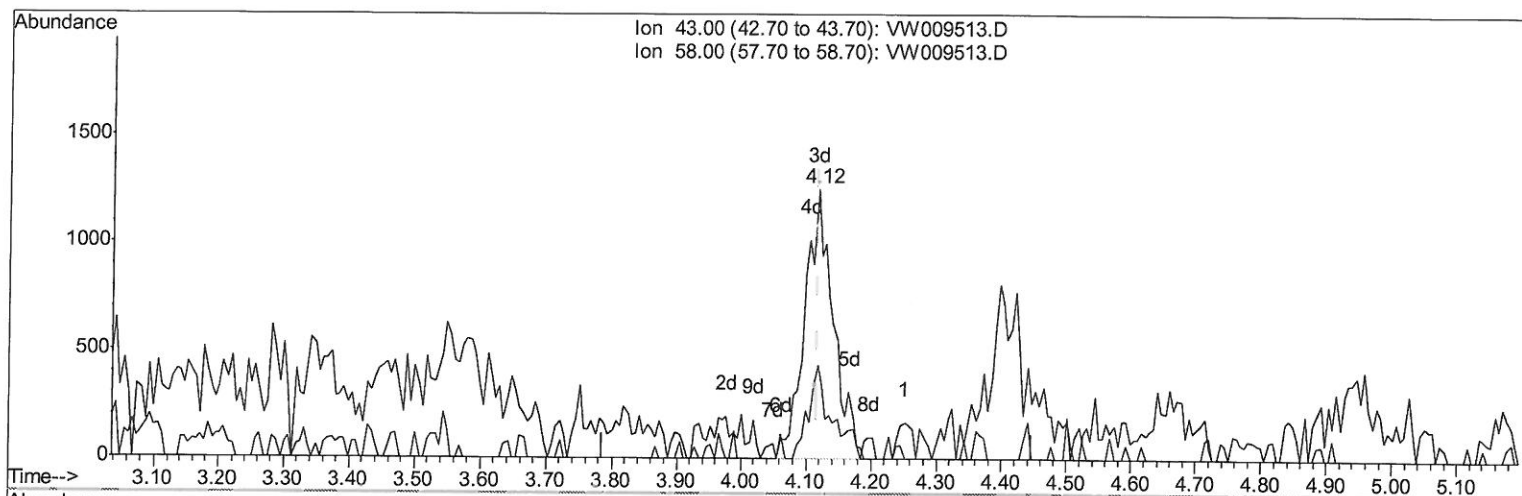

(13) Acetone (T)

4.117min (+0.000) 2.47ug/L m

response 3747

Ion	Exp%	Act%
43.00	100	100
58.00	28.10	1.20
0.00	0.00	0.00
0.00	0.00	0.00

7 MO
 4/6/19

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
 Data File : VW009513.D
 Acq On : 27 Mar 2019 21:37
 Operator : SY/VA
 Sample : VW0327SBL02
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK15

Manual Integrations
 APPROVED

MMDadoda
 3/28/2019 2:48:01 PM

Quant Time: Mar 28 07:46:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 07:41:43 2019
 Response via : Initial Calibration

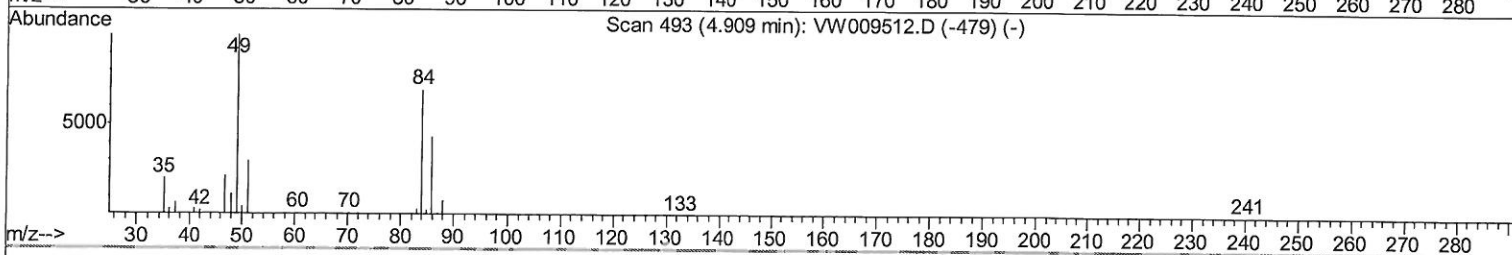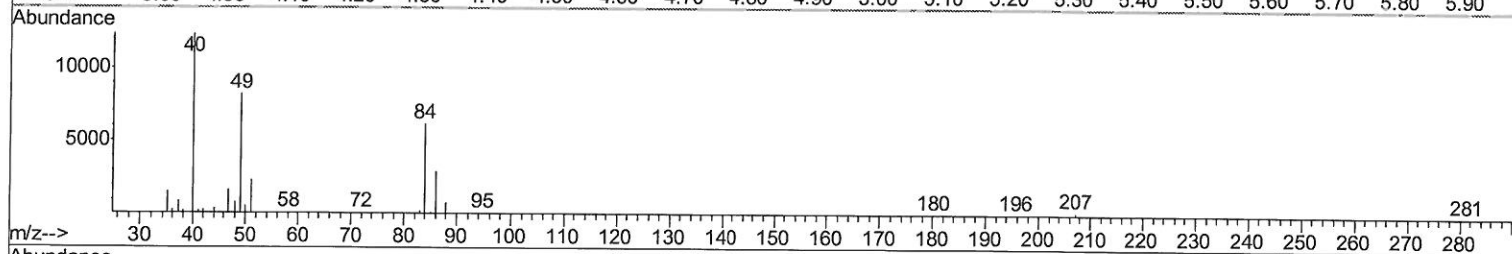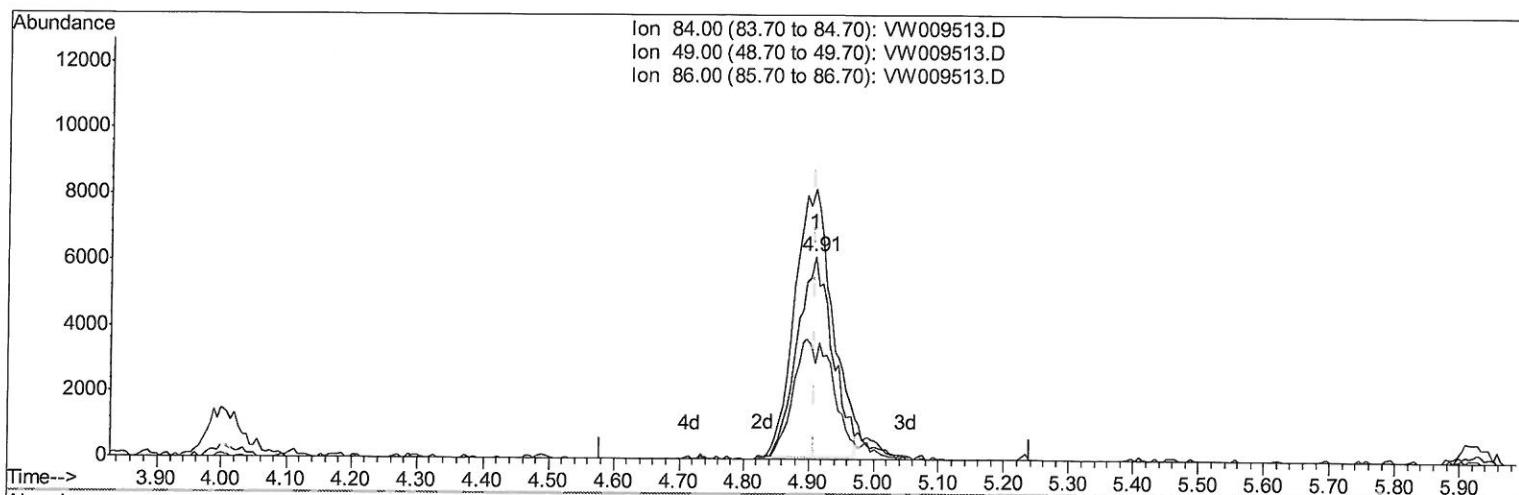

TIC: VW009513.D

(16) Methylene chloride (T)

4.909min (+0.000) 4.19ug/L

response 22887

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	132.98
86.00	63.50	47.28
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
 Data File : VW009513.D
 Acq On : 27 Mar 2019 21:37
 Operator : SY/VA
 Sample : VW0327SBL02
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK15

Manual Integrations
 APPROVED

MMDadoda
 3/28/2019 2:48:01 PM

Quant Time: Mar 28 07:46:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 07:41:43 2019
 Response via : Initial Calibration

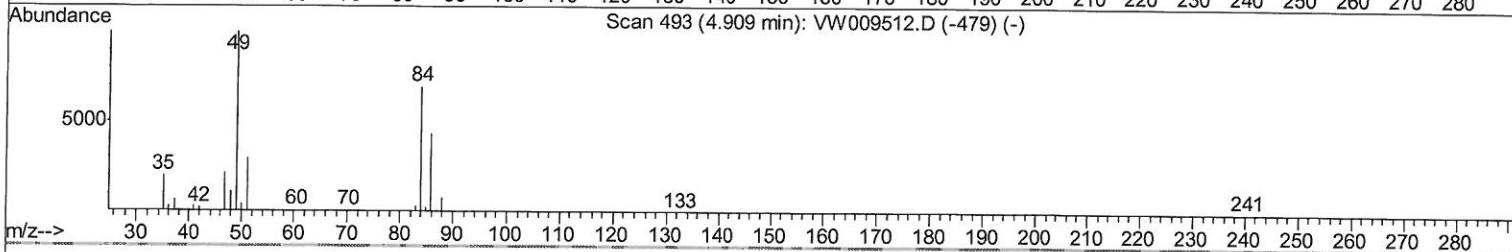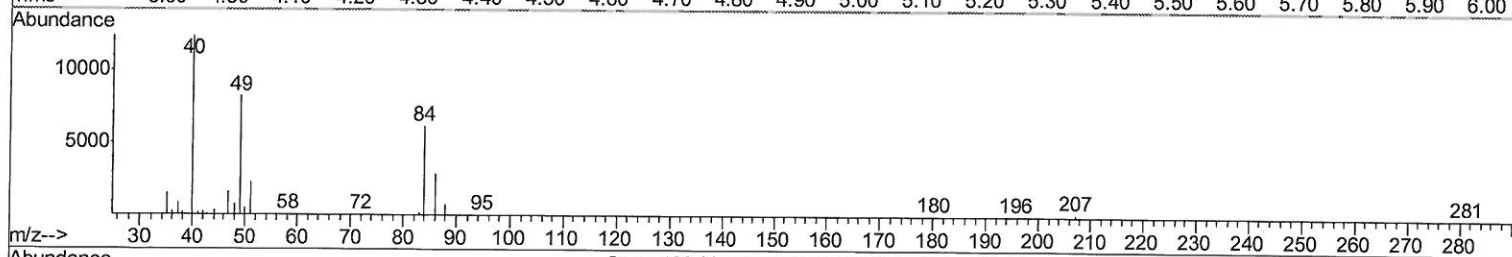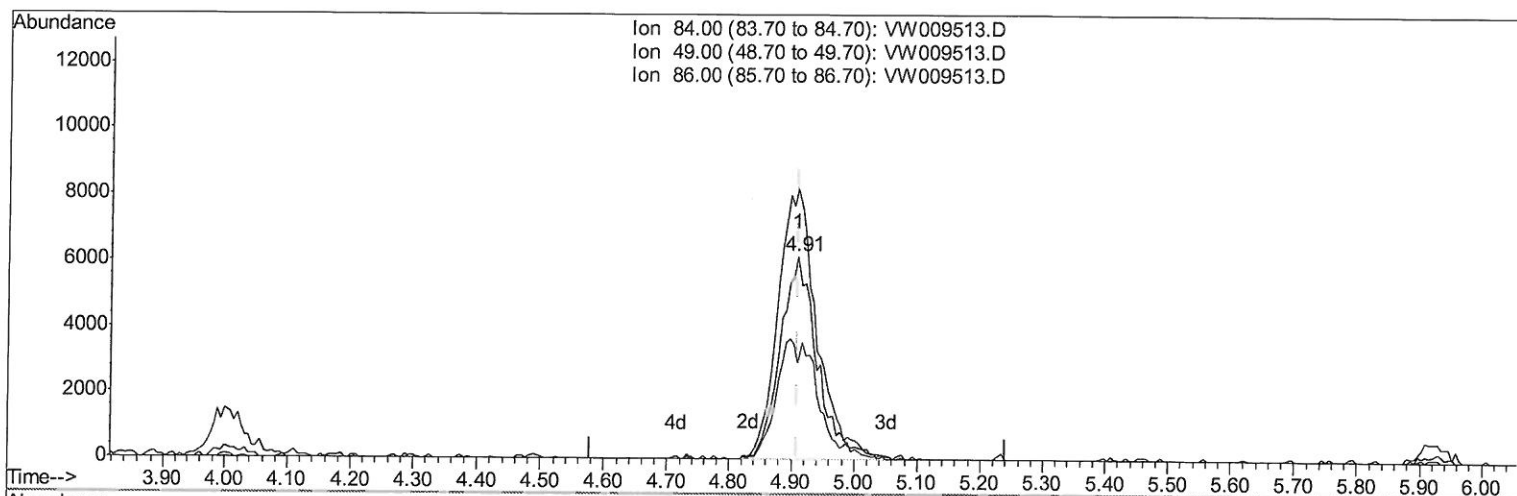

TIC: VW009513.D

(16) Methylene chloride (T)

4.909min (+0.000) 4.58ug/L m

response 25021

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	132.98
86.00	63.50	47.28
0.00	0.00	0.00

7 mg
 4/6/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW032719\
 Data File : VW009513.D
 Acq On : 27 Mar 2019 21:37
 Operator : SY/VA
 Sample : VW0327SBL02
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK15

Manual Integrations
 APPROVED

MMDadoda
 3/28/2019 2:48:01 PM

Quant Time: Mar 28 07:56:36 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Mar 28 07:41:43 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	374579	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	365479	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	173802	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	84117	18.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.16%
7) Chloroethane-d5	2.86	69	101923	19.46	ug/L	-0.03
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.84%
10) 1,1-Dichloroethene-d2	4.00	63	146408	15.13	ug/L	-0.02
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.52%
20) 2-Butanone-d5	7.07	46	86944	46.97	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.94%
24) Chloroform-d	7.64	84	223713	21.88	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.52%
26) 1,2-Dichloroethane-d4	8.30	65	141476	22.97	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.88%
29) Benzene-d6	8.27	84	409333	20.31	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.24%
33) 1,2-Dichloropropane-d6	9.27	67	132437	21.88	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.52%
37) Toluene-d8	10.32	98	368952	19.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.20%
38) trans-1,3-Dichloropropene-	10.57	79	56876	18.71	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.84%
39) 2-Hexanone-d5	10.92	63	61887	42.21	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.42%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	128765	21.60	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.40%
61) 1,2-Dichlorobenzene-d4	13.86	152	151237	22.69	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.76%

Target Compounds

13) Acetone	4.12	43	3747m	2.468	ug/L	Ovalue
16) Methylene chloride	4.91	84	25021m	4.581	ug/L	

} m2
 4/6/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed