


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032819\
Quantitation Report (QT Reviewed)
Data File : VW009550.D
Acq On : 28 Mar 2019 21:39
Operator : SY/VA
Sample : VW0328SBL02
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK17

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:06:12 AM

Quant Time: Mar 29 07:50:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 29 07:41:24 2019
Response via : Initial Calibration

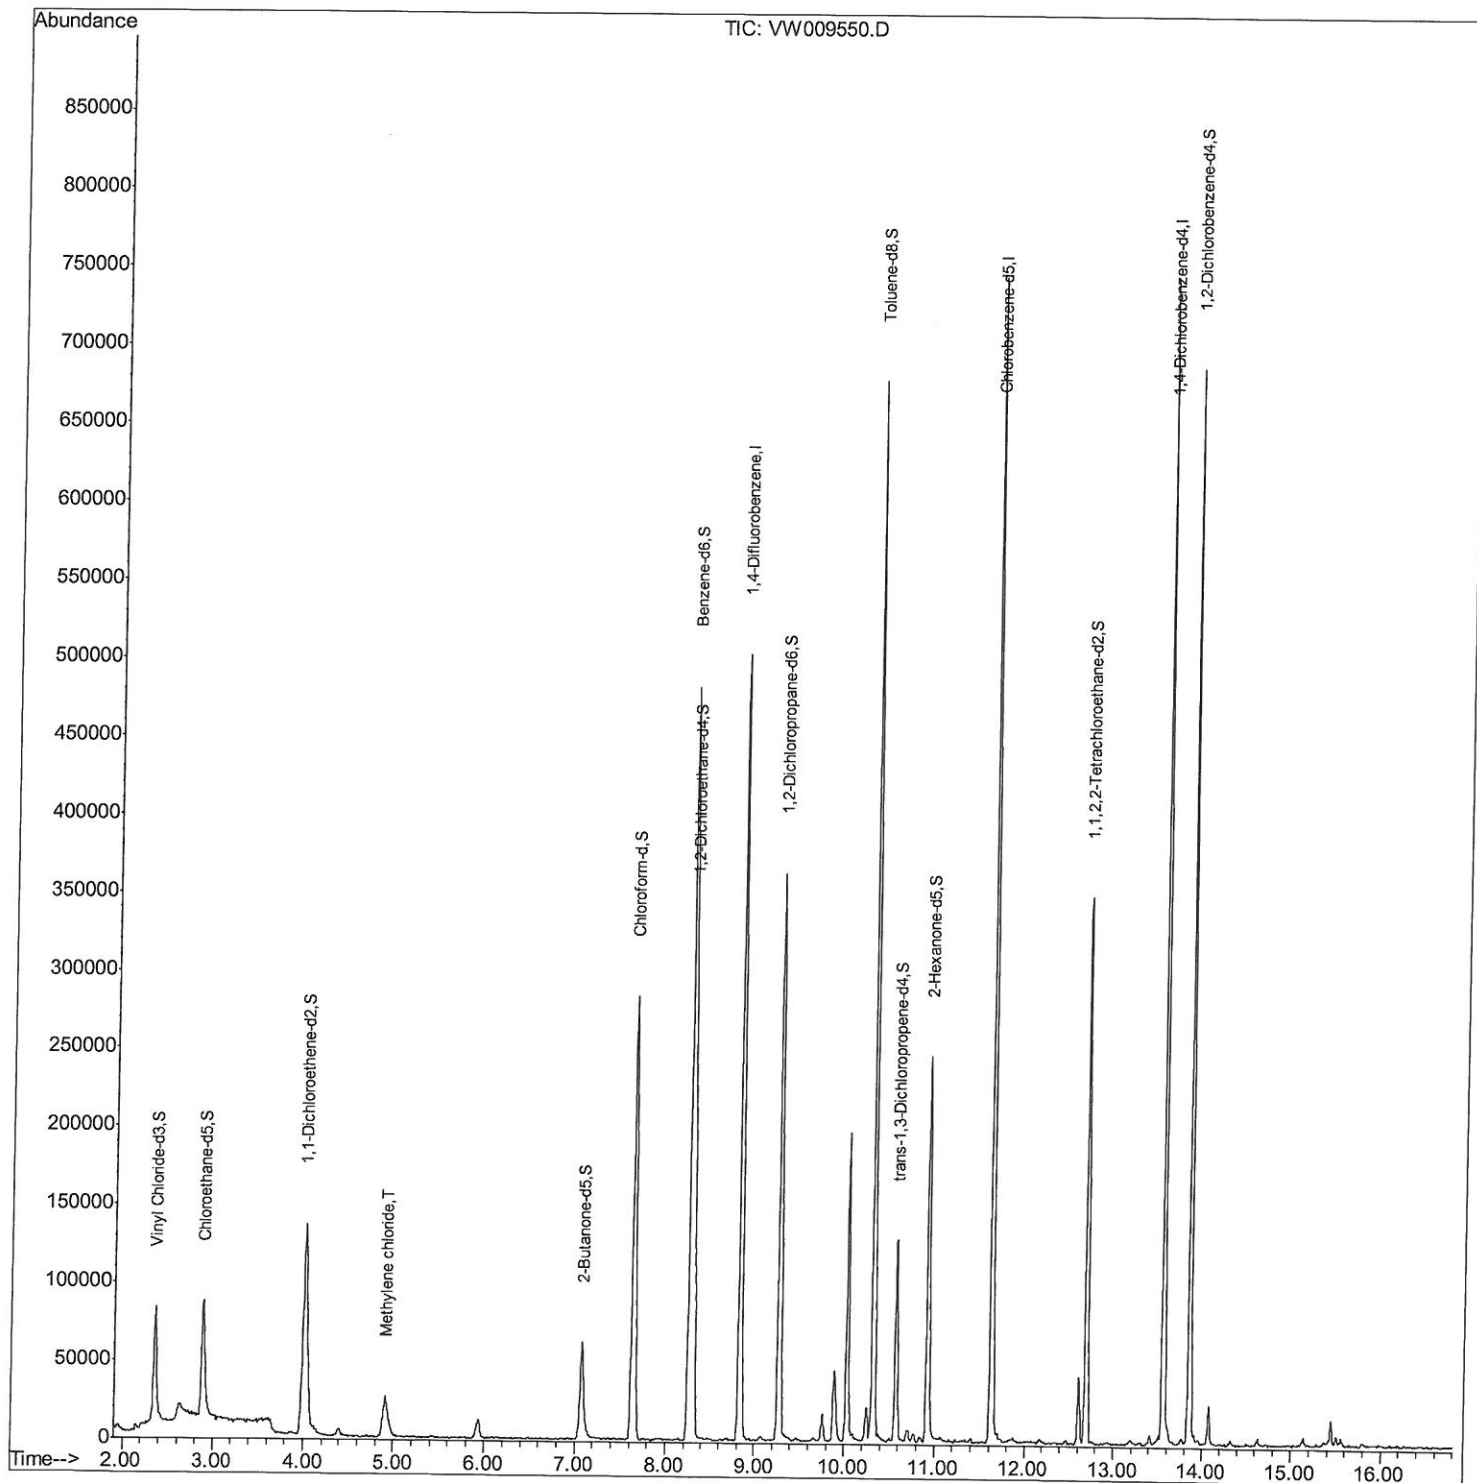

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032819\
Quantitation Report (Qedit)




Data File : VW009550.D
Acq On : 28 Mar 2019 21:39
Operator : SY/VA
Sample : VW0328SBL02
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VBLK17

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:06:12 AM

Quant Time: Mar 29 07:44:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 29 07:41:24 2019
Response via : Initial Calibration

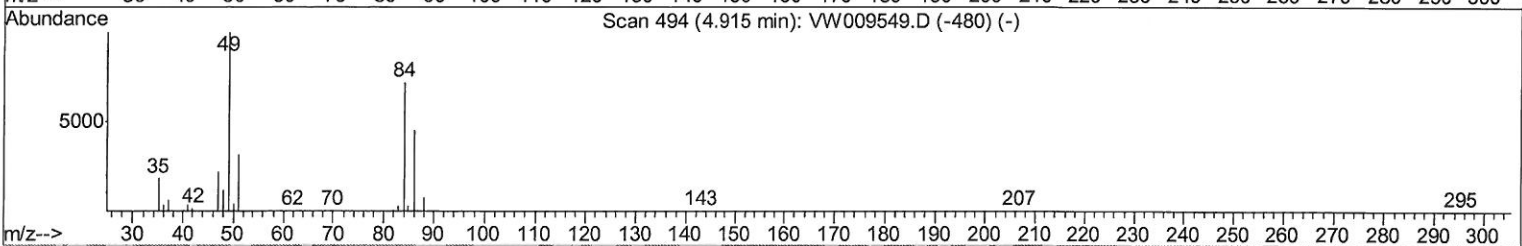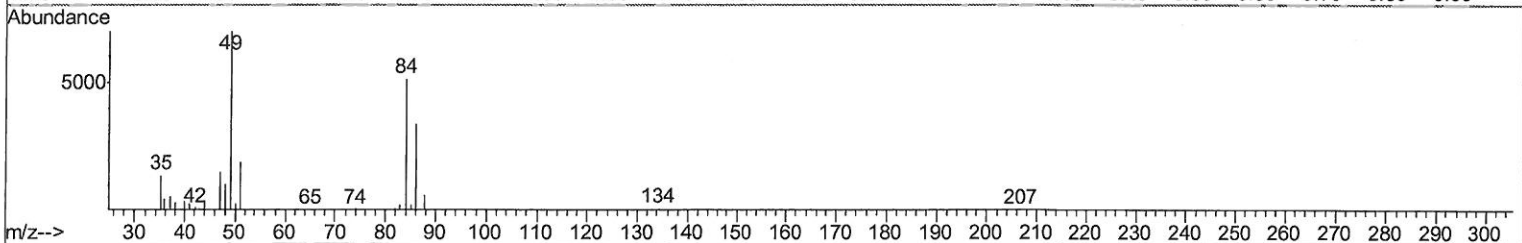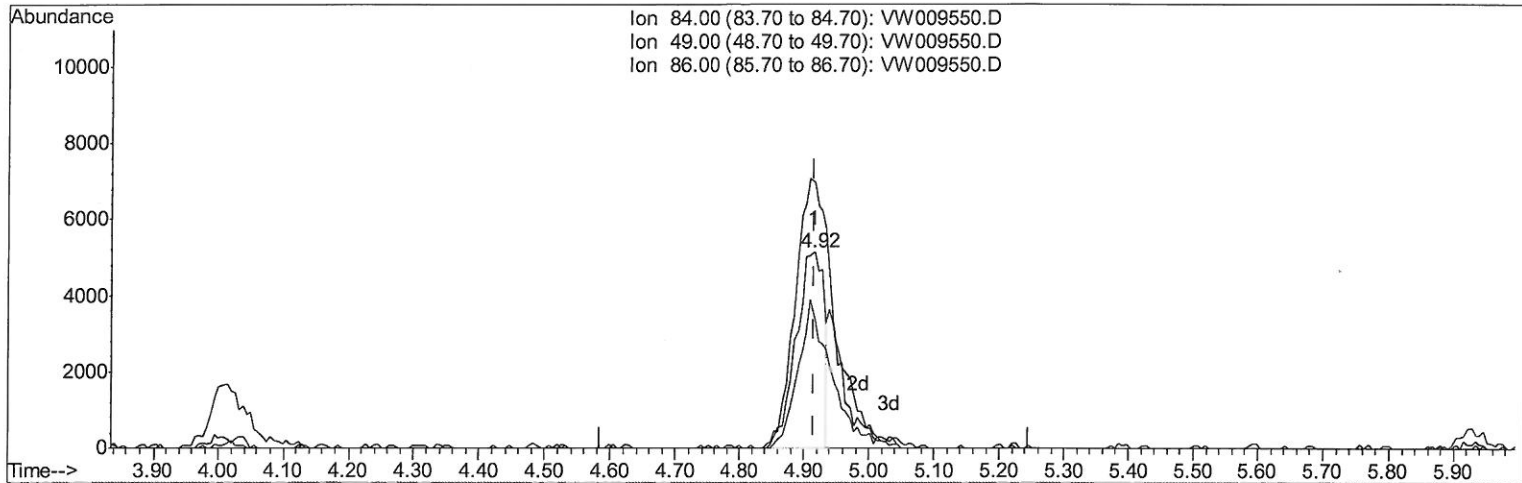

TIC: VW009550.D

(16) Methylene chloride (T)

4.916min (+0.000) 2.68ug/L

response 15370

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	135.67
86.00	63.50	65.87
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032819\
Quantitation Report (Qedit)




Data File : VW009550.D
Acq On : 28 Mar 2019 21:39
Operator : SY/VA
Sample : VW0328SBL02
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
VBLK17

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:06:12 AM

Quant Time: Mar 29 07:44:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 29 07:41:24 2019
Response via : Initial Calibration

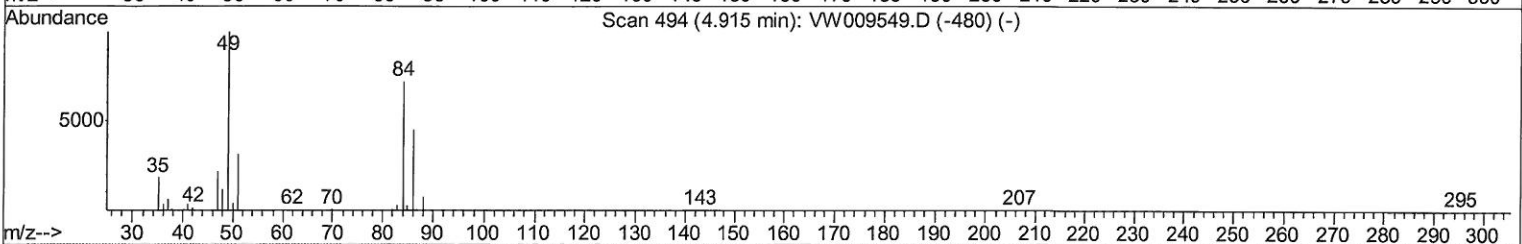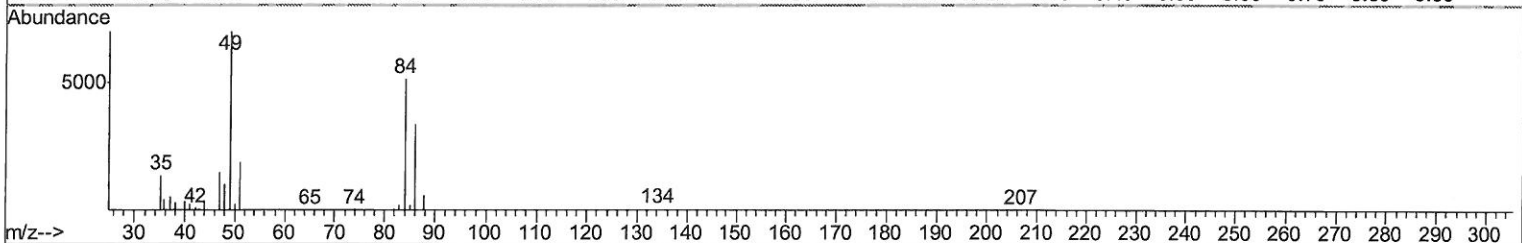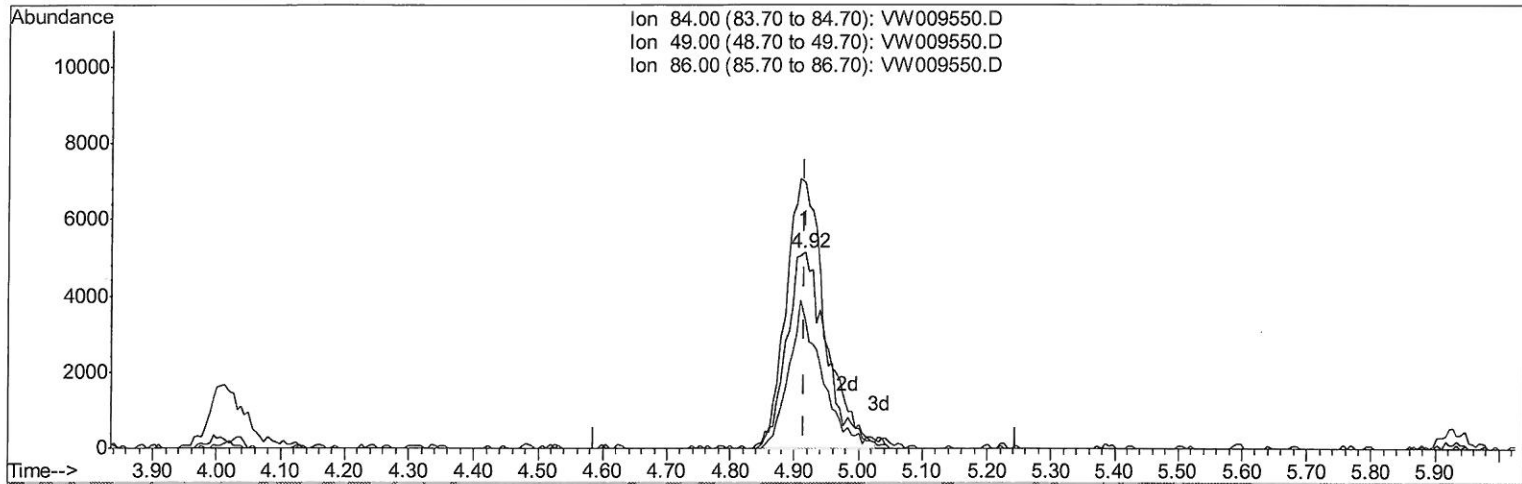

TIC: VW009550.D

(16) Methylene chloride (T)

4.916min (+0.000) 3.79ug/L m

response 21679

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	135.67
86.00	63.50	65.87
0.00	0.00	0.00

7 MD
4/1/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032819\
Quantitation Report (QT Reviewed)

Data File : VW009550.D
Acq On : 28 Mar 2019 21:39
Operator : SY/VA
Sample : VW0328SBL02
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
VBLK17

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:06:12 AM

Quant Time: Mar 29 07:50:40 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 29 07:41:24 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	392748	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	381857	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	172023	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	96505	20.56	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.24%
7) Chloroethane-d5	2.89	69	107785	19.63	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.52%
10) 1,1-Dichloroethene-d2	4.01	63	160643	15.84	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.36%
20) 2-Butanone-d5	7.07	46	105206	54.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.40%
24) Chloroform-d	7.64	84	259665	24.23	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.92%
26) 1,2-Dichloroethane-d4	8.30	65	165492	25.63	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.52%
29) Benzene-d6	8.27	84	460451	21.86	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.44%
33) 1,2-Dichloropropane-d6	9.27	67	149637	23.66	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.64%
37) Toluene-d8	10.32	98	420237	21.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.32%
38) trans-1,3-Dichloropropene-	10.58	79	66735	21.01	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.04%
39) 2-Hexanone-d5	10.93	63	71248	46.51	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.02%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	155380	24.94	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.76%
61) 1,2-Dichlorobenzene-d4	13.85	152	166462	25.24	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.96%

Target Compounds

16) Methylene chloride	4.92	84	21679m	3.785	ug/L	Qvalue
------------------------	------	----	--------	-------	------	--------

7 mQ
4/1/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed