

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032819\
Quantitation Report (QT Reviewed)


Data File : VW009553.D
Acq On : 28 Mar 2019 23:29
Operator : SY/VA
Sample : K2120-07
Misc : 5.55G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5D1

Quant Time: Mar 29 08:07:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 29 07:41:24 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:06:12 AM

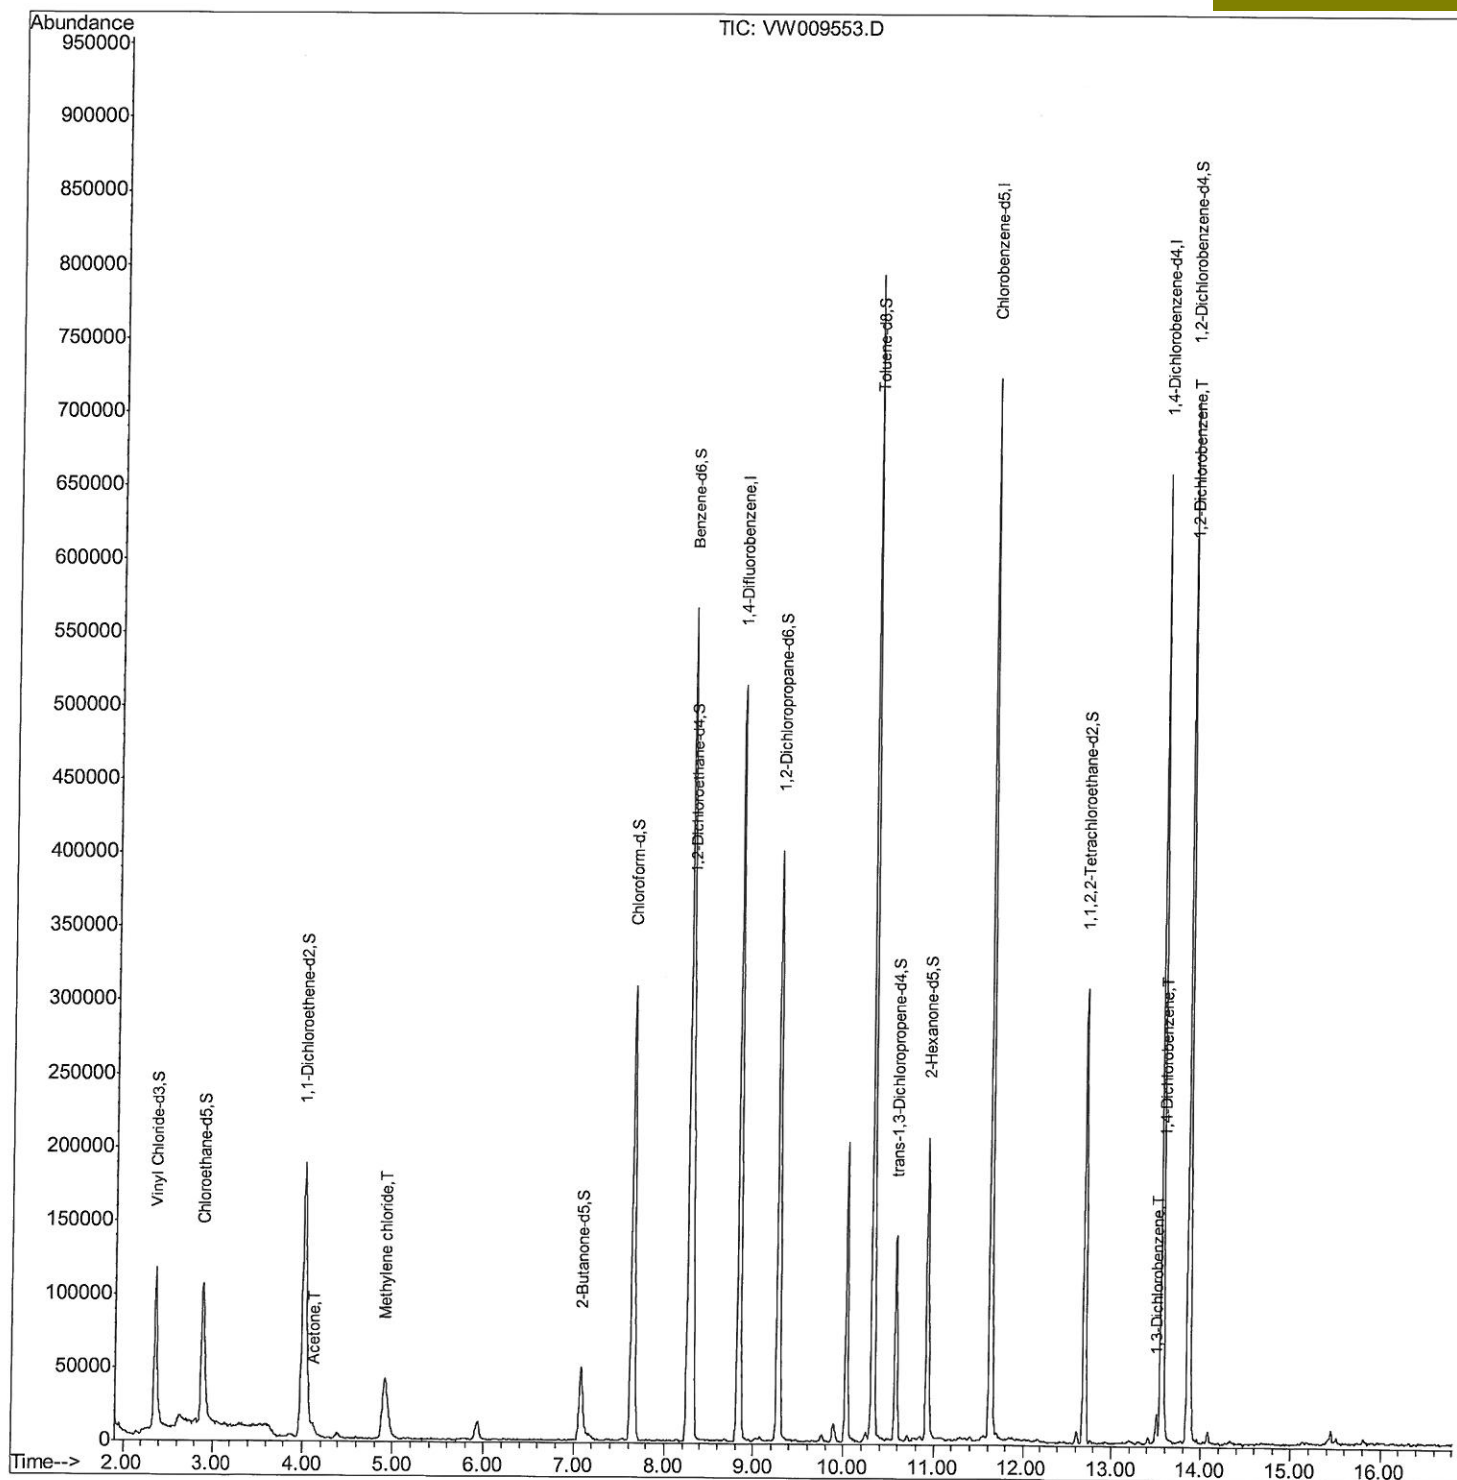

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032819\
Quantitation Report (Qedit)


Data File : VW009553.D
Acq On : 28 Mar 2019 23:29
Operator : SY/VA
Sample : K2120-07
Misc : 5.55G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BF5D1

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:06:12 AM

Quant Time: Mar 29 07:44:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 29 07:41:24 2019
Response via : Initial Calibration

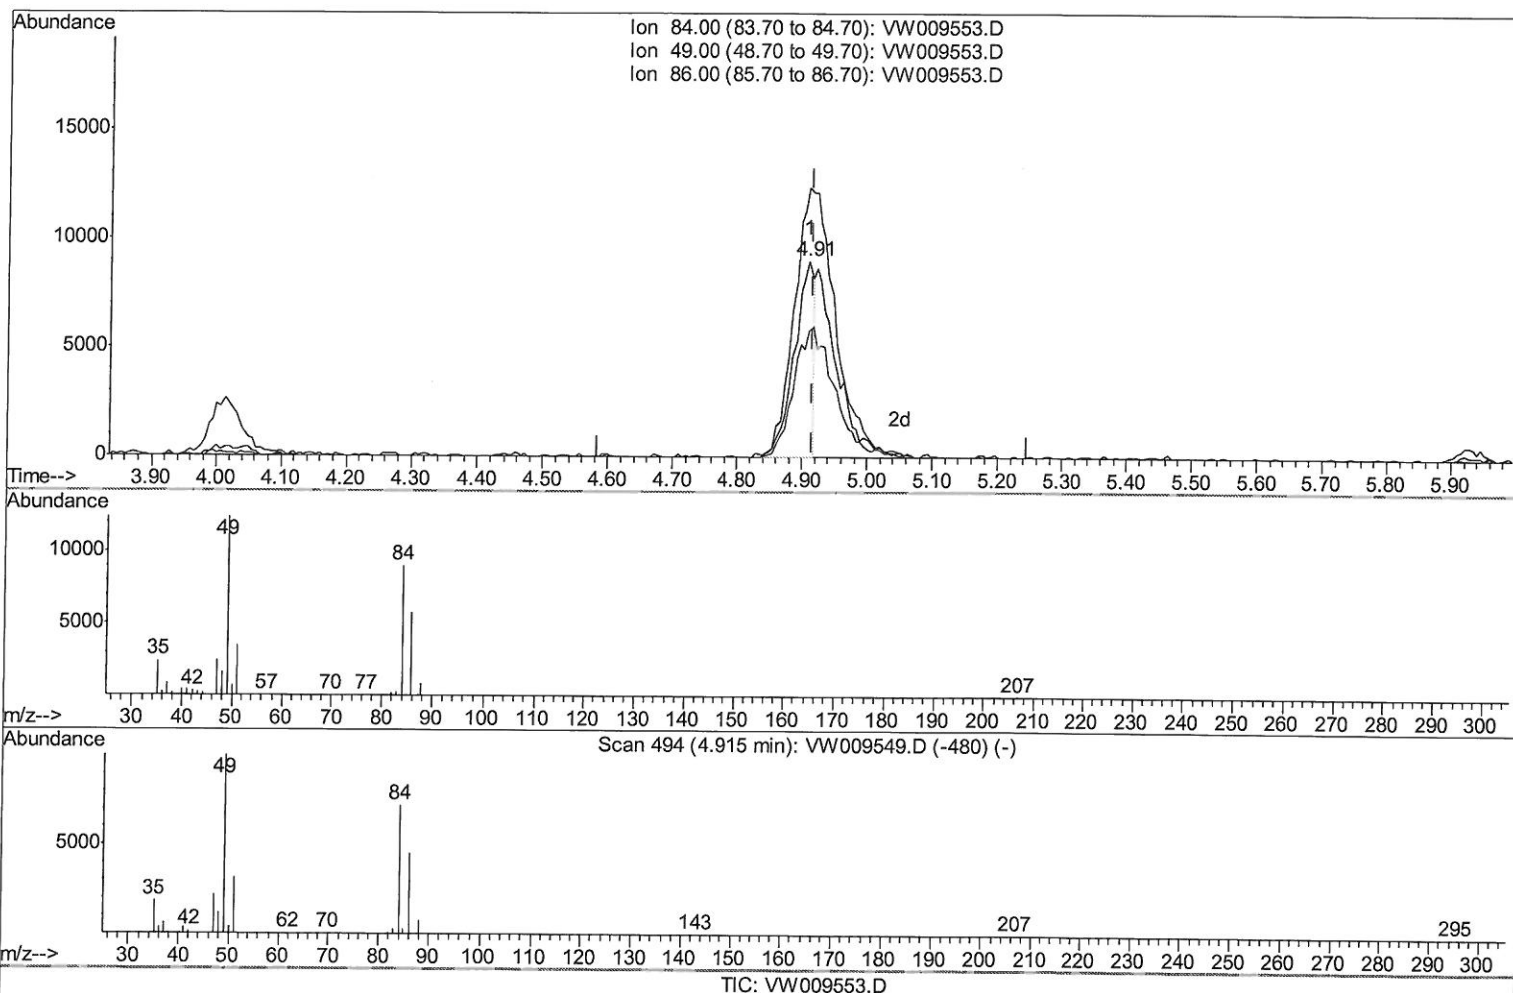

(16) Methylene chloride (T)

4.909min (-0.006) 3.23ug/L

response 18570

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	137.35
86.00	63.50	64.40
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032819\
Quantitation Report (Qedit)




Data File : VW009553.D
Acq On : 28 Mar 2019 23:29
Operator : SY/VA
Sample : K2120-07
Misc : 5.55G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BF5D1

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:06:12 AM

Quant Time: Mar 29 07:44:44 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 29 07:41:24 2019
Response via : Initial Calibration

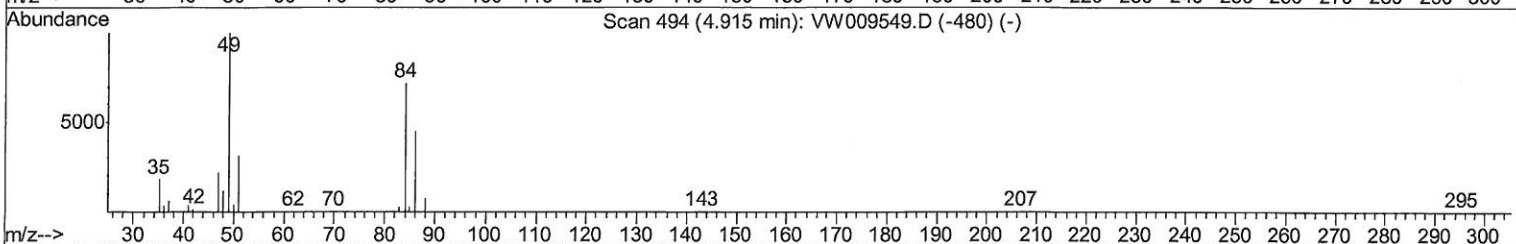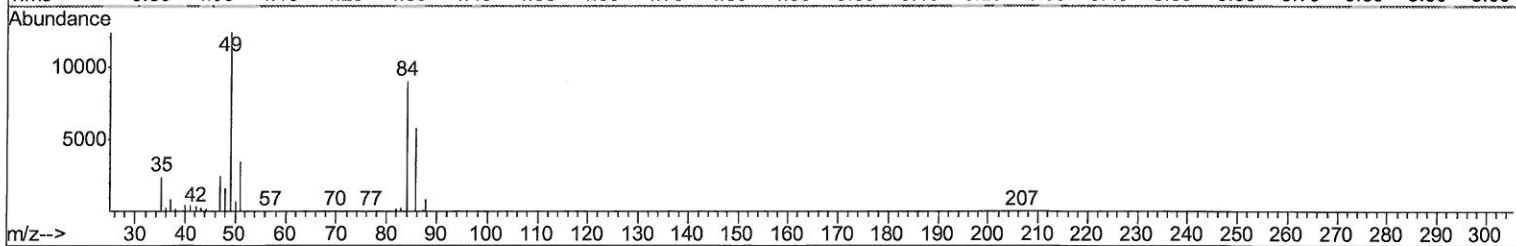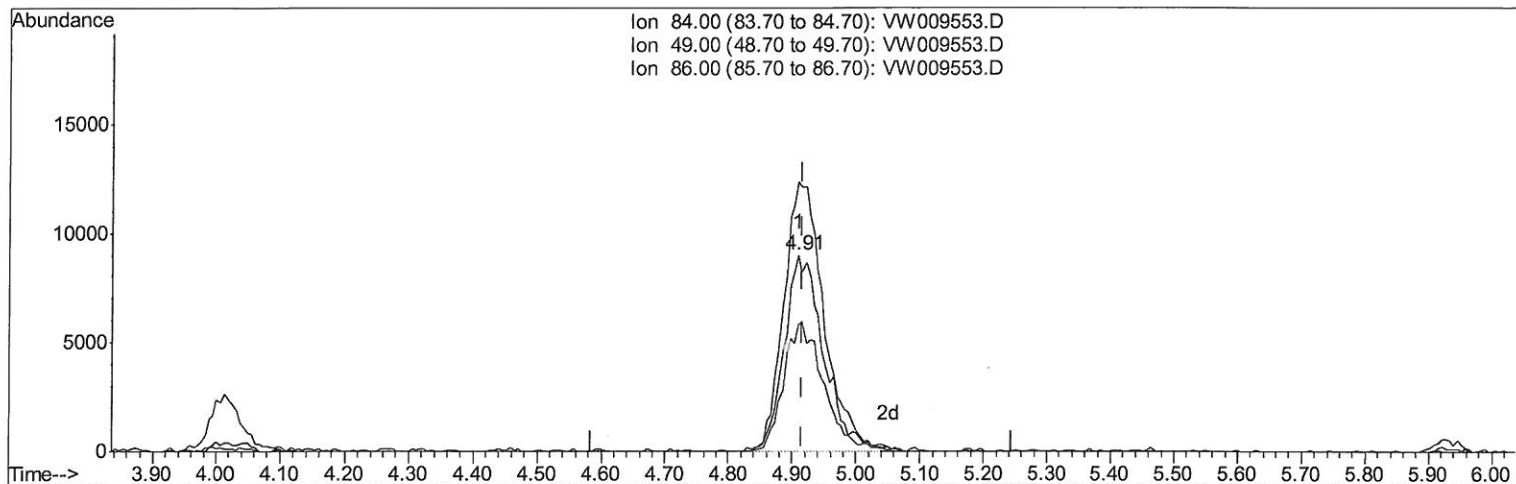

TIC: VW009553.D

(16) Methylene chloride (T)

4.909min (-0.006) 6.67ug/L m

response 38369

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	137.35
86.00	63.50	64.40
0.00	0.00	0.00

7 MB
4/1/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032819\
 Quantitation Report (QT Reviewed)
 Data File : VW009553.D
 Acq On : 28 Mar 2019 23:29
 Operator : SY/VA
 Sample : K2120-07
 Misc : 5.55G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF5D1

Quant Time: Mar 29 08:07:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 29 07:41:24 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:06:12 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	394356	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	378637	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	156492	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	150754	31.99	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	127.96%		
7) Chloroethane-d5	2.89	69	140711	25.52	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	102.08%		
10) 1,1-Dichloroethene-d2	4.01	63	225107	22.10	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	88.40%		
20) 2-Butanone-d5	7.07	46	86042	44.15	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	88.30%		
24) Chloroform-d	7.64	84	282079	26.21	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	104.84%		
26) 1,2-Dichloroethane-d4	8.30	65	175432	27.06	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	108.24%		
29) Benzene-d6	8.27	84	540048	25.86	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	103.44%		
33) 1,2-Dichloropropane-d6	9.27	67	165490	26.39	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	105.56%		
37) Toluene-d8	10.32	98	486587	25.20	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	100.80%		
38) trans-1,3-Dichloropropene-	10.58	79	69374	22.02	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.08%		
39) 2-Hexanone-d5	10.93	63	55467	36.52	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	73.04%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	142428	23.06	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	92.24%		
61) 1,2-Dichlorobenzene-d4	13.86	152	158926	26.48	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	105.92%		

Target Compounds

					Qvalue
13) Acetone	4.12	43	10857	6.793 ug/L	89
16) Methylene chloride	4.91	84	38369m	6.672 ug/L	89
63) 1,3-Dichlorobenzene	13.50	146	6512	0.698 ug/L	98
64) 1,4-Dichlorobenzene	13.58	146	8810	0.914 ug/L	97
65) 1,2-Dichlorobenzene	13.87	146	60533	6.806 ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

7 MD
 4/1/19