

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW032819\
 Data File : VW009541.D
 Acq On : 28 Mar 2019 16:35
 Operator : SY/VA
 Sample : K2084-09
 Misc : 5.48G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF7W0

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:06:09 AM

Quant Time: Mar 29 07:12:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Mar 29 05:35:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	381053	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	371276	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	164978	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	145362	31.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	127.68%
7) Chloroethane-d5	2.89	69	137573	25.82	ug/L	0.02
Spiked Amount	25.000	Range	30 - 150	Recovery	=	103.28%
10) 1,1-Dichloroethene-d2	4.01	63	218879	22.24	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	88.96%
20) 2-Butanone-d5	7.07	46	85769	45.55	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.10%
24) Chloroform-d	7.64	84	269981	25.96	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.84%
26) 1,2-Dichloroethane-d4	8.31	65	167017	26.66	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.64%
29) Benzene-d6	8.27	84	518831	25.34	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.36%
33) 1,2-Dichloropropane-d6	9.27	67	157151	25.55	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.20%
37) Toluene-d8	10.32	98	472920	24.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.92%
38) trans-1,3-Dichloropropene-	10.58	79	70347	22.78	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.12%
39) 2-Hexanone-d5	10.93	63	53595	35.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	141283	23.33	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.32%
61) 1,2-Dichlorobenzene-d4	13.86	152	167110	26.42	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.68%

Target Compounds					Qvalue
13) Acetone	4.12	43	5516m	3.572	ug/L
16) Methylene chloride	4.92	84	31910m	5.743	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW032819\
Data File : VW009541.D
Acq On : 28 Mar 2019 16:35
Operator : SY/VA
Sample : K2084-09
Misc : 5.48G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BF7W0

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:06:09 AM

Quant Time: Mar 29 07:12:42 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Fri Mar 29 05:35:33 2019
Response via : Initial Calibration

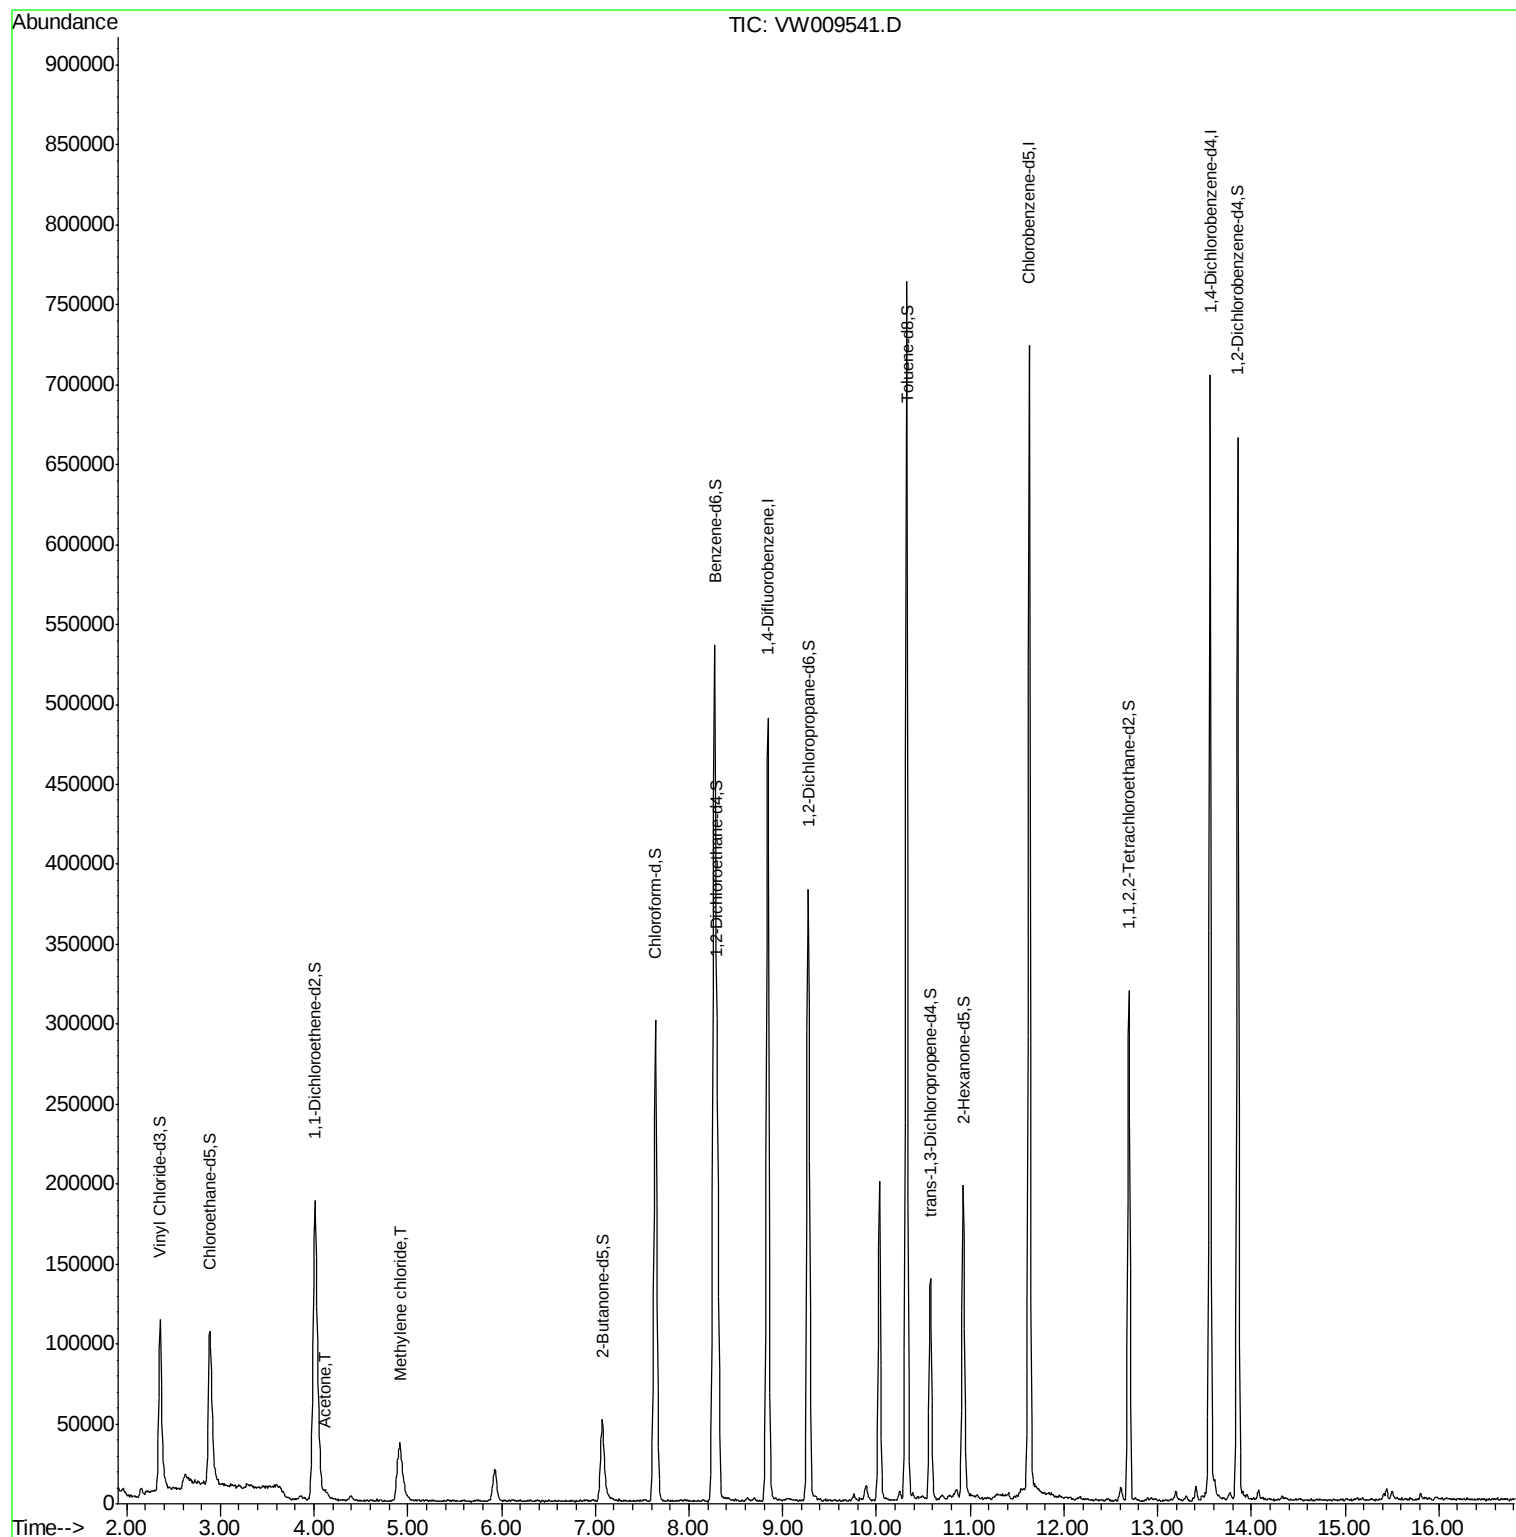

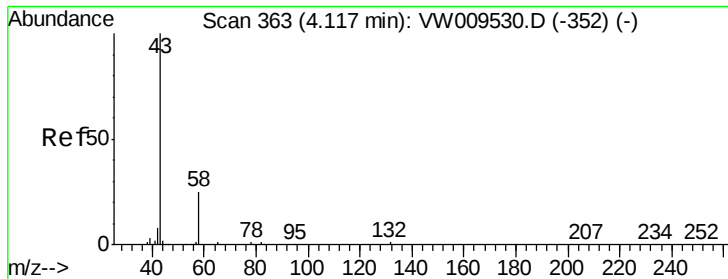

#13

Acetone

Concen: 3.572 ug/L m

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW009541.D





Acq: 28 Mar 2019 16:35

Tgt Ion	Ratio	Lower	Upper
43	100		
58	21.7	0.0	56.2

Instrument :
MSVOA_W
ClientSampleId :
BF7W0

Manual Integrations
APPROVED

MMDadoda
4/1/2019 4:06:09 AM

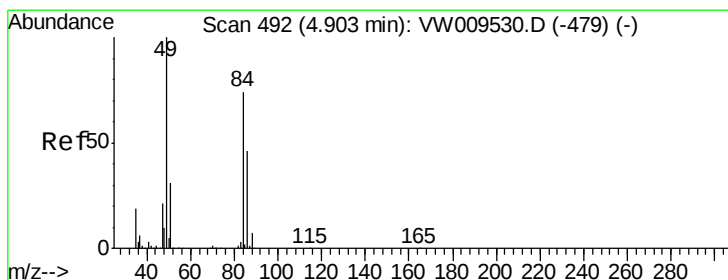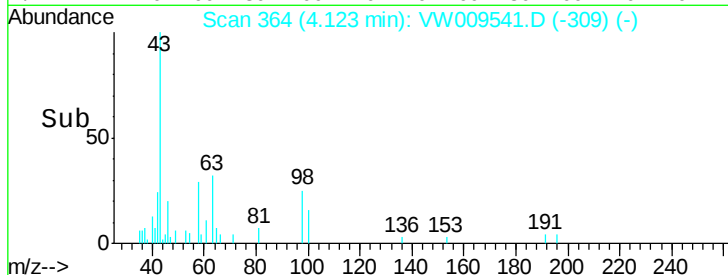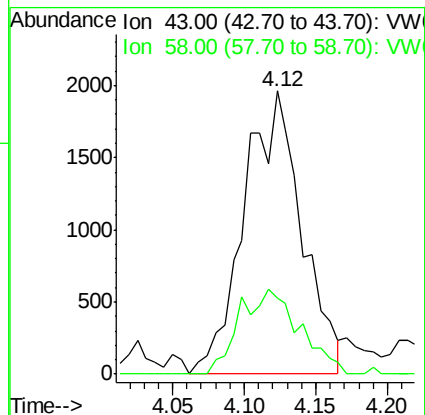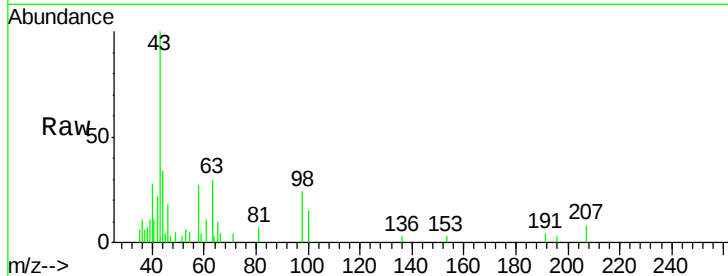

#16

Methylene chloride

Concen: 5.743 ug/L m

RT: 4.92 min Scan# 494

Delta R.T. 0.01 min

Lab File: VW009541.D

Acq: 28 Mar 2019 16:35

Tgt Ion	Ratio	Lower	Upper
84	100		
49	112.2	96.0	178.2
86	59.9	44.4	82.5

