



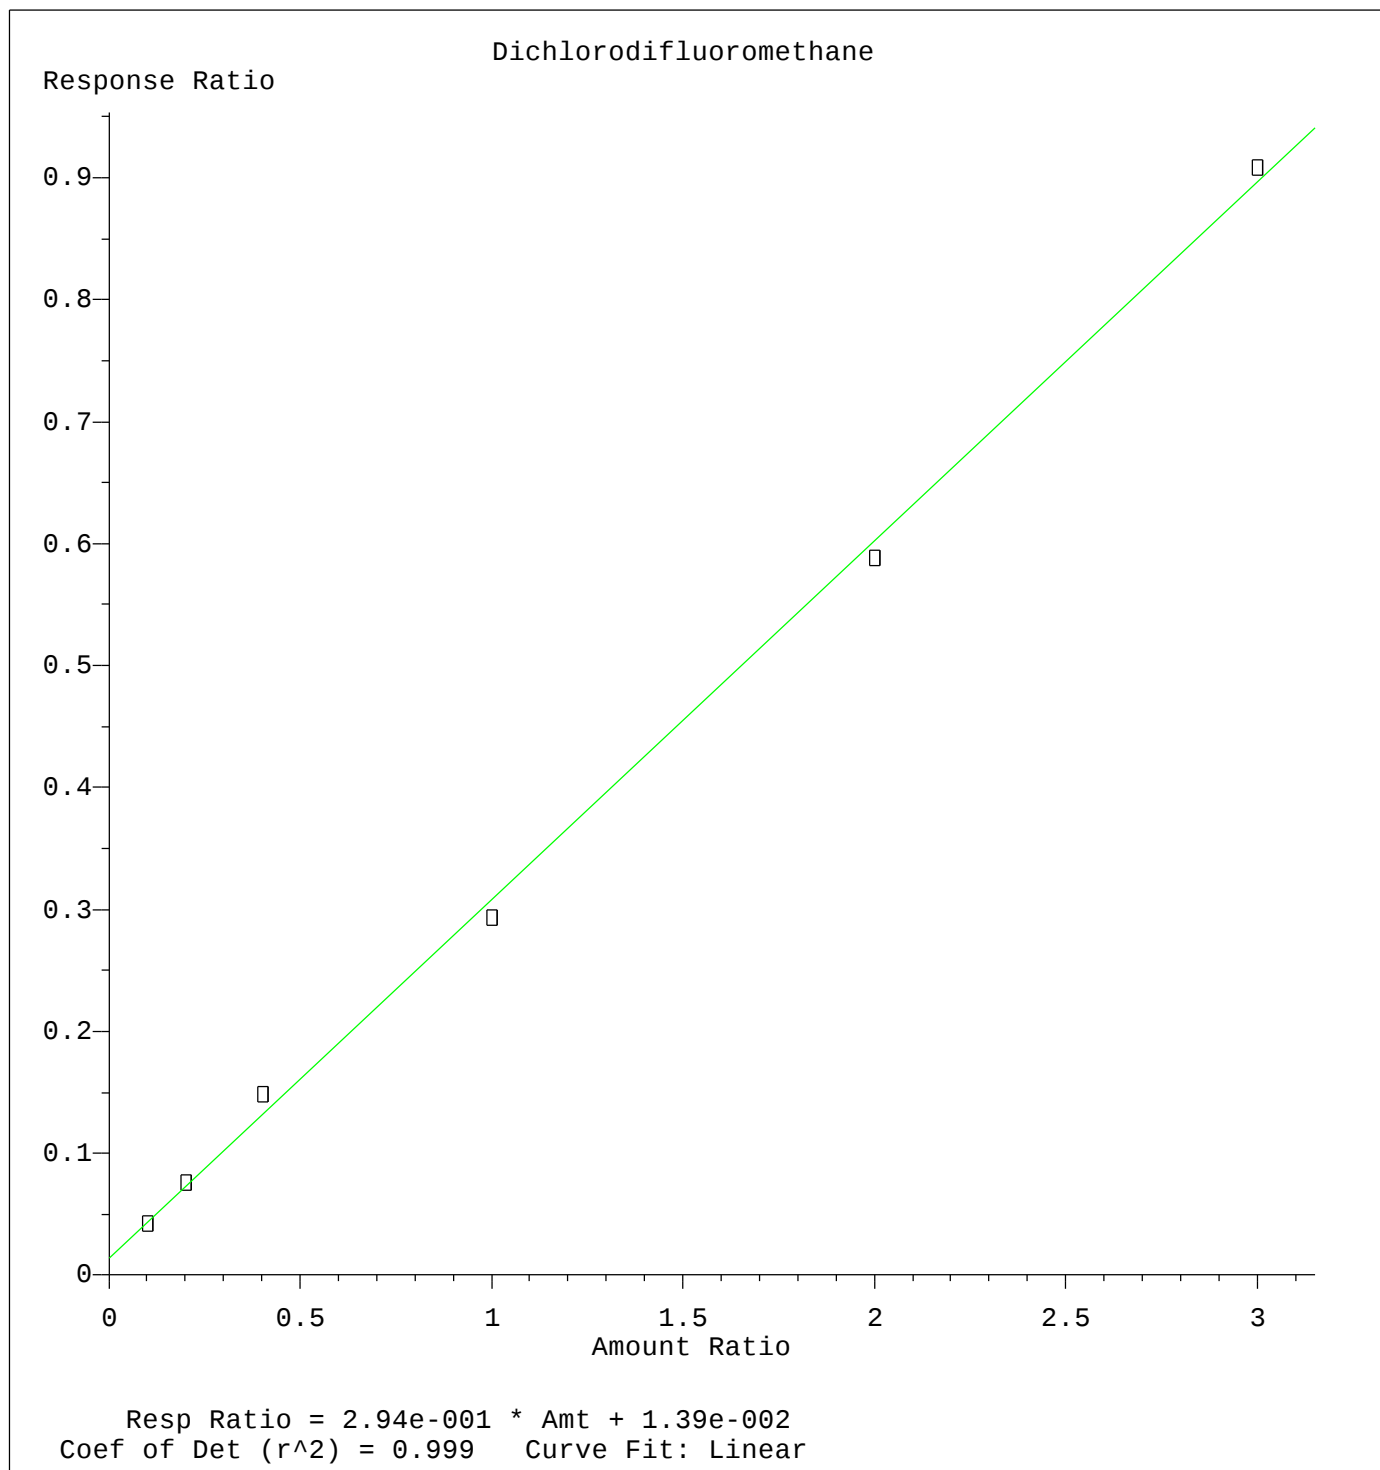

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W032919S.M
Calibration Table Last Updated: Fri Mar 29 13:24:53 2019


2-Chloroethyl Vinyl ether

Response Ratio

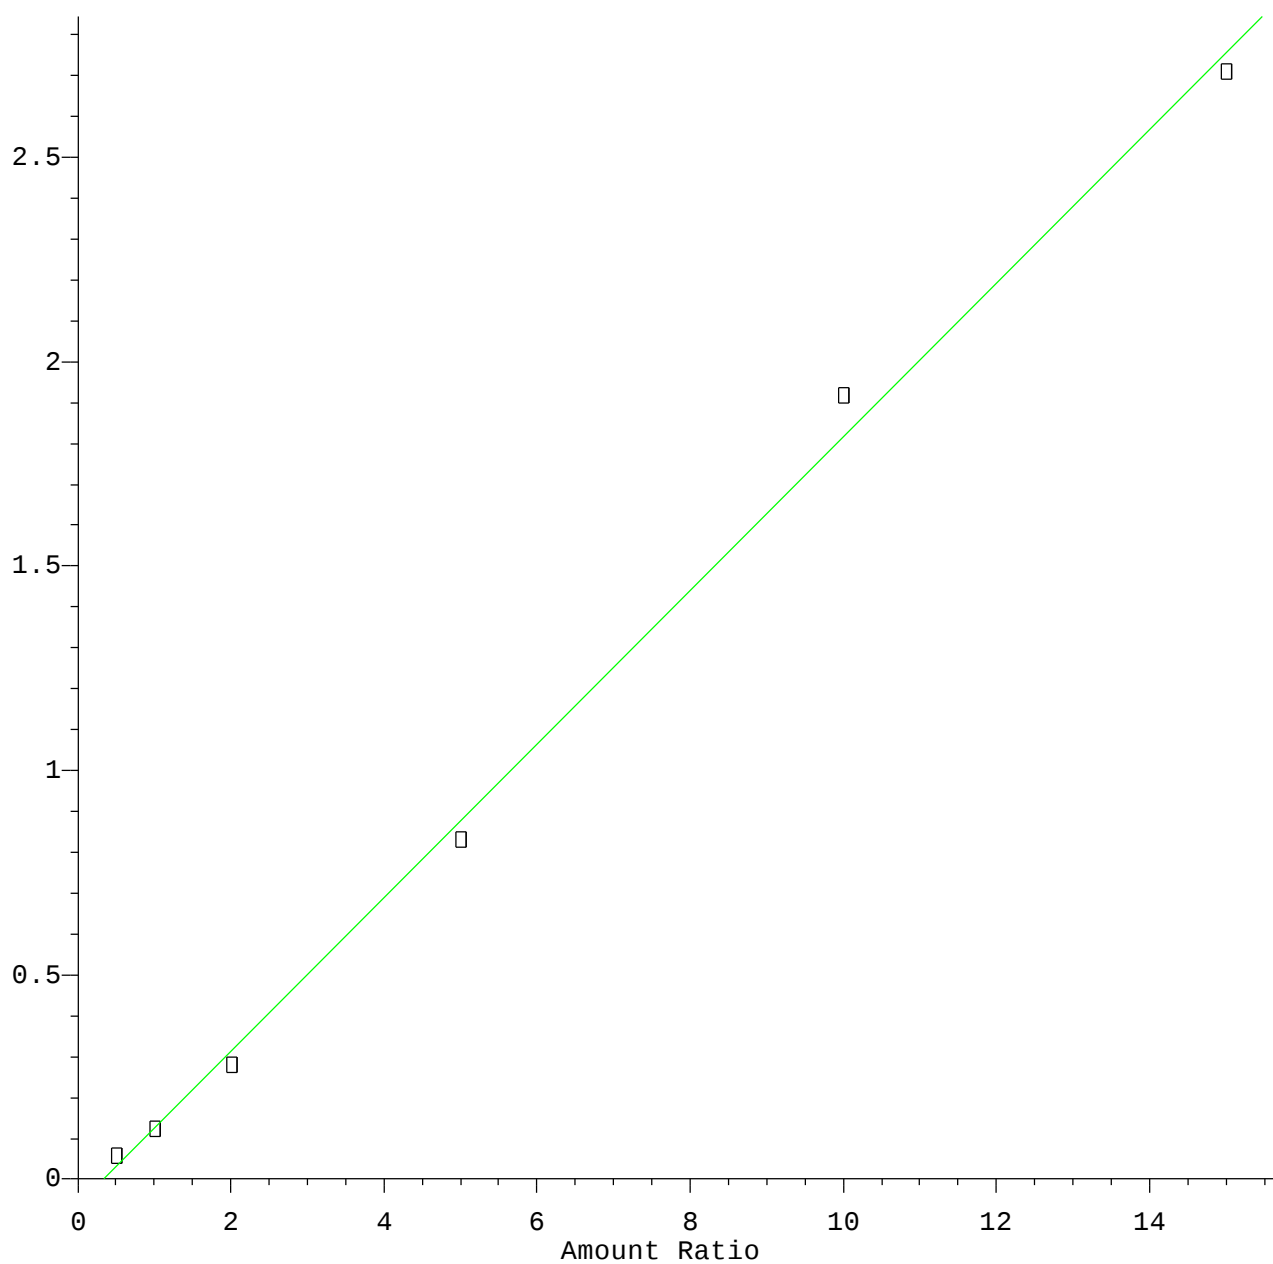


Resp Ratio = $1.88 \times 10^{-1} \times \text{Amt} - 6.40 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W032919S.M
Calibration Table Last Updated: Fri Mar 29 13:24:53 2019

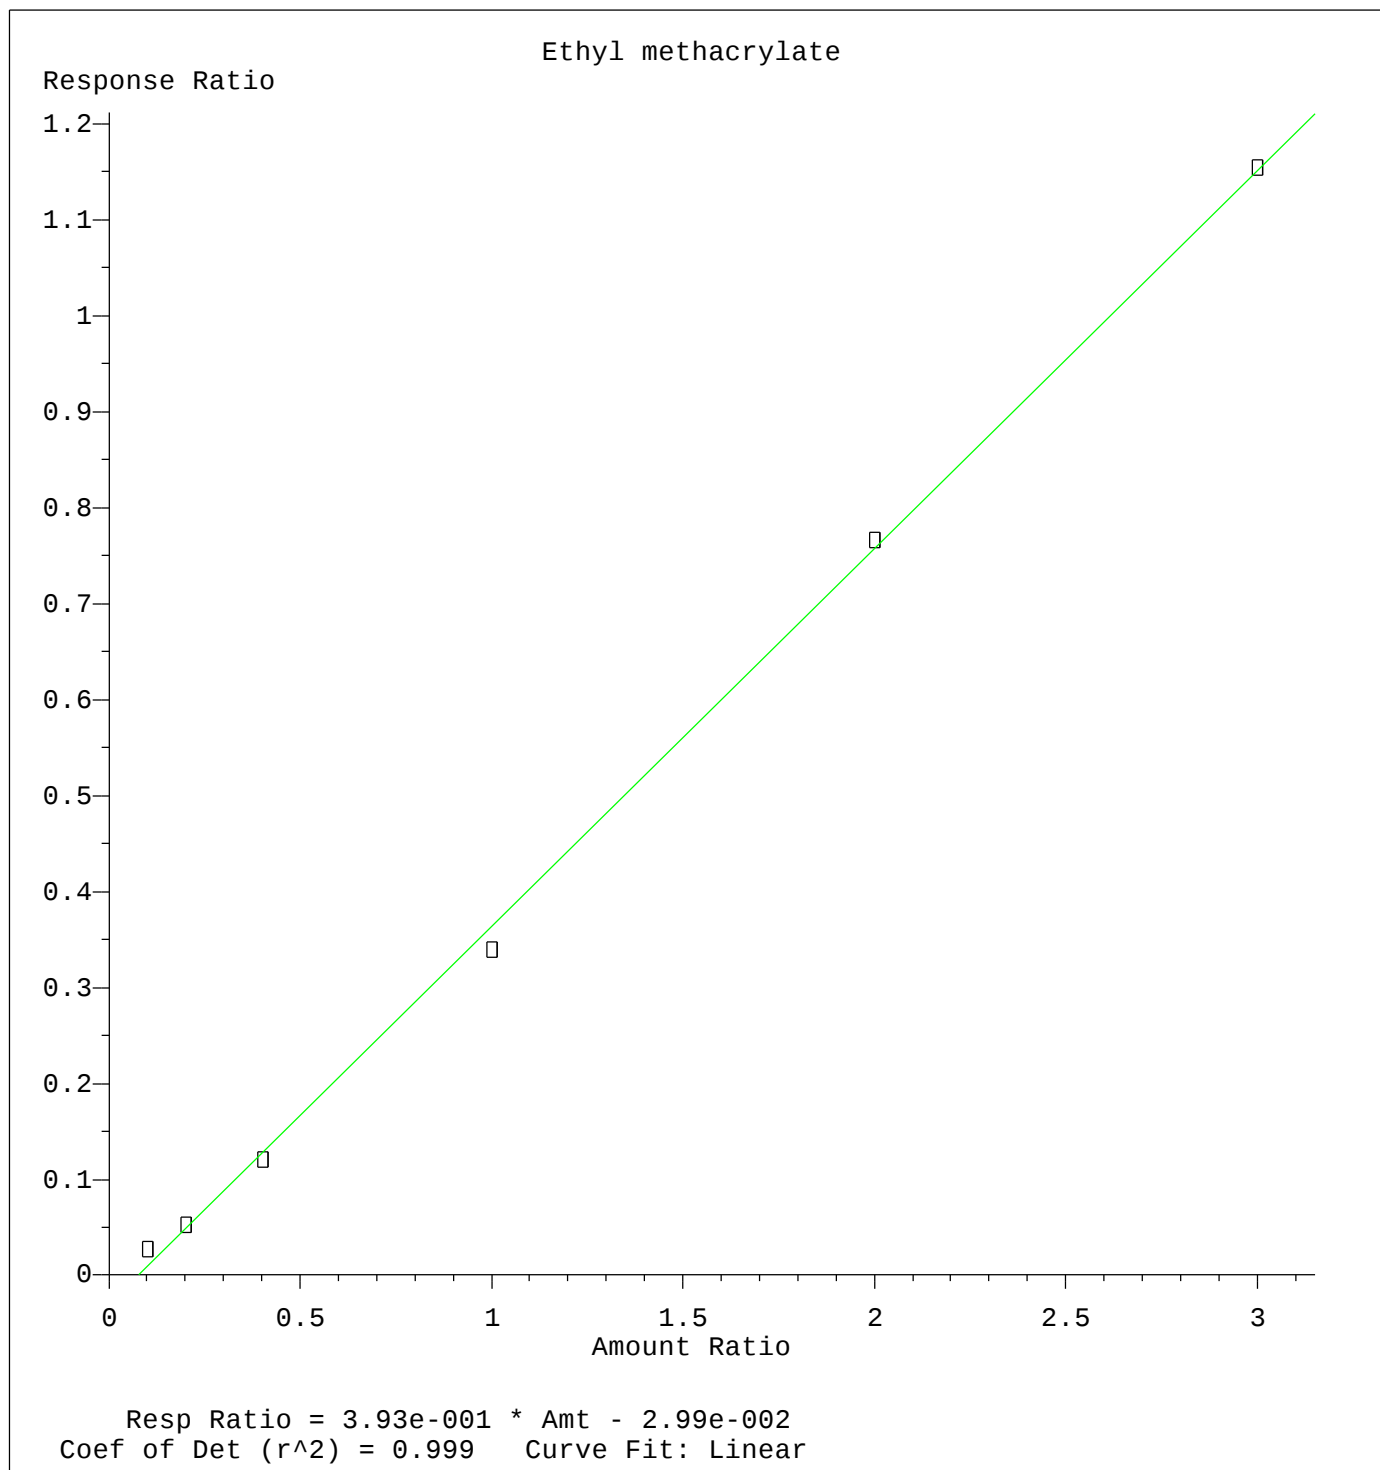


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W032919S.M
Calibration Table Last Updated: Fri Mar 29 13:24:53 2019

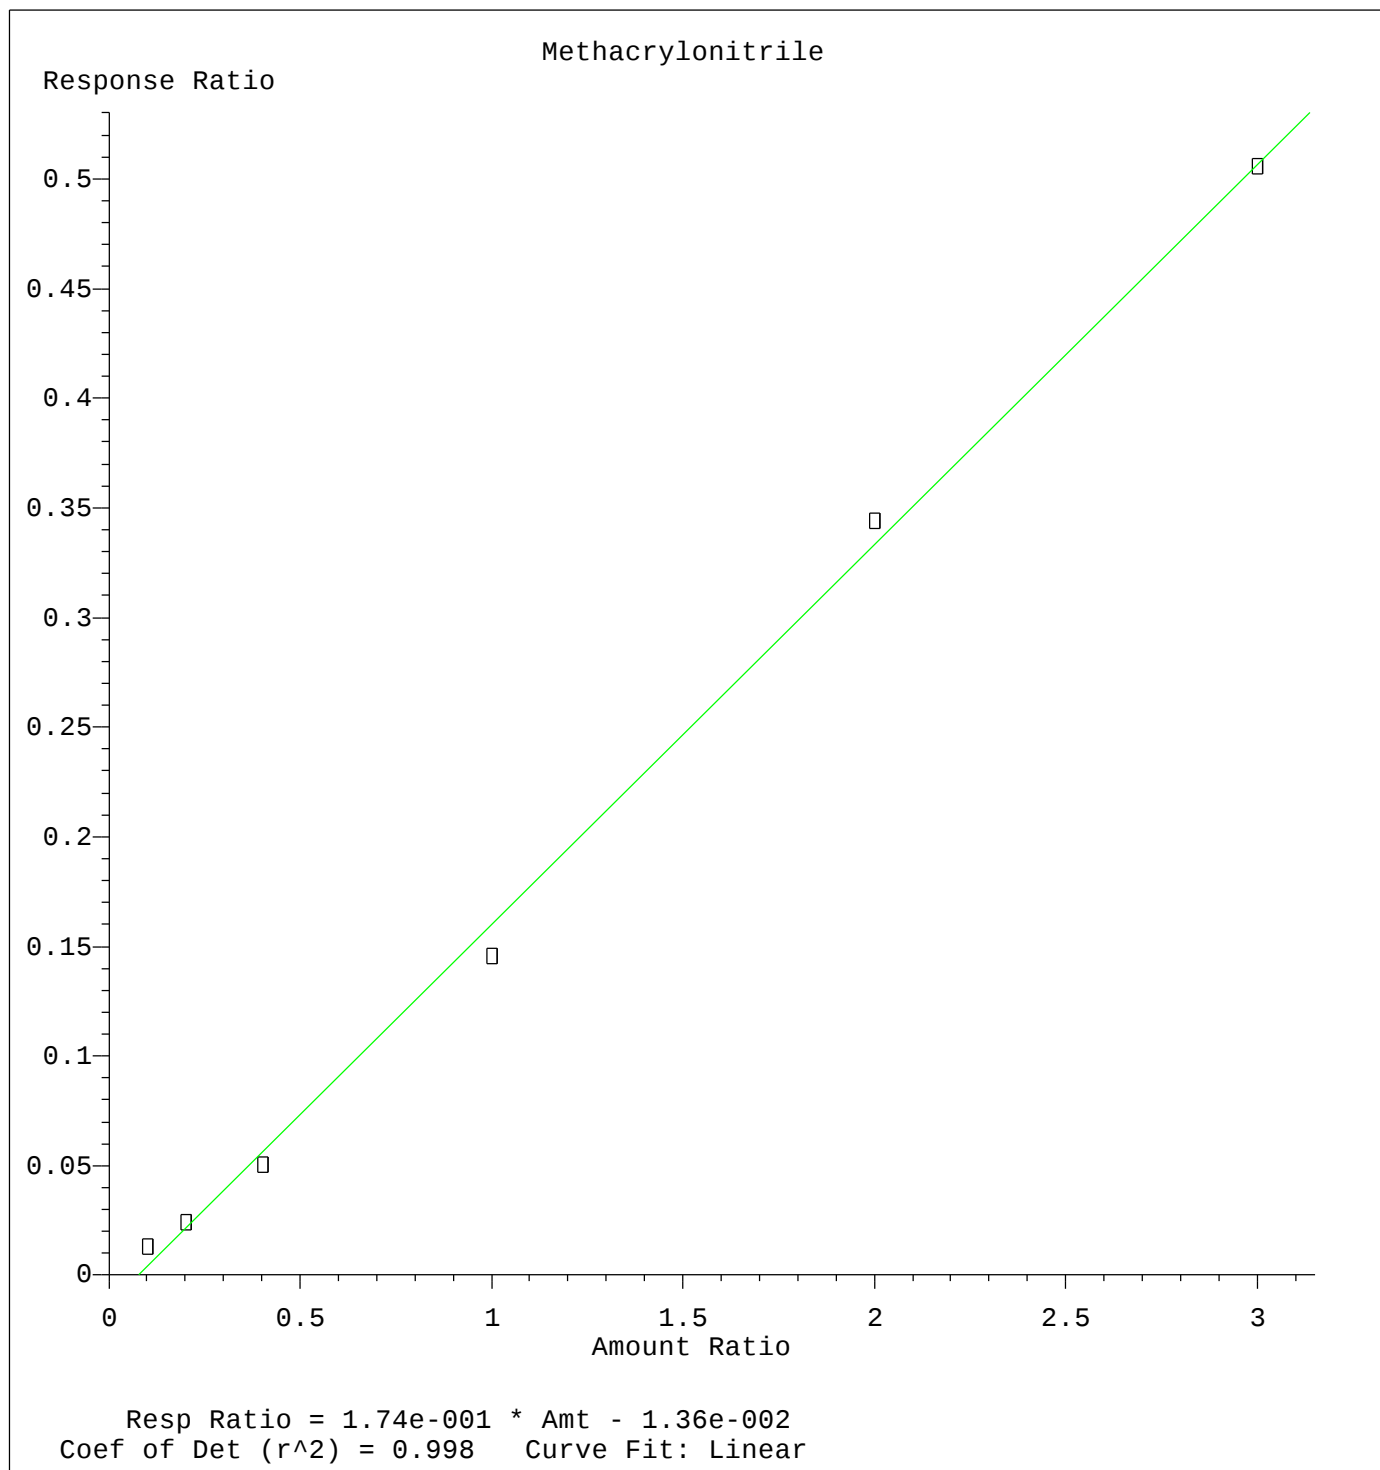

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W032919S.M
Calibration Table Last Updated: Fri Mar 29 13:24:53 2019

Methylene Chloride

Response Ratio

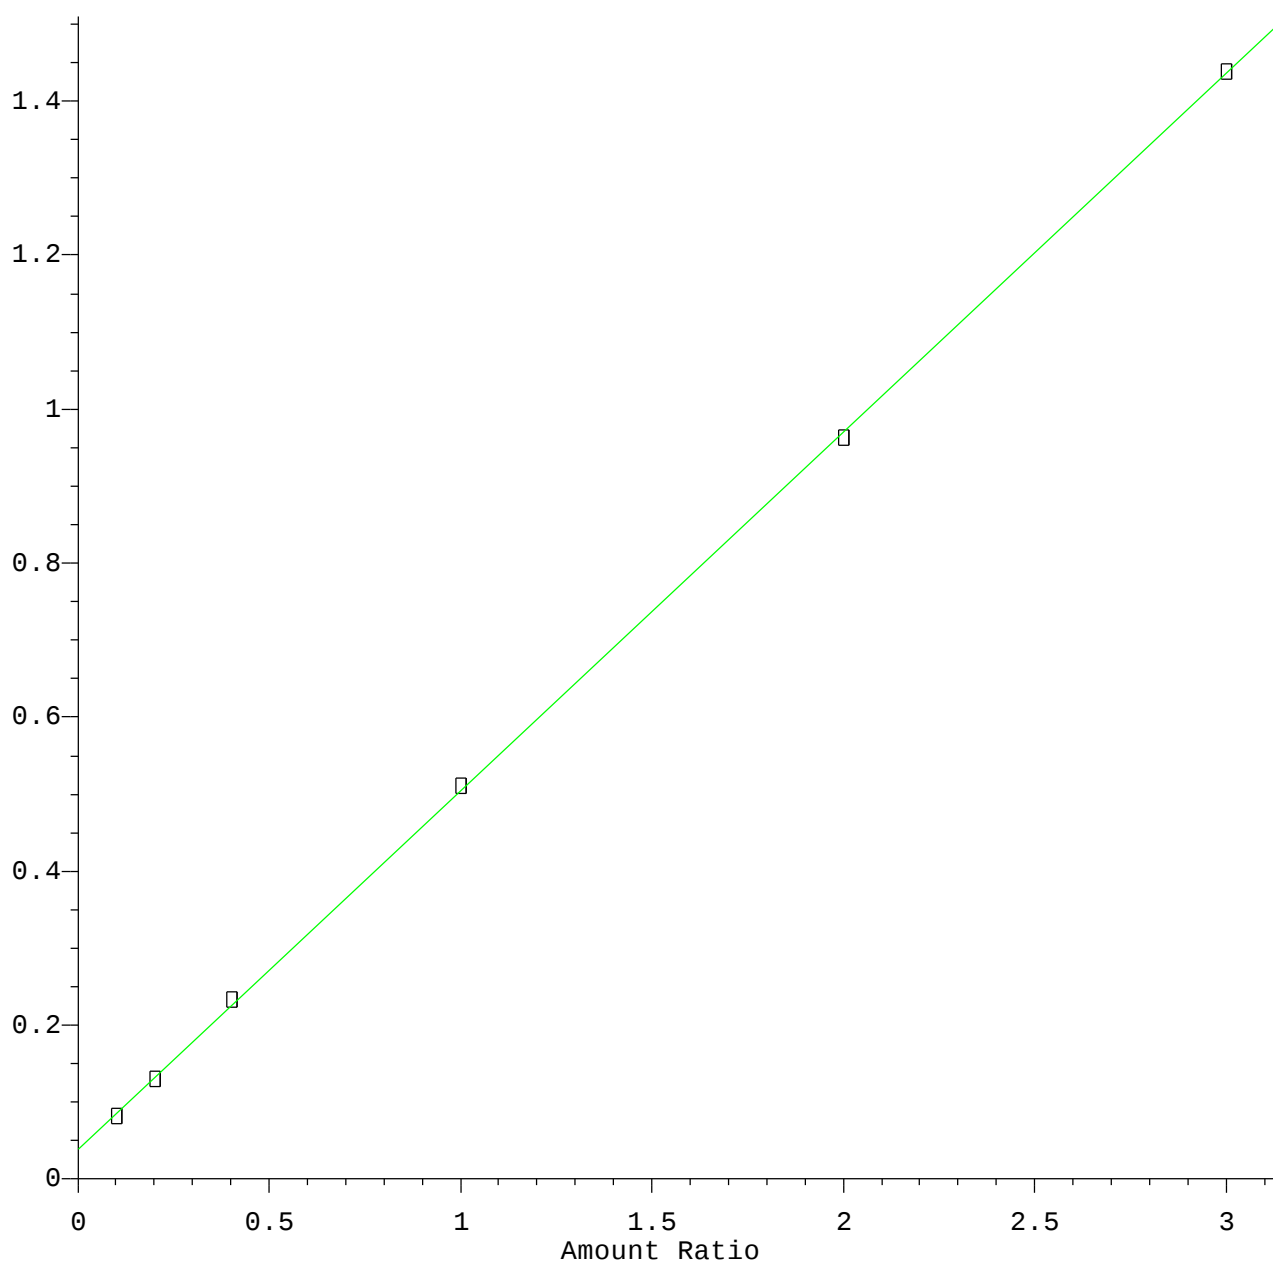


Resp Ratio = 4.65e-001 * Amt + 3.91e-002
Coef of Det (r²) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W032919S.M
Calibration Table Last Updated: Fri Mar 29 13:24:53 2019

Naphthalene

Response Ratio

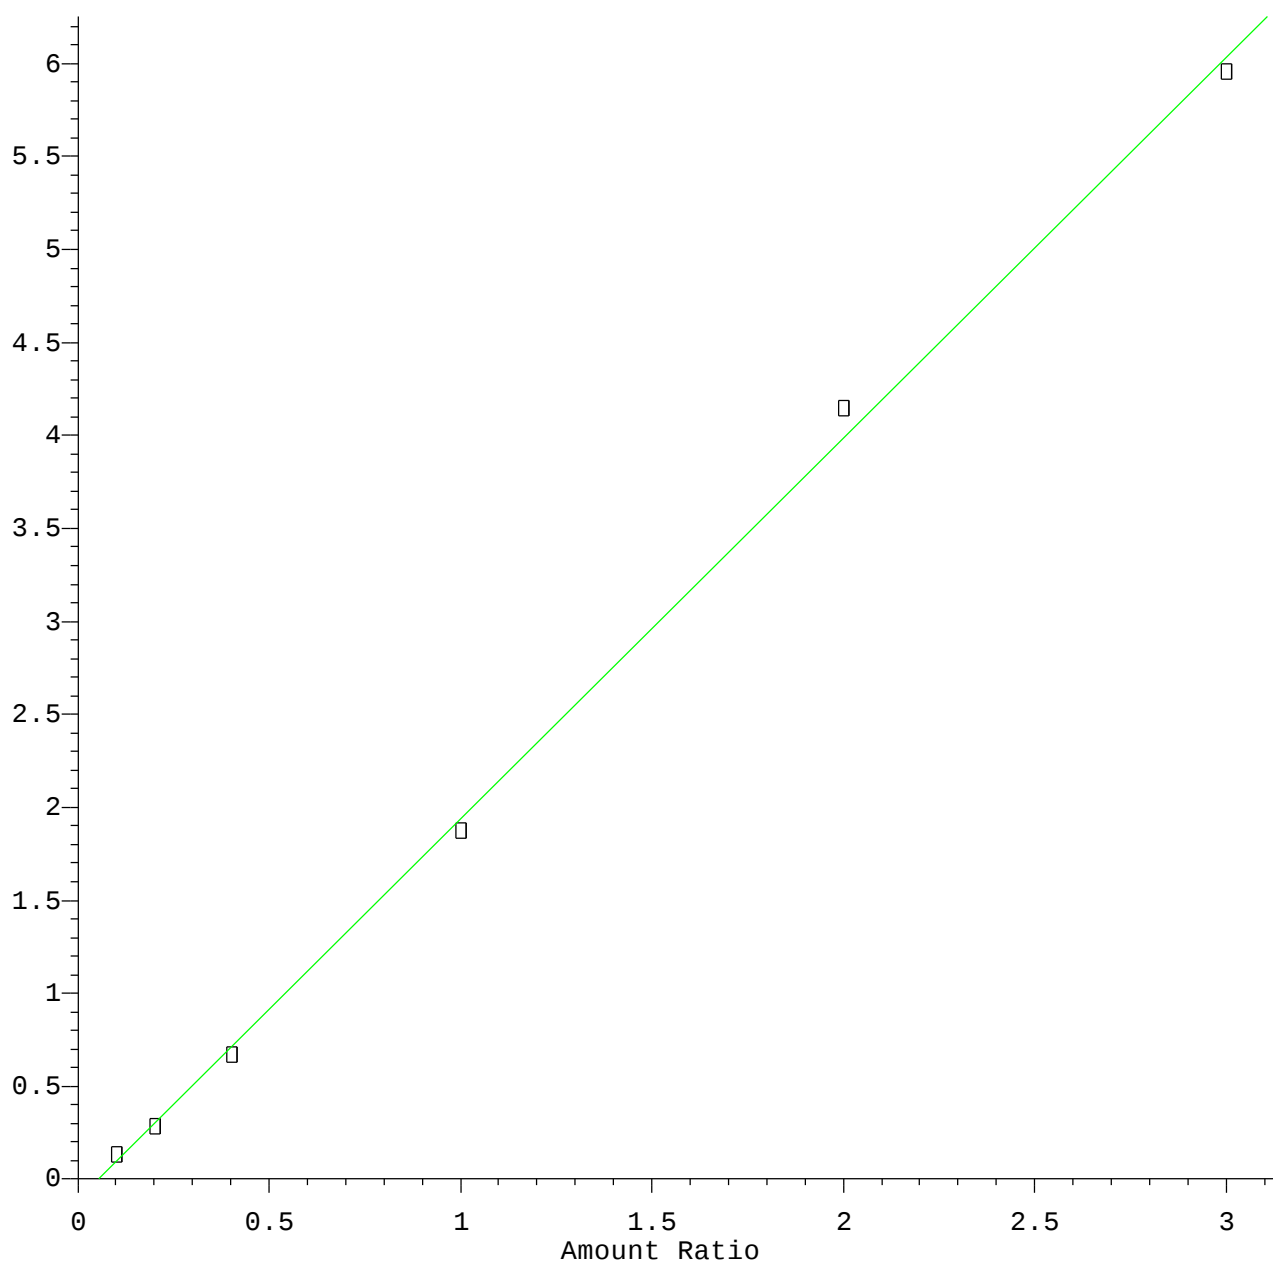

Resp Ratio = 2.05e+000 * Amt - 1.11e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W032919S.M
Calibration Table Last Updated: Fri Mar 29 13:24:53 2019