

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032921\
 Data File : VW018477.D
 Acq On : 29 Mar 2021 11:41
 Operator : SY/VA
 Sample : M1816-20
 Misc : 5.86G/10ML/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4S6

Quant Time: Mar 30 03:11:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 30 03:10:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	512100	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	459913	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	217947	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	151329	21.24	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	84.96%		
7) Chloroethane-d5	2.897	69	138290	22.17	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.68%		
10) 1,1-Dichloroethene-d2	4.019	63	196318	15.96	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	63.84%		
20) 2-Butanone-d5	7.073	46	63416	39.97	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.94%		
24) Chloroform-d	7.646	84	284872	21.84	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.36%		
26) 1,2-Dichloroethane-d4	8.494	65	62	0.01	ug/L	0.19
Spiked Amount 25.000	Range 70 - 130		Recovery =	0.04%#		
29) Benzene-d6	8.274	84	548119	22.42	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	89.68%		
33) 1,2-Dichloropropane-d6	9.274	67	157780	22.37	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	89.48%		
37) Toluene-d8	10.323	98	507476	21.56	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.24%		
38) trans-1,3-Dichloroprop...	10.579	79	68063	18.71	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	74.84%		
39) 2-Hexanone-d5	10.926	63	52563	38.08	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	76.16%		
48) 1,1,2,2-Tetrachloroeth...	12.694	84	126393	20.03	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	80.12%		
61) 1,2-Dichlorobenzene-d4	13.853	152	164801	21.27	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	85.08%		
Target Compounds						
11) 1,1,2-Trichloro-1,2,2-...	4.031	101	2229	0.35	ug/L #	22
12) 1,1-Dichloroethene	4.019	96	1734	0.27	ug/L #	1
13) Acetone	4.129	43	10121	8.88	ug/L	100
14) Carbon disulfide	4.391	76	14065	0.73	ug/L	98
16) Methylene chloride	4.915	84	10009	1.19	ug/L	99
21) 2-Butanone	7.183	43	2988	1.65	ug/L	84
45) trans-1,3-Dichloropropene	10.579	75	3804	0.38	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032921\
Data File : VW018477.D
Acq On : 29 Mar 2021 11:41
Operator : SY/VA
Sample : M1816-20
Misc : 5.86G/10ML/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG4S6

Quant Time: Mar 30 03:11:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 30 03:10:03 2021
Response via : Initial Calibration




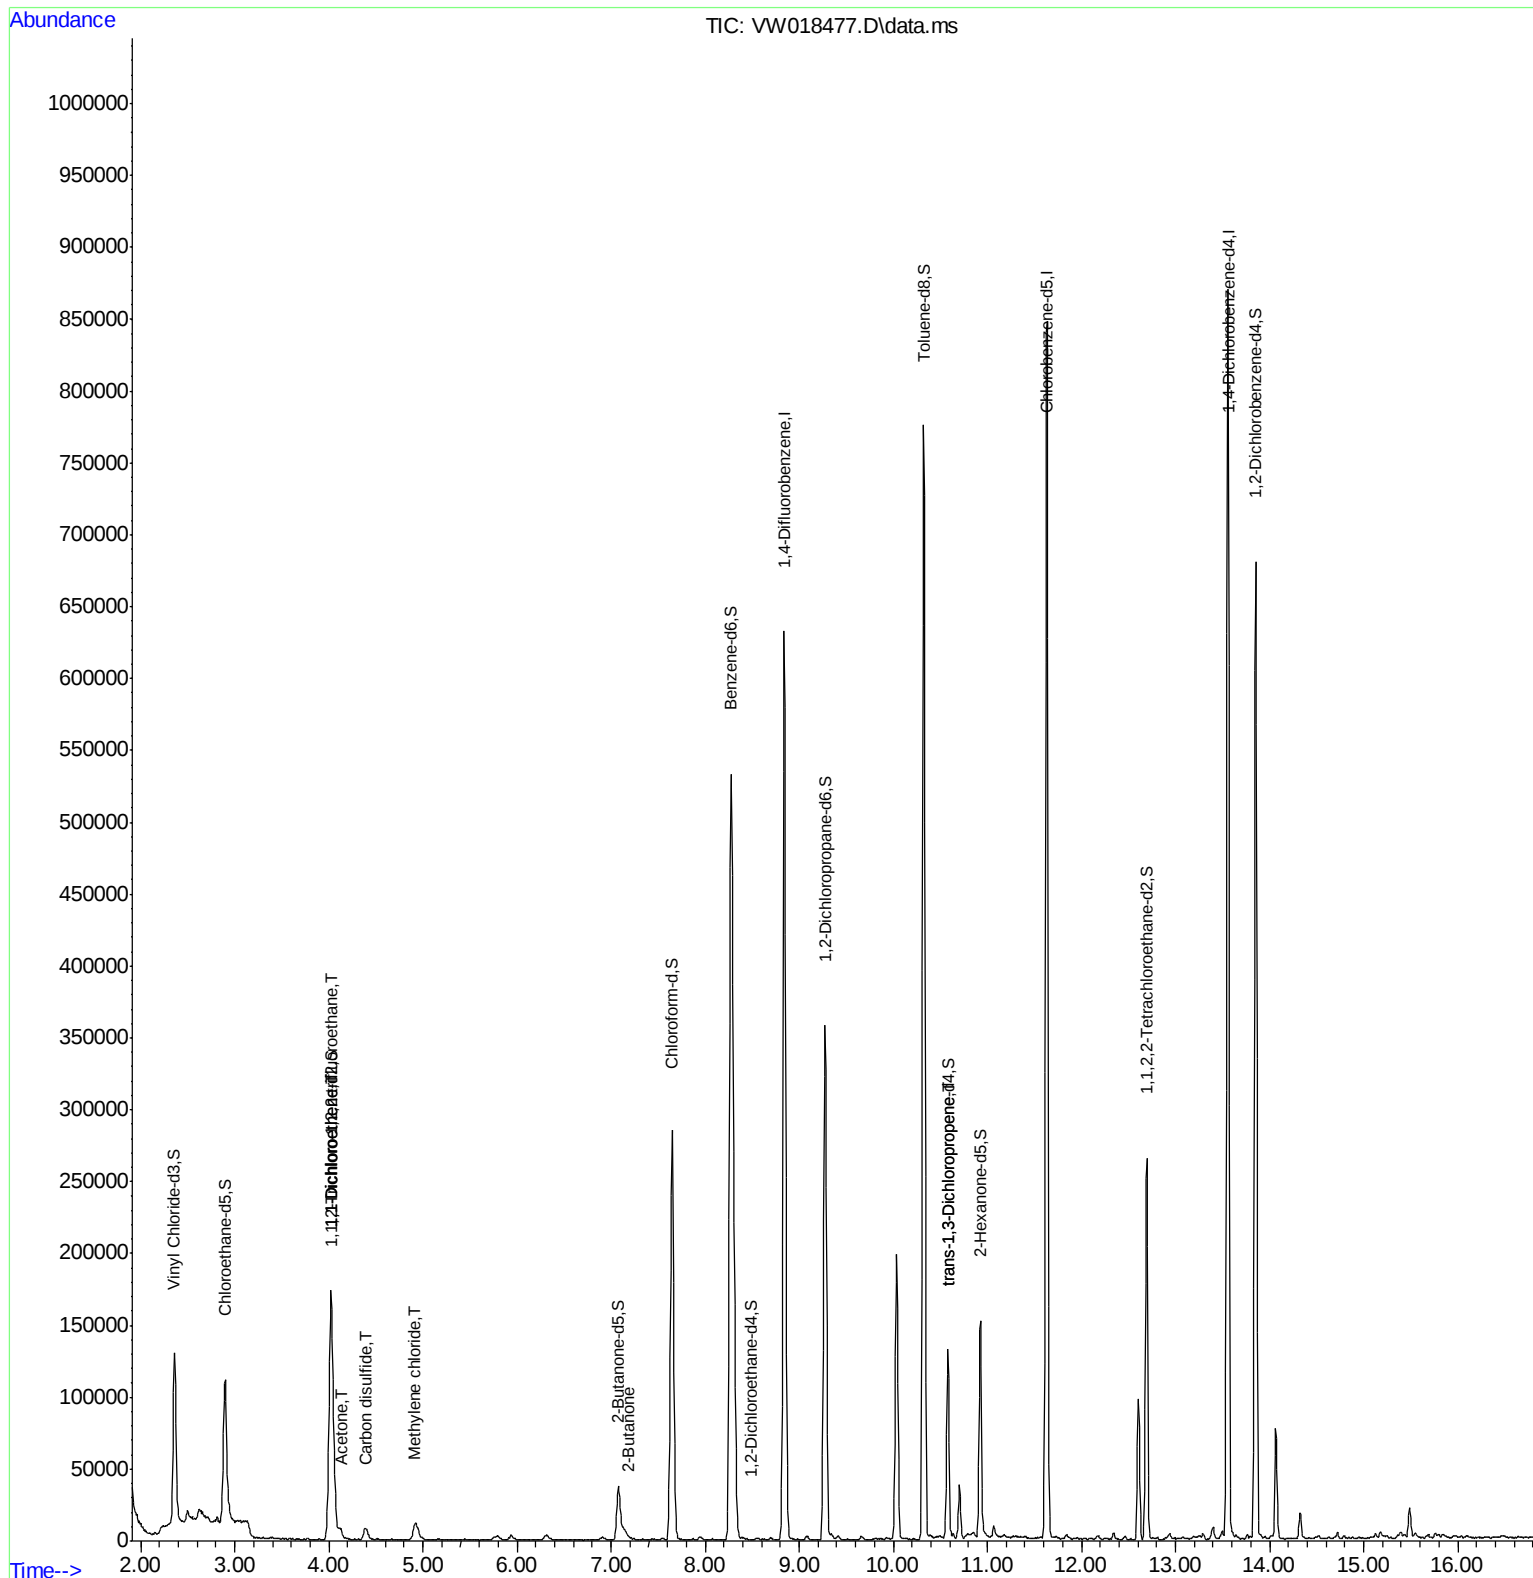


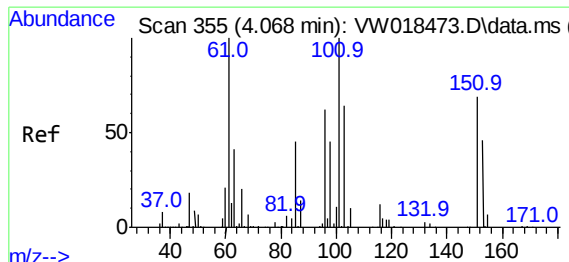

#11
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.35 ug/L
 RT: 4.031 min Scan# 349
 Delta R.T. -0.037 min
 Lab File: VW018477.D
 Acq: 29 Mar 2021 11:41




Instrument :
 MSVOA_W
 ClientSampled :
 BG4S6


Tgt Ion:101 Resp: 2229
 Ion Ratio Lower Upper
 101 100
 85 0.0 35.6 53.4#
 151 2.0 58.1 87.1#

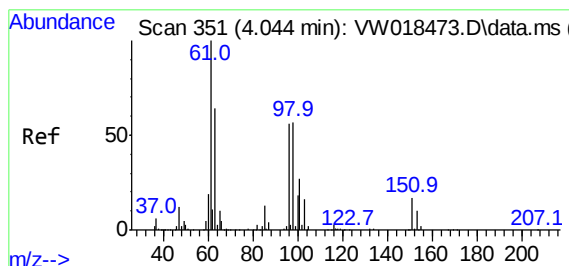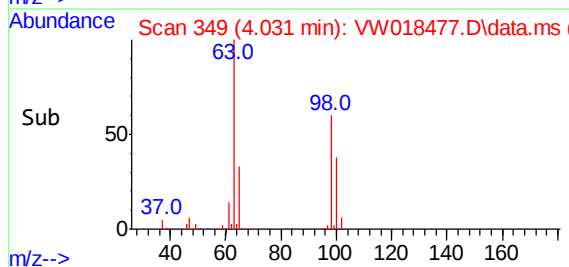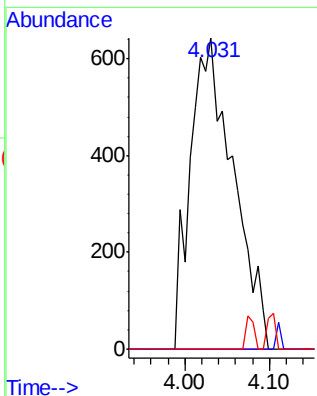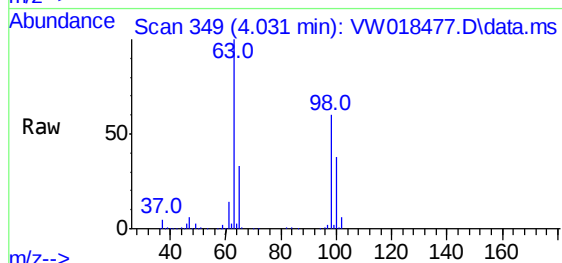

#12
 1,1-Dichloroethene
 Concen: 0.27 ug/L
 RT: 4.019 min Scan# 347
 Delta R.T. -0.025 min
 Lab File: VW018477.D
 Acq: 29 Mar 2021 11:41

Tgt Ion: 96 Resp: 1734
 Ion Ratio Lower Upper
 96 100
 61 1137.6 118.6 220.2#
 63 8644.0 82.4 153.0#


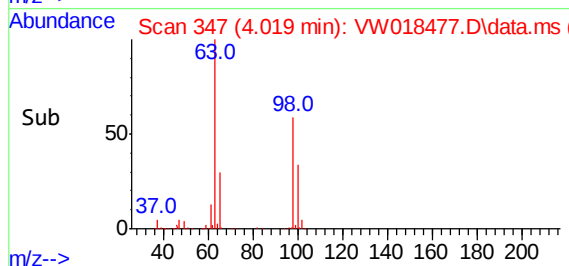
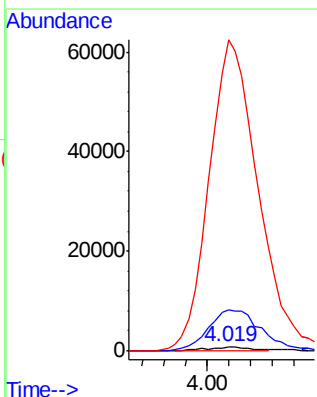
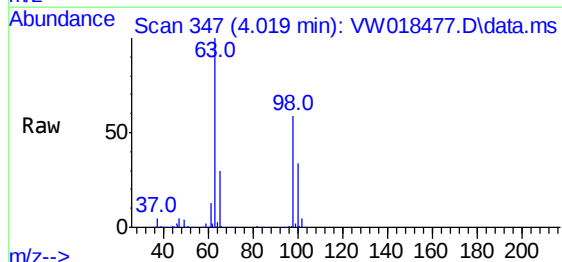


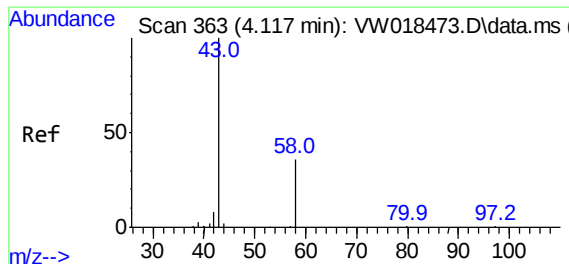

#13
Acetone
Concen: 8.88 ug/L
RT: 4.129 min Scan# 365
Delta R.T. 0.012 min
Lab File: VW018477.D
Acq: 29 Mar 2021 11:41




Instrument :
MSVOA_W
ClientSampled :
BG4S6


Tgt Ion: 43 Resp: 10121
Ion Ratio Lower Upper
43 100
58 31.2 0.0 62.2

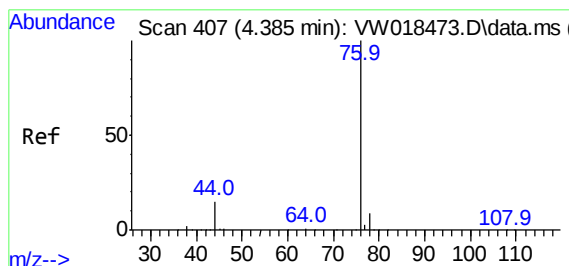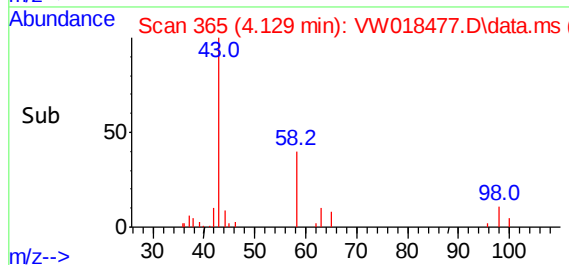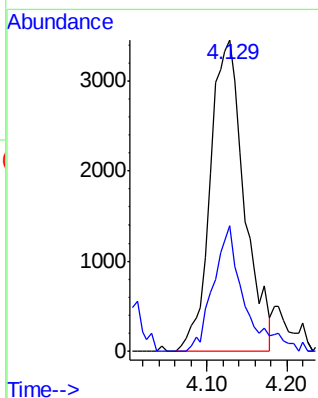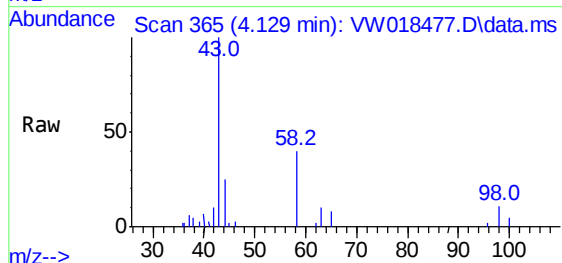

#14
Carbon disulfide
Concen: 0.73 ug/L
RT: 4.391 min Scan# 408
Delta R.T. 0.006 min
Lab File: VW018477.D
Acq: 29 Mar 2021 11:41

Tgt Ion: 76 Resp: 14065
Ion Ratio Lower Upper
76 100
78 8.5 7.4 11.2

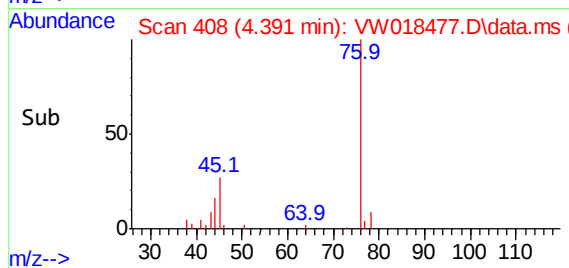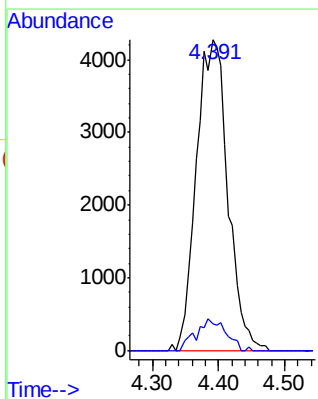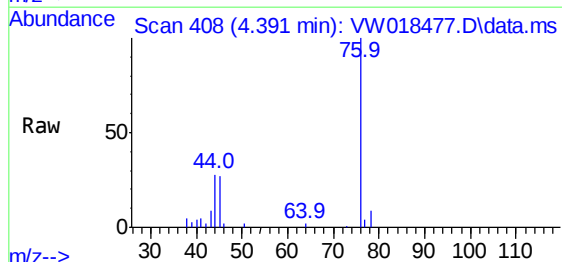




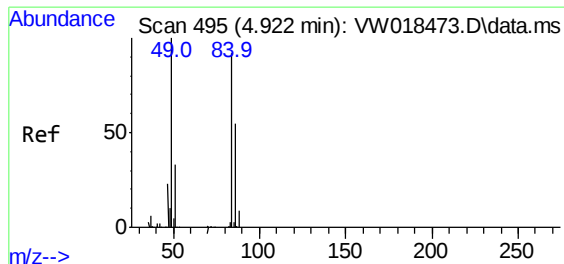


#16
Methylene chloride
Concen: 1.19 ug/L
RT: 4.915 min Scan# 494
Delta R.T. -0.006 min
Lab File: VW018477.D
Acq: 29 Mar 2021 11:41

Instrument :
MSVOA_W
ClientSampleId :
BG4S6

Tgt Ion: 84 Resp: 10009




Ion	Ratio	Lower	Upper
84	100		
49	105.0	74.4	138.2
86	67.0	46.1	85.7

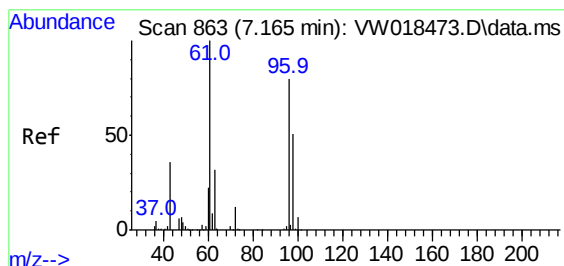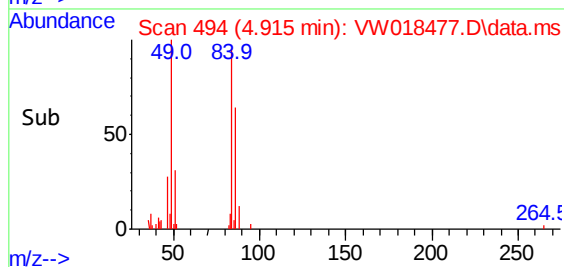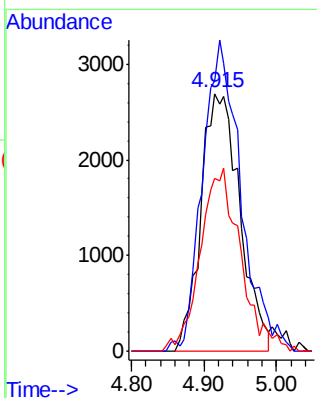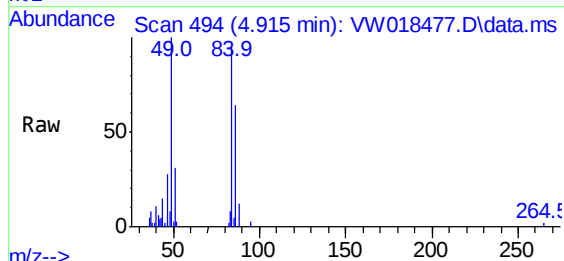


#21
2-Butanone
Concen: 1.65 ug/L
RT: 7.183 min Scan# 866
Delta R.T. 0.018 min
Lab File: VW018477.D
Acq: 29 Mar 2021 11:41

Tgt Ion: 43 Resp: 2988

Ion	Ratio	Lower	Upper
43	100		
72	24.0	16.5	49.5

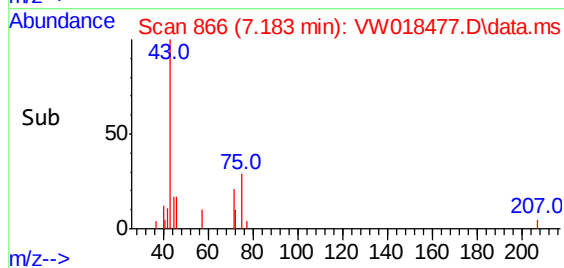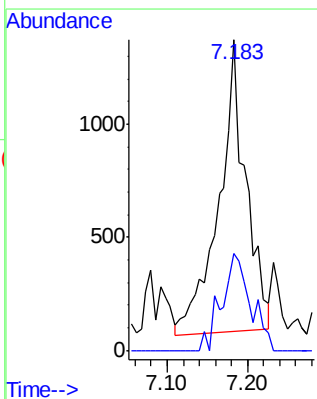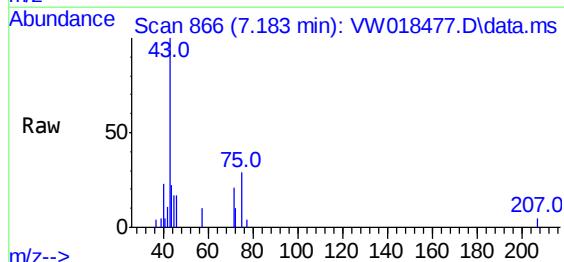

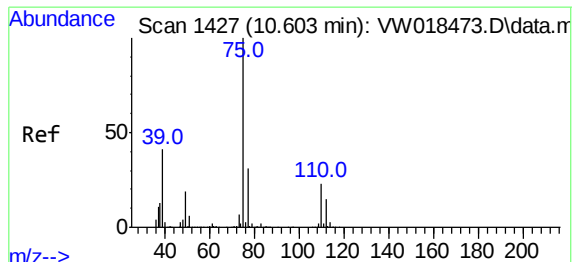

#45
 trans-1,3-Dichloropropene
 Concen: 0.38 ug/L
 RT: 10.579 min Scan# 1423
 Delta R.T. -0.025 min
 Lab File: VW018477.D
 Acq: 29 Mar 2021 11:41

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4S6

Tgt Ion: 75 Resp: 3804
 Ion Ratio Lower Upper
 75 100
 77 30.6 22.6 42.0

