

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032921\
 Data File : VW018480.D
 Acq On : 29 Mar 2021 12:53
 Operator : SY/VA
 Sample : M1816-13
 Misc : 5.87G/10ML/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG3P6

Manual Integrations
 APPROVED

MMDadoda
 3/31/2021 10:55:51 AM

Quant Time: Mar 30 03:12:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Mar 30 03:10:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	207899	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	185632	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	86999	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	71090	24.57	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	98.28%		
7) Chloroethane-d5	2.885	69	63318	25.00	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	100.00%		
10) 1,1-Dichloroethene-d2	4.013	63	89557	17.93	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	71.72%		
20) 2-Butanone-d5	7.080	46	35583	55.25	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	110.50%		
24) Chloroform-d	7.647	84	122955	23.22	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	92.88%		
26) 1,2-Dichloroethane-d4	8.305	65	77360	25.03	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	100.12%		
29) Benzene-d6	8.275	84	232810	23.59	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.36%		
33) 1,2-Dichloropropane-d6	9.274	67	68012	23.89	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.56%		
37) Toluene-d8	10.323	98	211584	22.27	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	89.08%		
38) trans-1,3-Dichloroprop...	10.579	79	29626	20.18	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.72%		
39) 2-Hexanone-d5	10.927	63	29623	53.18	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	106.36%		
48) 1,1,2,2-Tetrachloroeth...	12.689	84	64557	25.35	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	101.40%		
61) 1,2-Dichlorobenzene-d4	13.853	152	70518	22.80	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.20%		
Target Compounds					Qvalue	
13) Acetone	4.135	43	2455m	5.31	ug/L	
16) Methylene chloride	4.916	84	4501m	1.32	ug/L	
47) Tetrachloroethene	10.872	164	686	0.30	ug/L #	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW032921\
Data File : VW018480.D
Acq On : 29 Mar 2021 12:53
Operator : SY/VA
Sample : M1816-13
Misc : 5.87G/10ML/MSVOA_W/SOIL
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BG3P6

Manual Integrations
APPROVED

MMDadoda
3/31/2021 10:55:51 AM


Quant Time: Mar 30 03:12:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Tue Mar 30 03:10:03 2021
Response via : Initial Calibration

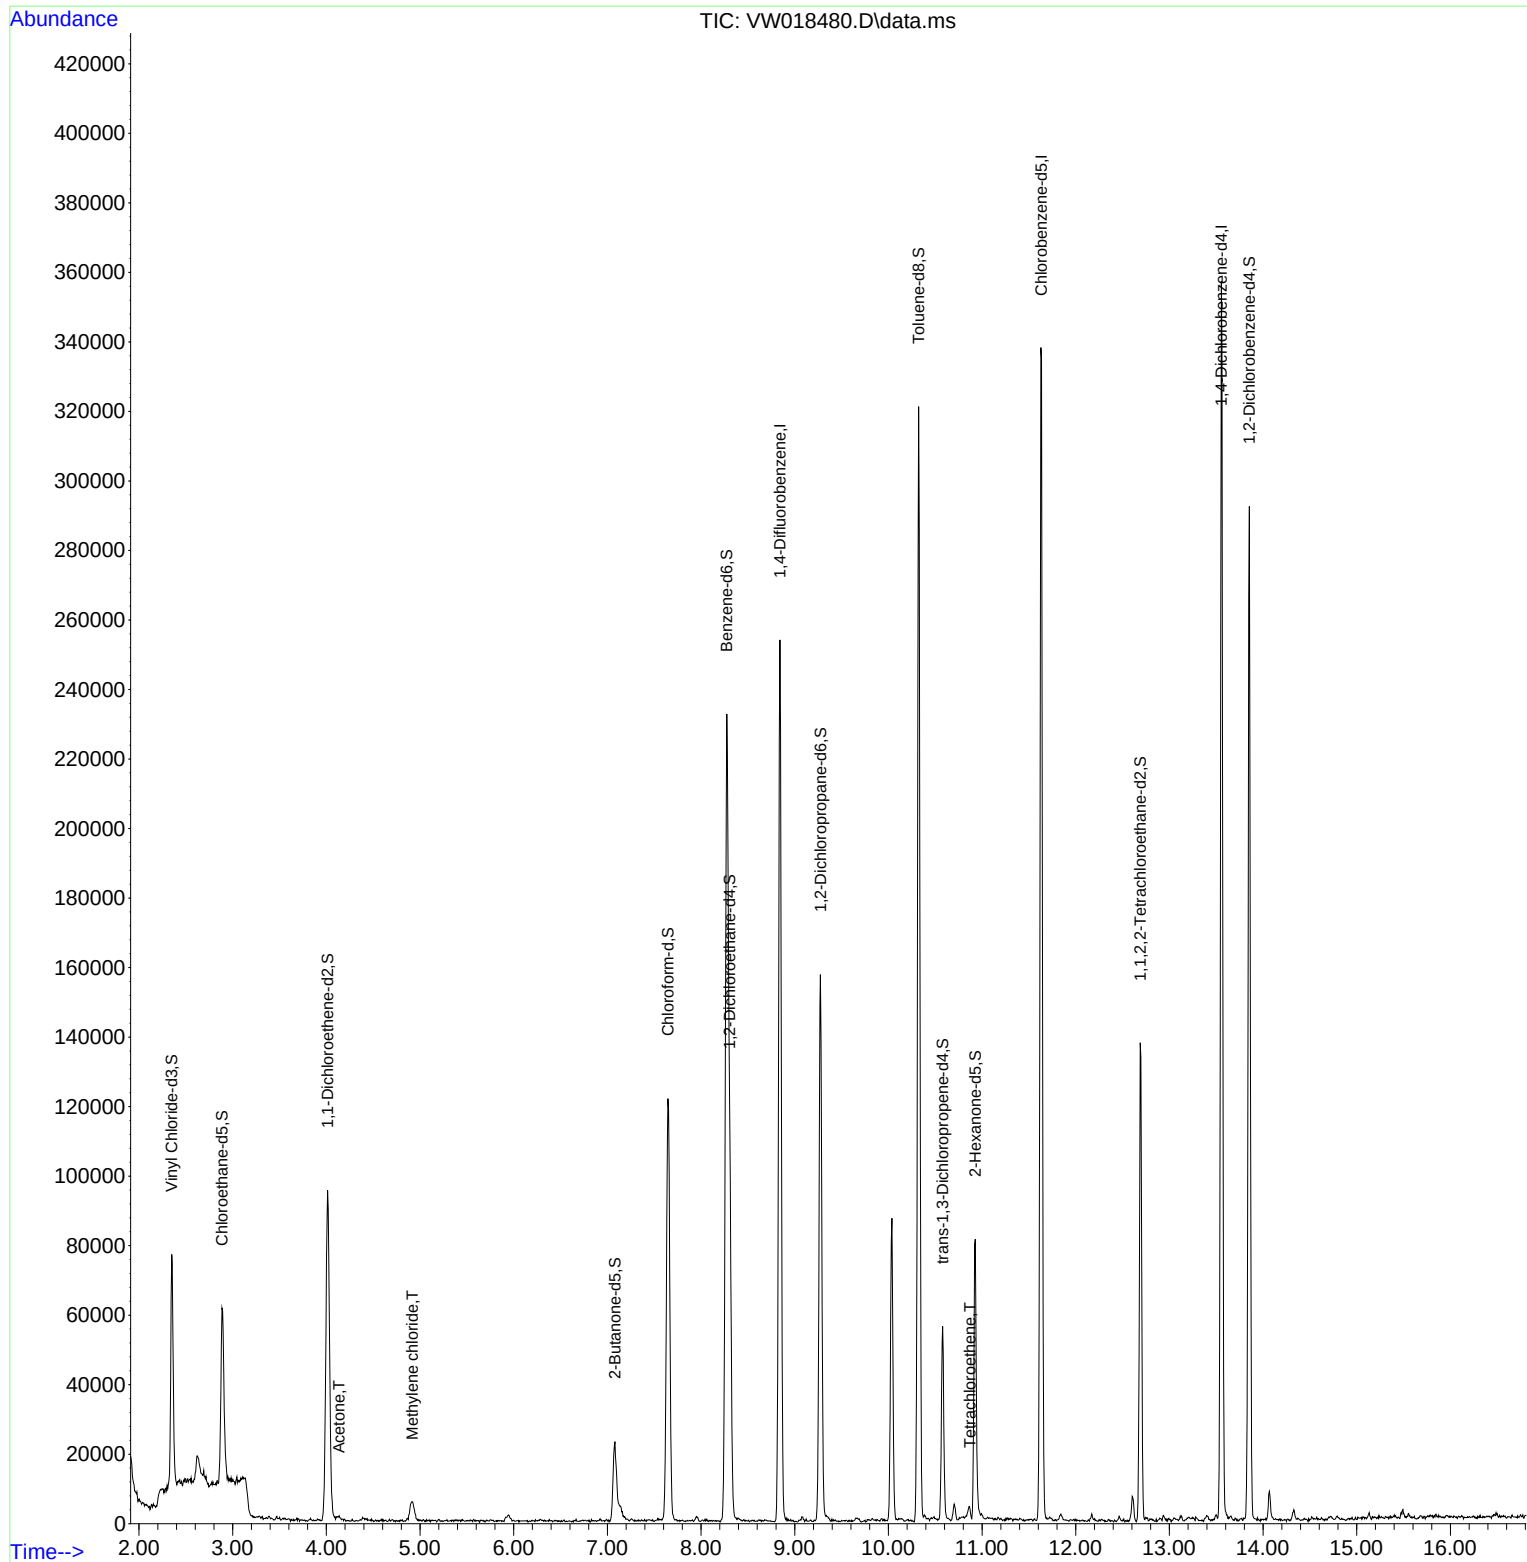

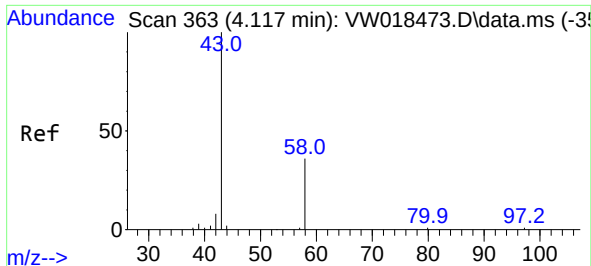

#13
Acetone
Concen: 5.31 ug/L m
RT: 4.135 min Scan# 366
Delta R.T. 0.018 min
Lab File: VW018480.D
Acq: 29 Mar 2021 12:53




Instrument :
MSVOA_W
ClientSampled :
BG3P6

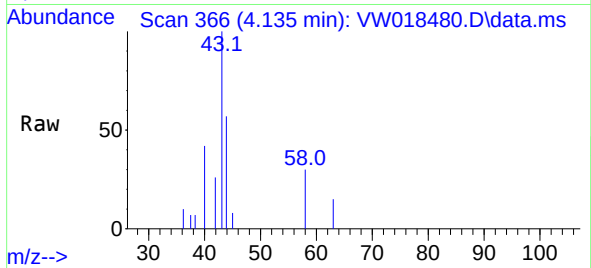


Tgt Ion: 43 Resp: 2455
Ion Ratio Lower Upper
43 100
58 1.2 0.0 62.2

Manual Integrations
APPROVED



MMDadoda
3/31/2021 10:55:51 AM

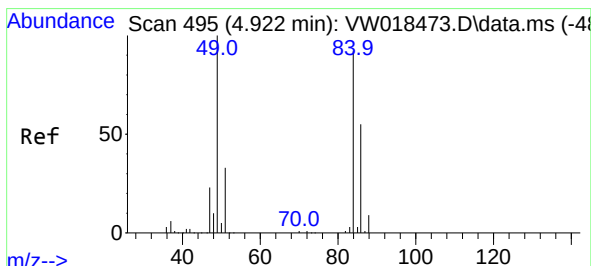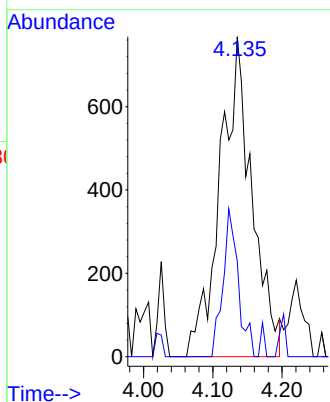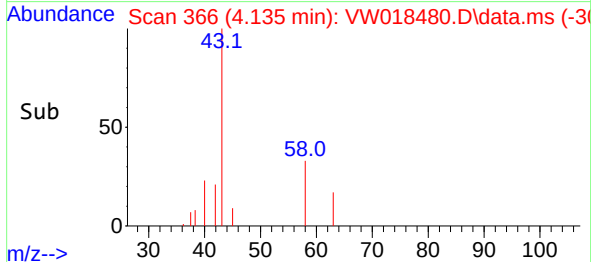


#16
Methylene chloride
Concen: 1.32 ug/L m
RT: 4.916 min Scan# 494
Delta R.T. -0.006 min
Lab File: VW018480.D
Acq: 29 Mar 2021 12:53

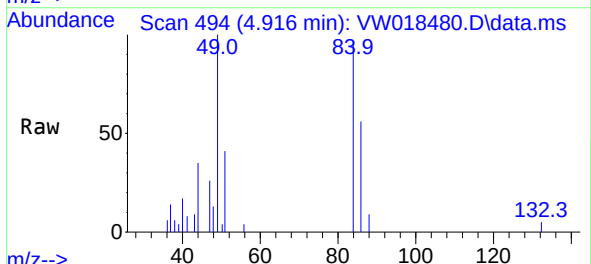

Tgt Ion: 84 Resp: 4501
Ion Ratio Lower Upper
84 100
49 104.2 74.4 138.2
86 58.3 46.1 85.7

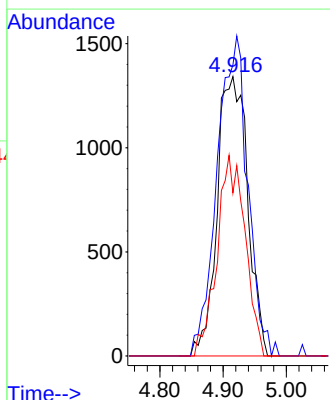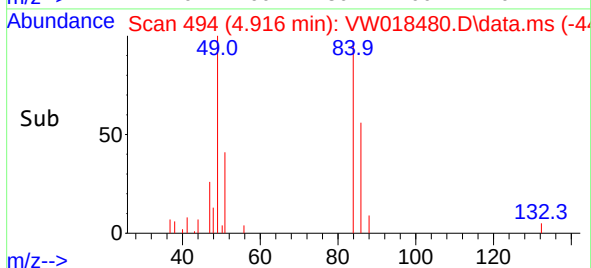

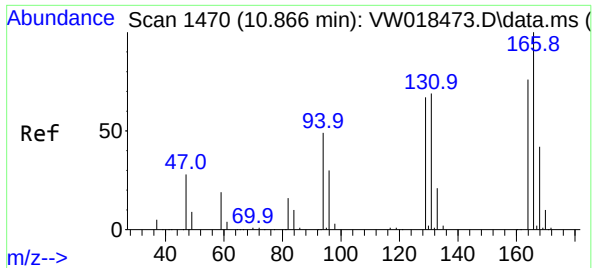

#47
Tetrachloroethene
Concen: 0.30 ug/L
RT: 10.872 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VW018480.D
Acq: 29 Mar 2021 12:53

Tgt Ion:	164	Resp:	686
Ion	Ratio	Lower	Upper
164	100		
129	72.2	68.8	127.8
131	61.8	68.3	126.8#
166	103.2	95.4	177.2

Instrument :
MSVOA_W
ClientSampled :
BG3P6

Manual Integrations
APPROVED

MMDadoda
3/31/2021 10:55:51 AM

