

Quantitation Report (QT Reviewed)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW033019\
 Data File : VW009587.D
 Acq On : 30 Mar 2019 13:48
 Operator : SY/VA
 Sample : K2128-21
 Misc : 5.40G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BF101

Quant Time: Mar 30 21:38:16 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 21:16:55 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:02:08 AM

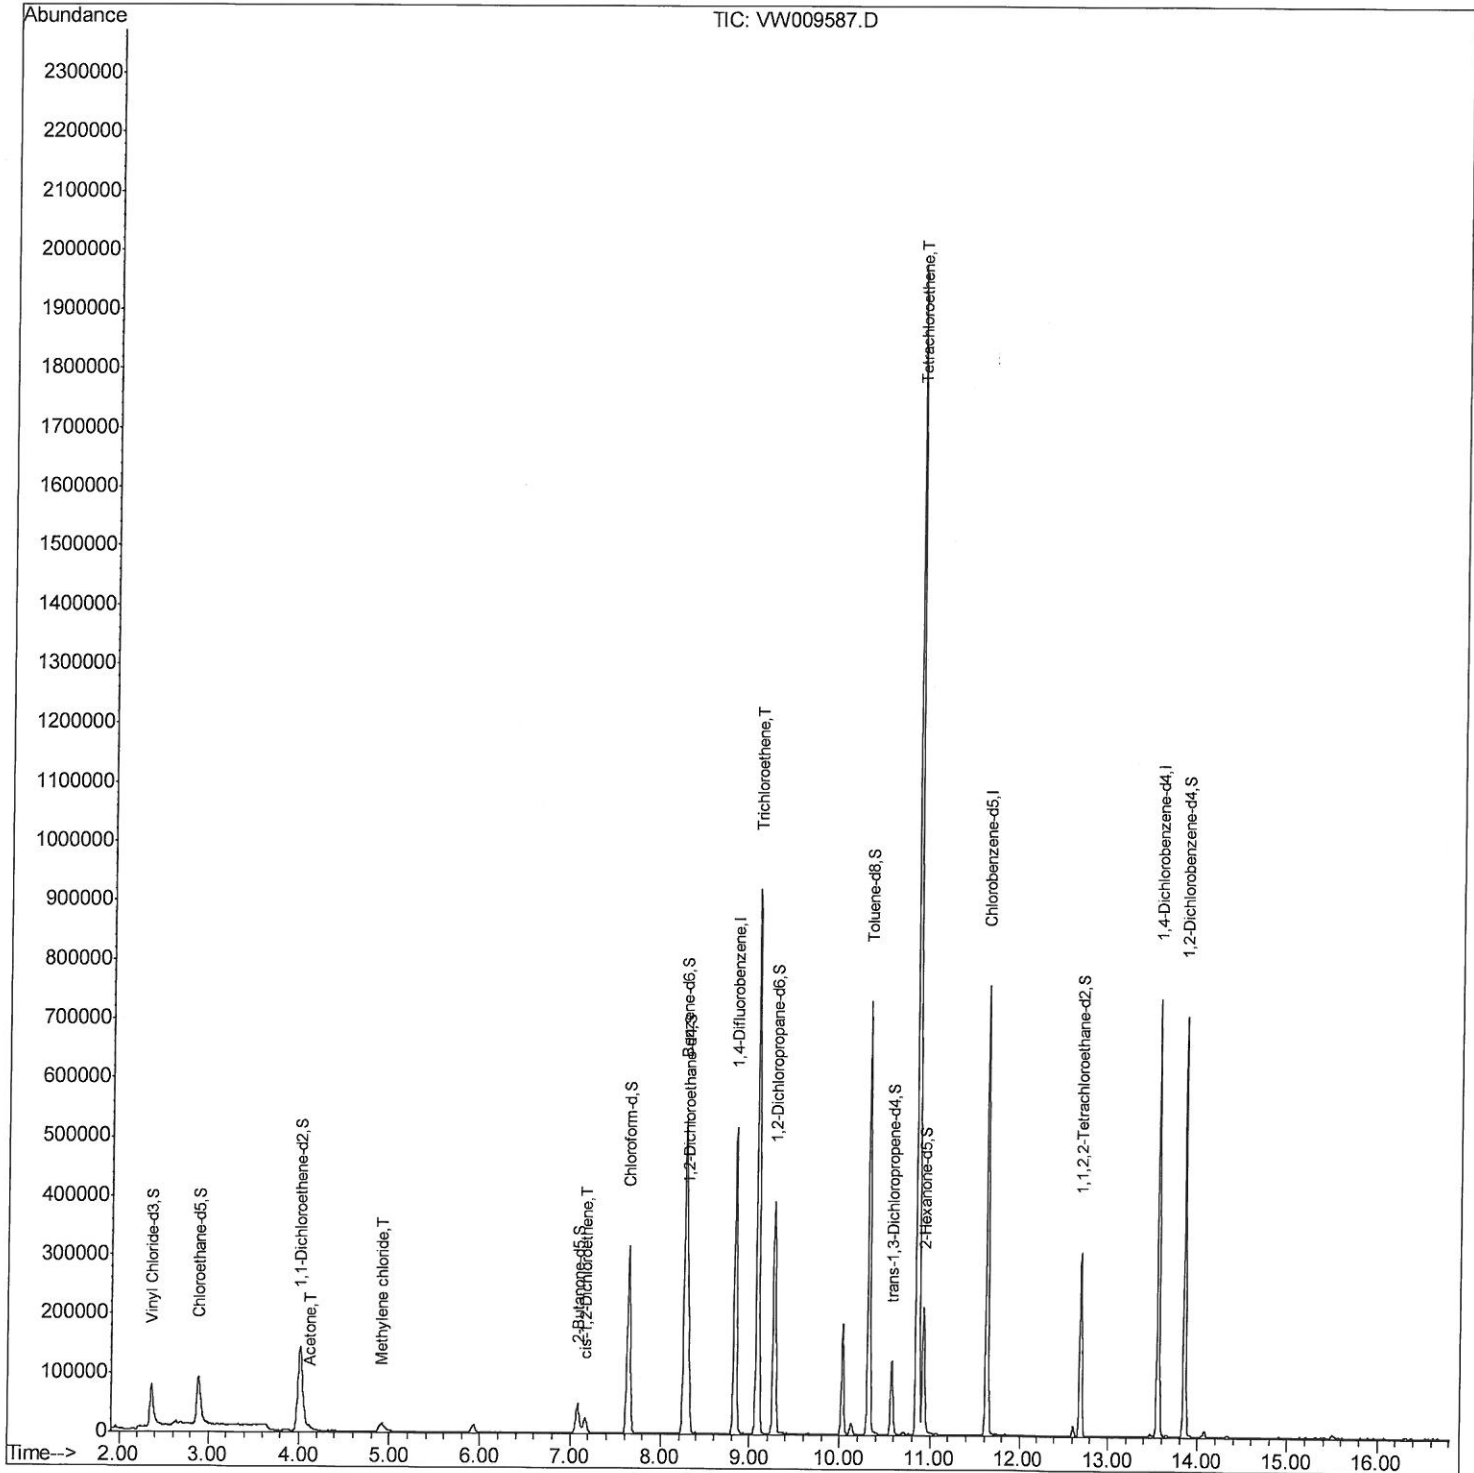

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW033019\
 Data File : VW009587.D
 Acq On : 30 Mar 2019 13:48
 Operator : SY/VA
 Sample : K2128-21
 Misc : 5.40G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BF101

Quant Time: Mar 30 21:20:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 21:16:55 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:02:08 AM

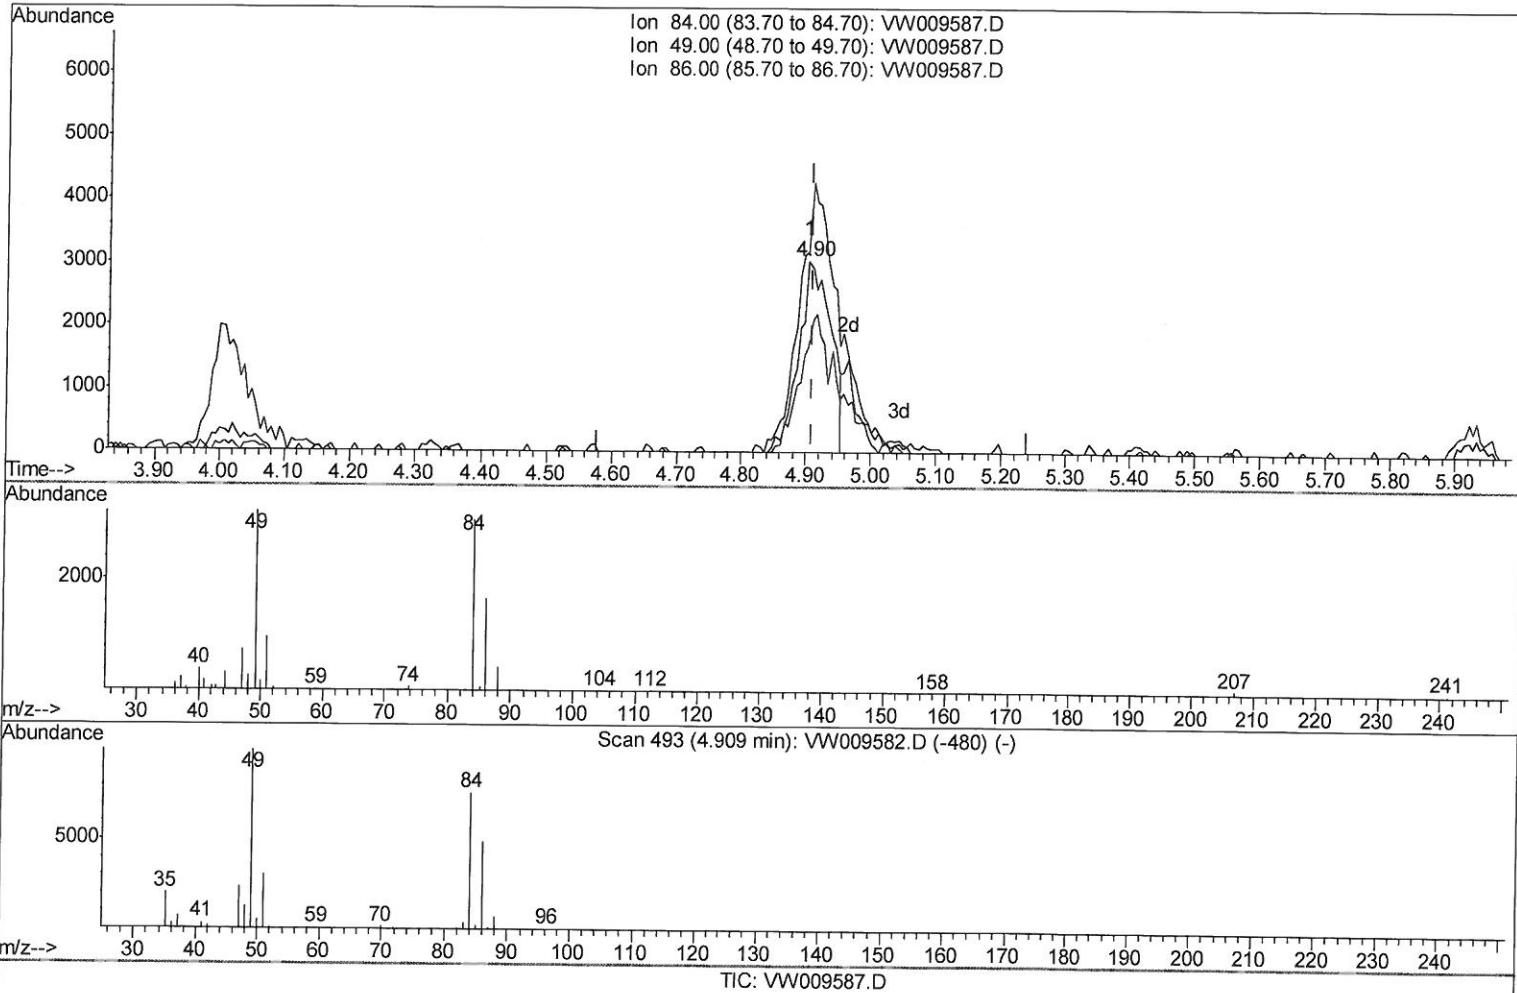

(16) Methylene chloride (T)

4.903min (-0.006) 1.78ug/L

response 10458

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	104.98
86.00	63.50	55.08
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW033019\
 Data File : VW009587.D
 Acq On : 30 Mar 2019 13:48
 Operator : SY/VA
 Sample : K2128-21
 Misc : 5.40G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BF101

Quant Time: Mar 30 21:20:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 21:16:55 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:02:08 AM

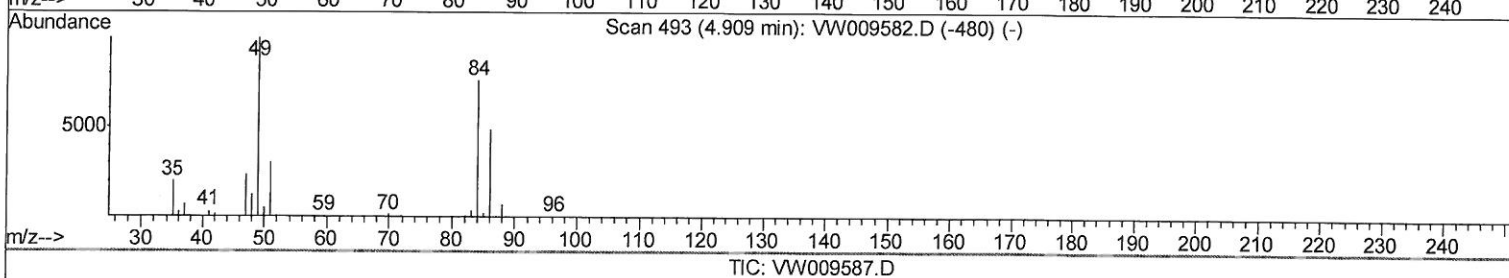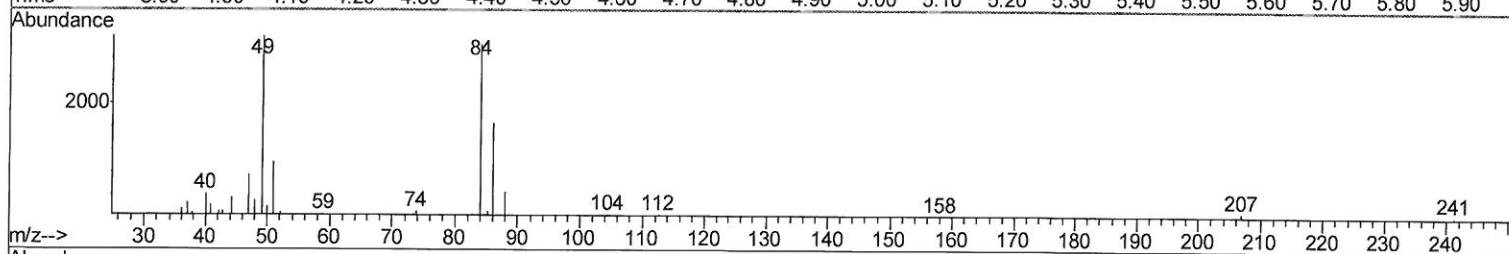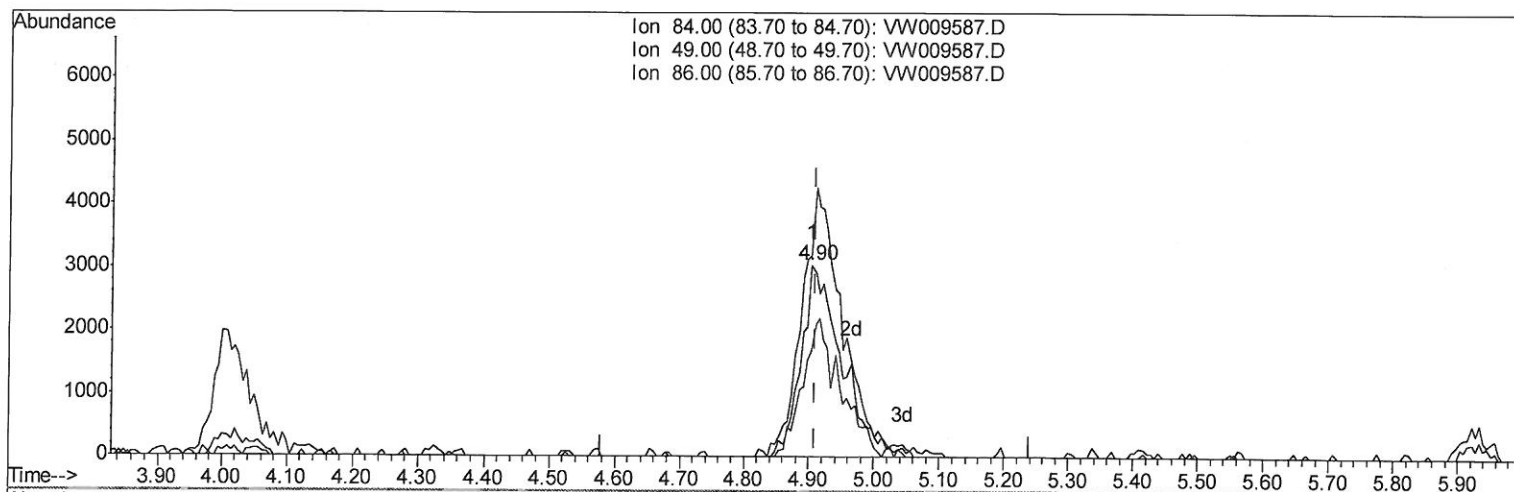

TIC: VW009587.D

(16) Methylene chloride (T)

4.903min (-0.006) 2.25ug/L m

response 13202

MO
 4/11/19

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	104.98
86.00	63.50	55.08
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW033019\
 Data File : VW009587.D
 Acq On : 30 Mar 2019 13:48
 Operator : SY/VA
 Sample : K2128-21
 Misc : 5.40G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BF101

Quant Time: Mar 30 21:38:16 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 21:16:55 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/1/2019 4:02:08 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	403017	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	390836	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	170200	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	122371	25.41	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	101.64%		
7) Chloroethane-d5	2.89	69	124020	22.01	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.04%		
10) 1,1-Dichloroethene-d2	4.01	63	189107	18.17	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	72.68%		
20) 2-Butanone-d5	7.07	46	84279	42.31	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	84.62%		
24) Chloroform-d	7.64	84	283576	25.78	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	103.12%		
26) 1,2-Dichloroethane-d4	8.30	65	170425	25.72	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	102.88%		
29) Benzene-d6	8.27	84	511050	23.71	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.84%		
33) 1,2-Dichloropropane-d6	9.27	67	166678	25.75	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	103.00%		
37) Toluene-d8	10.32	98	456998	22.93	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	91.72%		
38) trans-1,3-Dichloropropene-	10.58	79	62730	19.29	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.16%		
39) 2-Hexanone-d5	10.93	63	62220	39.68	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	79.36%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	142420	22.34	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	89.36%		
61) 1,2-Dichlorobenzene-d4	13.85	152	169195	25.92	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	103.68%		

Target Compounds

					Qvalue
13) Acetone	4.12	43	8779	5.375 ug/L	90
16) Methylene chloride	4.90	84	13202m	2.246 ug/L	97
22) cis-1,2-Dichloroethene	7.16	96	12376	2.190 ug/L	97
35) Trichloroethene	9.09	95	300828	52.775 ug/L	98
47) Tetrachloroethene	10.86	164	394112	81.828 ug/L	98

MQ
 4/1/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed