


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW033019\
Data File : VW009602.D
Acq On : 30 Mar 2019 20:53
Operator : SY/VA
Sample : K2084-23
Misc : 5.08G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 22:32:02 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 21:16:55 2019
Response via : Initial Calibration

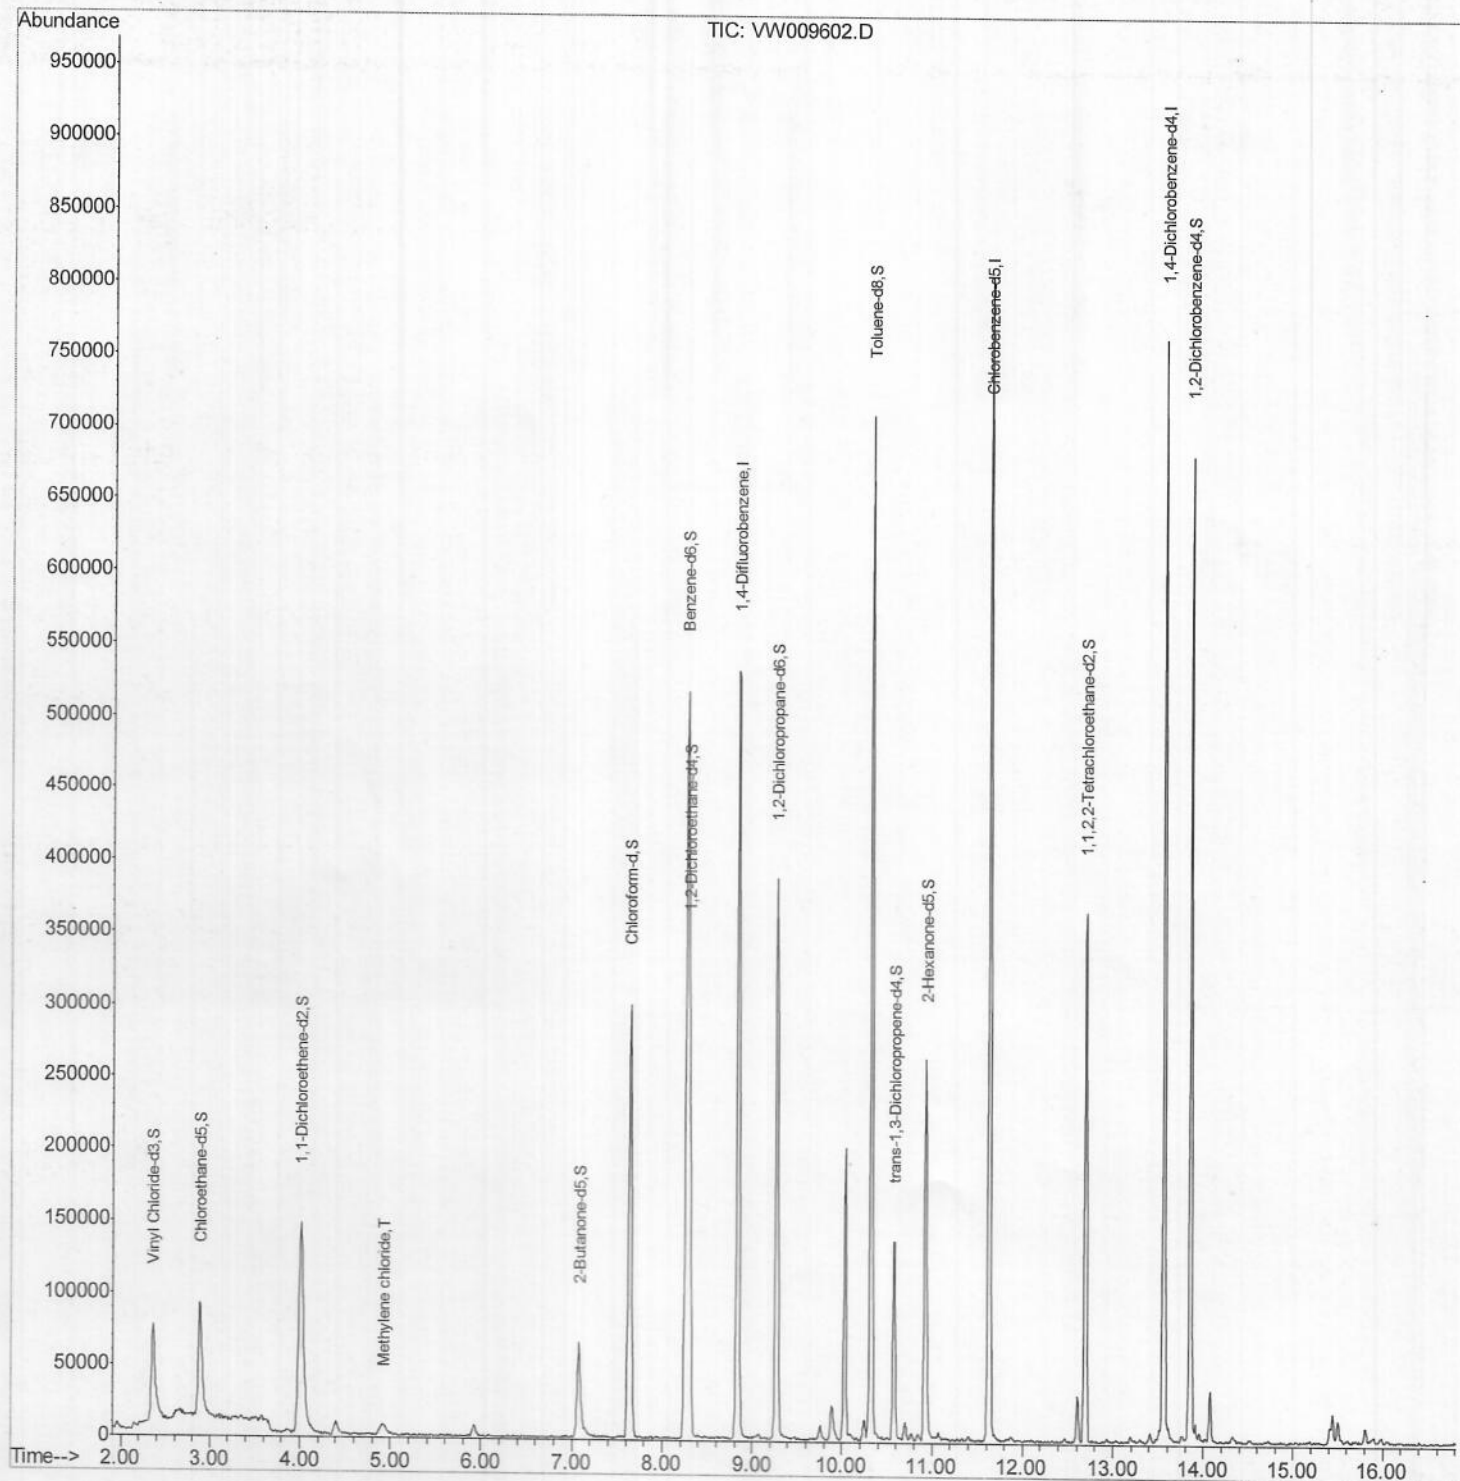

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW033019\

Data File : VW009602.D

Acq On : 30 Mar 2019 20:53

Operator : SY/VA

Sample : K2084-23

Misc : 5.08G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Apr 11 11:04:23 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Thu Apr 11 10:44:34 2019

Response via : Initial Calibration

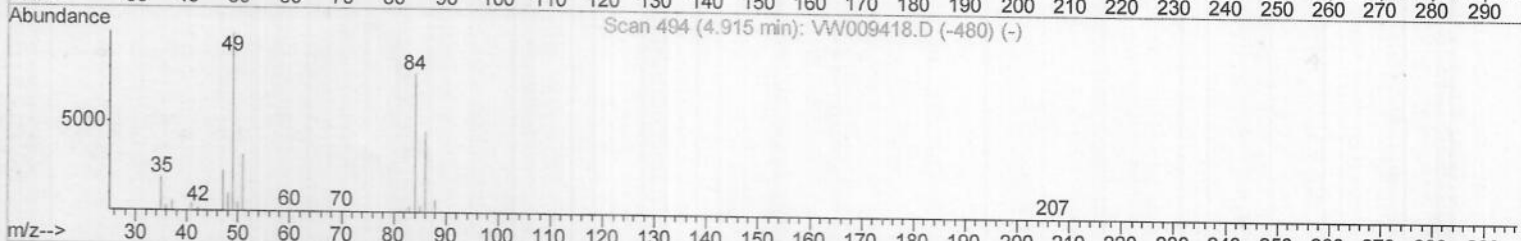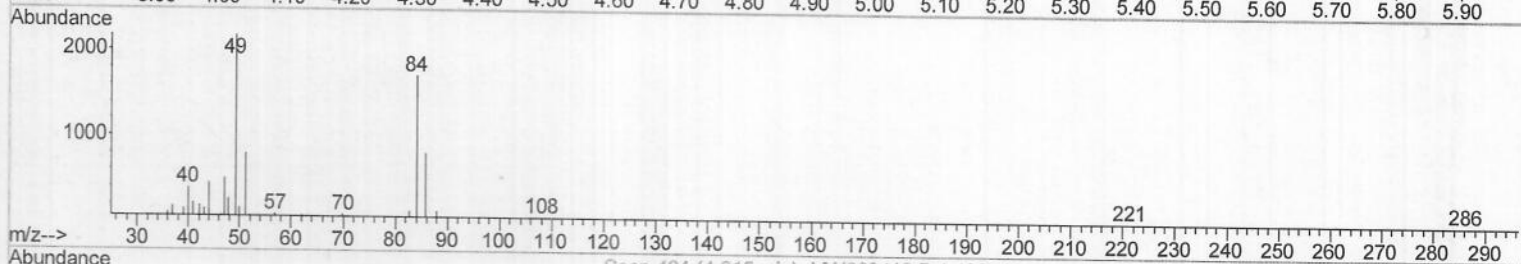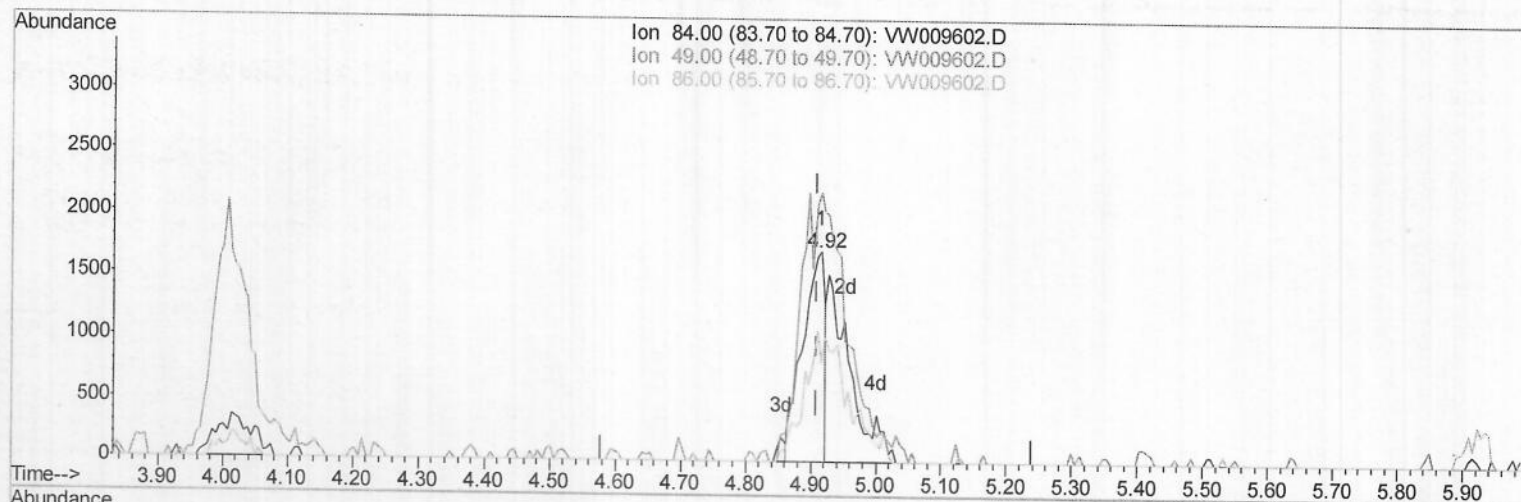

TIC: VW009602.D

(16) Methylene chloride (T)

4.915min (+0.006) 0.68ug/L

response 4095

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	127.69
86.00	63.50	47.42
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW033019\

Data File : VW009602.D

Acq On : 30 Mar 2019 20:53

Operator : SY/VA

Sample : K2084-23

Misc : 5.08G/10ML/MSVOA W/SOIL

ALS Vial : 1 Sample Multiplier: 1


Quant Time: Mar 30 22:32:02 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Sat Mar 30 21:16:55 2019

Response via : Initial Calibration

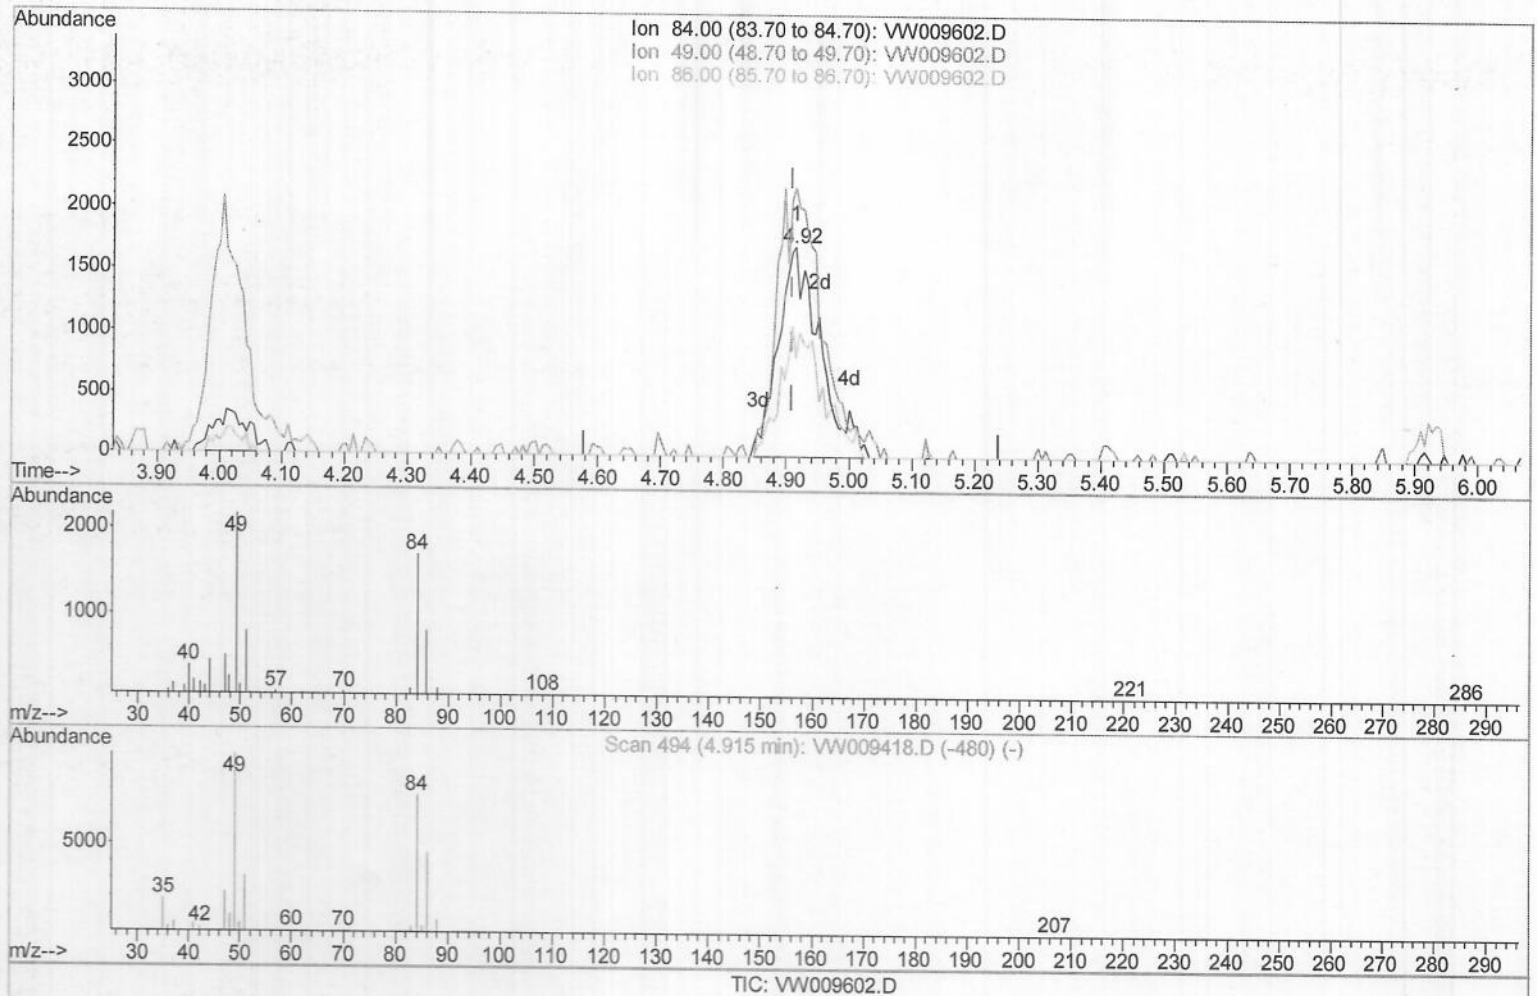

(16) Methylene chloride (T)

4.915min (+0.006) 1.32ug/L m

response 7983

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	127.69
86.00	63.50	47.42
0.00	0.00	0.00

M.P
4/11/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW033019\
 Data File : VW009602.D
 Acq On : 30 Mar 2019 20:53
 Operator : SY/VA
 Sample : K2084-23
 Misc : 5.08G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 22:32:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Mar 30 21:16:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	415137	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	411838	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	180573	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	130848	26.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	105.52%
7) Chloroethane-d5	2.89	69	122924	21.18	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.72%
10) 1,1-Dichloroethene-d2	4.01	63	192468	17.95	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.80%
20) 2-Butanone-d5	7.07	46	108845	53.05	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.10%
24) Chloroform-d	7.64	84	271153	23.93	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.72%
26) 1,2-Dichloroethane-d4	8.30	65	180028	26.38	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	105.52%
29) Benzene-d6	8.27	84	497248	21.89	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.56%
33) 1,2-Dichloropropane-d6	9.27	67	158766	23.27	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.08%
37) Toluene-d8	10.32	98	445344	21.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.84%
38) trans-1,3-Dichloropropene-	10.57	79	69037	20.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.60%
39) 2-Hexanone-d5	10.93	63	72484	43.87	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.74%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	159879	23.80	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.20%
61) 1,2-Dichlorobenzene-d4	13.85	152	164874	23.81	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.24%

Target Compounds

16) Methylene chloride	4.92	84	7983m	1.319	ug/L	Qvalue
------------------------	------	----	-------	-------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed