


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033021\
Data File : VW018499.D
Acq On : 30 Mar 2021 11:18
Operator : SY/VA
Sample : M1816-17RE
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 31 01:13:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 31 01:12:37 2021
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
BG3Q4RE

Manual Integrations
APPROVED

MMDadoda
4/2/2021 1:09:21 PM

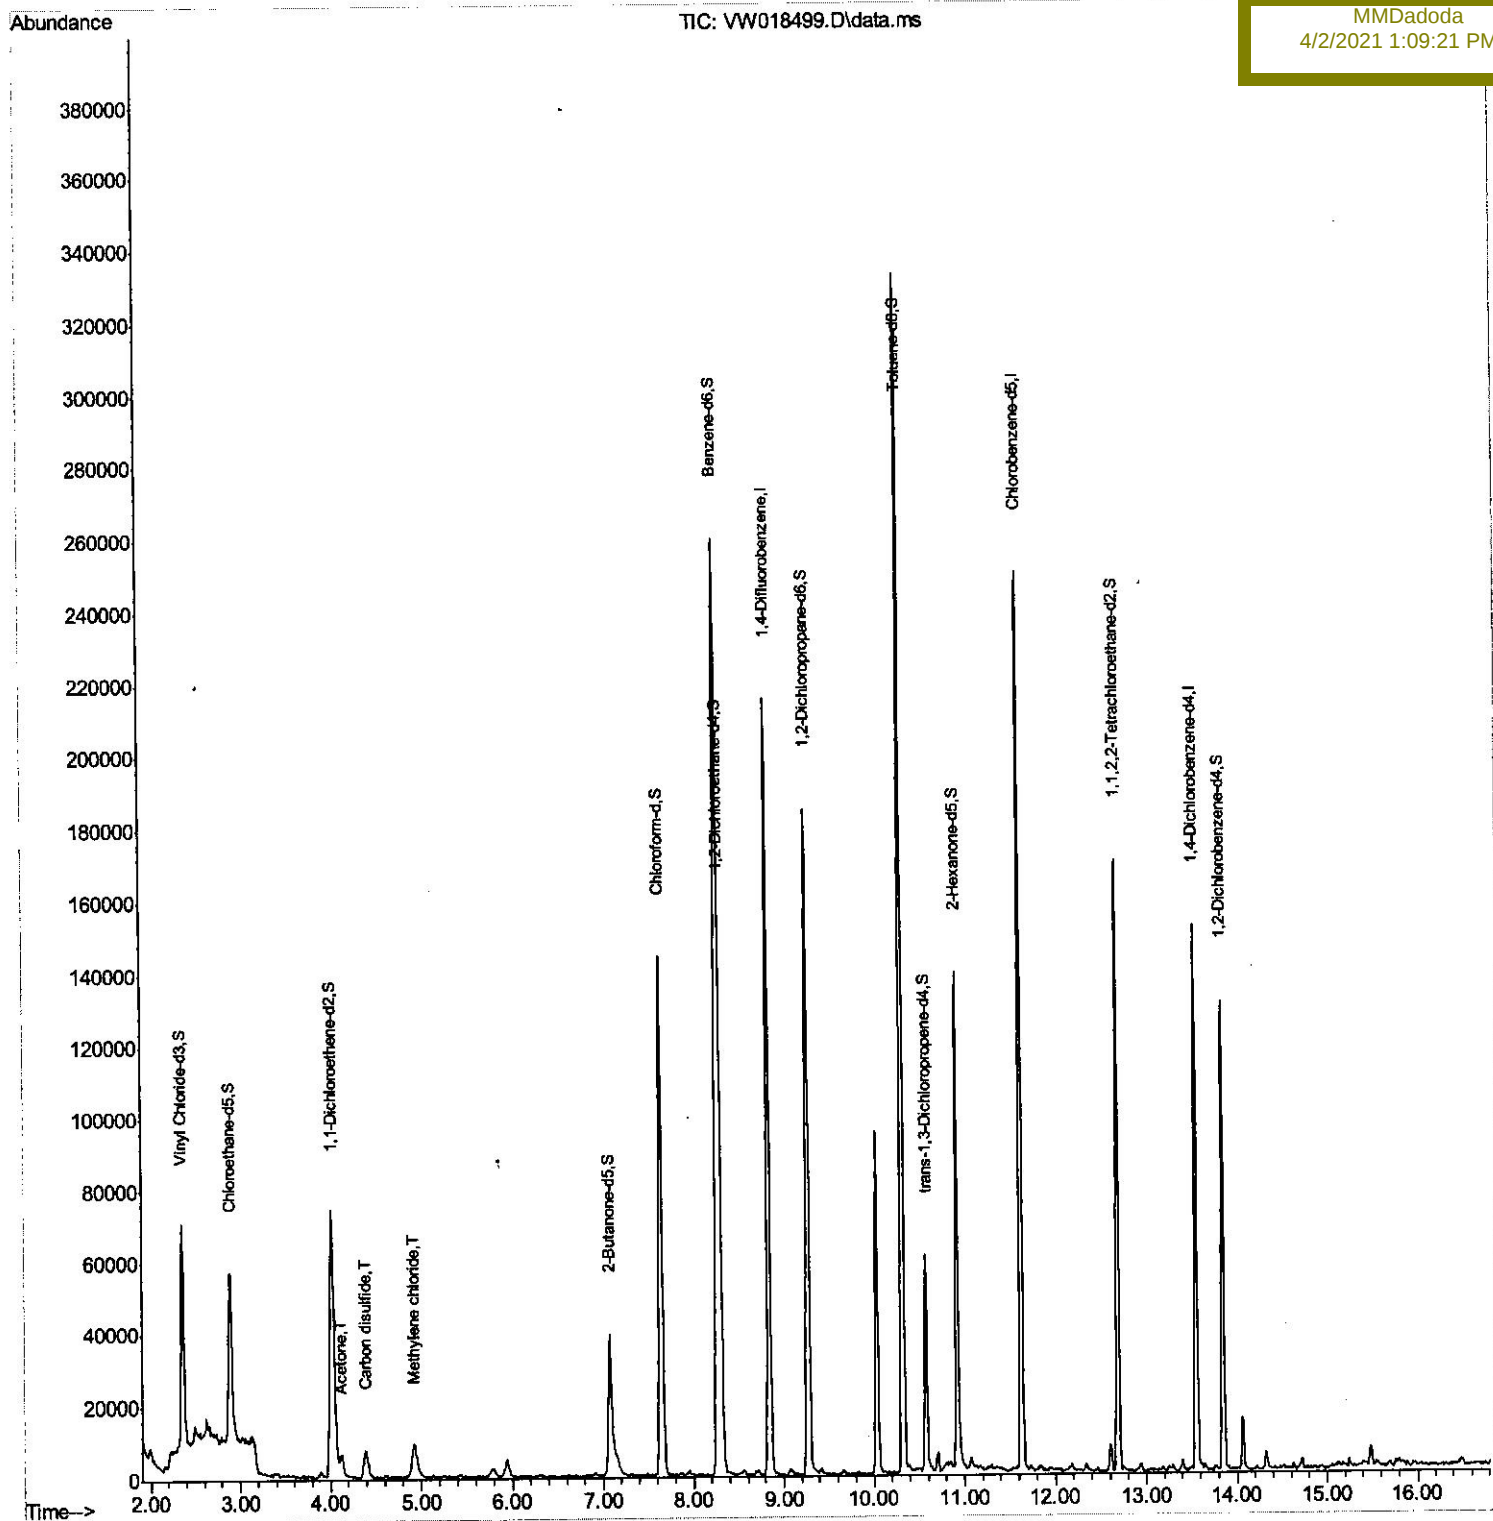




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033021\
Data File : VW018499.D
Acq On : 30 Mar 2021 11:18
Operator : SY/VA
Sample : M1816-17RE
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Mar 31 01:13:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 31 01:12:37 2021
Response via : Initial Calibration

Instrument :
MSVOA_W
ClientSampleId :
BG3Q4RE

Manual Integrations
APPROVED

MMDadoda
4/2/2021 1:09:21 PM

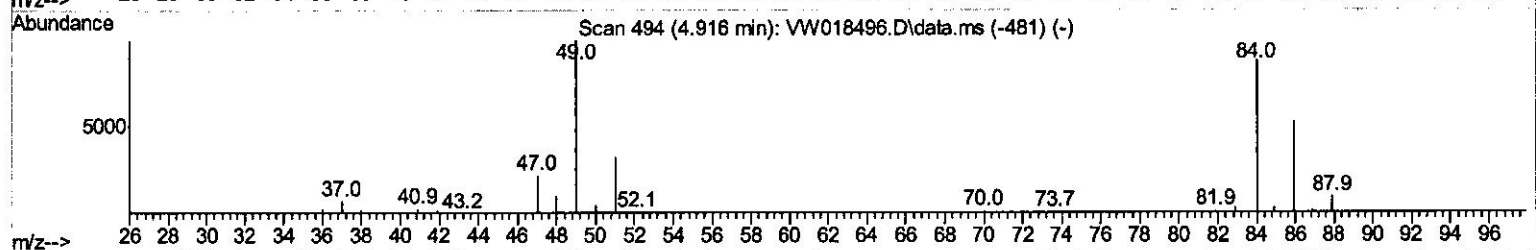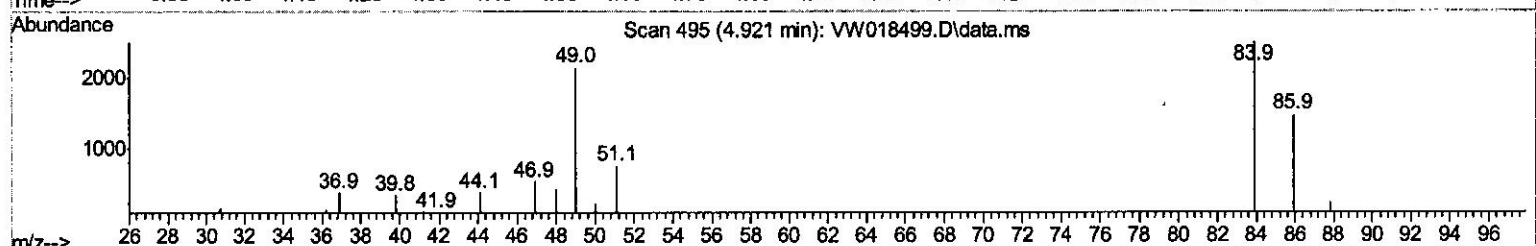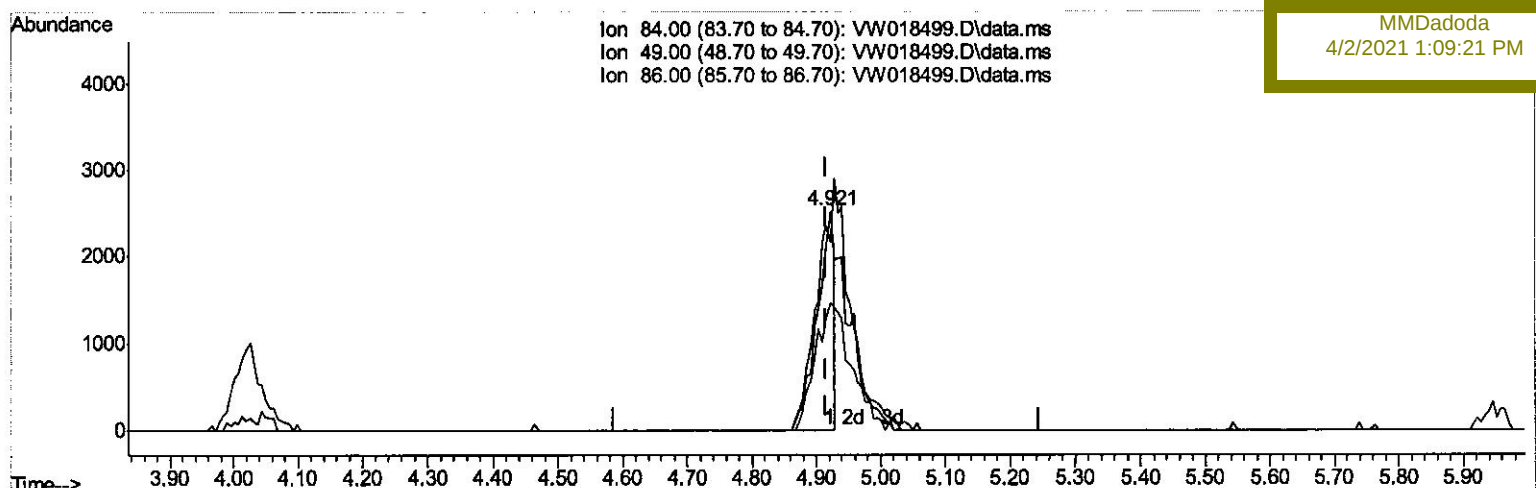

TIC: VW018499.D\data.ms

(16) Methylene chloride (T)

4.921min (+ 0.006) 1.60 ug/L

response 4624

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	106.30	85.57
86.00	65.90	58.41
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033021\
 Data File : VW018499.D
 Acq On : 30 Mar 2021 11:18
 Operator : SY/VA
 Sample : M1816-17RE
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG3Q4RE

Manual Integrations
 APPROVED

MMDadoda
 4/2/2021 1:09:21 PM

Quant Time: Mar 31 01:13:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 31 01:12:37 2021
 Response via : Initial Calibration

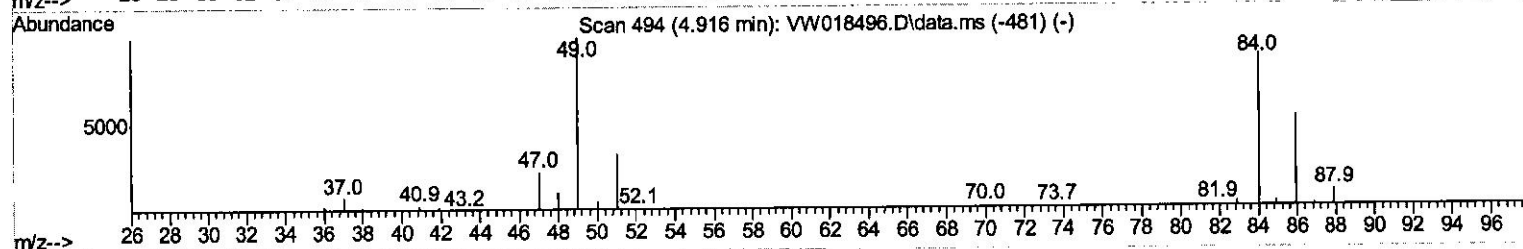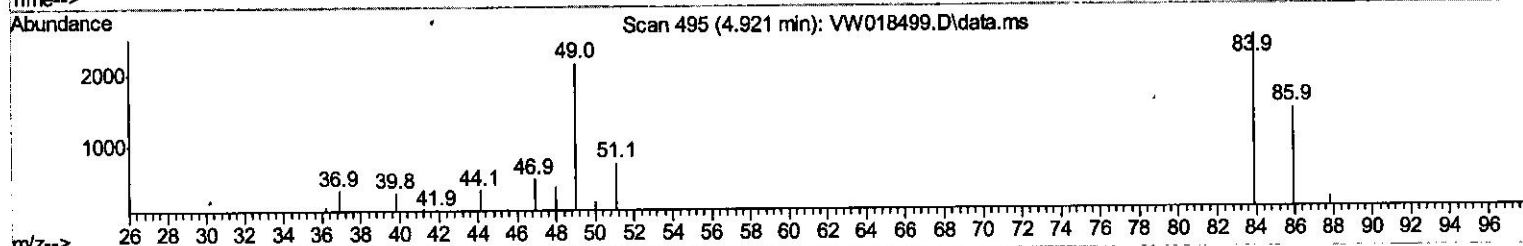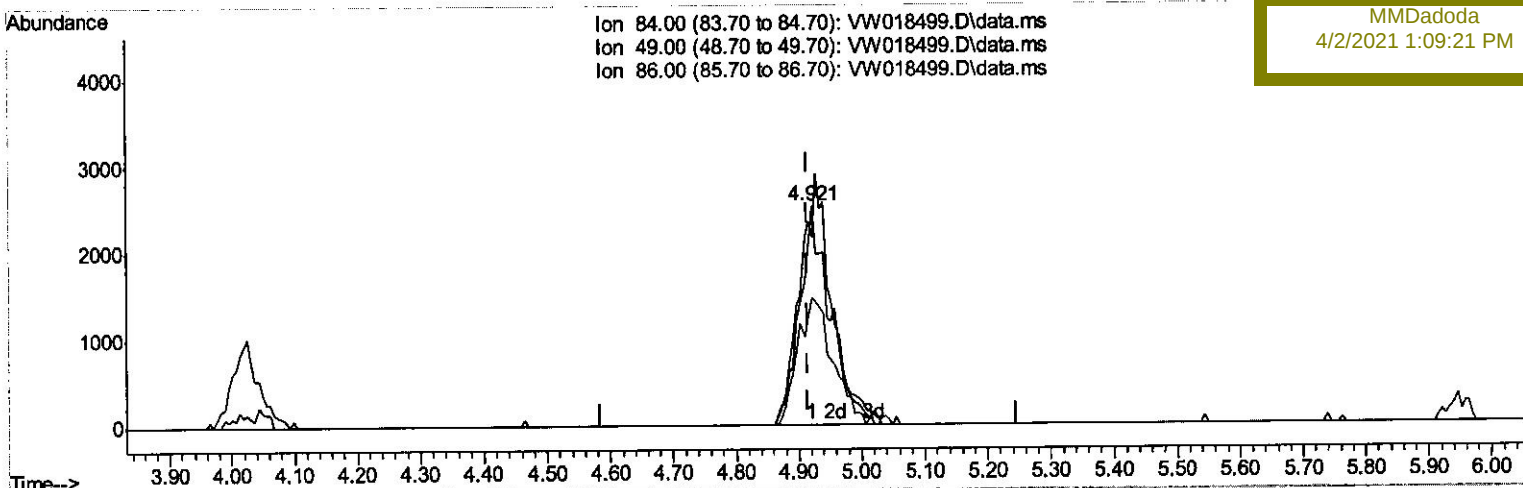

TIC: VW018499.D\data.ms

(16) Methylene chloride (T)

4.921min (+ 0.006) 2.98 ug/L m

response 8606

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	106.30	85.57
86.00	65.90	58.41
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033021\
 Data File : VW018499.D
 Acq On : 30 Mar 2021 11:18
 Operator : SY/VA
 Sample : M1816-17RE
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG3Q4RE

Manual Integrations
 APPROVED

MMDadoda
 4/2/2021 1:09:21 PM

Quant Time: Mar 31 01:13:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 31 01:12:37 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	175981	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	132501	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	36735	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	71187	29.07	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	= 116.28%		
7) Chloroethane-d5	2.891	69	68448	31.93	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	= 127.72%		
10) 1,1-Dichloroethene-d2	4.025	63	80911	19.14	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	= 76.56%		
20) 2-Butanone-d5	7.080	46	63795	117.01	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	= 234.02%#		
24) Chloroform-d	7.646	84	142465	31.78	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	= 127.12%		
26) 1,2-Dichloroethane-d4	8.305	65	96172	36.76	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	= 147.04%#		
29) Benzene-d6	8.274	84	256038	36.35	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	= 145.40%#		
33) 1,2-Dichloropropane-d6	9.274	67	81638	40.18	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	= 160.72%#		
37) Toluene-d8	10.323	98	214524	31.63	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	= 126.52%		
38) trans-1,3-Dichloroprop...	10.579	79	32516	31.03	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	= 124.12%		
39) 2-Hexanone-d5	10.926	63	47348	119.07	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	= 238.14%#		
48) 1,1,2,2-Tetrachloroeth...	12.694	84	82152	45.20	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	= 180.80%#		
61) 1,2-Dichlorobenzene-d4	13.853	152	31041	23.77	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	= 95.08%		
Target Compounds						Qvalue
13) Acetone	4.123	43	9626	24.58	ug/L	98
14) Carbon disulfide	4.391	76	15872	2.39	ug/L	96
16) Methylene chloride	4.921	84	8606m	2.98	ug/L	

m D
 4/2/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed