




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025498.D
 Acq On : 30 Mar 2023 13:02
 Operator : SY/MD
 Sample : VW0330SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK476

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Mar 31 02:22:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

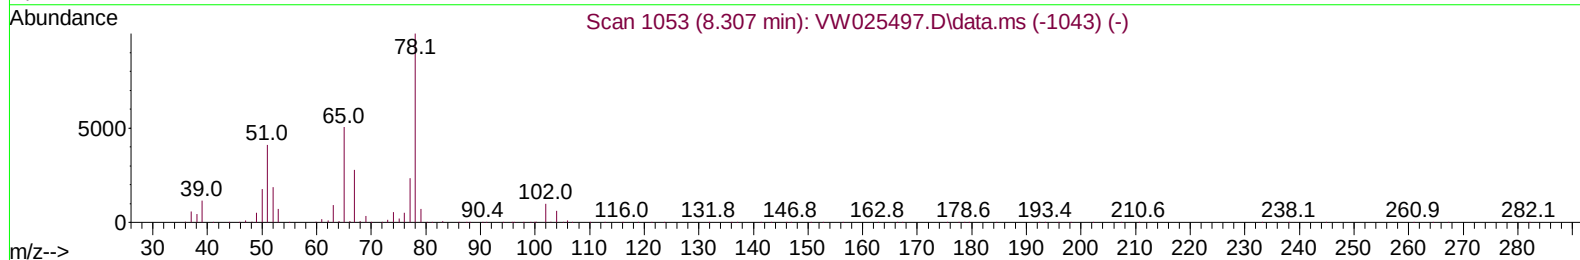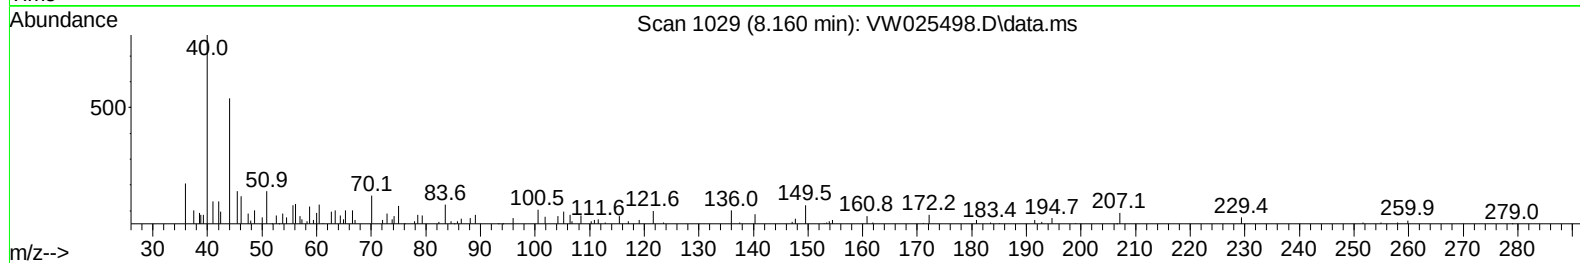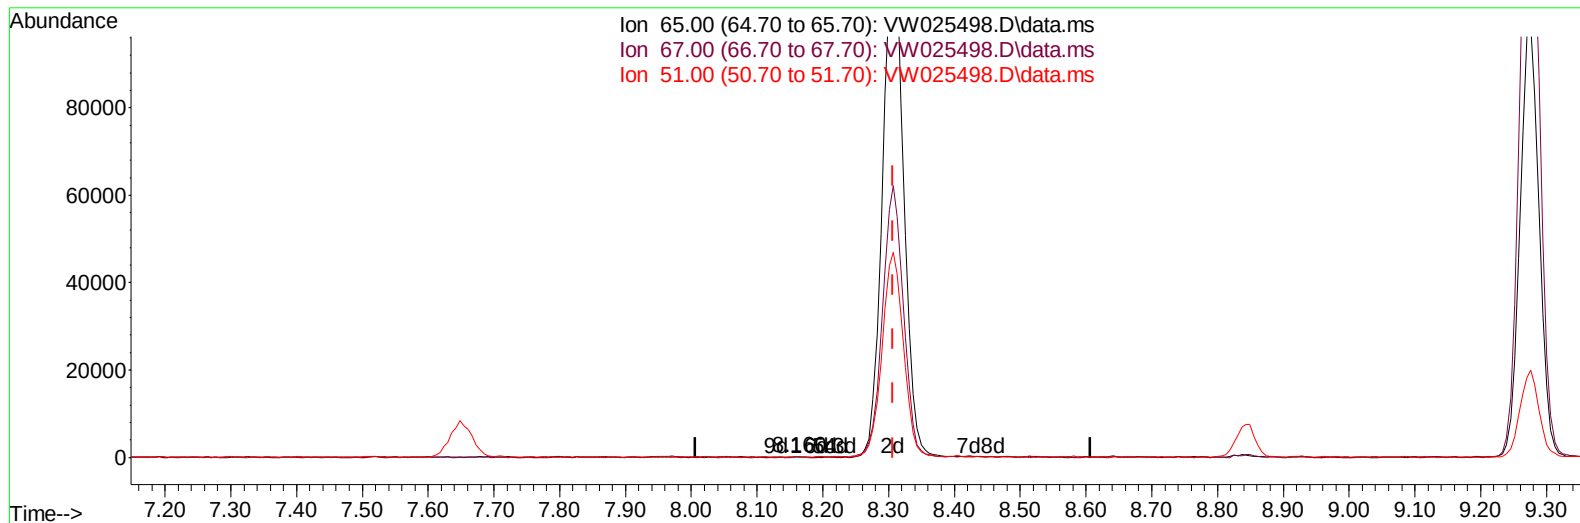

TIC: VW025498.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.160min (-0.146) 0.02 ug/L

response 182

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	37.36
51.00	111.10	116.48
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025498.D
 Acq On : 30 Mar 2023 13:02
 Operator : SY/MD
 Sample : VW0330SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK476

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Mar 31 02:22:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

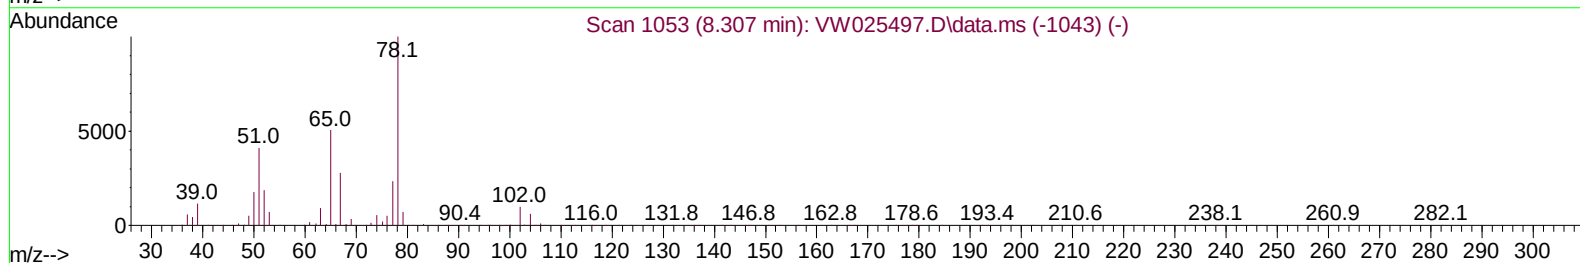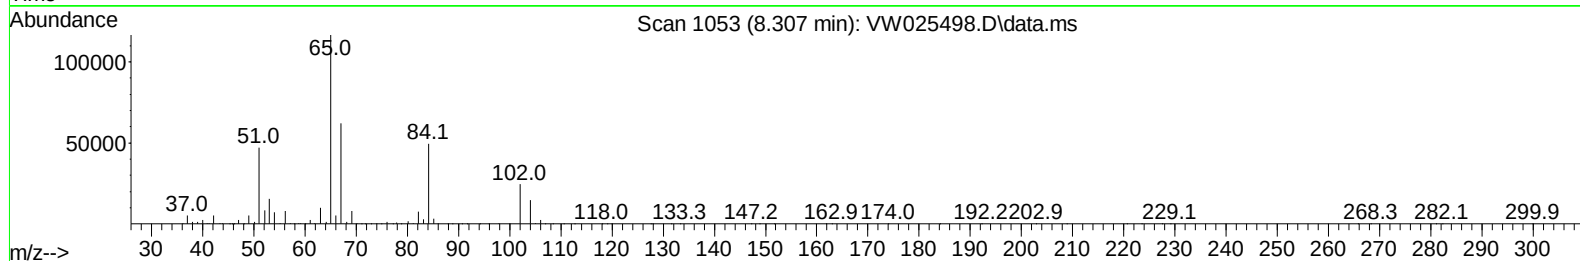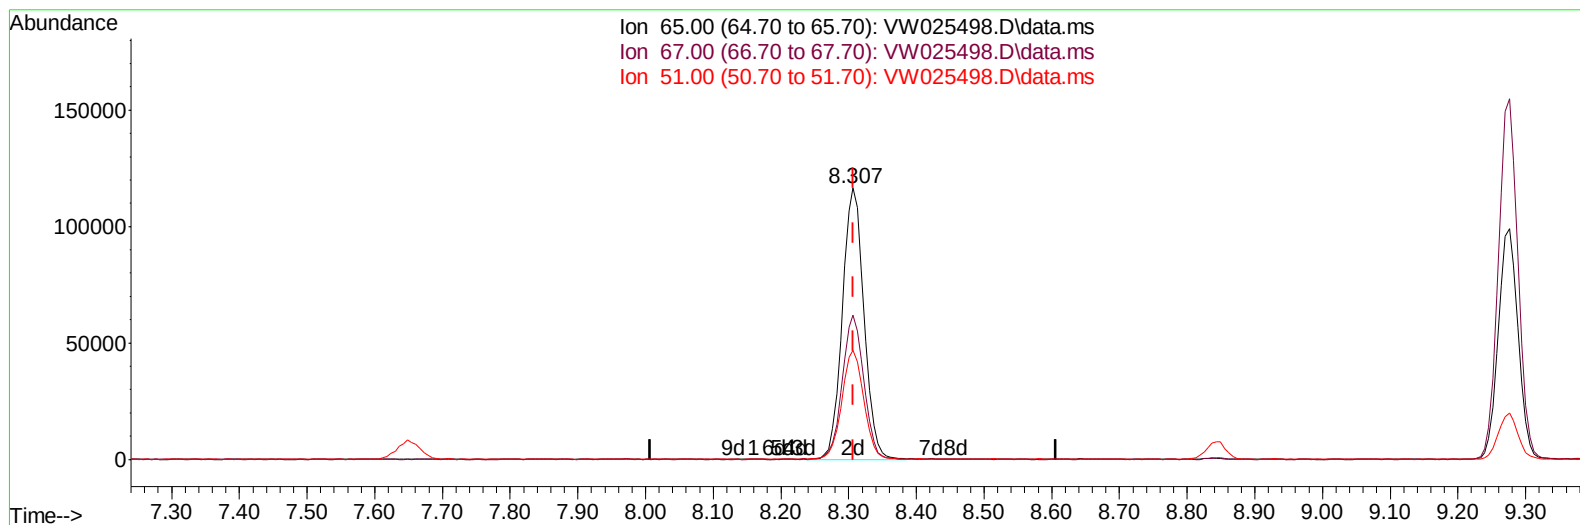

TIC: VW025498.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 24.25 ug/L m

response 257457

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	0.03#
51.00	111.10	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025498.D
 Acq On : 30 Mar 2023 13:02
 Operator : SY/MD
 Sample : VW0330SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK476

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Mar 31 02:22:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	686068	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	621744	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	294095	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	198328	17.386	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	69.560%	
7) Chloroethane-d5	2.899	69	167954	20.462	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	81.840%	
11) 1,1-Dichloroethene-d2	4.027	63	341902	15.518	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.080%	
21) 2-Butanone-d5	7.081	46	133871	47.811	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	95.620%	
24) Chloroform-d	7.648	84	467416	23.633	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	94.520%	
26) 1,2-Dichloroethane-d4	8.307	65	257457m	24.252	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	97.000%	
32) Benzene-d6	8.276	84	947996	22.315	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	89.240%	
36) 1,2-Dichloropropane-d6	9.276	67	310276	23.608	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	94.440%	
41) Toluene-d8	10.325	98	818721	21.858	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	87.440%	
43) trans-1,3-Dichloroprop...	10.581	79	110013	21.021	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	84.080%	
47) 2-Hexanone-d5	10.922	63	82196	43.493	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	86.980%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	219574	22.804	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	91.200%	
66) 1,2-Dichlorobenzene-d4	13.848	152	270104	24.697	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	98.800%	
Target Compounds					Qvalue	
16) Methylene chloride	4.929	84	26302	2.753	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
Data File : VW025498.D
Acq On : 30 Mar 2023 13:02
Operator : SY/MD
Sample : VW0330SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK476

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Mar 31 02:22:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 31 02:21:49 2023
Response via : Initial Calibration

