




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025506.D
 Acq On : 30 Mar 2023 16:36
 Operator : SY/MD
 Sample : 02130-06
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1195

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Mar 31 02:24:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

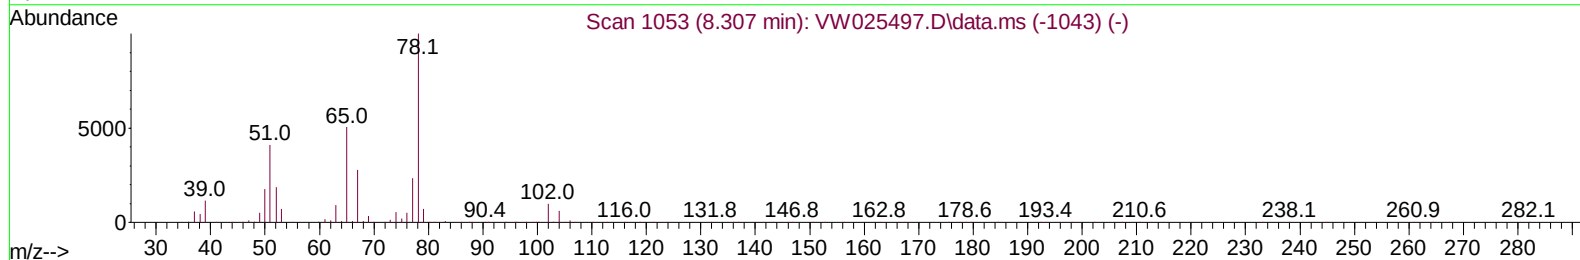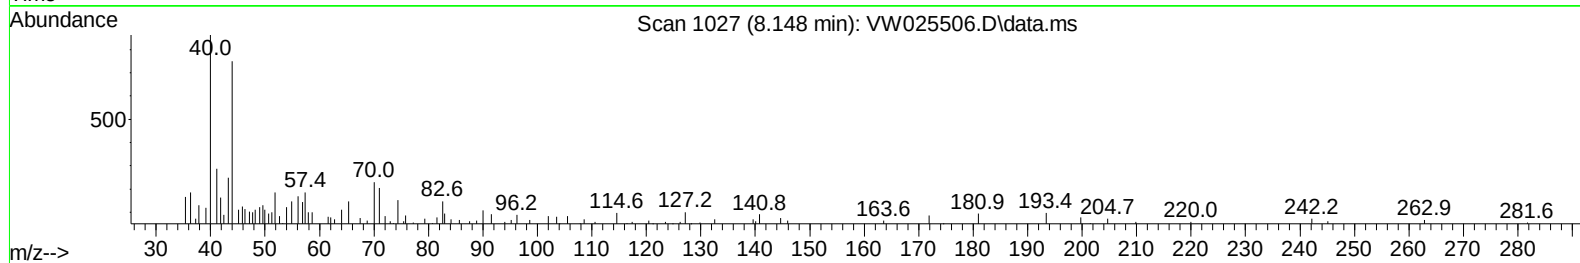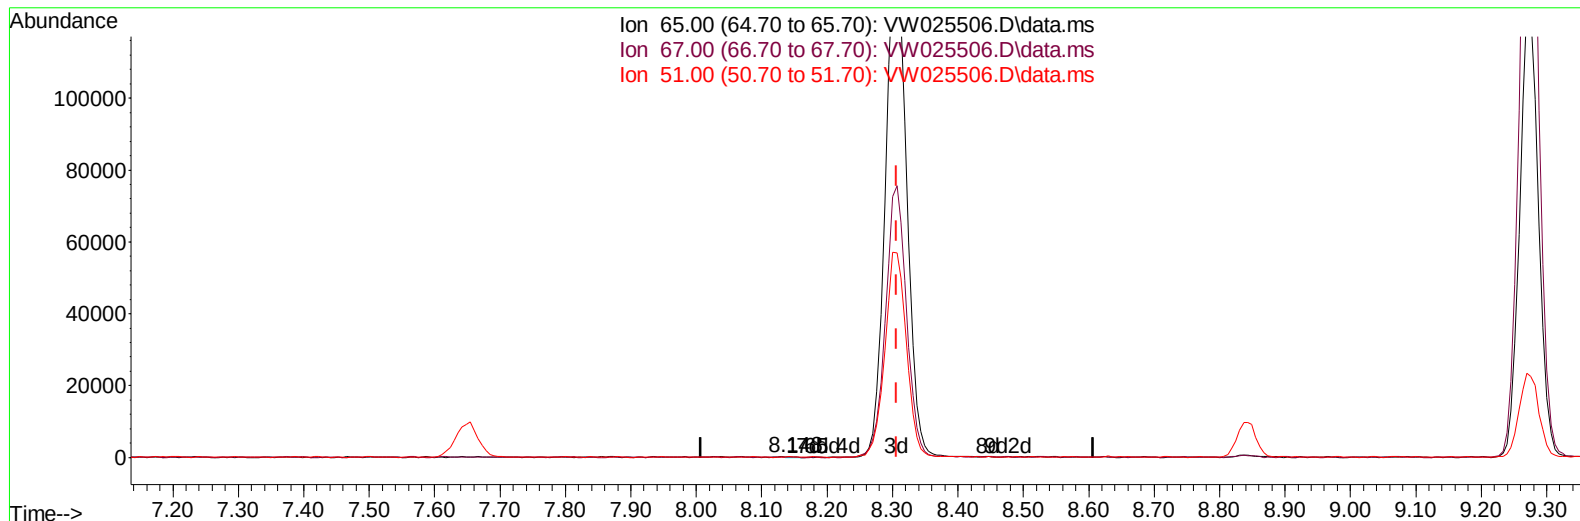

TIC: VW025506.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.148min (-0.159) 0.01 ug/L

response 115

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	47.83
51.00	111.10	136.52
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025506.D
 Acq On : 30 Mar 2023 16:36
 Operator : SY/MD
 Sample : 02130-06
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1195

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:24:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

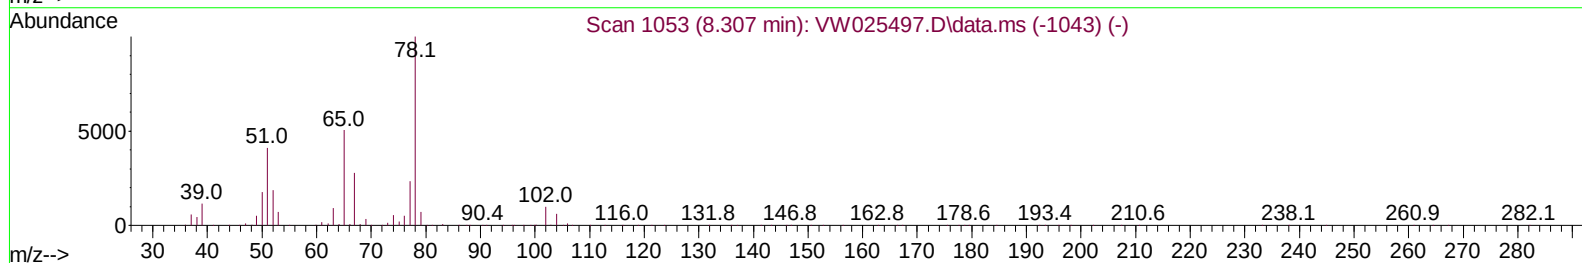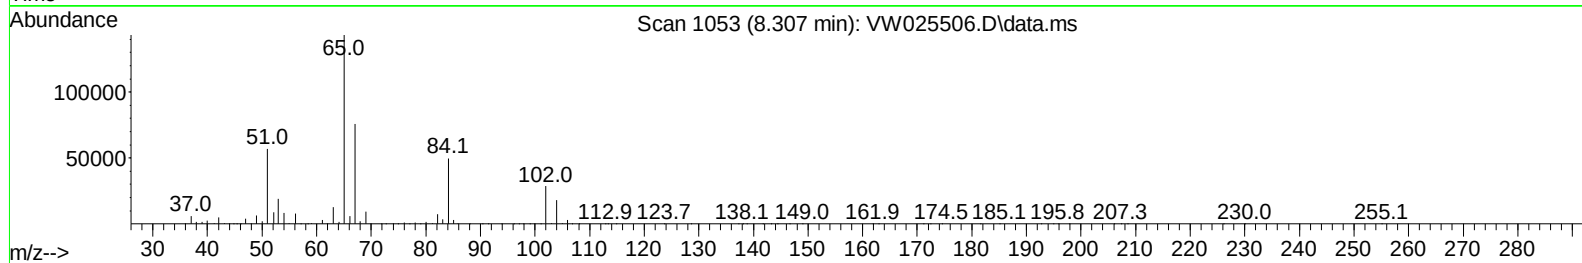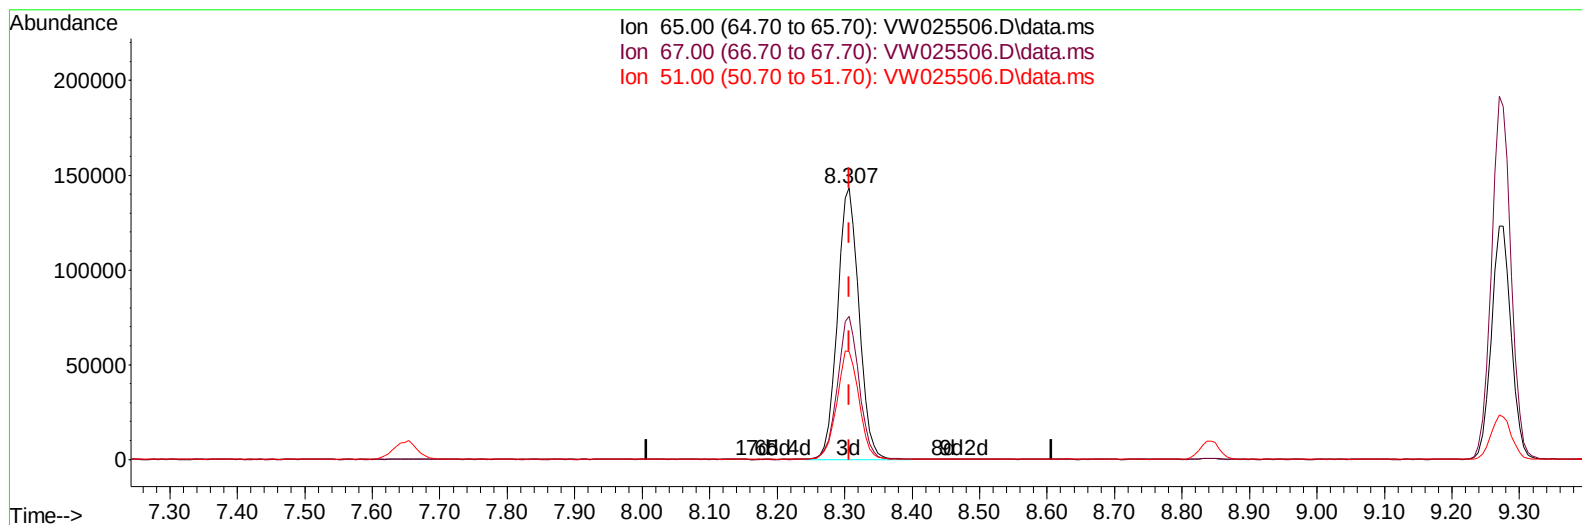

TIC: VW025506.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 22.72 ug/L m

response 318238

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	0.02#
51.00	111.10	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025506.D
 Acq On : 30 Mar 2023 16:36
 Operator : SY/MD
 Sample : 02130-06
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1195

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:24:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	905296	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	756273	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	297187	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	155077	10.303	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	41.200%	
7) Chloroethane-d5	2.899	69	169289	15.630	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	62.520%	
11) 1,1-Dichloroethene-d2	4.021	63	353814	12.170	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	48.680%	
21) 2-Butanone-d5	7.075	46	174867	47.329	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	94.660%	
24) Chloroform-d	7.648	84	577072	22.111	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.440%	
26) 1,2-Dichloroethane-d4	8.307	65	318238m	22.718	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	90.880%	
32) Benzene-d6	8.276	84	1167926	22.601	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	90.400%	
36) 1,2-Dichloropropane-d6	9.270	67	385150	24.092	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	96.360%	
41) Toluene-d8	10.324	98	1006909	22.100	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	88.400%	
43) trans-1,3-Dichloroprop...	10.581	79	125192	19.666	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	78.680%	
47) 2-Hexanone-d5	10.922	63	111338	48.433	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	96.860%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	278316	23.763	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	95.040%	
66) 1,2-Dichlorobenzene-d4	13.848	152	271608	24.576	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	98.320%	
Target Compounds						
					Qvalue	
13) Acetone	4.130	43	21842	6.150	ug/L	68
16) Methylene chloride	4.923	84	31044	2.463	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
Data File : VW025506.D
Acq On : 30 Mar 2023 16:36
Operator : SY/MD
Sample : 02130-06
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C1195

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Mar 31 02:24:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 31 02:21:49 2023
Response via : Initial Calibration

