




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025509.D
 Acq On : 30 Mar 2023 17:48
 Operator : SY/MD
 Sample : 02130-09
 Misc : 5.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1198

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:25:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

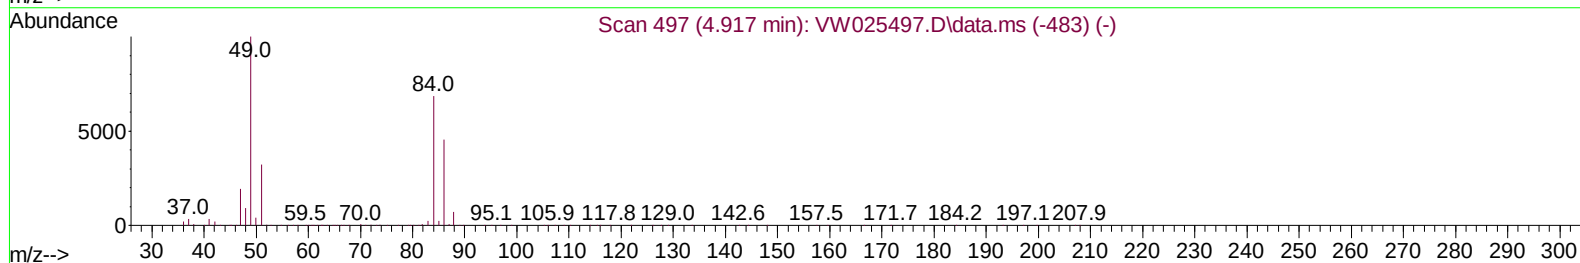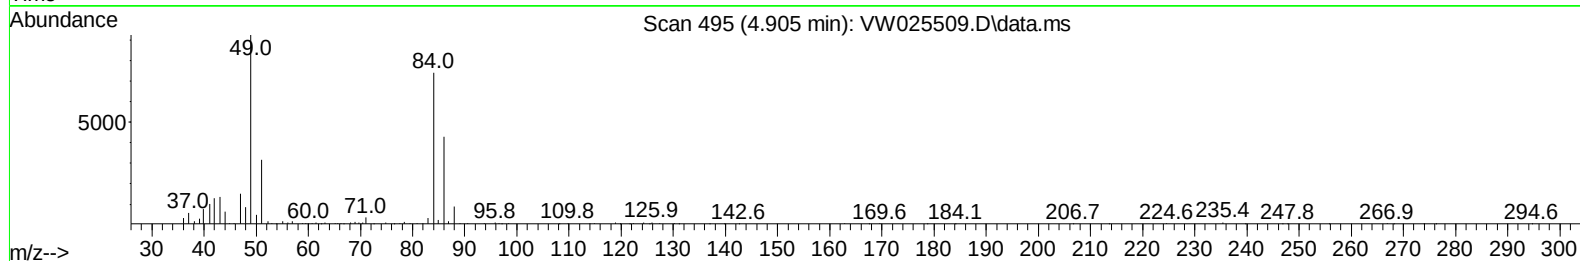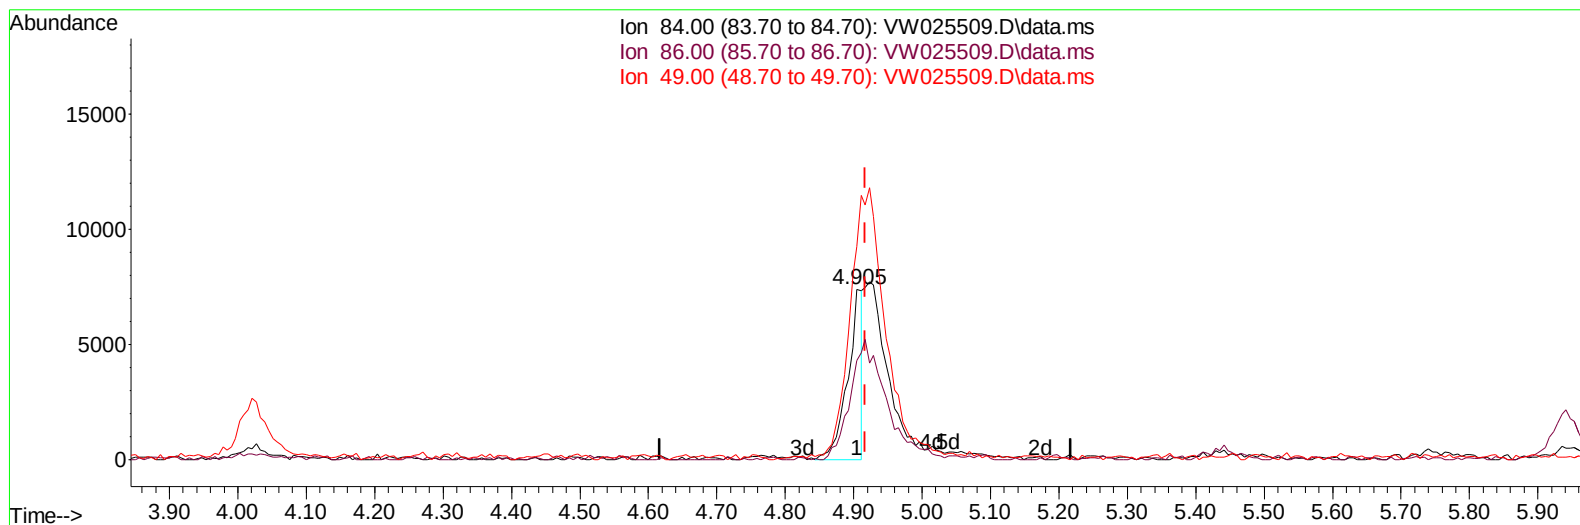

TIC: VW025509.D\data.ms

(16) Methylene chloride (T)

4.905min (-0.012) 1.08 ug/L

response 10991

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.40	58.05
49.00	135.30	125.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025509.D
 Acq On : 30 Mar 2023 17:48
 Operator : SY/MD
 Sample : 02130-09
 Misc : 5.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1198

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:25:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

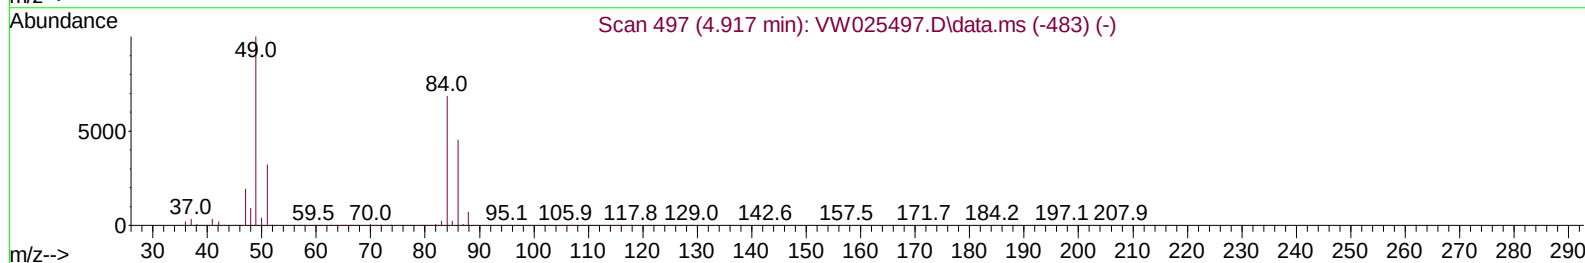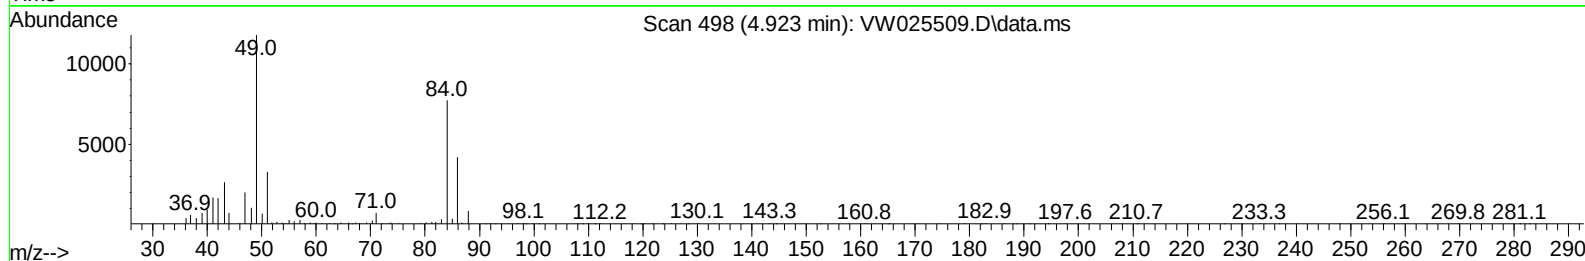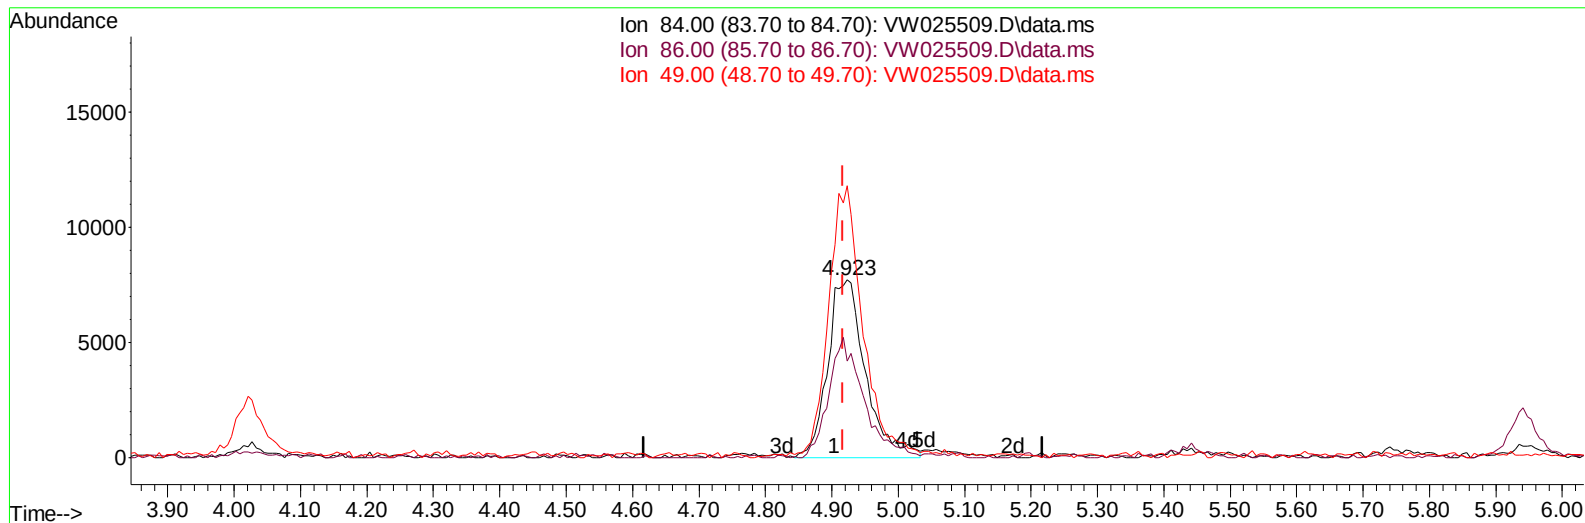

TIC: VW025509.D\data.ms

(16) Methylene chloride (T)

4.923min (+ 0.006) 2.99 ug/L m

response 30341

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.40	54.29
49.00	135.30	152.63
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025509.D
 Acq On : 30 Mar 2023 17:48
 Operator : SY/MD
 Sample : 02130-09
 Misc : 5.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1198

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:25:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

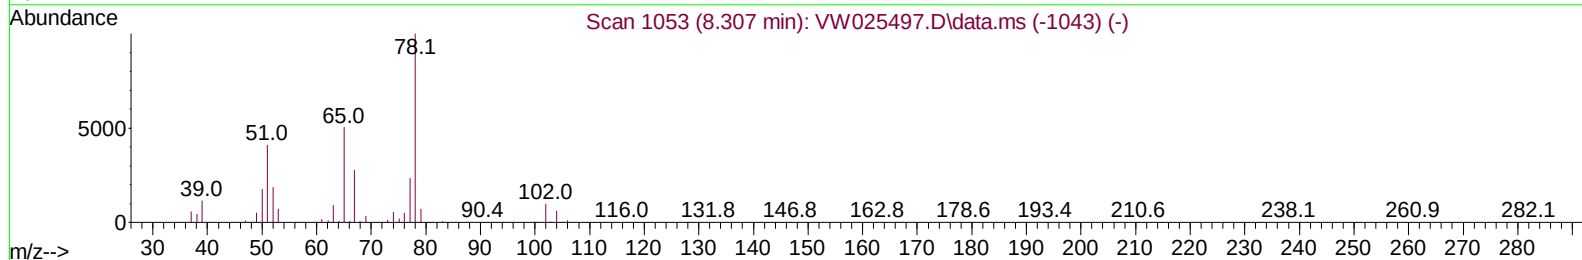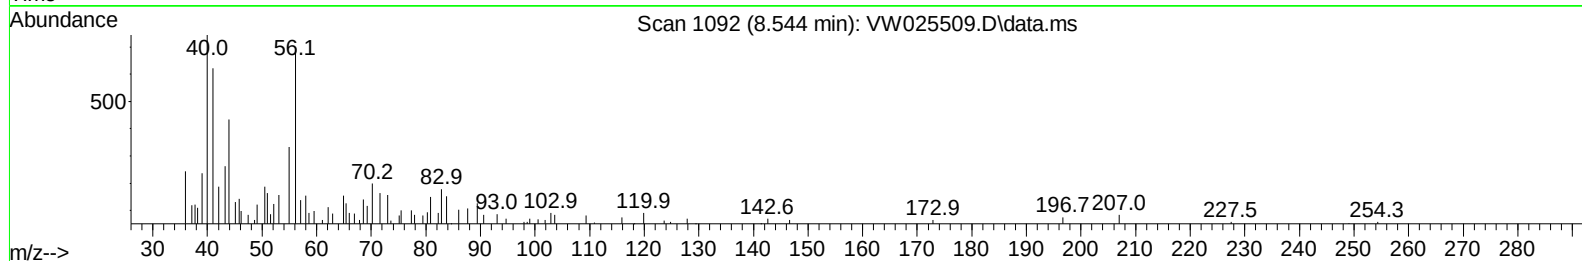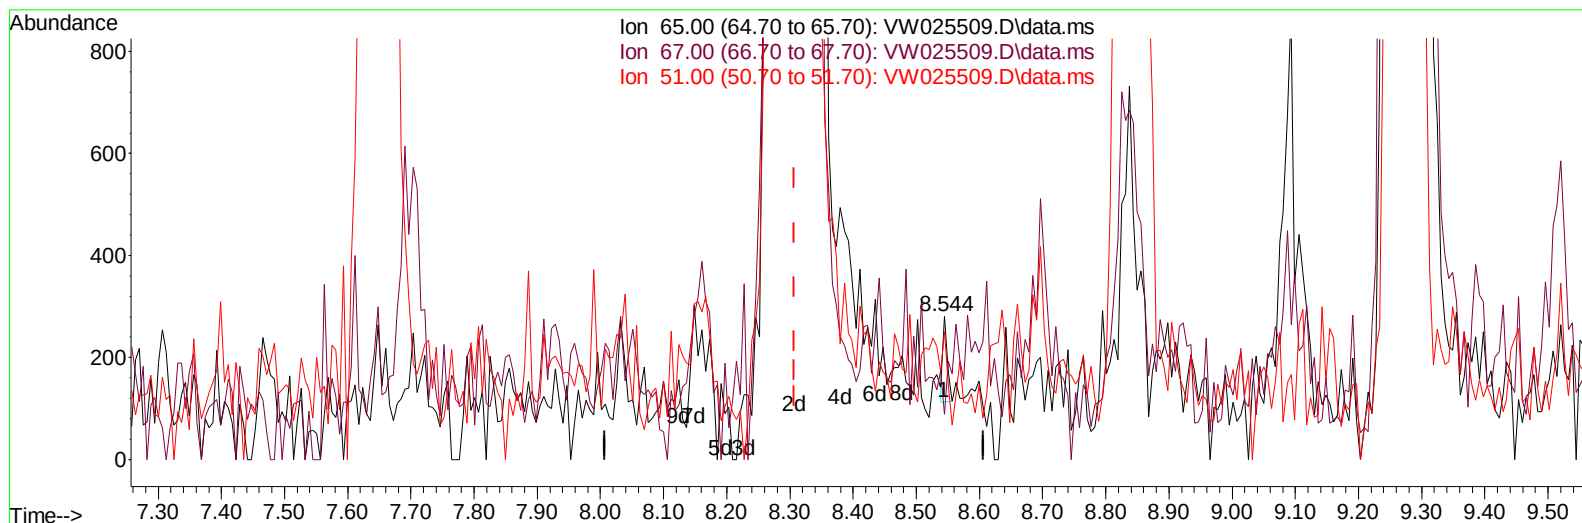

TIC: VW025509.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.544min (+ 0.238) 0.01 ug/L

response 83

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	37.35
51.00	111.10	115.66
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025509.D
 Acq On : 30 Mar 2023 17:48
 Operator : SY/MD
 Sample : 02130-09
 Misc : 5.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1198

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:25:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

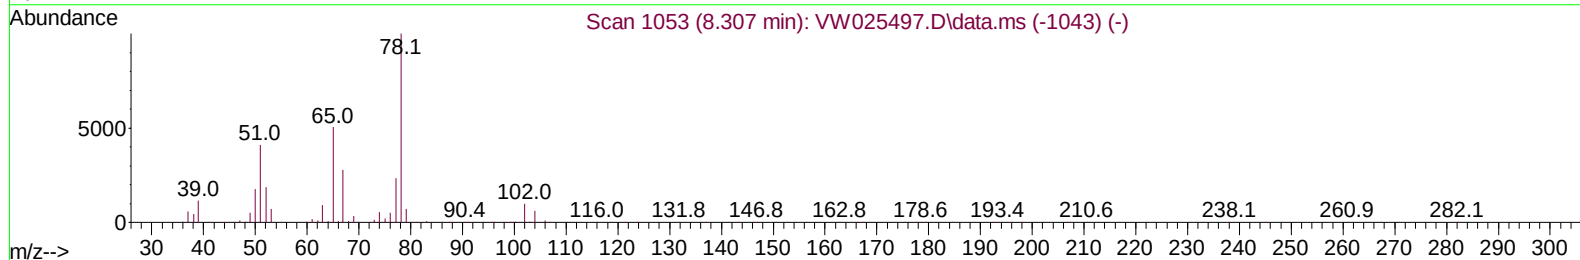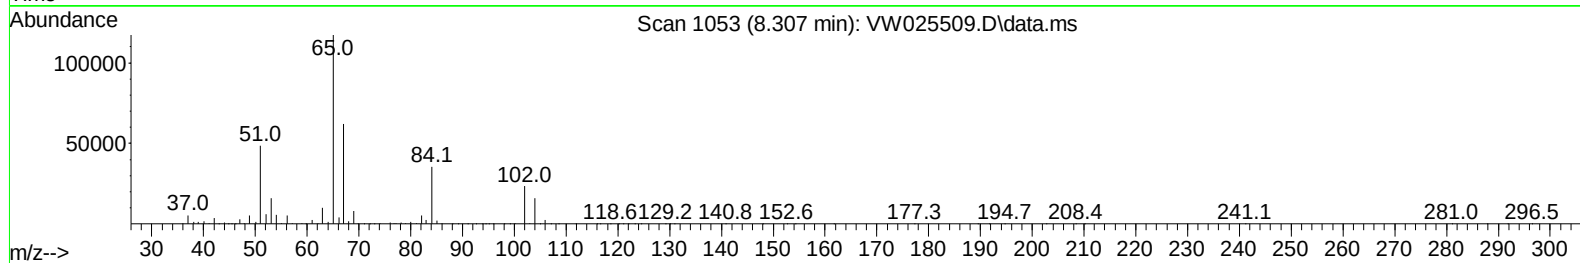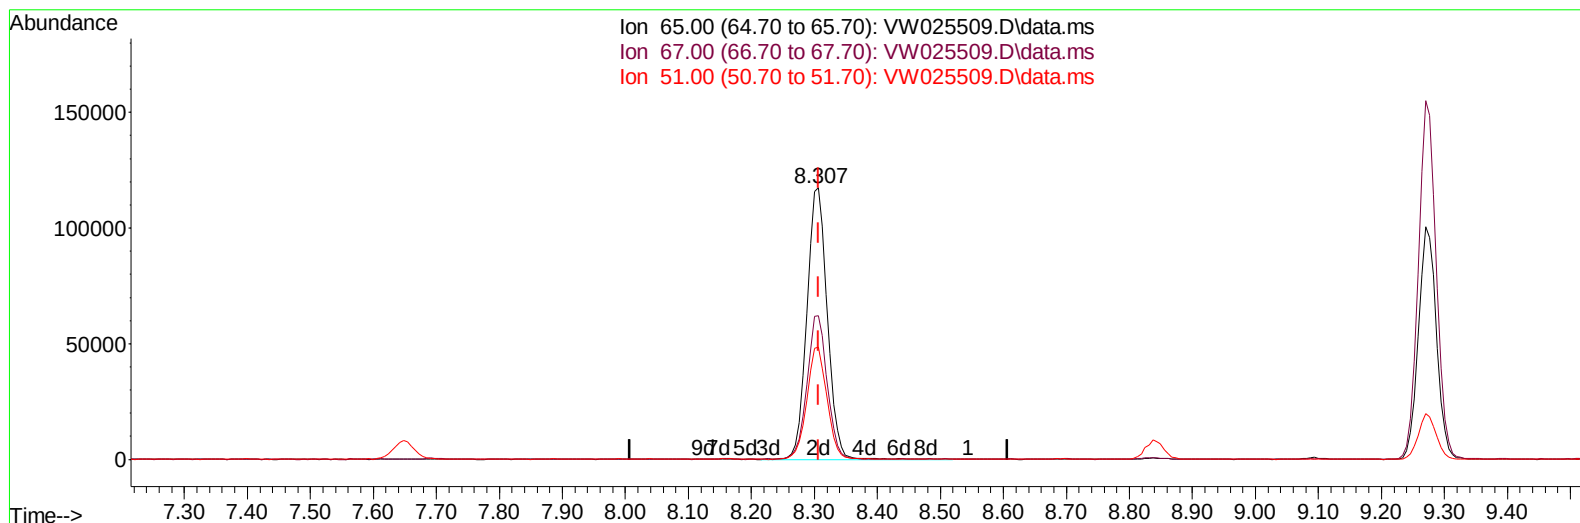

TIC: VW025509.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 23.41 ug/L m

response 264122

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	0.01#
51.00	111.10	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025509.D
 Acq On : 30 Mar 2023 17:48
 Operator : SY/MD
 Sample : 02130-09
 Misc : 5.71g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1198

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:25:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	729295	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	567452	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	184329	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	124050	10.230	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	40.920%	
7) Chloroethane-d5	2.899	69	131422	15.062	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	60.240%	
11) 1,1-Dichloroethene-d2	4.021	63	273721	11.687	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	46.760%	
21) 2-Butanone-d5	7.075	46	160263	53.844	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	107.680%	
24) Chloroform-d	7.648	84	451972	21.497	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	86.000%	
26) 1,2-Dichloroethane-d4	8.307	65	264122m	23.405	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	93.640%	
32) Benzene-d6	8.276	84	894412	23.068	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	92.280%	
36) 1,2-Dichloropropane-d6	9.270	67	305487	25.468	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	101.880%	
41) Toluene-d8	10.325	98	720545	21.077	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	84.320%	
43) trans-1,3-Dichloroprop...	10.575	79	95190	19.929	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	79.720%	
47) 2-Hexanone-d5	10.922	63	103157	59.806	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	119.620%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	237271	27.000	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	108.000%	
66) 1,2-Dichlorobenzene-d4	13.848	152	165796	24.187	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	96.760%	
Target Compounds						
					Qvalue	
13) Acetone	4.124	43	21077	7.366	ug/L	99
16) Methylene chloride	4.923	84	30341m	2.988	ug/L	
20) cis-1,2-Dichloroethene	7.173	96	15041	1.441	ug/L #	95
34) Trichloroethene	9.093	95	54596	5.734	ug/L	97
46) Tetrachloroethene	10.861	164	1045123	154.255	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
Data File : VW025509.D
Acq On : 30 Mar 2023 17:48
Operator : SY/MD
Sample : 02130-09
Misc : 5.71g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C1198

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Mar 31 02:25:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 31 02:21:49 2023
Response via : Initial Calibration

