




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025512.D
 Acq On : 30 Mar 2023 18:59
 Operator : SY/MD
 Sample : 02130-14
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11A3

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:25:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

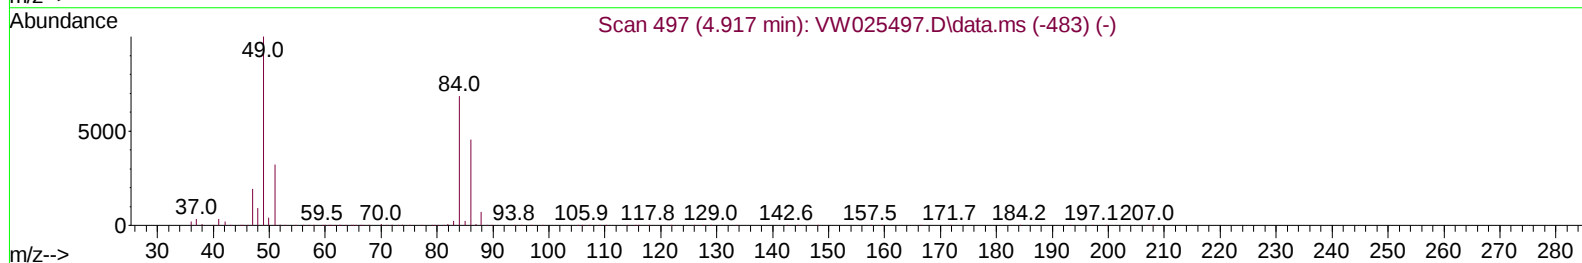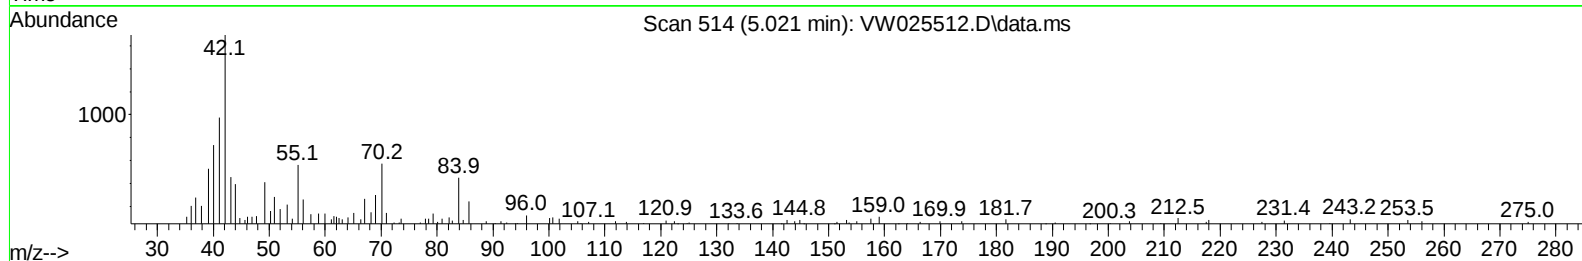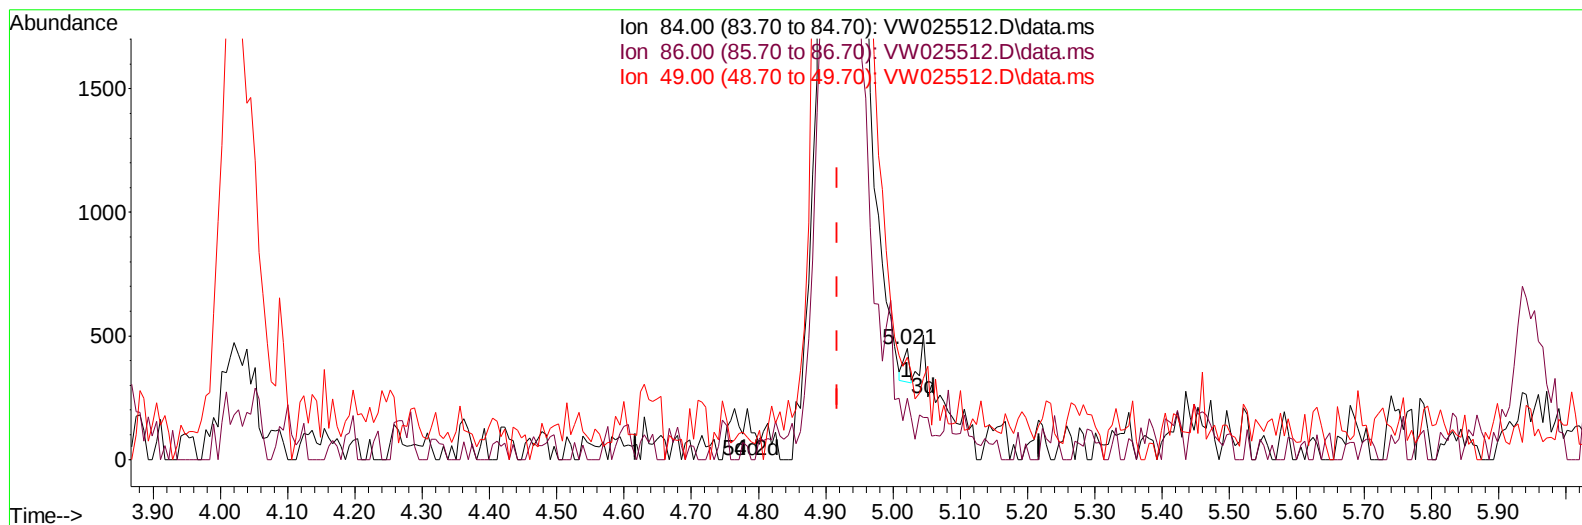

TIC: VW025512.D\data.ms

(16) Methylene chloride (T)

5.021min (+ 0.103) 0.01 ug/L

response 80

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.40	46.17
49.00	135.30	77.20#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025512.D
 Acq On : 30 Mar 2023 18:59
 Operator : SY/MD
 Sample : 02130-14
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11A3

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:25:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

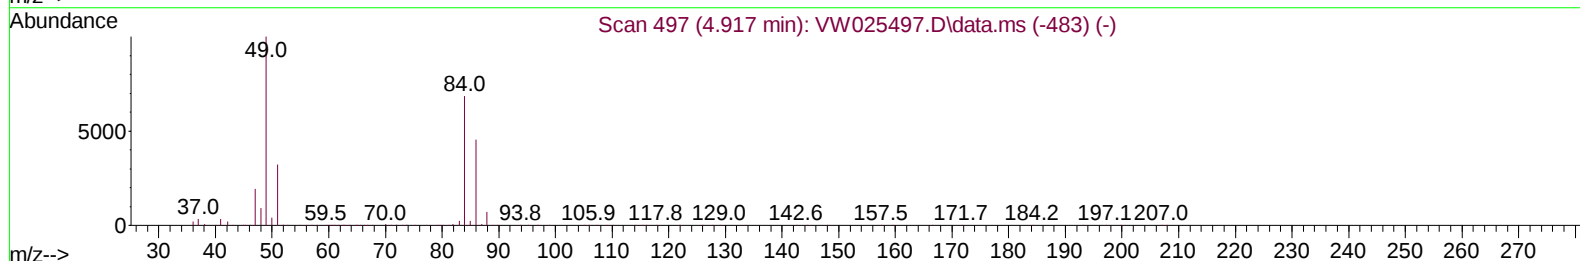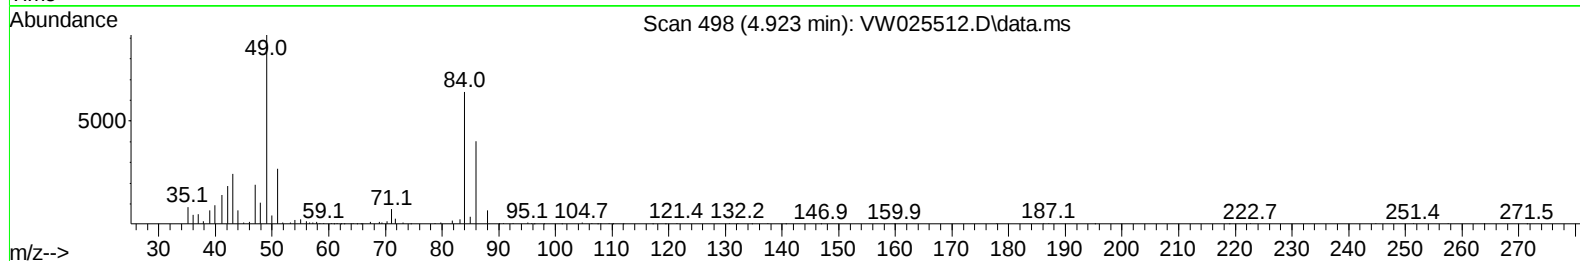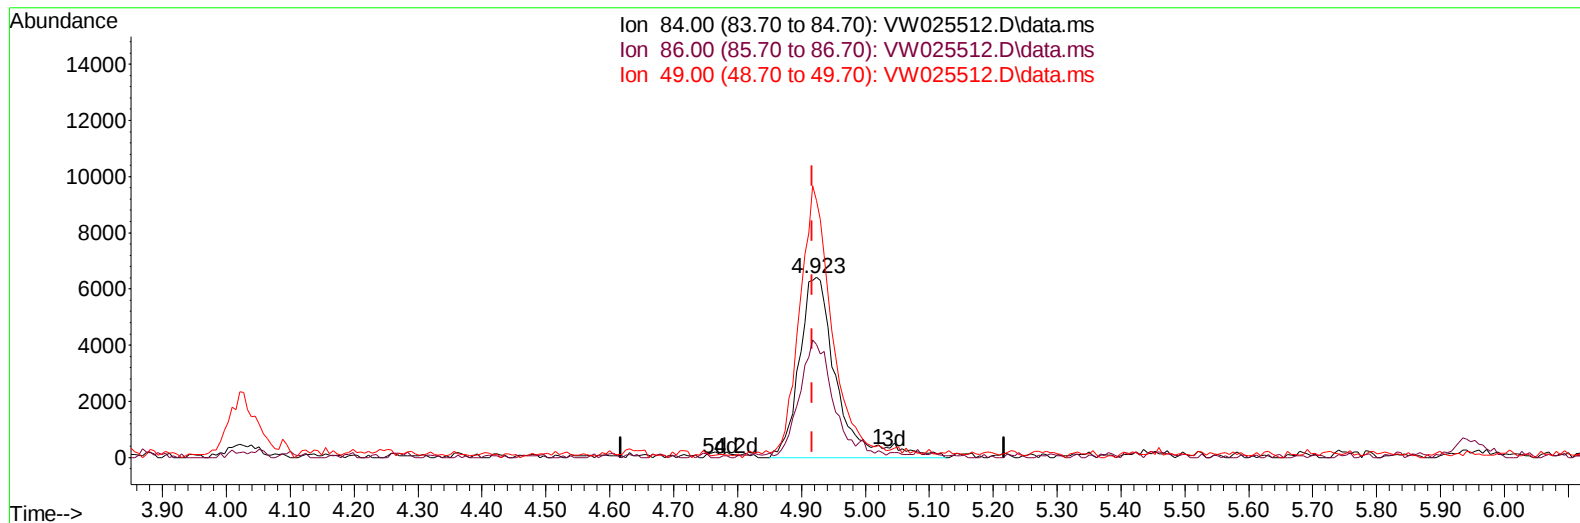

TIC: VW025512.D\data.ms

(16) Methylene chloride (T)

4.923min (+ 0.006) 3.46 ug/L m

response 25991

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.40	62.75
49.00	135.30	142.70
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025512.D
 Acq On : 30 Mar 2023 18:59
 Operator : SY/MD
 Sample : 02130-14
 Misc : 6.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11A3

Manual IntegrationsAPPROVED

Quant Time: Mar 31 02:25:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		540043	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		279431	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		38396	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		118585	13.207	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	52.840%		
7) Chloroethane-d5	2.899	69		144400	22.350	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	89.400%		
11) 1,1-Dichloroethene-d2	4.021	63		261211	15.061	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	60.240%		
21) 2-Butanone-d5	7.081	46		185438	84.135	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	168.280%#		
24) Chloroform-d	7.648	84		504172	32.384	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	129.520%		
26) 1,2-Dichloroethane-d4	8.307	65		235264	28.154	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	112.600%		
32) Benzene-d6	8.276	84		930585	48.739	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	194.960%#		
36) 1,2-Dichloropropane-d6	9.270	67		343834	58.210	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	232.840%#		
41) Toluene-d8	10.325	98		615358	36.554	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	146.200%#		
43) trans-1,3-Dichloroprop...	10.581	79		39629	16.849	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	67.400%		
47) 2-Hexanone-d5	10.922	63		74885	88.165	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	176.340%#		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		225783	52.175	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	208.720%#		
66) 1,2-Dichlorobenzene-d4	13.848	152		64083	44.881	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	179.520%#		
Target Compounds							
13) Acetone	4.124	43		53013	25.021	ug/L	98
16) Methylene chloride	4.923	84		25991m	3.456	ug/L	
22) 2-Butanone	7.179	43		16448	6.001	ug/L	92
46) Tetrachloroethene	10.861	164		5310	1.592	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
Data File : VW025512.D
Acq On : 30 Mar 2023 18:59
Operator : SY/MD
Sample : 02130-14
Misc : 6.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C11A3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Mar 31 02:25:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 31 02:21:49 2023
Response via : Initial Calibration

