

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
 Data File : VW025499.D
 Acq On : 30 Mar 2023 13:30
 Operator : SY/MD
 Sample : 02121-07
 Misc : 5.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C1180

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Mar 31 02:22:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Mar 31 02:21:49 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	668864	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	515372	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	160796	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	132437	11.909	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	47.640%		
7) Chloroethane-d5	2.899	69	135422	16.923	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	67.680%		
11) 1,1-Dichloroethene-d2	4.021	63	278937	12.986	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	51.960%		
21) 2-Butanone-d5	7.081	46	154214	56.493	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	112.980%		
24) Chloroform-d	7.648	84	426325	22.110	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.440%		
26) 1,2-Dichloroethane-d4	8.307	65	242911m	23.471	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	93.880%		
32) Benzene-d6	8.276	84	868059	24.650	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	98.600%		
36) 1,2-Dichloropropane-d6	9.276	67	294199	27.005	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	108.040%		
41) Toluene-d8	10.325	98	692732	22.311	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	89.240%		
43) trans-1,3-Dichloroprop...	10.575	79	89924	20.729	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.920%		
47) 2-Hexanone-d5	10.922	63	88972	56.795	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	113.600%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	209871	26.295	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	105.200%		
66) 1,2-Dichlorobenzene-d4	13.854	152	152659	25.530	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	102.120%		
Target Compounds						
5) Vinyl chloride	2.375	62	844024	82.177	ug/L	96
13) Acetone	4.124	43	253172	96.477	ug/L	99
16) Methylene chloride	4.923	84	19195	2.061	ug/L	96
17) trans-1,2-Dichloroethene	5.429	96	320321	36.635	ug/L	94
20) cis-1,2-Dichloroethene	7.167	96	19385077	2024.924	ug/L #	86
42) Toluene	10.386	91	39525	1.162	ug/L	99
53) m,p-Xylene	11.837	106	10695	0.747	ug/L	99
54) o-Xylene	12.166	106	16691	1.239	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033023\
Data File : VW025499.D
Acq On : 30 Mar 2023 13:30
Operator : SY/MD
Sample : 02121-07
Misc : 5.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C1180

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Mar 31 02:22:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Mar 31 02:21:49 2023
Response via : Initial Calibration

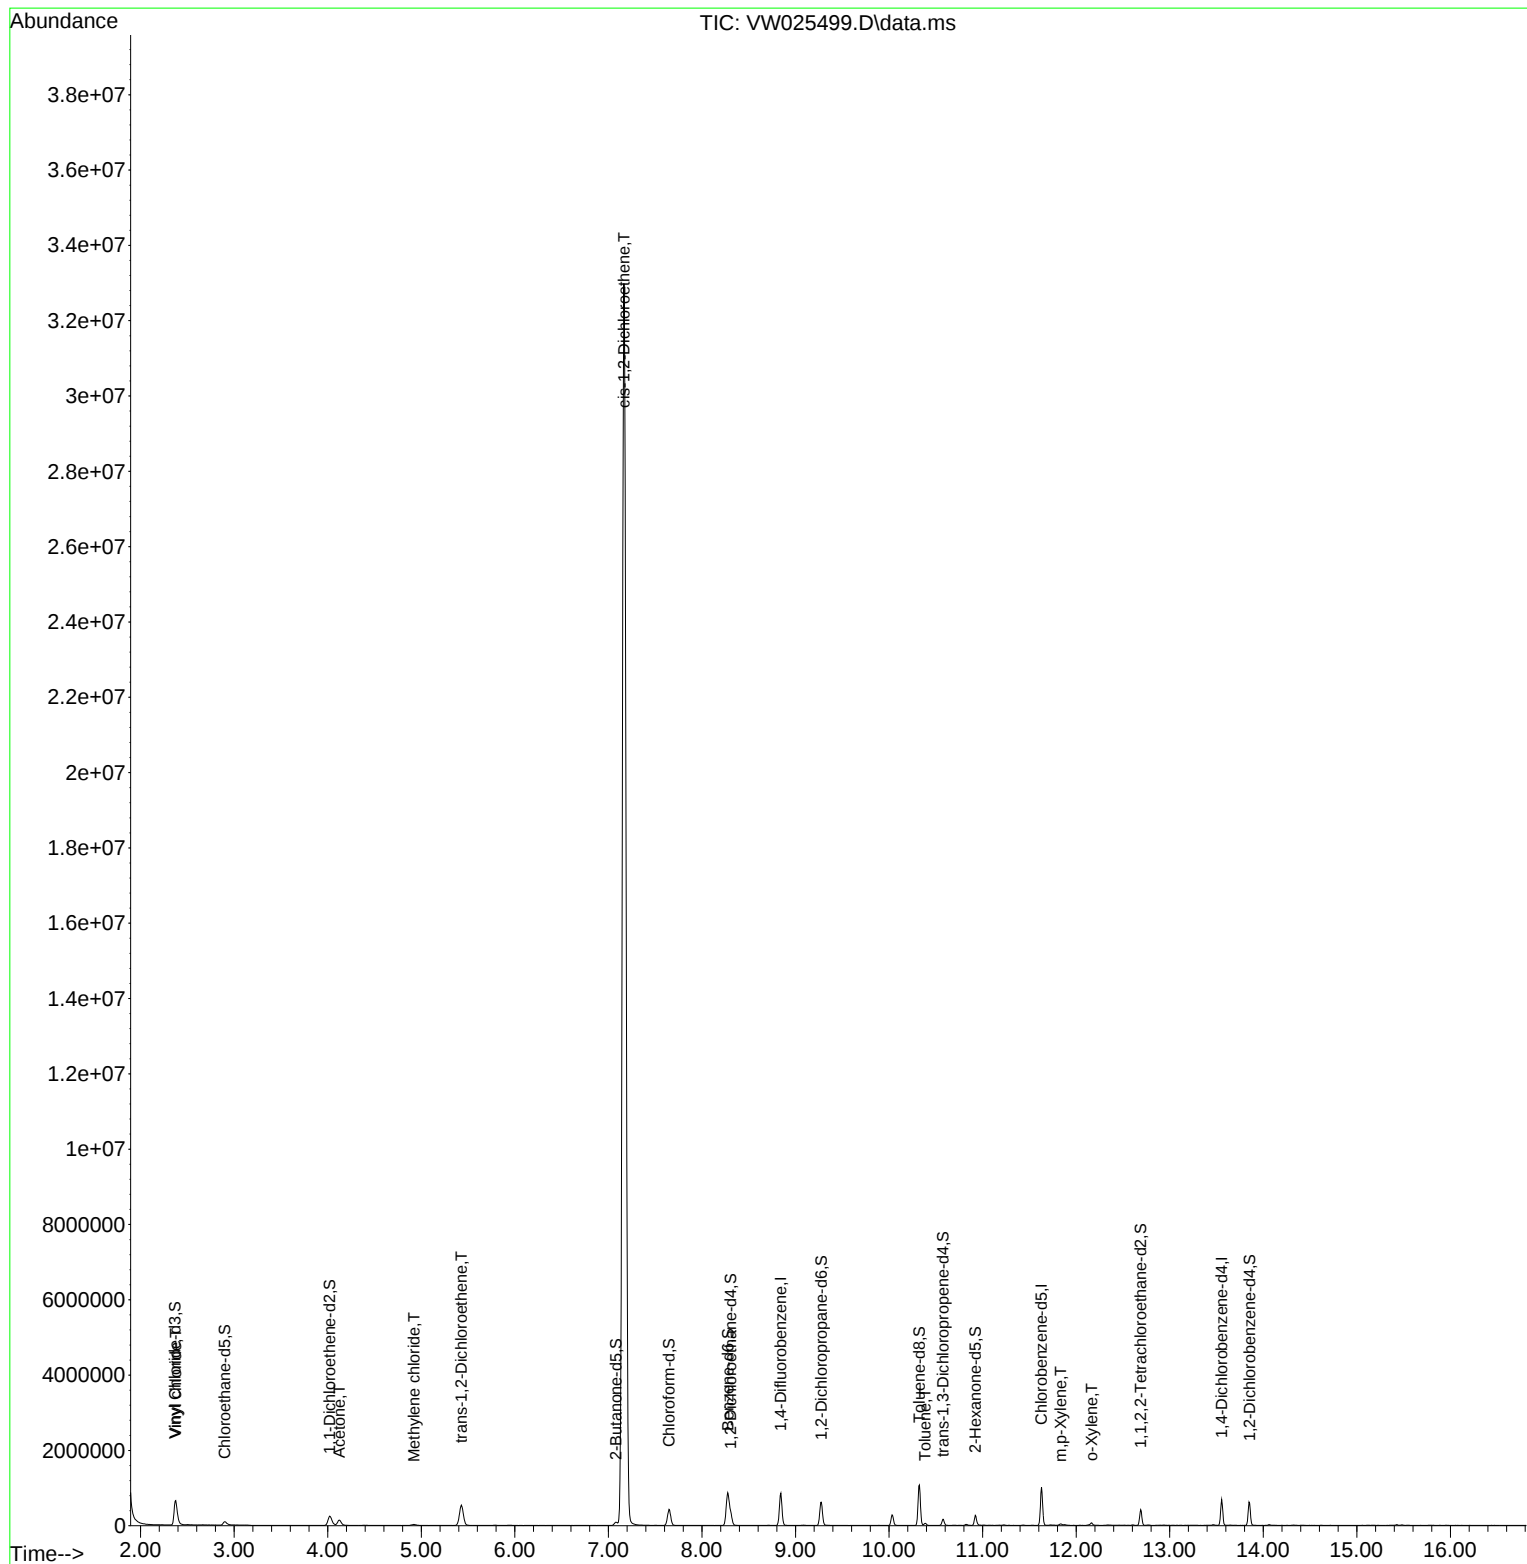

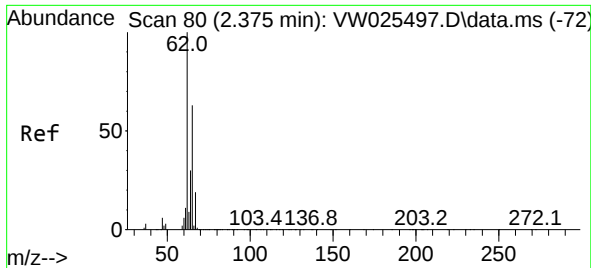





#5
 Vinyl chloride
 Concen: 82.177 ug/L
 RT: 2.375 min Scan# 80
 Delta R.T. -0.000 min
 Lab File: VW025499.D
 Acq: 30 Mar 2023 13:30

Instrument :
 MSVOA_W
 Client Sample Id :
 C1180

Tgt Ion: 62 Resp: 844024
 Ion Ratio Lower Upper
 62 100
 64 31.1 23.4 43.6




Manual Integrations
 APPROVED


Reviewed By :Semsettin Yesilyurt 03/31/2023
 Supervised By :Mahesh Dadoda 04/03/2023

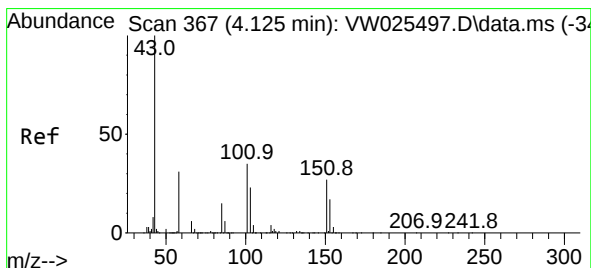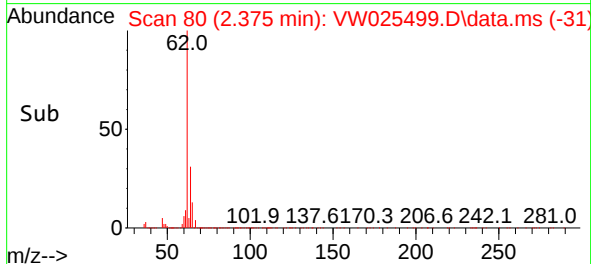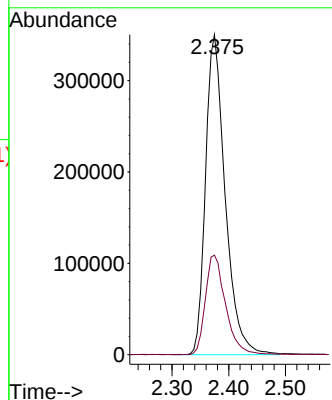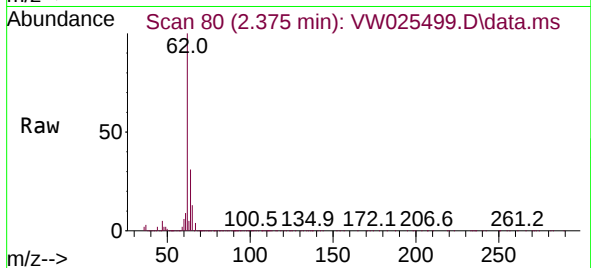

#13
 Acetone
 Concen: 96.477 ug/L
 RT: 4.124 min Scan# 367
 Delta R.T. -0.000 min
 Lab File: VW025499.D
 Acq: 30 Mar 2023 13:30

Tgt Ion: 43 Resp: 253172
 Ion Ratio Lower Upper
 43 100
 58 29.3 0.0 60.0

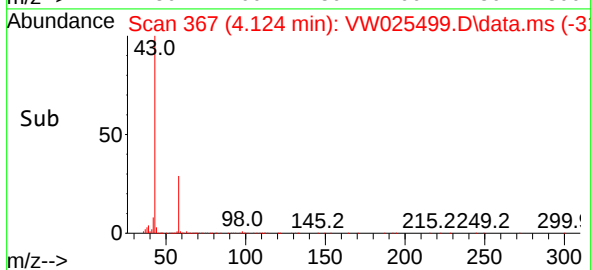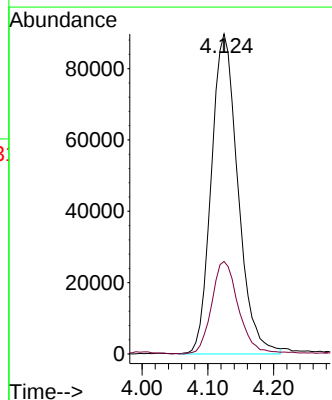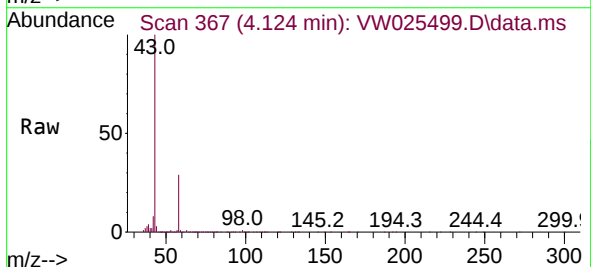

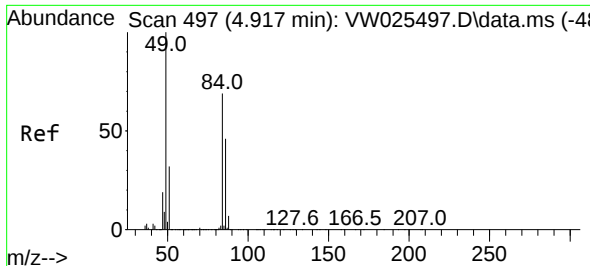





#16
Methylene chloride
Concen: 2.061 ug/L
RT: 4.923 min Scan# 497
Delta R.T. 0.006 min
Lab File: VW025499.D
Acq: 30 Mar 2023 13:30

Instrument :
MSVOA_W
ClientSampleId :
C1180

Tgt Ion: 84 Resp: 1919
Ion Ratio Lower Upper
84 100
86 62.4 45.1 83.7
49 140.3 94.7 175.9




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 03/31/2023
Supervised By :Mahesh Dadoda 04/03/2023

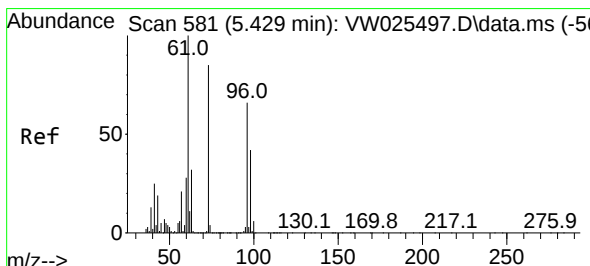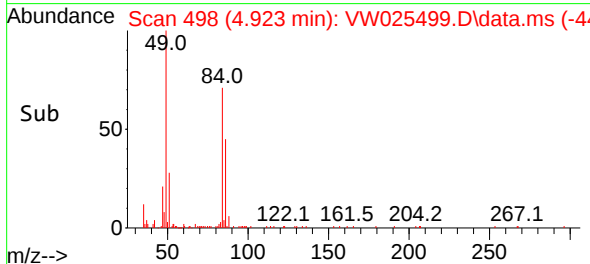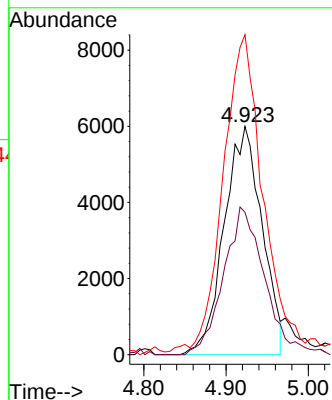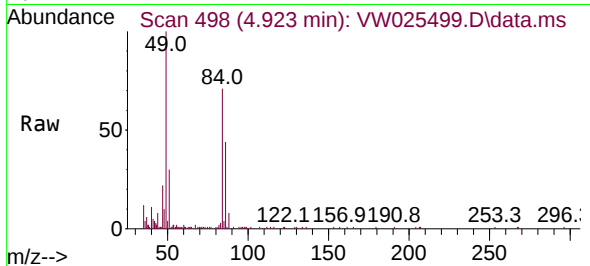

#17
trans-1,2-Dichloroethene
Concen: 36.635 ug/L
RT: 5.429 min Scan# 581
Delta R.T. -0.000 min
Lab File: VW025499.D
Acq: 30 Mar 2023 13:30


Tgt Ion: 96 Resp: 320321
Ion Ratio Lower Upper
96 100
61 155.1 103.0 191.4
98 65.4 43.4 80.6

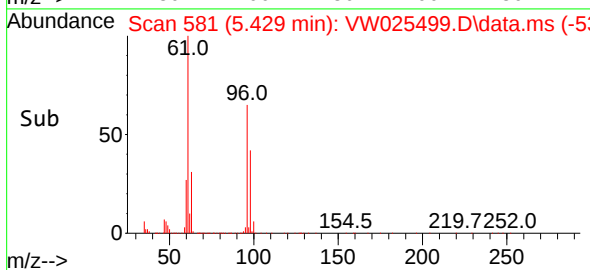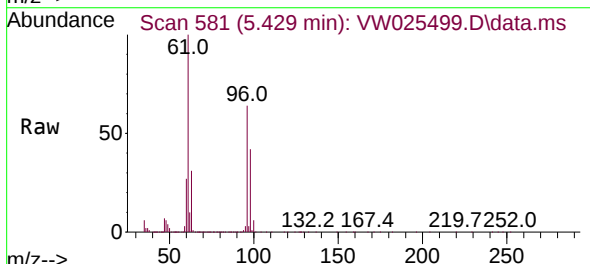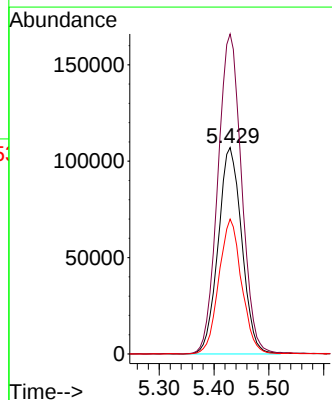

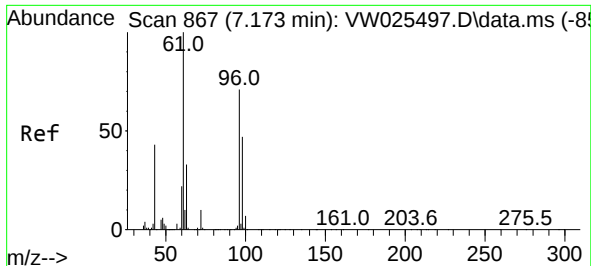

#20
cis-1,2-Dichloroethene
Concen: 2024.924 ug/L
RT: 7.167 min Scan# 867
Delta R.T. -0.006 min
Lab File: VW025499.D
Acq: 30 Mar 2023 13:30




Instrument :
MSVOA_W
ClientSampleId :
C1180

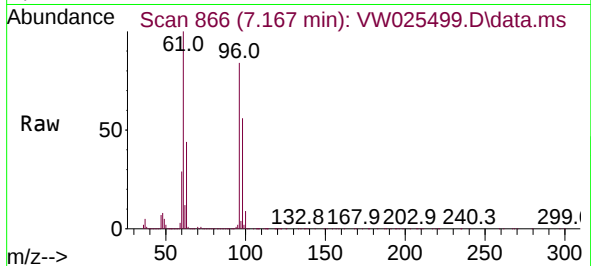


Tgt Ion: 96 Resp:1938507
Ion Ratio Lower Upper
96 100
61 119.5 95.5 177.4
68 0.0 0.1 0.1

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 03/31/2023
Supervised By :Mahesh Dadoda 04/03/2023

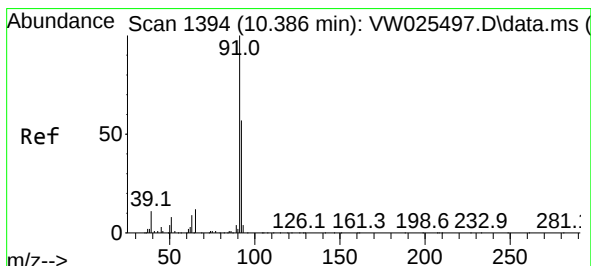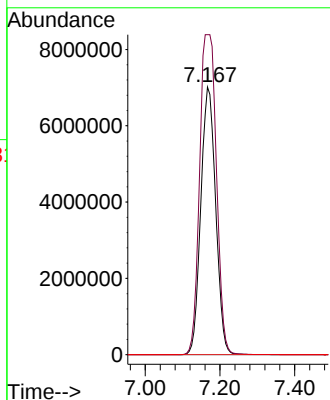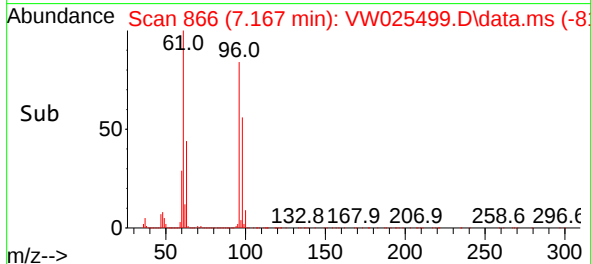


#42
Toluene
Concen: 1.162 ug/L
RT: 10.386 min Scan# 1394
Delta R.T. -0.000 min
Lab File: VW025499.D
Acq: 30 Mar 2023 13:30

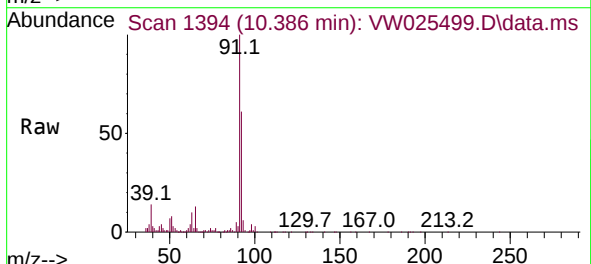


Tgt Ion: 91 Resp: 39525
Ion Ratio Lower Upper
91 100
92 60.6 41.6 77.3

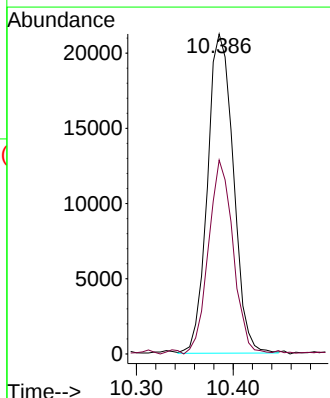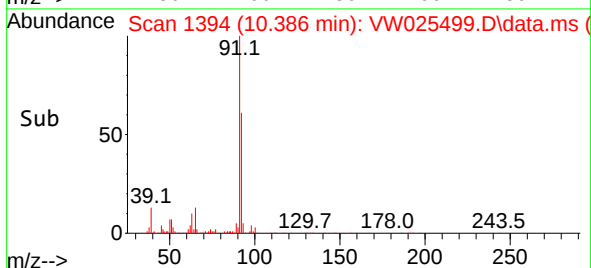

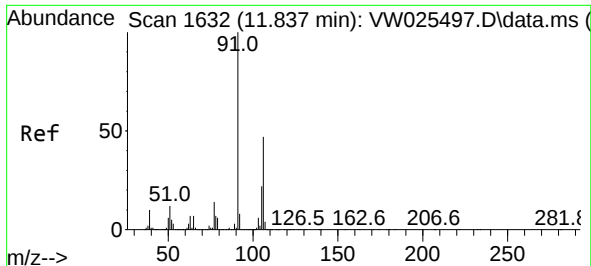

#53
m,p-Xylene
Concen: 0.747 ug/L
RT: 11.837 min Scan# 1632
Delta R.T. -0.000 min
Lab File: VW025499.D
Acq: 30 Mar 2023 13:30




Instrument :
MSVOA_W
ClientSampleId :
C1180

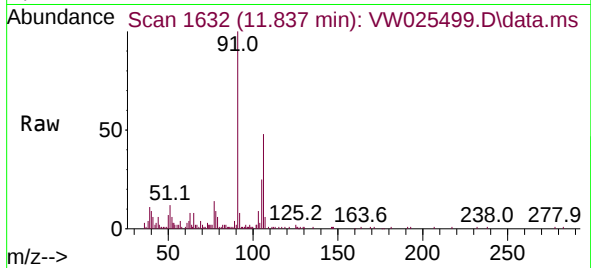


Tgt Ion:106 Resp: 1069
Ion Ratio Lower Upper
106 100
91 208.1 144.2 267.8

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 03/31/2023
Supervised By :Mahesh Dadoda 04/03/2023

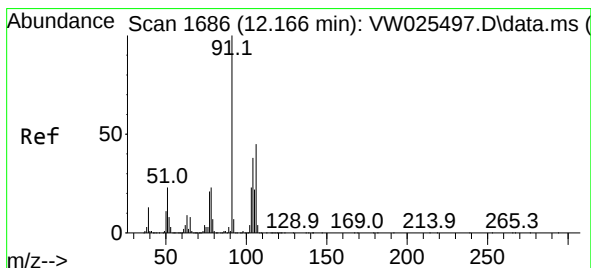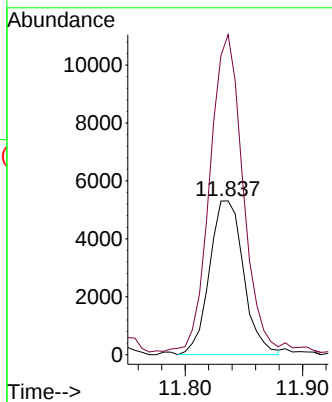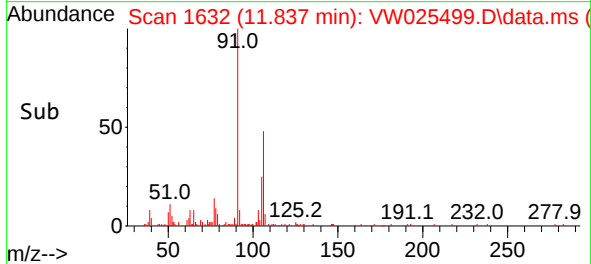

#54
o-Xylene
Concen: 1.239 ug/L
RT: 12.166 min Scan# 1686
Delta R.T. -0.000 min
Lab File: VW025499.D
Acq: 30 Mar 2023 13:30

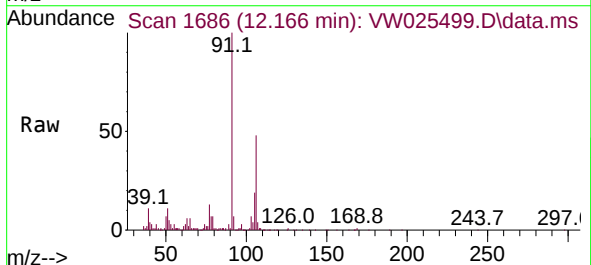

Tgt Ion:106 Resp: 16691
Ion Ratio Lower Upper
106 100
91 210.5 154.6 287.2

