

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033123\
 Data File : VW025531.D
 Acq On : 31 Mar 2023 14:37
 Operator : SY/MD
 Sample : 02151-02
 Misc : 4.38g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 01 00:38:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 01 00:35:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	933366	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	842859	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	388649	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	149036	9.603	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	38.400%
7) Chloroethane-d5	2.899	69	157012	14.061	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.240%
11) 1,1-Dichloroethene-d2	4.021	63	339704	11.333	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	45.320%
21) 2-Butanone-d5	7.075	46	188289	49.429	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.860%
24) Chloroform-d	7.648	84	522569	19.421	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	77.680%
26) 1,2-Dichloroethane-d4	8.307	65	304706	21.098	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.400%
32) Benzene-d6	8.276	84	1075054	18.667	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.680%
36) 1,2-Dichloropropane-d6	9.276	67	355140	19.933	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.720%
41) Toluene-d8	10.325	98	949413	18.697	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.800%
43) trans-1,3-Dichloroprop...	10.575	79	134904	19.015	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	76.080%
47) 2-Hexanone-d5	10.922	63	120462	47.019	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.040%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	285401	21.865	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.440%
66) 1,2-Dichlorobenzene-d4	13.848	152	313686	21.704	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	86.800%
Target Compounds					Qvalue	
48) 2-Hexanone	10.922	43	16356	2.550	ug/L	# 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033123\
Data File : VW025531.D
Acq On : 31 Mar 2023 14:37
Operator : SY/MD
Sample : 02151-02
Misc : 4.38g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Apr 01 00:38:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 01 00:35:04 2023
Response via : Initial Calibration

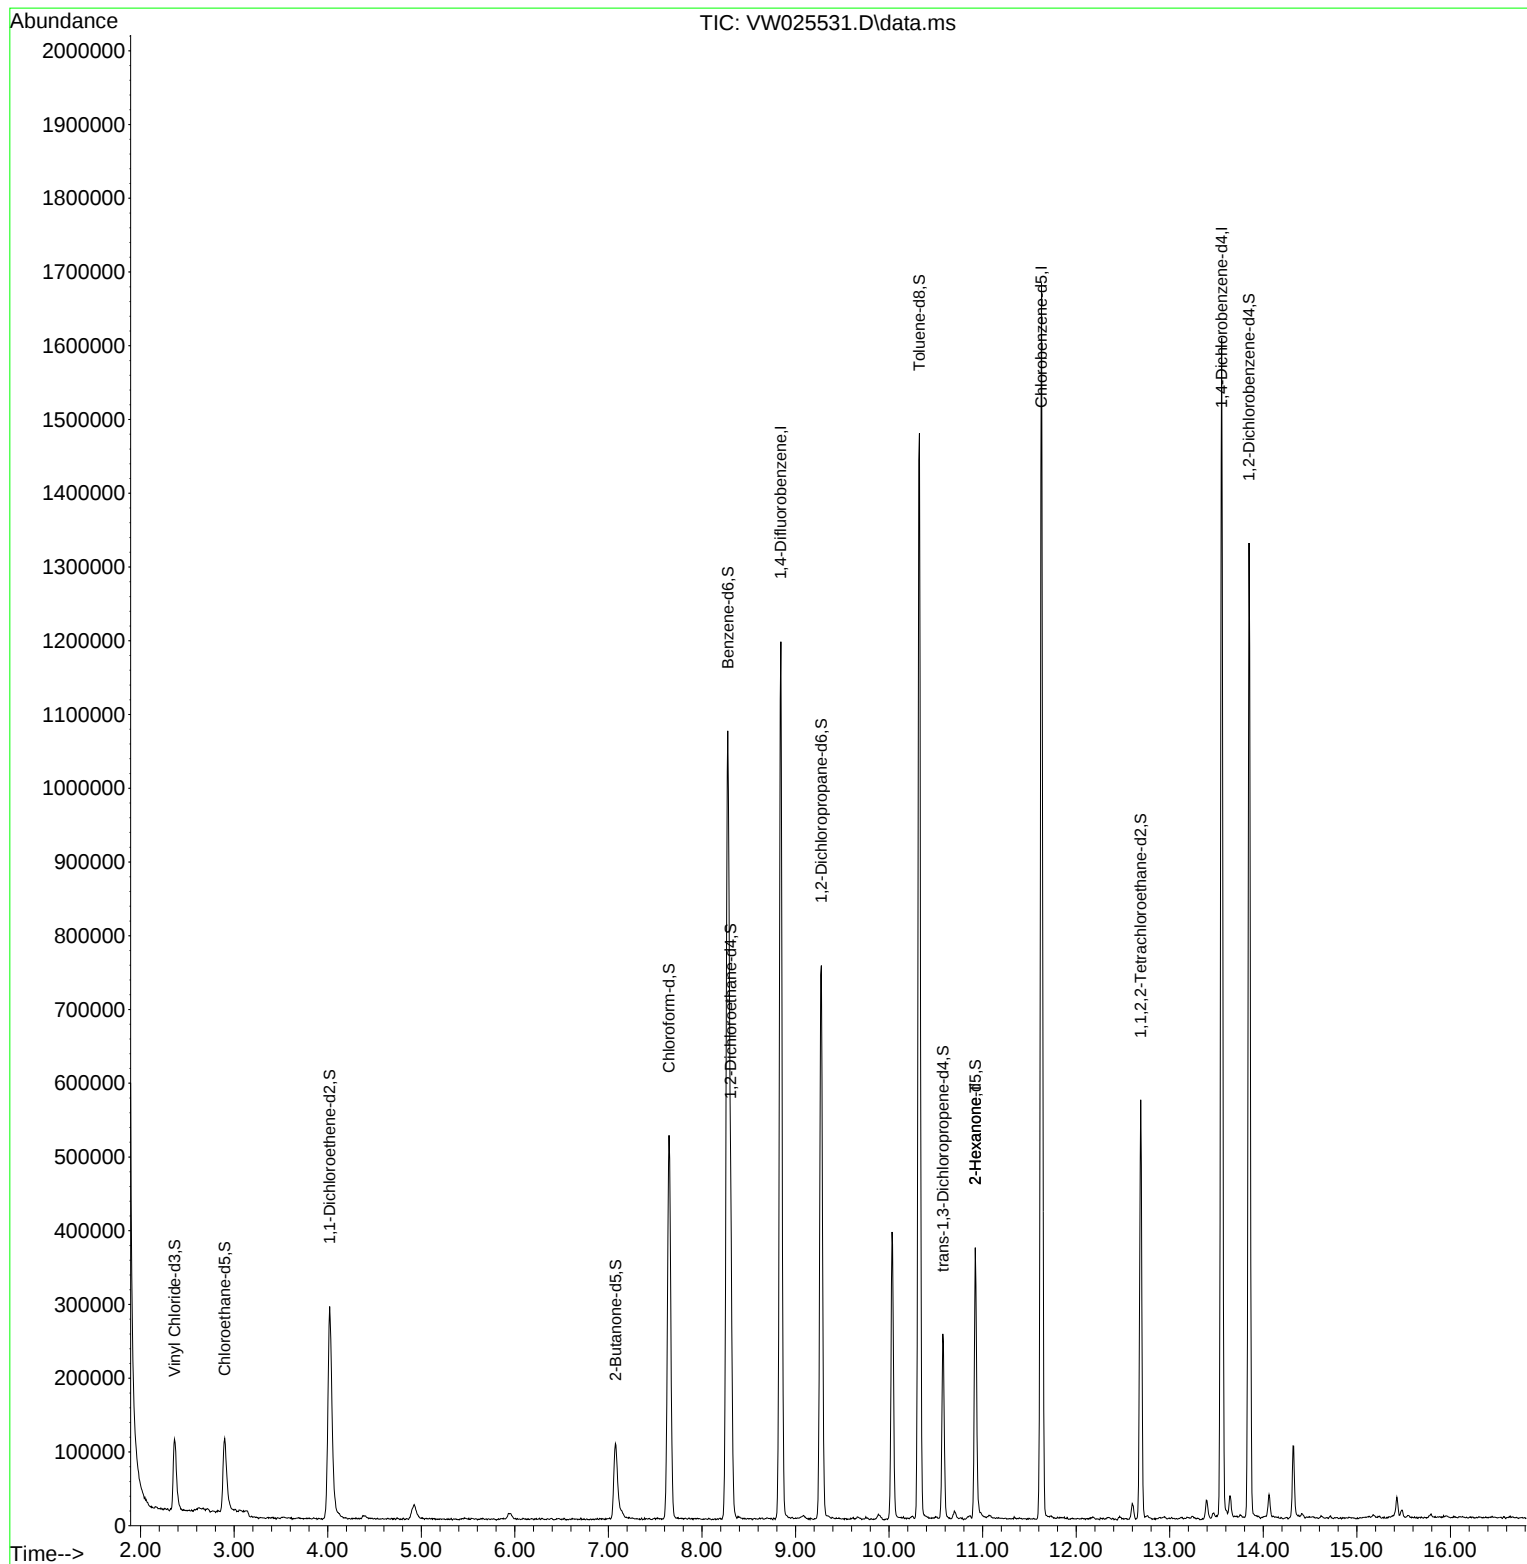

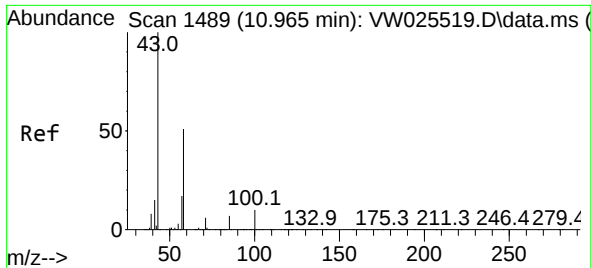

#48
 2-Hexanone
 Concen: 2.550 ug/L
 RT: 10.922 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW025531.D
 Acq: 31 Mar 2023 14:37

Instrument :
 MSVOA_W
 ClientSampleId :

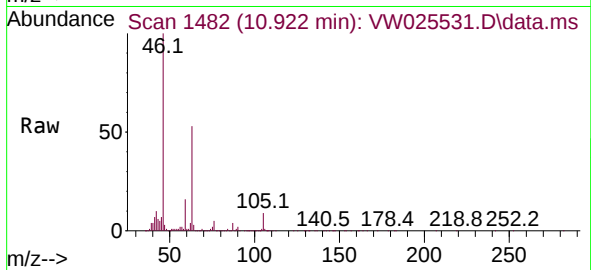

Tgt Ion: 43	Resp: 16356
Ion Ratio	Lower Upper
43	100
58	22.6 41.2 61.8#
57	26.1 14.2 21.4#
100	0.5 8.5 12.7#

