




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033123\
 Data File : VW025526.D
 Acq On : 31 Mar 2023 12:38
 Operator : SY/MD
 Sample : VIBLK434
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK434

Manual IntegrationsAPPROVED

Quant Time: Apr 01 00:37:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 01 00:35:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/01/2023
 Supervised By :Mahesh Dadoda 04/03/2023

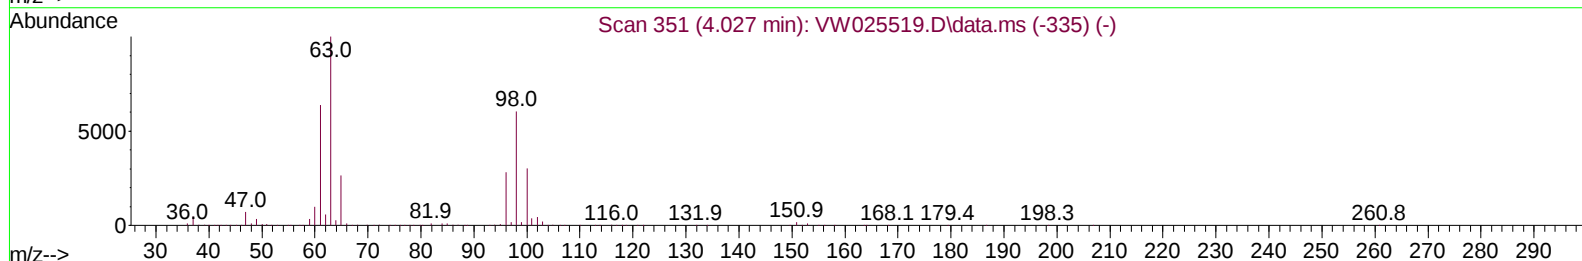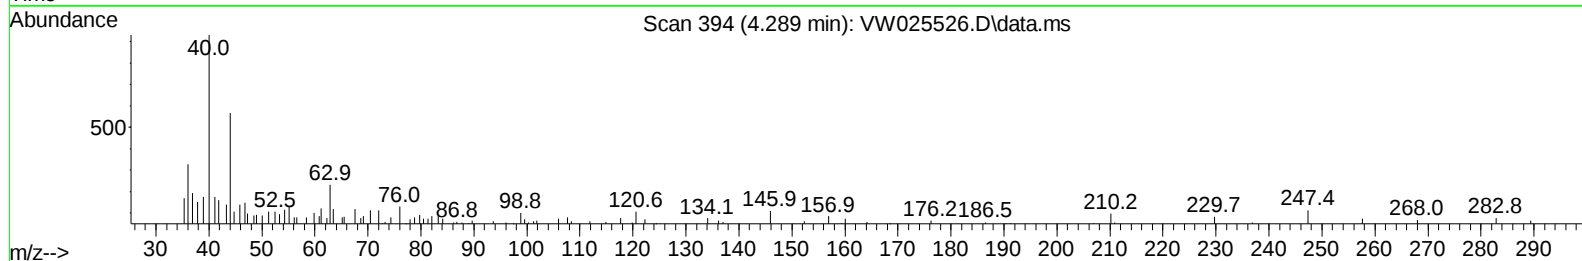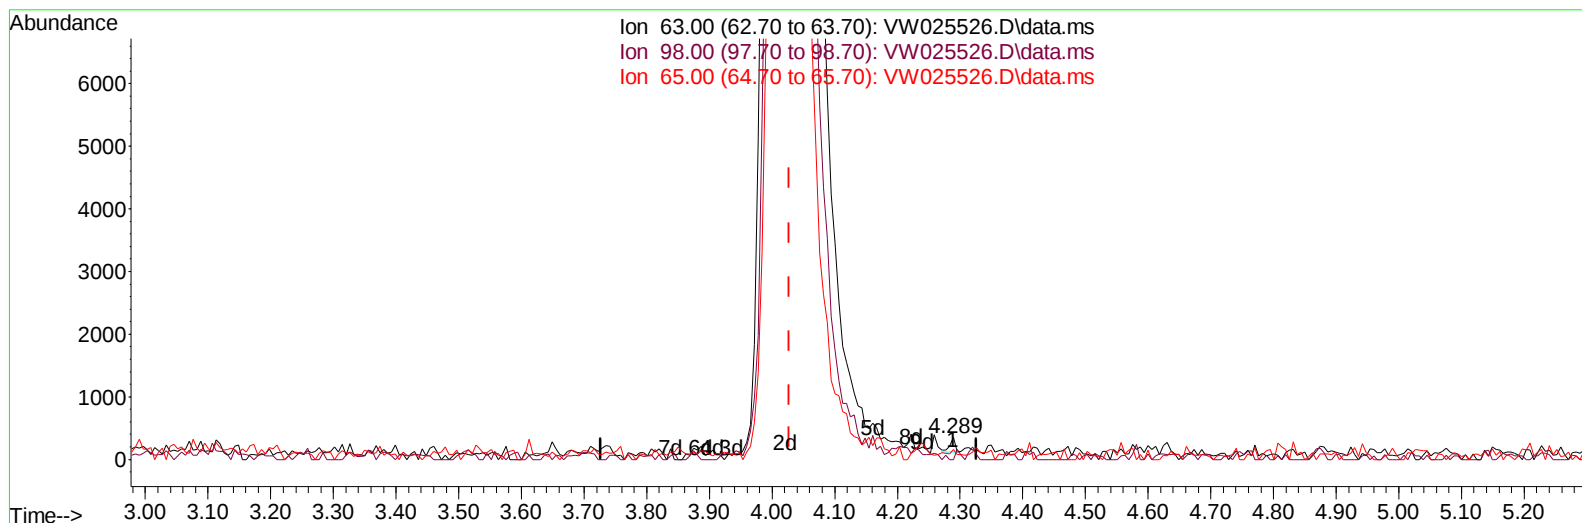

TIC: VW025526.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.289min (+ 0.262) 0.01 ug/L

response 129

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	62.02
65.00	23.70	25.58
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033123\
 Data File : VW025526.D
 Acq On : 31 Mar 2023 12:38
 Operator : SY/MD
 Sample : VIBLK434
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK434

Manual IntegrationsAPPROVED

Quant Time: Apr 01 00:37:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 01 00:35:04 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/01/2023
 Supervised By :Mahesh Dadoda 04/03/2023

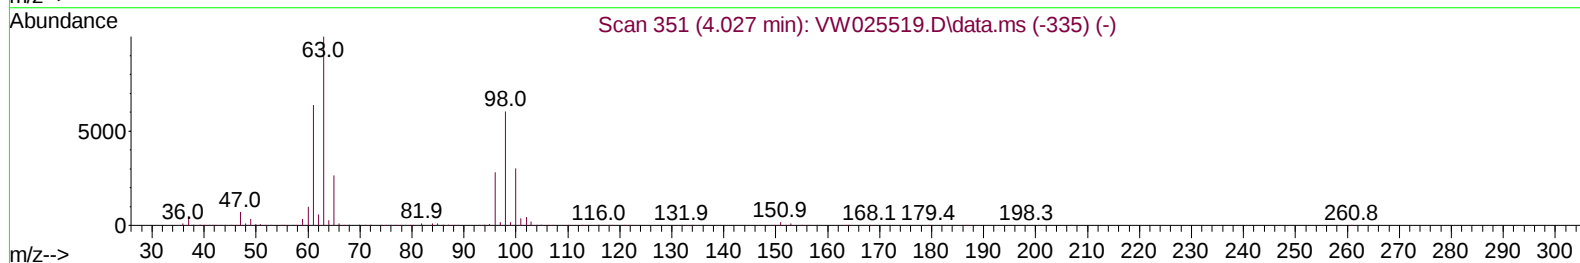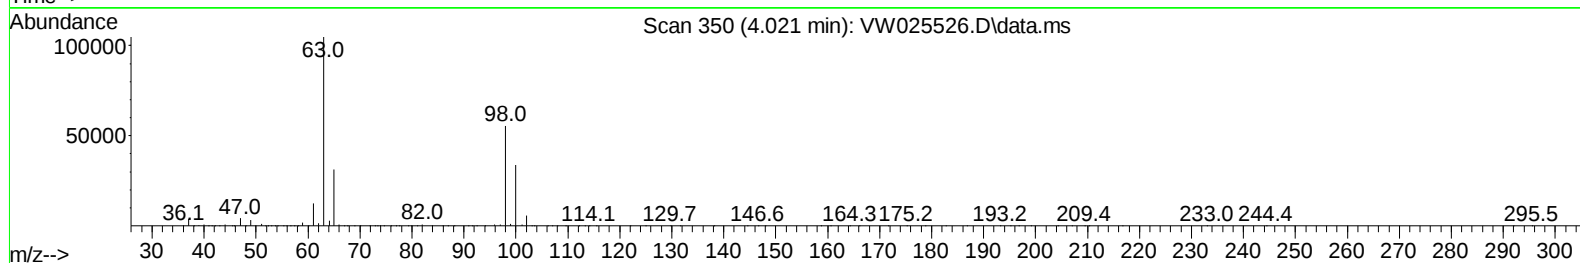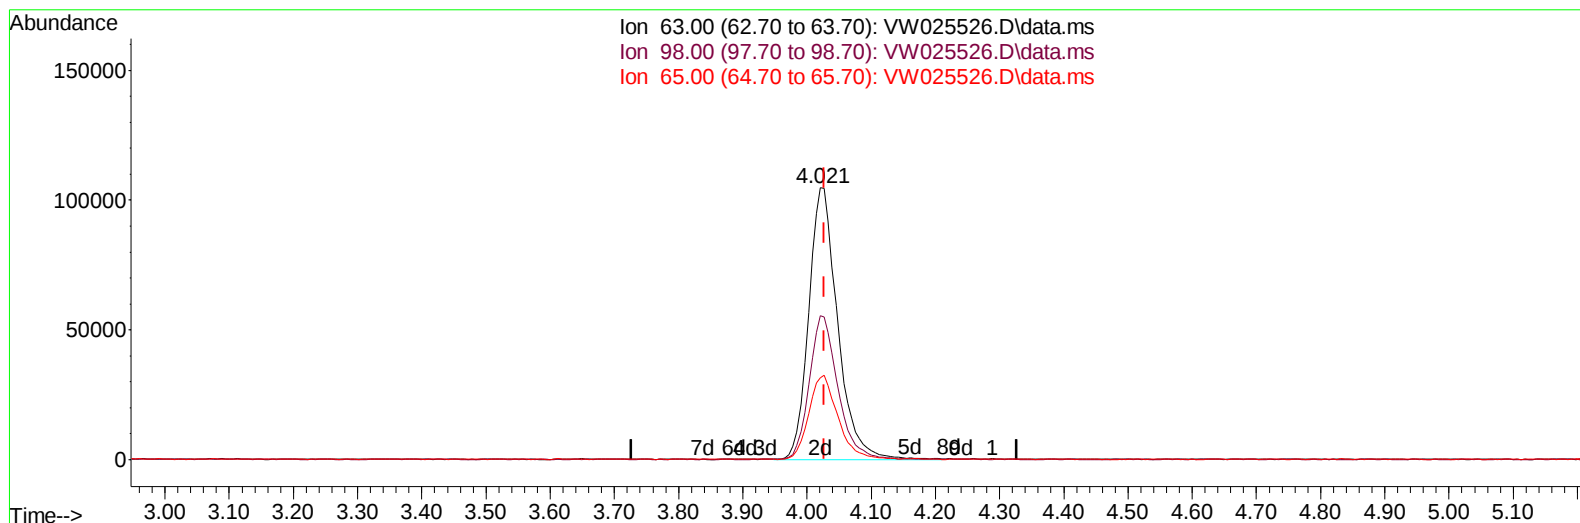

TIC: VW025526.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.021min (-0.006) 15.34 ug/L m

response 329152

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	66.90	0.02#
65.00	23.70	0.01#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033123\
 Data File : VW025526.D
 Acq On : 31 Mar 2023 12:38
 Operator : SY/MD
 Sample : VIBLK434
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK434

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/01/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Apr 01 00:37:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 01 00:35:04 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		668259	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		585158	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		277660	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		191555	17.240	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	68.960%		
7) Chloroethane-d5	2.899	69		163055	20.395	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	81.560%		
11) 1,1-Dichloroethene-d2	4.021	63		329152m	15.338	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	61.360%		
21) 2-Butanone-d5	7.075	46		129516	47.488	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	94.980%		
24) Chloroform-d	7.648	84		445965	23.149	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	92.600%		
26) 1,2-Dichloroethane-d4	8.307	65		246375	23.827	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	95.320%		
32) Benzene-d6	8.276	84		890604	22.274	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	89.080%		
36) 1,2-Dichloropropane-d6	9.276	67		295695	23.905	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	95.640%		
41) Toluene-d8	10.325	98		775207	21.990	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	87.960%		
43) trans-1,3-Dichloroprop...	10.581	79		103795	21.073	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	84.280%		
47) 2-Hexanone-d5	10.922	63		81247	45.679	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	91.360%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		213055	23.511	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	94.040%		
66) 1,2-Dichlorobenzene-d4	13.848	152		249468	24.160	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	96.640%		
Target Compounds							
16) Methylene chloride	4.917	84		31004	3.332	ug/L	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033123\
Data File : VW025526.D
Acq On : 31 Mar 2023 12:38
Operator : SY/MD
Sample : VIBLK434
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK434

Manual IntegrationsAPPROVED

Quant Time: Apr 01 00:37:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 01 00:35:04 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 04/01/2023
Supervised By :Mahesh Dadoda 04/03/2023

