

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033123\
 Data File : VW025542.D
 Acq On : 31 Mar 2023 19:00
 Operator : SY/MD
 Sample : 02151-10
 Misc : 6.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C11B3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/01/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Supervised By :Mahesh
 Dadoda
 04/03/2023

Quant Time: Apr 01 00:41:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 01 00:35:04 2023
 Response via : Initial Calibration

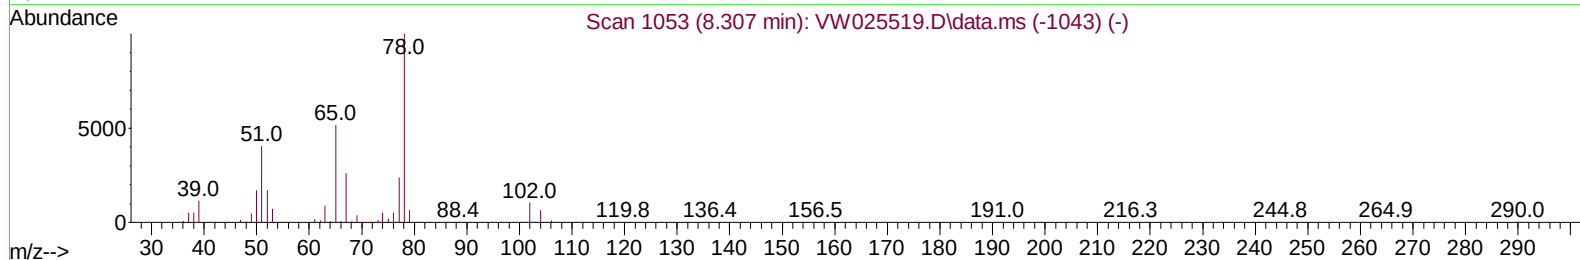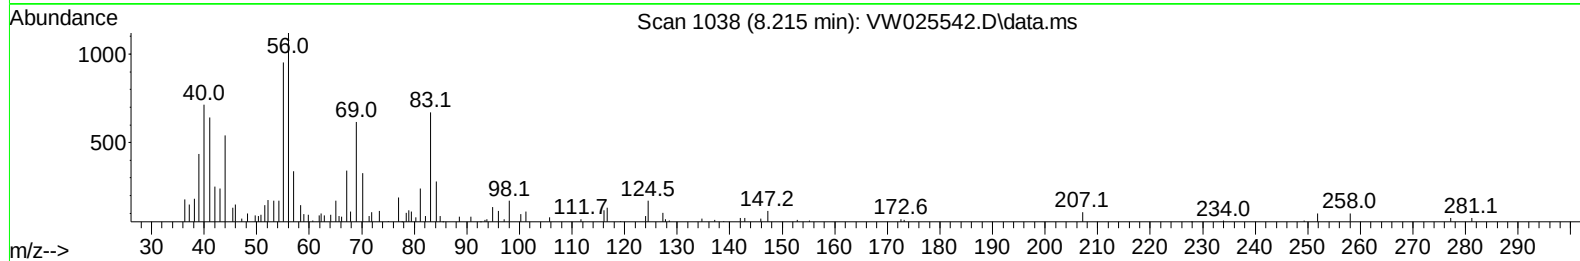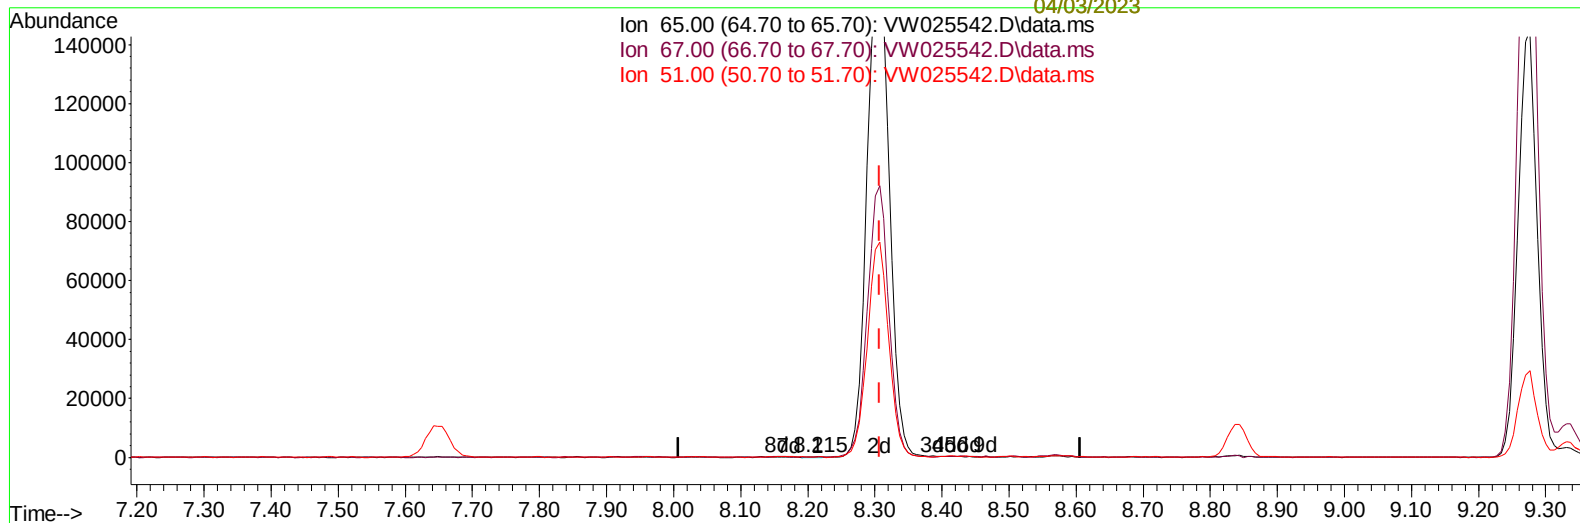

TIC: VW025542.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.215min (-0.091) 0.01 ug/L

response 226

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	56.64
51.00	111.10	100.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033123\
 Data File : VW025542.D
 Acq On : 31 Mar 2023 19:00
 Operator : SY/MD
 Sample : 02151-10
 Misc : 6.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 C11B3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/01/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Quant Time: Apr 01 00:41:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 01 00:35:04 2023
 Response via : Initial Calibration

Supervised By :Mahesh
 Dadoda
 04/03/2023

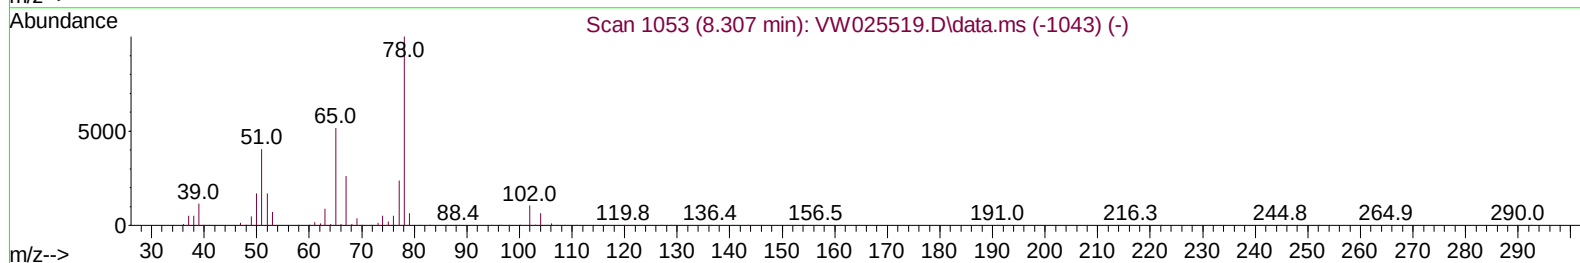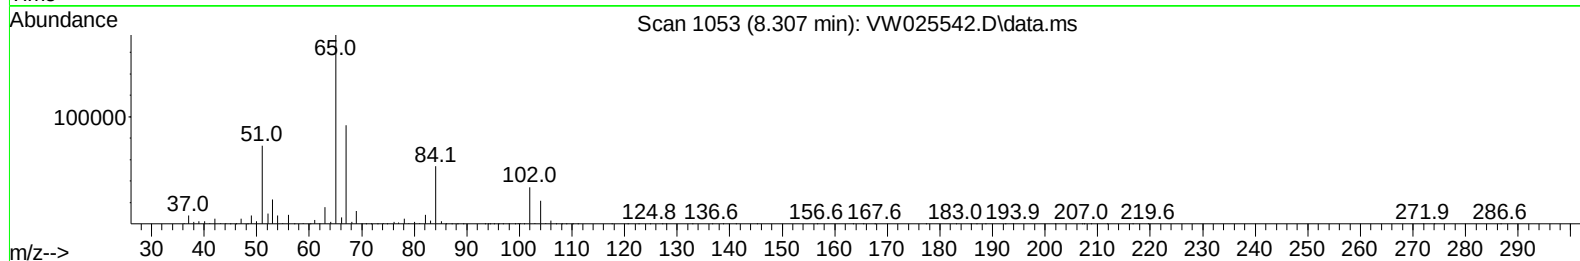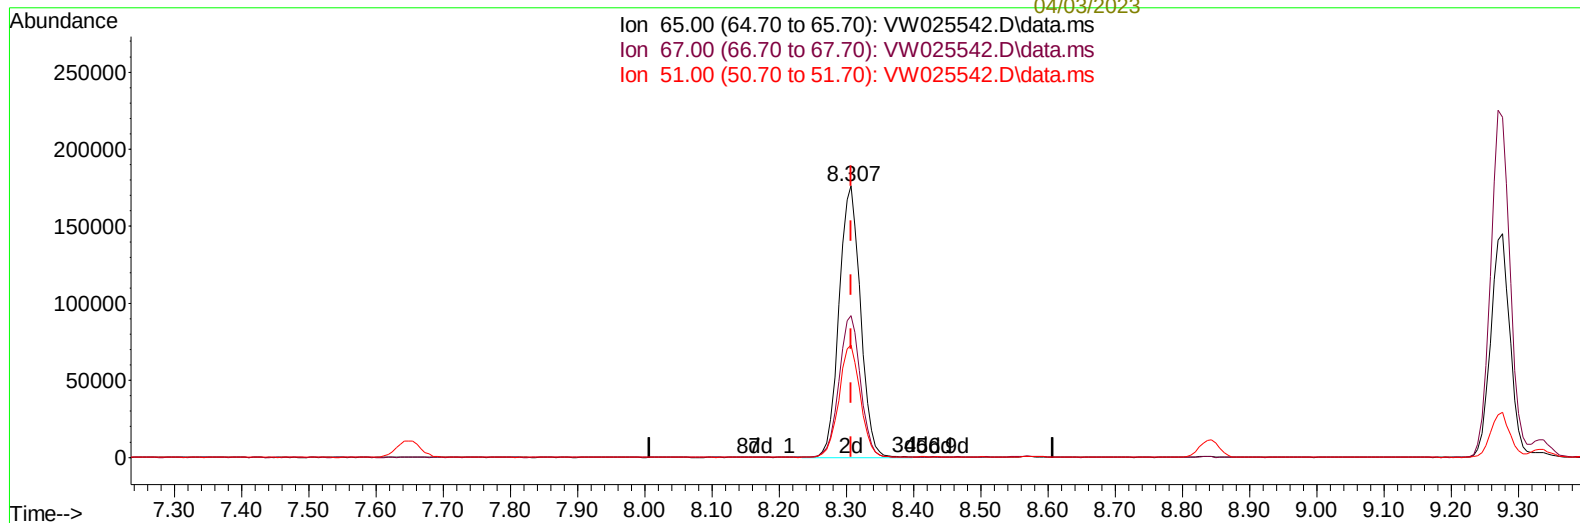

TIC: VW025542.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 24.64 ug/L m

response 392062

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.30	0.03#
51.00	111.10	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033123\
 Data File : VW025542.D
 Acq On : 31 Mar 2023 19:00
 Operator : SY/MD
 Sample : 02151-10
 Misc : 6.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C11B3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/01/2023
 Supervised By :Mahesh Dadoda 04/03/2023

Supervised By :Mahesh
 Dadoda
 04/03/2023

Quant Time: Apr 01 00:41:30 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 01 00:35:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1028508	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	864657	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	362106	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	169887	9.934	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	39.720%	
7) Chloroethane-d5	2.899	69	185530	15.078	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	60.320%	
11) 1,1-Dichloroethene-d2	4.027	63	396379	12.001	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	48.000%	
21) 2-Butanone-d5	7.075	46	243114	57.918	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	115.840%	
24) Chloroform-d	7.648	84	659752	22.251	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	89.000%	
26) 1,2-Dichloroethane-d4	8.307	65	392062m	24.635	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	98.560%	
32) Benzene-d6	8.276	84	1337088	22.631	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	90.520%	
36) 1,2-Dichloropropane-d6	9.270	67	451502	24.703	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	98.800%	
41) Toluene-d8	10.325	98	1171925	22.498	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	90.000%	
43) trans-1,3-Dichloroprop...	10.575	79	162165	22.281	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	89.120%	
47) 2-Hexanone-d5	10.922	63	164589	62.623	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	125.240%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	355493	26.548	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	106.200%	
66) 1,2-Dichlorobenzene-d4	13.849	152	338216	25.117	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	100.480%	
Target Compounds						
13) Acetone	4.125	43	29855	7.399	ug/L	99
16) Methylene chloride	4.917	84	39383	2.750	ug/L	95
35) Methylcyclohexane	9.337	83	266324	10.655	ug/L	92
52) Ethylbenzene	11.727	91	128178	1.969	ug/L	96
53) m,p-Xylene	11.831	106	105693	4.402	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW033123\
Data File : VW025542.D
Acq On : 31 Mar 2023 19:00
Operator : SY/MD
Sample : 02151-10
Misc : 6.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C11B3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 04/01/2023
Supervised By :Mahesh Dadoda 04/03/2023

Supervised By :Mahesh
Dadoda
04/03/2023

Quant Time: Apr 01 00:41:30 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM030623SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 01 00:35:04 2023
Response via : Initial Calibration

