
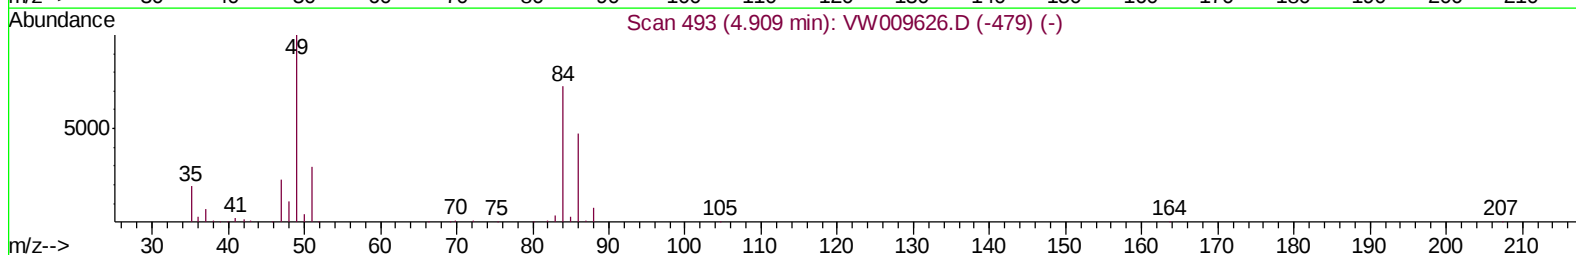
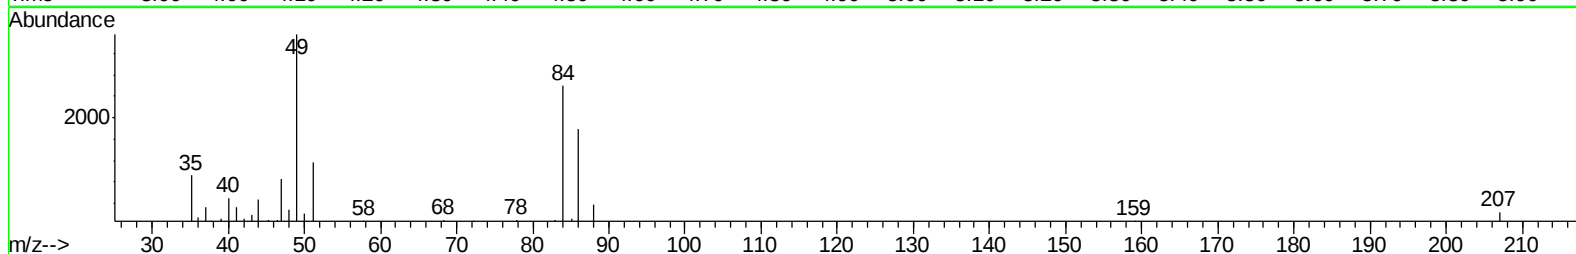


Data File : VW009627.D
Acq On : 01 Apr 2019 16:02
Operator : SY/VA
Sample : VW0401SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 02 01:37:31 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 02 01:34:09 2019
Response via : Initial Calibration

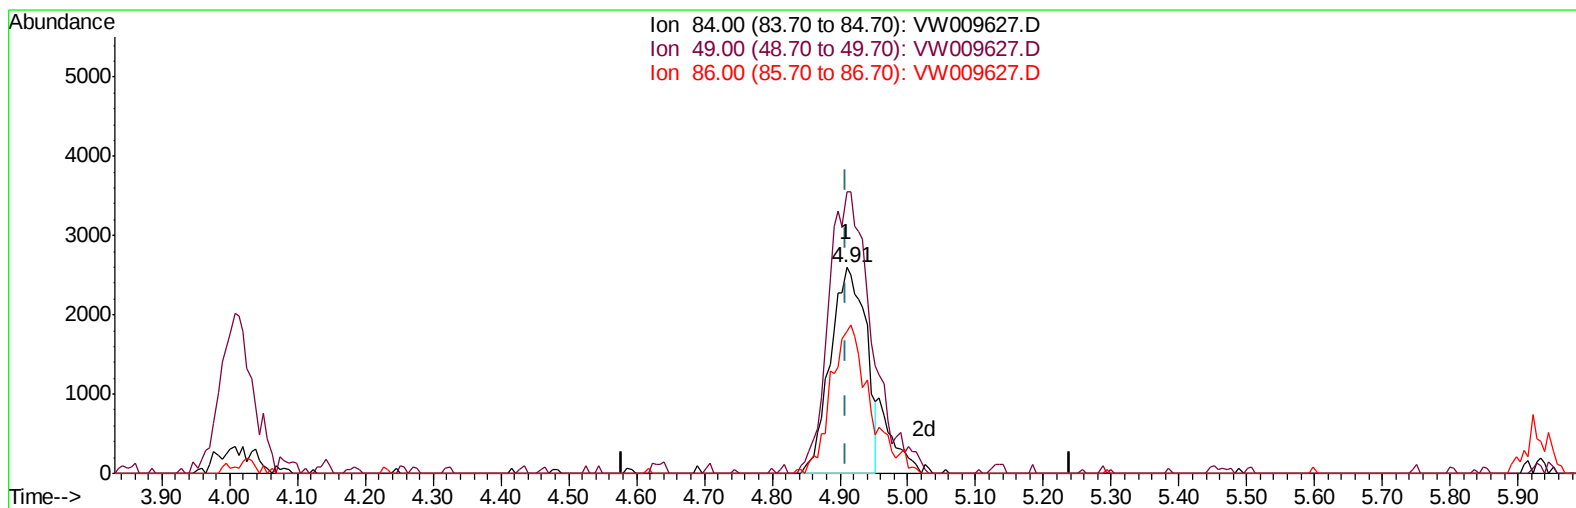

TIC: VW009627.D

(16) Methylene chloride (T)

4.909min (-0.000) 1.38ug/L

response 9503

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	136.81
86.00	63.50	68.96
0.00	0.00	0.00