

Data File : VW009627.D

Acq On : 01 Apr 2019 16:02

Operator : SY/VA

Sample : VW0401SBL01

Misc : 5.00G/10ML/MSVOA\_W/SOIL

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Apr 02 01:37:31 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\SOM2WLM031419S.M

Quant Title : VOC Analysis

QLast Update : Tue Apr 02 01:34:09 2019

Response via : Initial Calibration

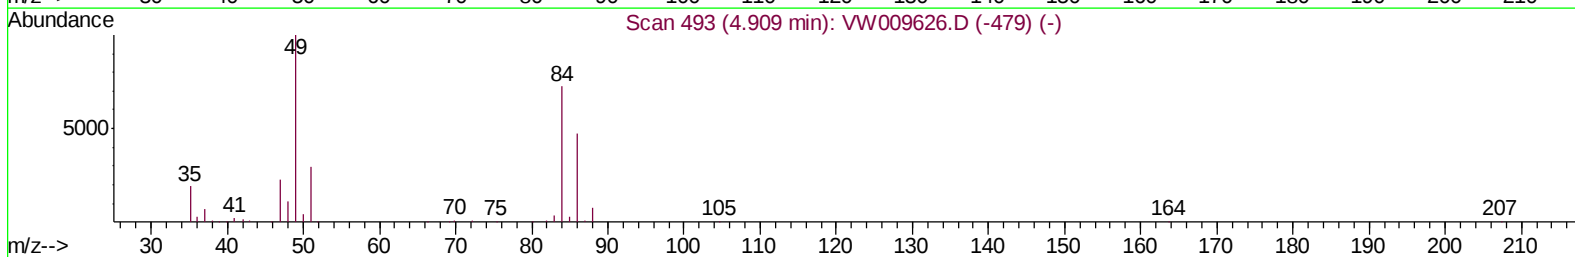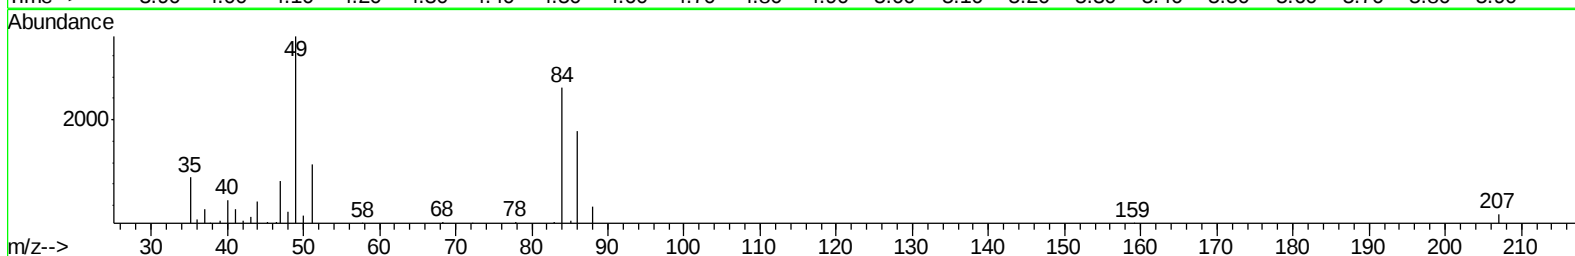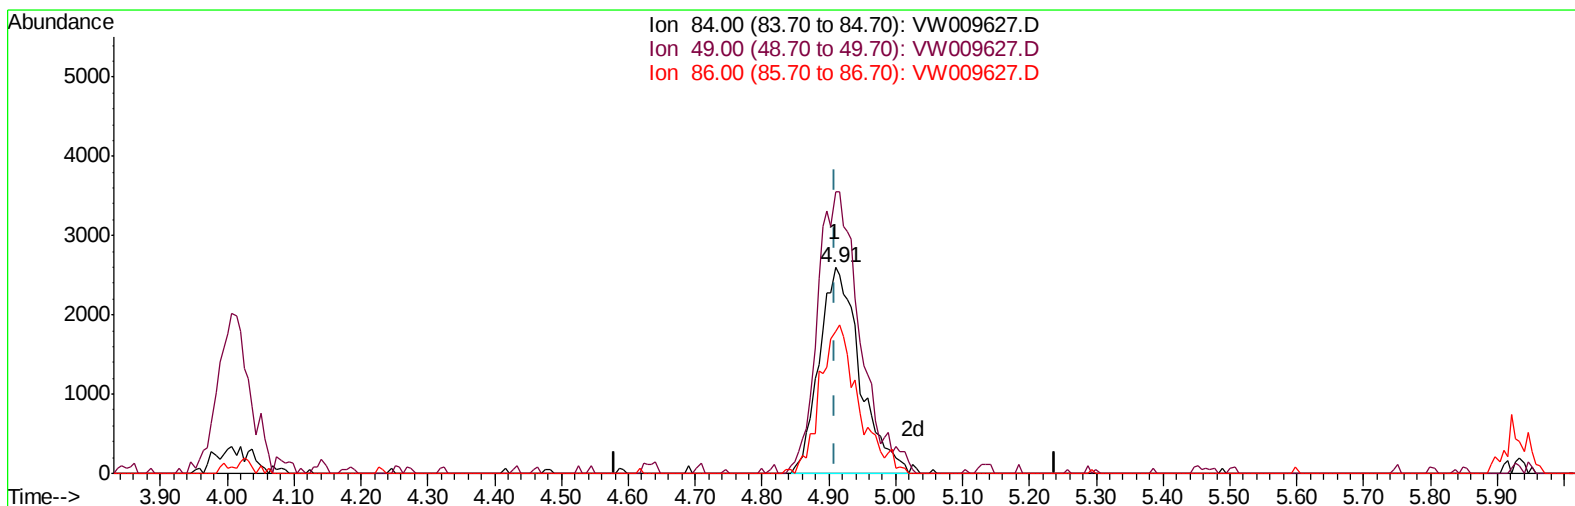

TIC: VW009627.D

(16) Methylene chloride (T)

4.909min (-0.000) 1.60ug/L m

response 10987

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 84.00 | 100    | 100    |
| 49.00 | 137.10 | 136.81 |
| 86.00 | 63.50  | 68.96  |
| 0.00  | 0.00   | 0.00   |