


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040119\
Quantitation Report (QT Reviewed)

Data File : VW009638.D
Acq On : 01 Apr 2019 22:00
Operator : SY/VA
Sample : K2119-09
Misc : 5.08G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5D2

Quant Time: Apr 02 03:02:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 02 01:34:09 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

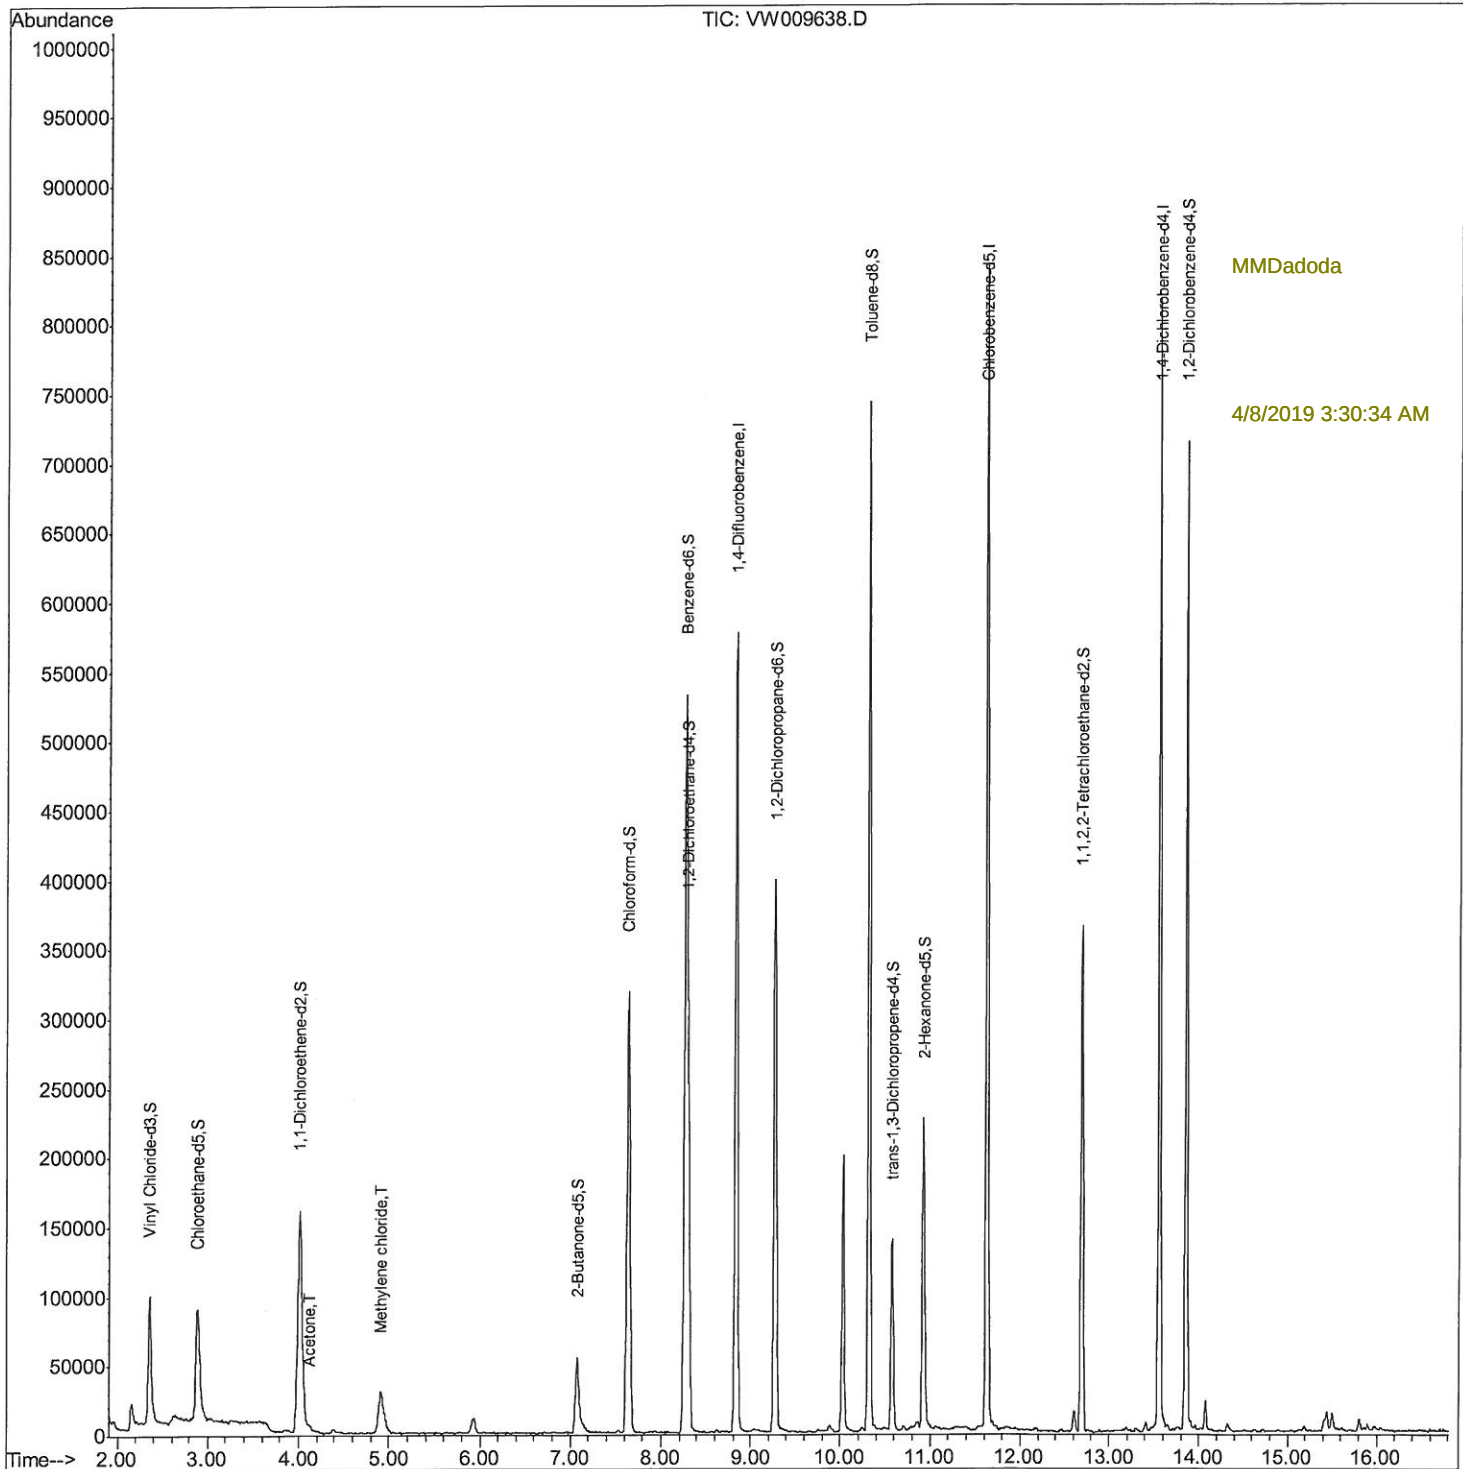




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040119\
Quantitation Report (Qedit)

Data File : VW009638.D
Acq On : 01 Apr 2019 22:00
Operator : SY/VA
Sample : K2119-09
Misc : 5.08G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5D2

Quant Time: Apr 02 01:39:12 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 02 01:34:09 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

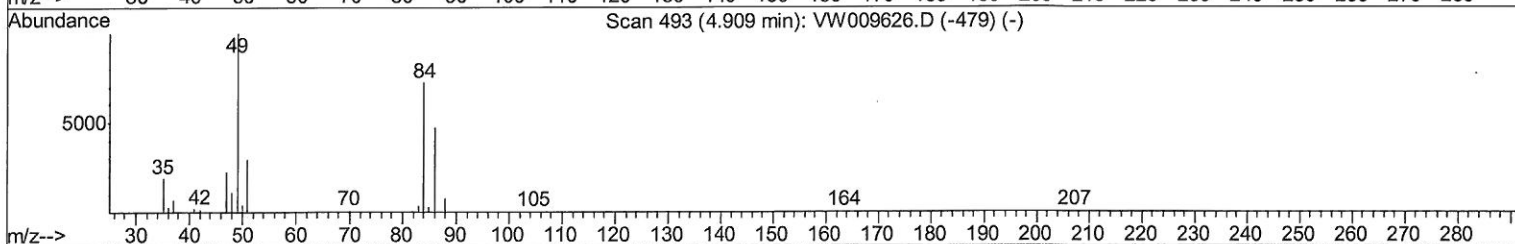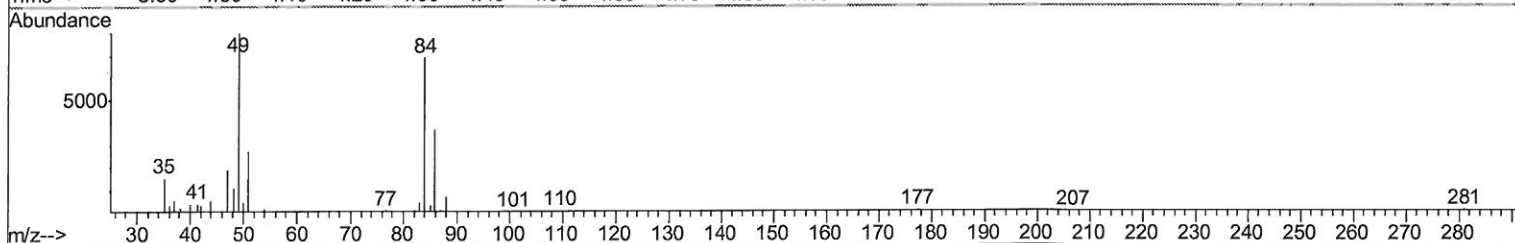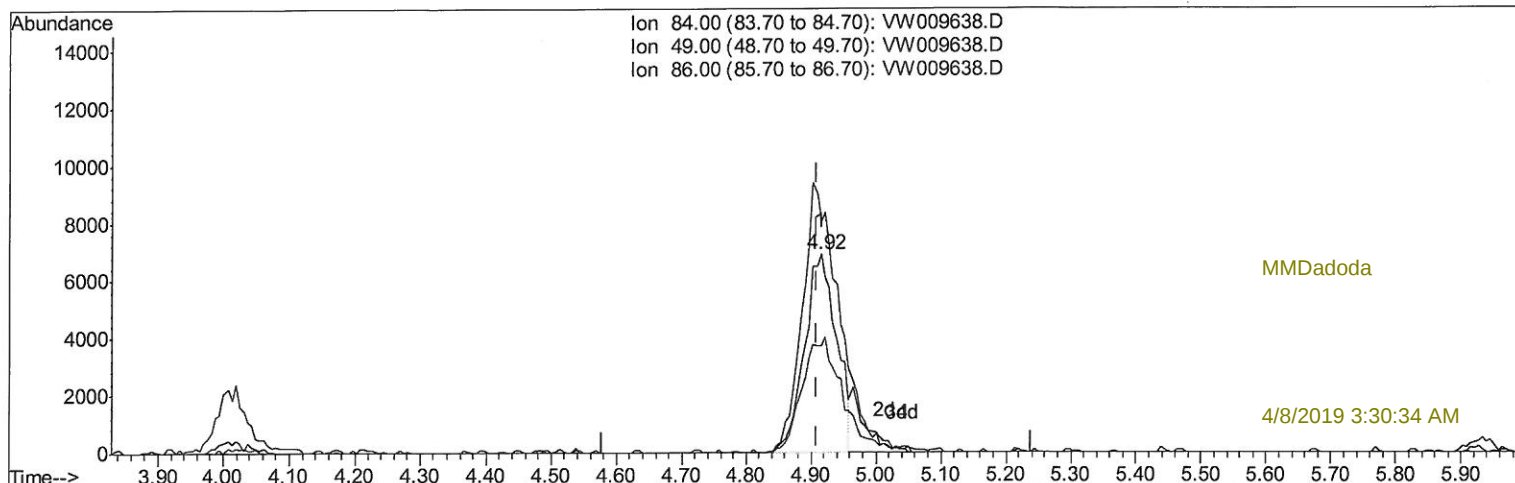

TIC: VW009638.D

(16) Methylene chloride (T)

4.915min (+0.006) 3.65ug/L

response 23616

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	116.05
86.00	63.50	53.48
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040119\
Quantitation Report (Qedit)

Data File : VW009638.D
Acq On : 01 Apr 2019 22:00
Operator : SY/VA
Sample : K2119-09
Misc : 5.08G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BF5D2

Quant Time: Apr 02 01:39:12 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 02 01:34:09 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

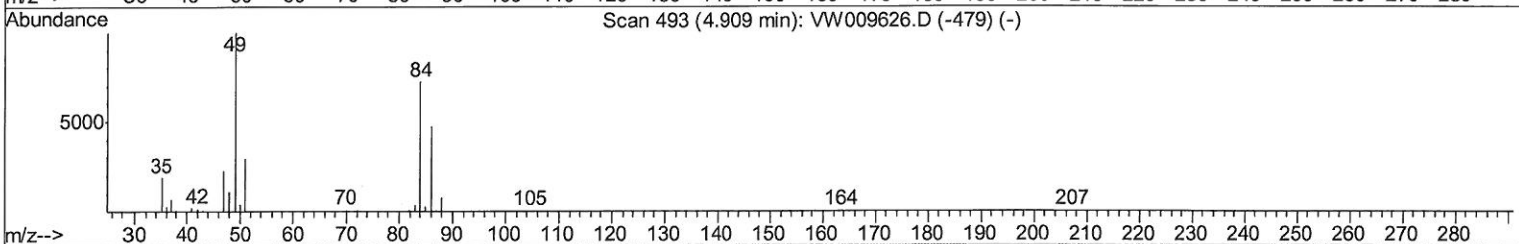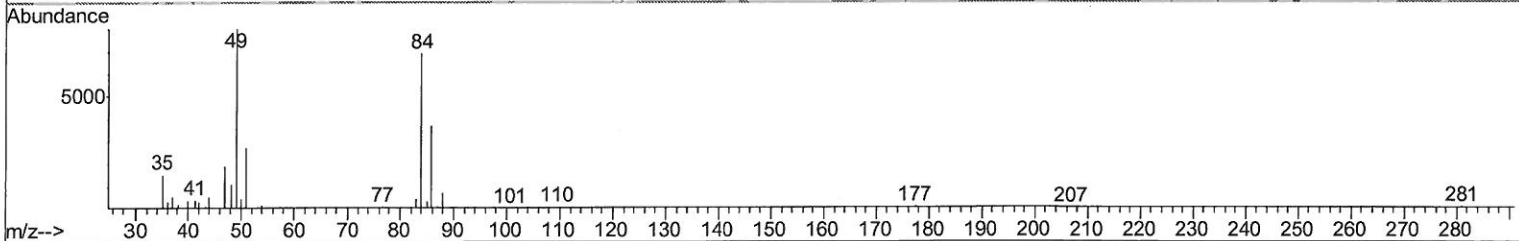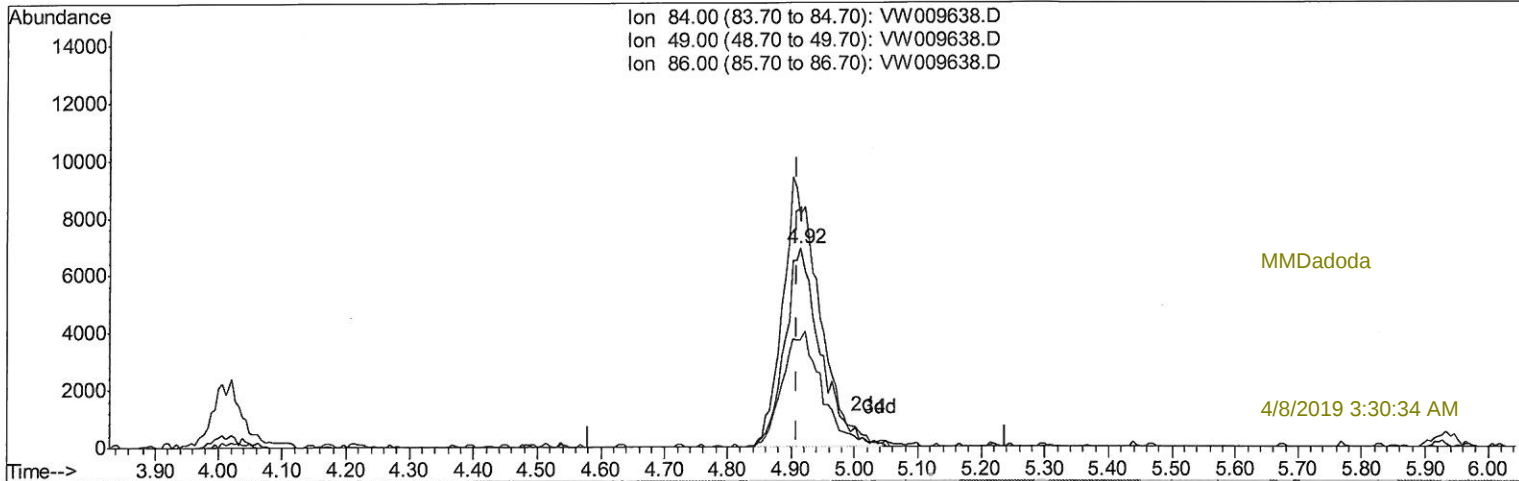

TIC: VW009638.D

(16) Methylene chloride (T)

4.915min (+0.006) 4.17ug/L m

response 27000

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	116.05
86.00	63.50	53.48
0.00	0.00	0.00

7 mg
4/13/19

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040119\
Quantitation Report (QT Reviewed)

Data File : VW009638.D
Acq On : 01 Apr 2019 22:00
Operator : SY/VA
Sample : K2119-09
Misc : 5.08G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5D2

Quant Time: Apr 02 03:02:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 02 01:34:09 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	444283	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	435403	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	190679	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	127046	23.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.72%
7) Chloroethane-d5	2.89	69	119702	19.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.08%
10) 1,1-Dichloroethene-d2	4.01	63	196488	17.12	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.48%
20) 2-Butanone-d5	7.08	46	92713	42.23	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.46%
24) Chloroform-d	7.64	84	291504	24.04	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.16%
26) 1,2-Dichloroethane-d4	8.30	65	178363	24.42	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.68%
29) Benzene-d6	8.27	84	511882	21.32	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	85.28%
33) 1,2-Dichloropropane-d6	9.27	67	167649	23.25	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.00%
37) Toluene-d8	10.32	98	449696	20.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.00%
38) trans-1,3-Dichloropropene-	10.57	79	70125	19.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.44%
39) 2-Hexanone-d5	10.93	63	60169	34.45	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	68.90%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	156818	22.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.32%
61) 1,2-Dichlorobenzene-d4	13.86	152	178438	24.40	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.60%

MMDadoda

4/8/2019 3:30:34 AM

Target Compounds

					Qvalue
13) Acetone	4.12	43	4454	2.474	ug/L
16) Methylene chloride	4.92	84	27000m	4.167	ug/L

72
7MLO
4/13/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed