
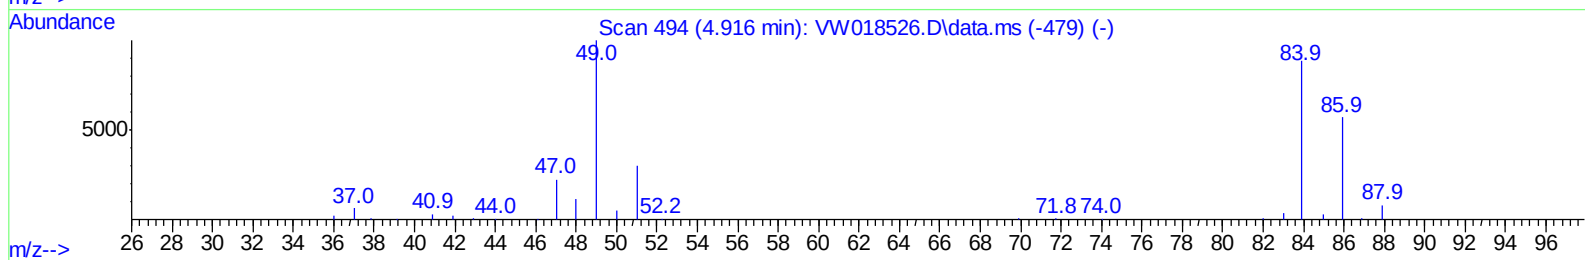
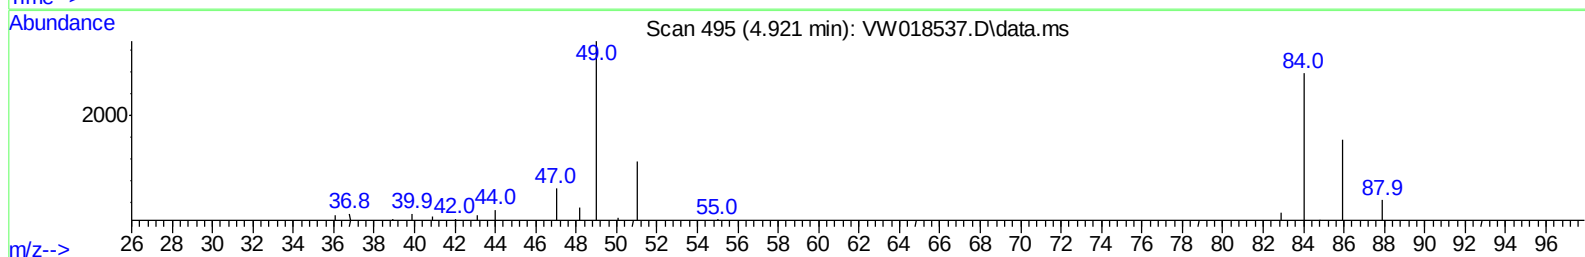


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040121\
Data File : VW018537.D
Acq On : 01 Apr 2021 15:45
Operator : SY/VA
Sample : M1896-04
Misc : 4.28G/10ML/MSVOA_W/SOIL
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Apr 02 03:32:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 02 03:28:33 2021
Response via : Initial Calibration

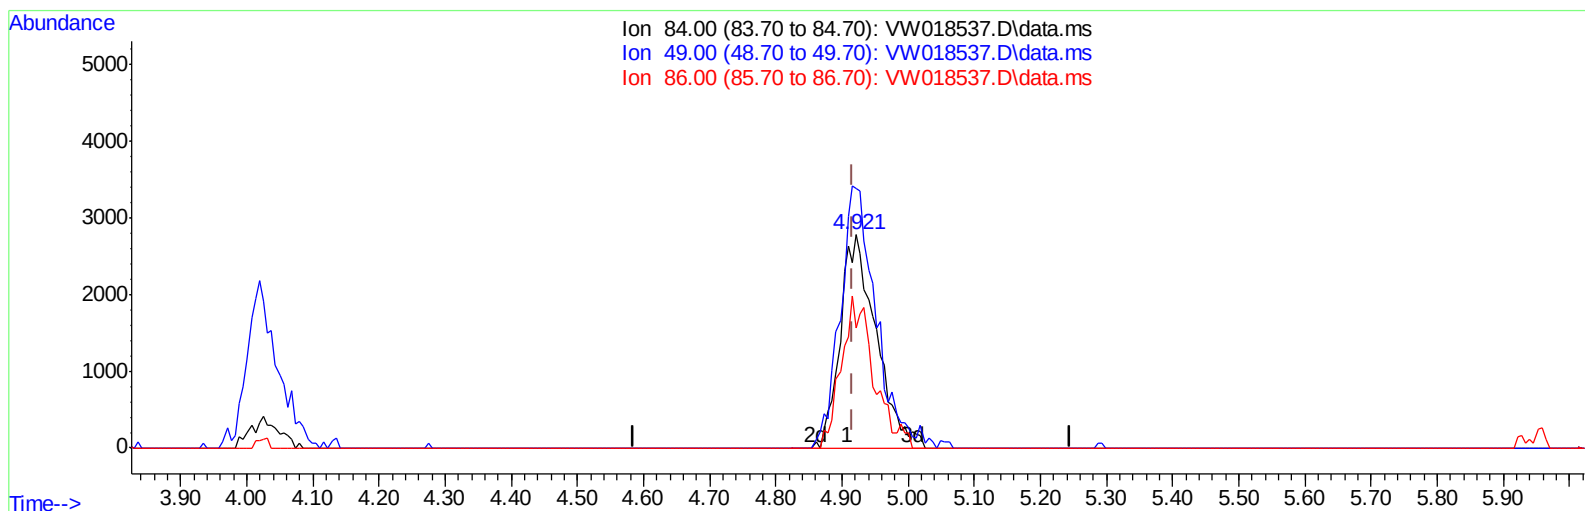

TIC: VW018537.D\data.ms

(16) Methylene chloride (T)




4.921min (+ 0.006) 1.10 ug/L m

response 10478

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	106.30	121.69
86.00	65.90	56.01
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040121\
 Data File : VW018537.D
 Acq On : 01 Apr 2021 15:45
 Operator : SY/VA
 Sample : M1896-04
 Misc : 4.28G/10ML/MSVOA_W/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Quant Time: Apr 02 03:32:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 02 03:28:33 2021
 Response via : Initial Calibration

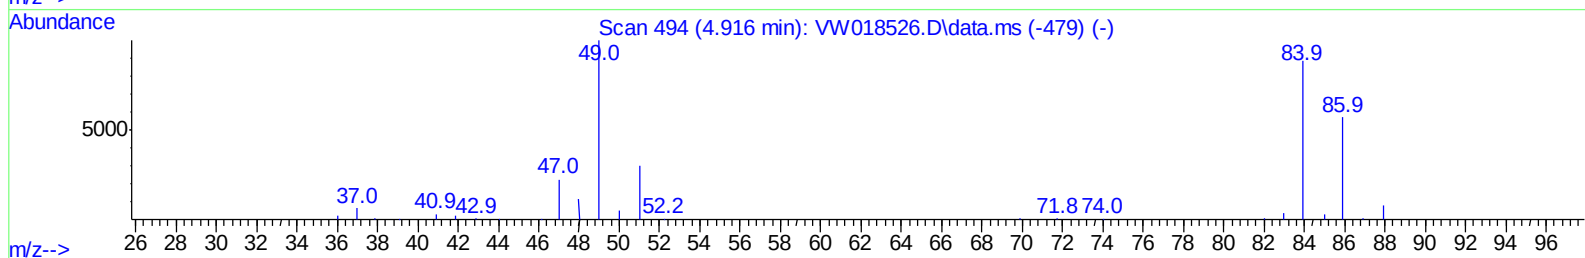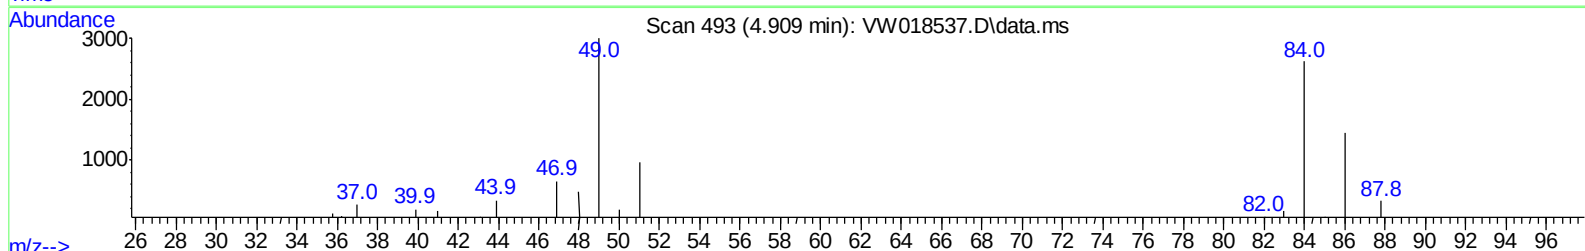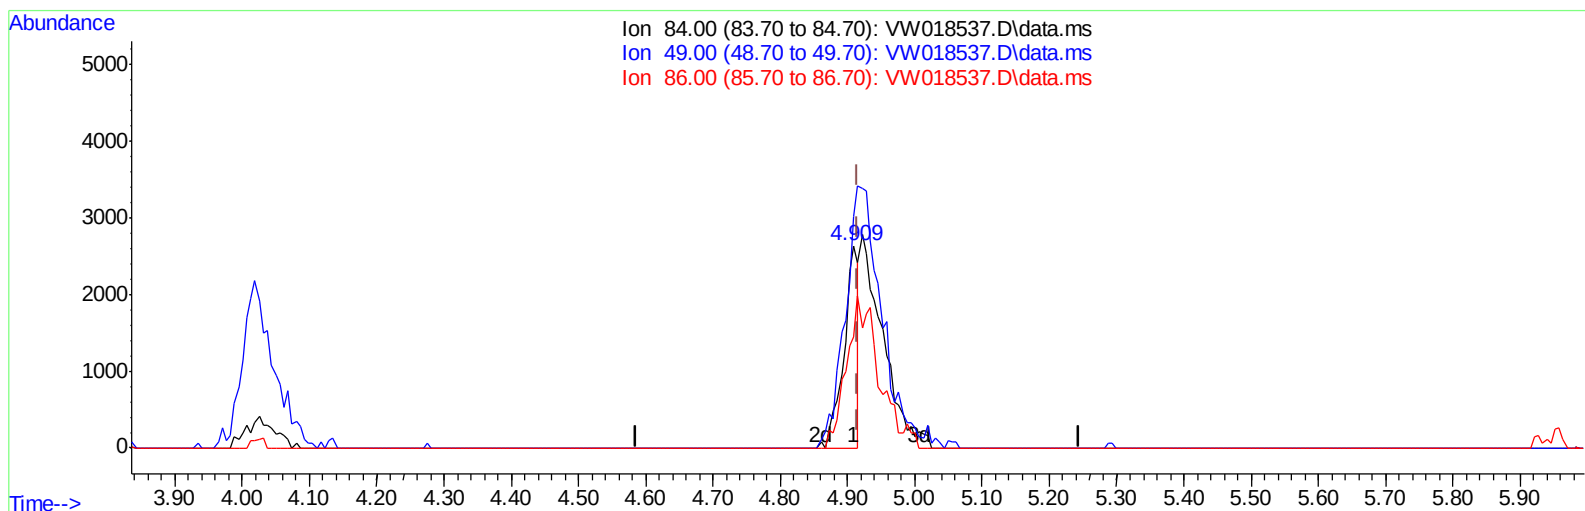

TIC: VW018537.D\data.ms

(16) Methylene chloride (T)

4.909min (-0.006) 0.42 ug/L

response 4017

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	106.30	114.13
86.00	65.90	55.09
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040121\
 Data File : VW018537.D
 Acq On : 01 Apr 2021 15:45
 Operator : SY/VA
 Sample : M1896-04
 Misc : 4.28G/10ML/MSVOA_W/SOIL
 ALS Vial : 29 Sample Multiplier: 1

Quant Time: Apr 02 03:32:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 02 03:28:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	578227	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	523010	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.560	152	247524	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	182498	22.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.72%
7) Chloroethane-d5	2.891	69	142361	20.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.84%
10) 1,1-Dichloroethene-d2	4.019	63	195141	14.05	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.20%
20) 2-Butanone-d5	7.074	46	69339	38.71	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.42%
24) Chloroform-d	7.647	84	270820	18.39	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	73.56%
26) 1,2-Dichloroethane-d4	8.305	65	168040	19.55	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.20%
29) Benzene-d6	8.274	84	542748	19.52	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.08%
33) 1,2-Dichloropropane-d6	9.274	67	152930	19.07	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.28%
37) Toluene-d8	10.323	98	526742	19.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.72%
38) trans-1,3-Dichloroprop...	10.579	79	67801	16.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	65.56%
39) 2-Hexanone-d5	10.926	63	56238	35.83	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.66%
48) 1,1,2,2-Tetrachloroeth...	12.694	84	131842	18.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	73.52%
61) 1,2-Dichlorobenzene-d4	13.853	152	163960	18.63	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	74.52%#
Target Compounds						
13) Acetone	4.123	43	7811	6.07	ug/L	98
14) Carbon disulfide	4.391	76	9907	0.45	ug/L	100
16) Methylene chloride	4.921	84	10478m	1.10	ug/L	
44) Toluene	10.384	91	8778	0.25	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040121\
Data File : VW018537.D
Acq On : 01 Apr 2021 15:45
Operator : SY/VA
Sample : M1896-04
Misc : 4.28G/10ML/MSVOA_W/SOIL
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Apr 02 03:32:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 02 03:28:33 2021
Response via : Initial Calibration

