


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040121\
Data File : VW018540.D
Acq On : 01 Apr 2021 16:57
Operator : SY/VA
Sample : M1896-07
Misc : 5.66G/10ML/MSVOA_W/SOIL
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG583

Manual Integrations
APPROVED

MMDadoda
4/6/2021 1:05:41 PM

Quant Time: Apr 02 03:33:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 02 03:28:33 2021
Response via : Initial Calibration

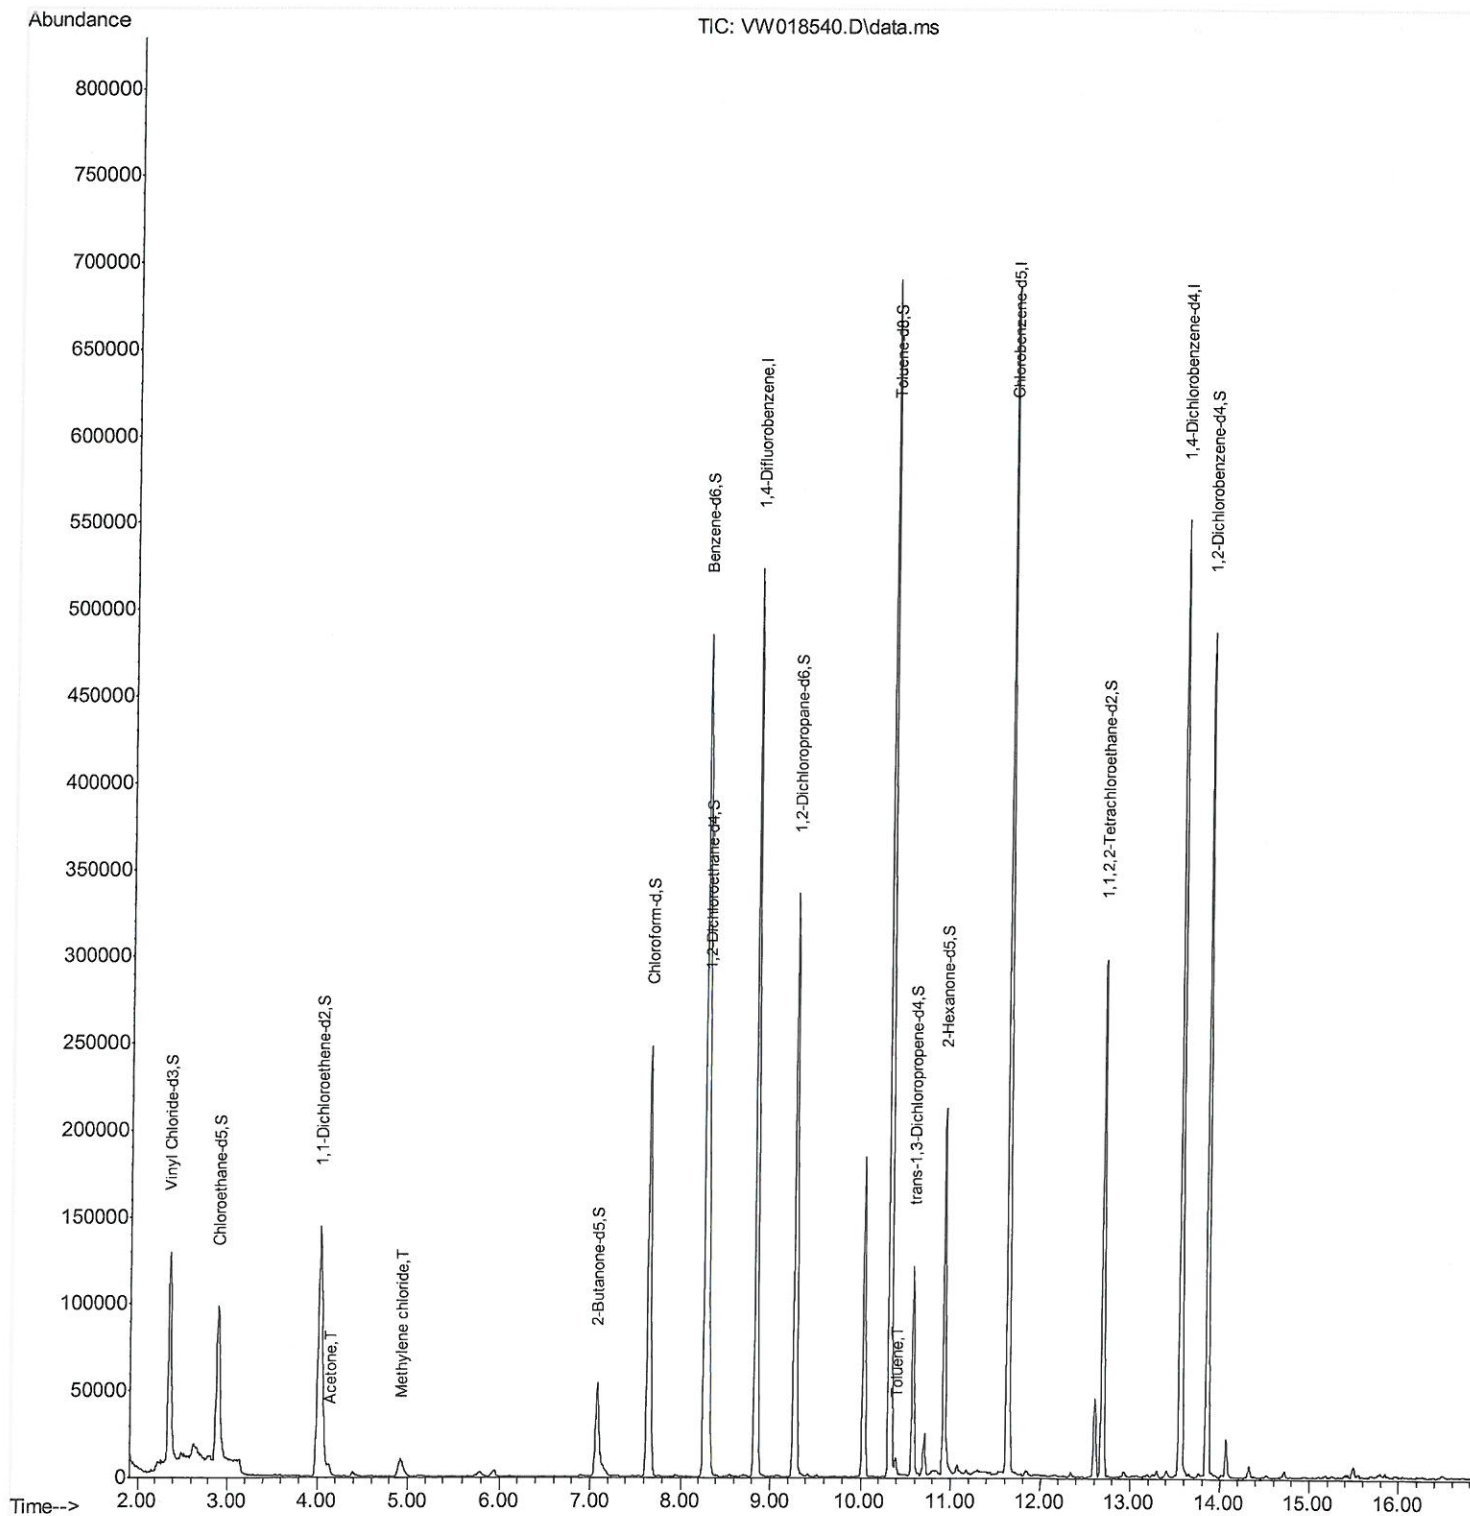

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040121\
 Data File : VW018540.D
 Acq On : 01 Apr 2021 16:57
 Operator : SY/VA
 Sample : M1896-07
 Misc : 5.66G/10ML/MSVOA_W/SOIL
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG583

Manual Integrations
 APPROVED

MMDadoda
 4/6/2021 1:05:41 PM

Quant Time: Apr 02 03:33:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 02 03:28:33 2021
 Response via : Initial Calibration

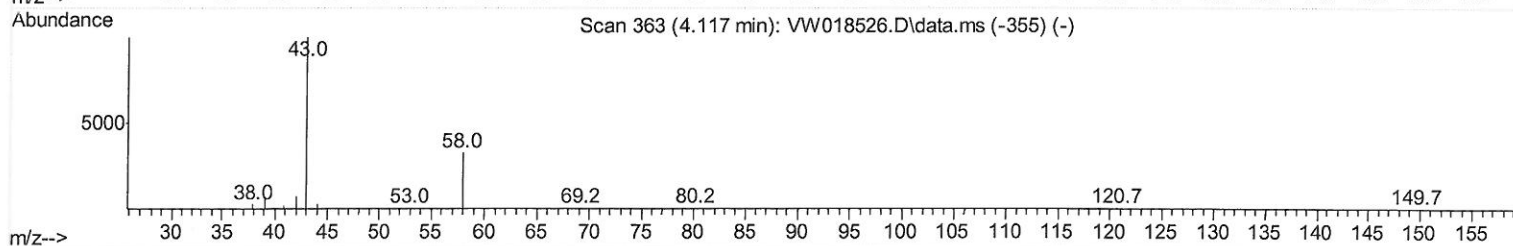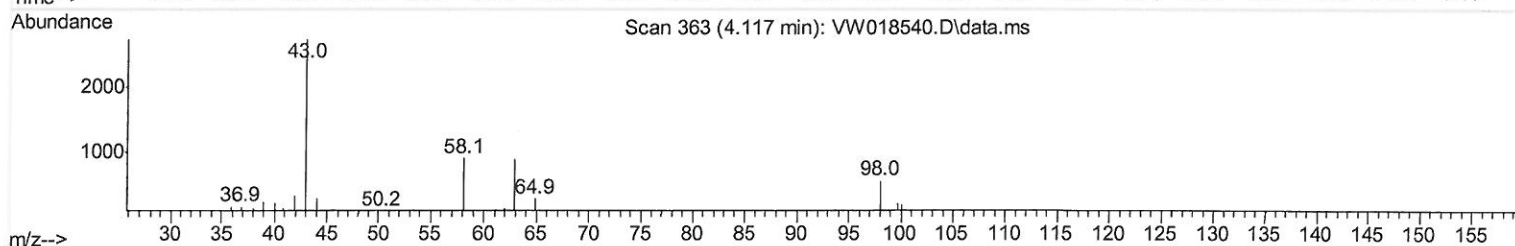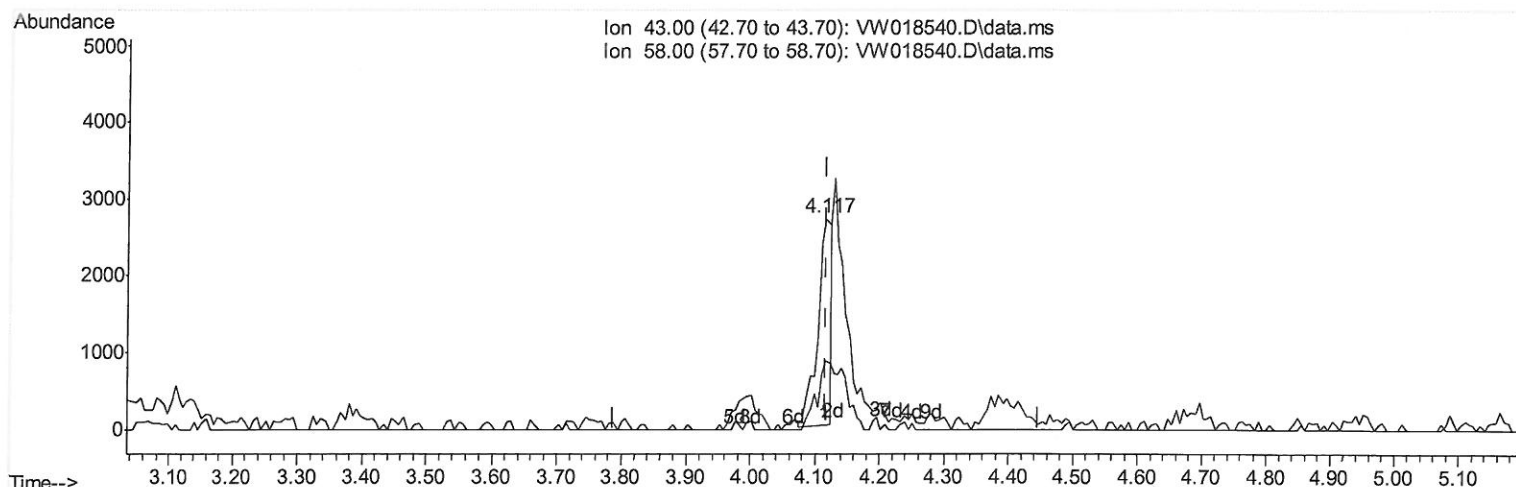

TIC: VW018540.D\data.ms

(13) Acetone (T)

4.117min (-0.000) 4.16 ug/L

response 3871

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.10	23.87
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040121\
Data File : VW018540.D
Acq On : 01 Apr 2021 16:57
Operator : SY/VA
Sample : M1896-07
Misc : 5.66G/10ML/MSVOA_W/SOIL
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG583

Manual Integrations
APPROVED

MMDadoda
4/6/2021 1:05:41 PM

Quant Time: Apr 02 03:33:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 02 03:28:33 2021
Response via : Initial Calibration

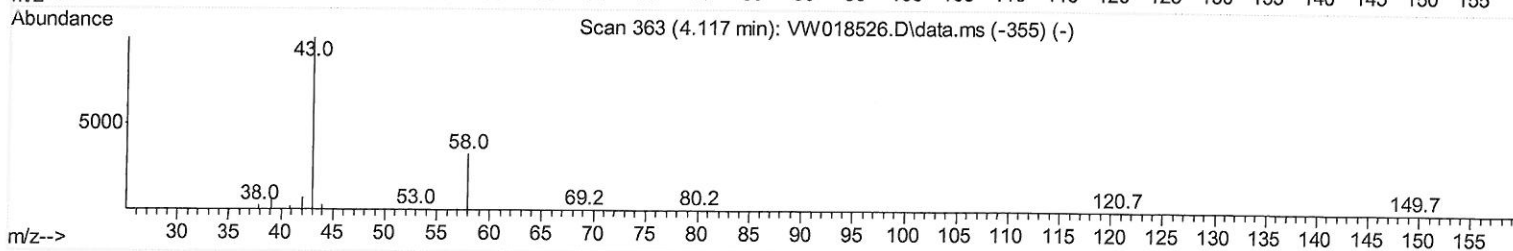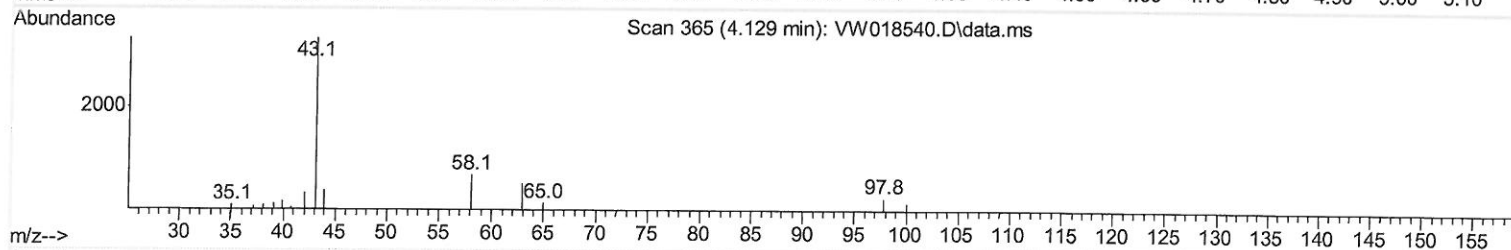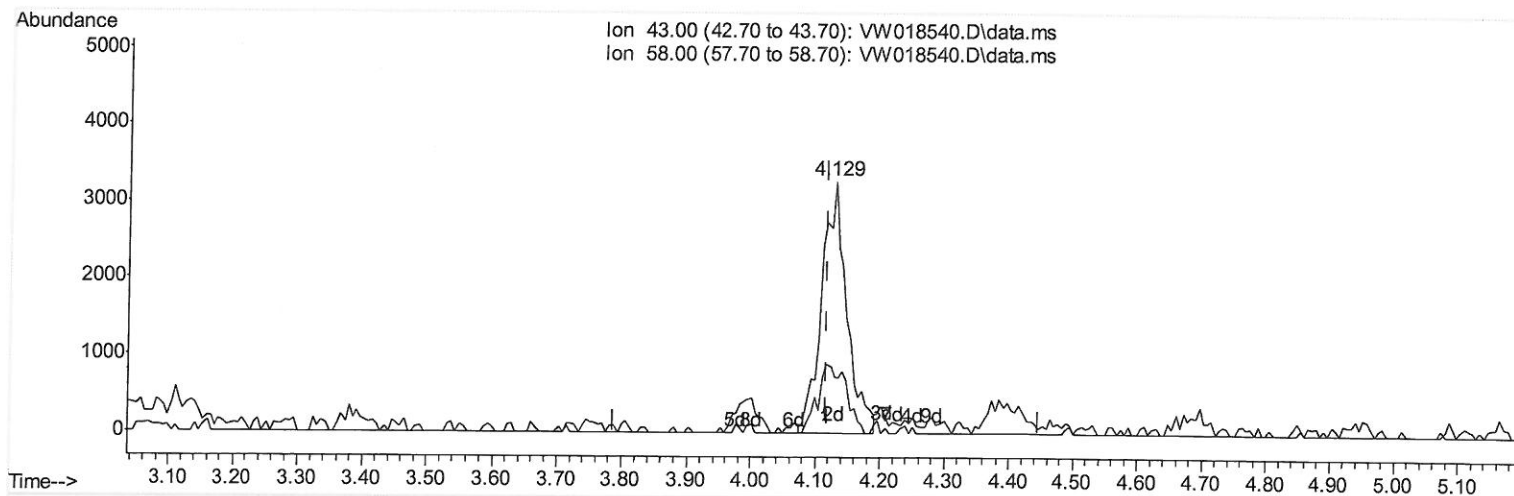

TIC: VW018540.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 9.41 ug/L m

response 8746

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	31.10	10.56
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
4/9/21

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040121\
Data File : VW018540.D
Acq On : 01 Apr 2021 16:57
Operator : SY/VA
Sample : M1896-07
Misc : 5.66G/10ML/MSVOA_W/SOIL
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG583

Manual Integrations
APPROVED

MMDadoda
4/6/2021 1:05:41 PM

Quant Time: Apr 02 03:33:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 02 03:28:33 2021
Response via : Initial Calibration

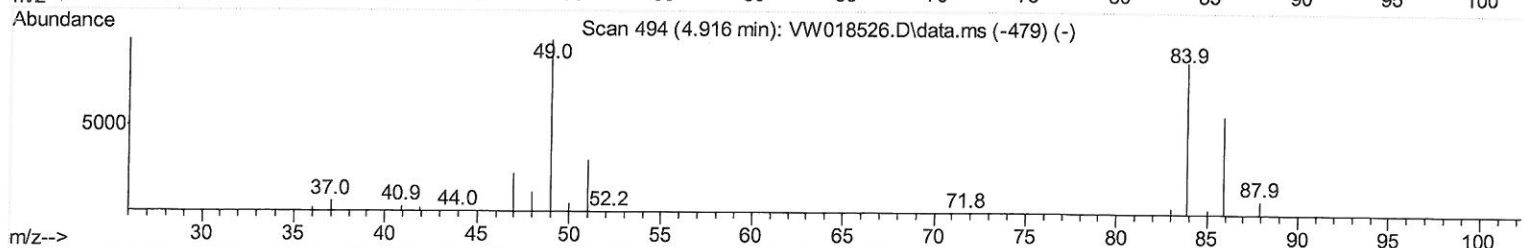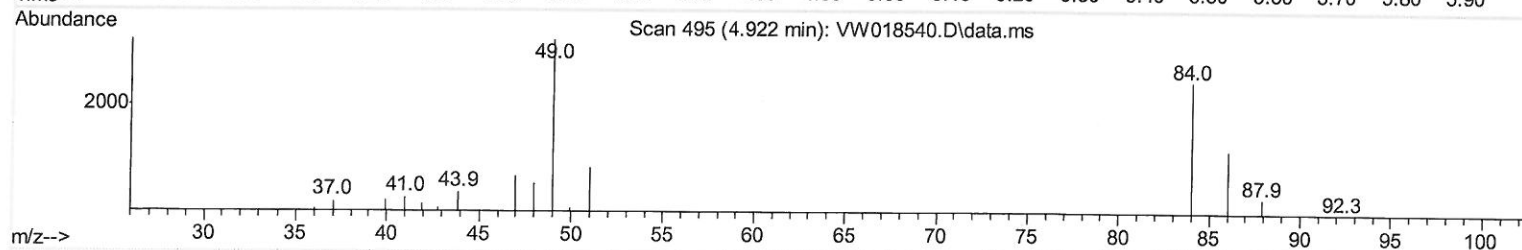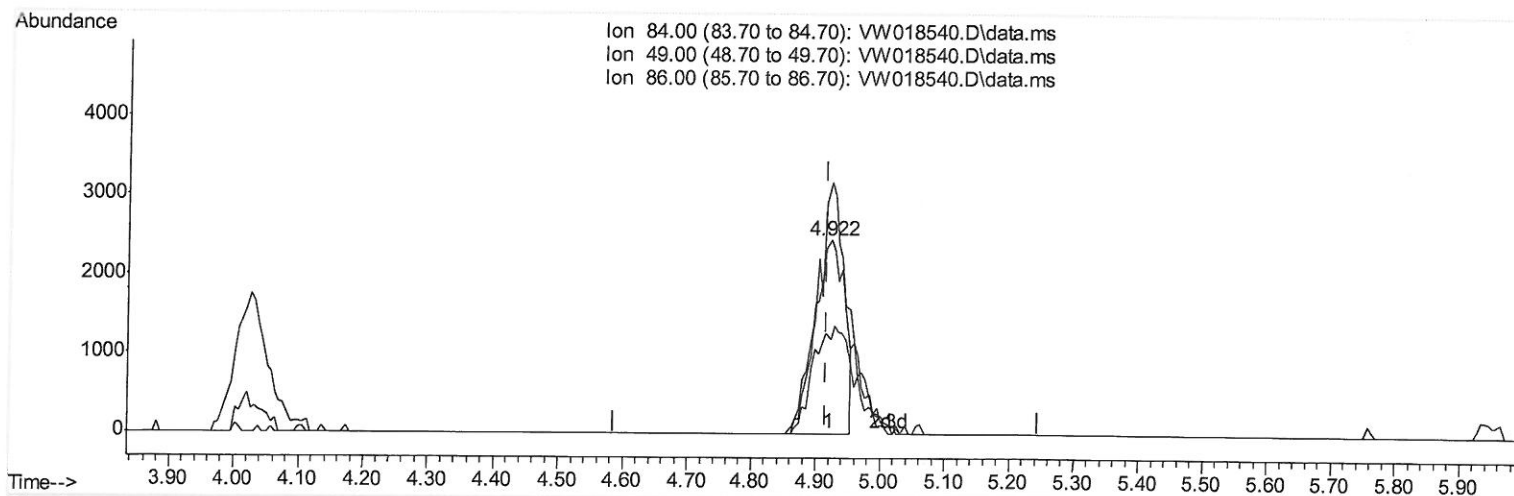

TIC: VW018540.D\data.ms

(16) Methylene chloride (T)

4.922min (+ 0.006) 1.14 ug/L

response 7822

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	106.30	130.19
86.00	65.90	48.50
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040121\
Data File : VW018540.D
Acq On : 01 Apr 2021 16:57
Operator : SY/VA
Sample : M1896-07
Misc : 5.66G/10ML/MSVOA_W/SOIL
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG583

Manual Integrations
APPROVED

MMDadoda
4/6/2021 1:05:41 PM

Quant Time: Apr 02 03:33:08 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 02 03:28:33 2021
Response via : Initial Calibration

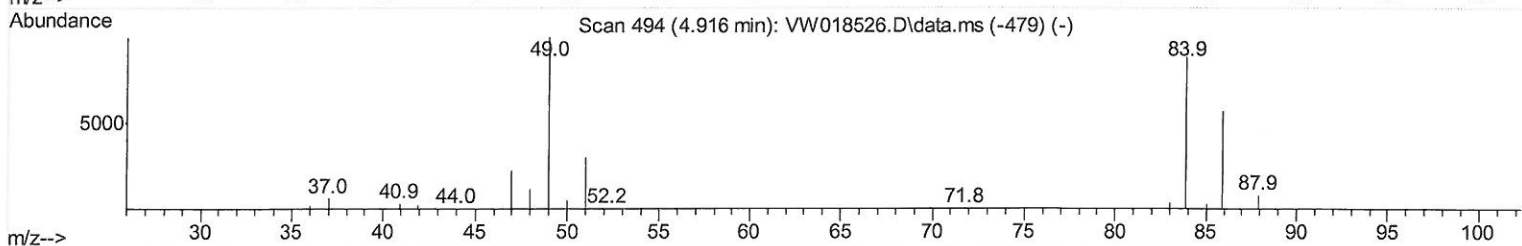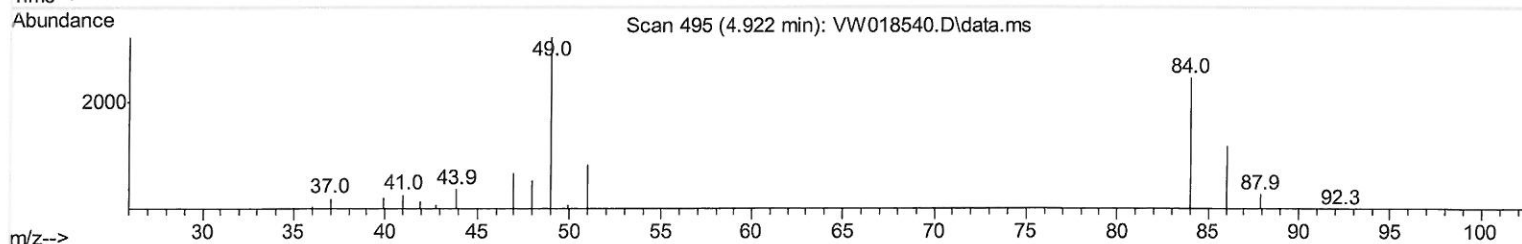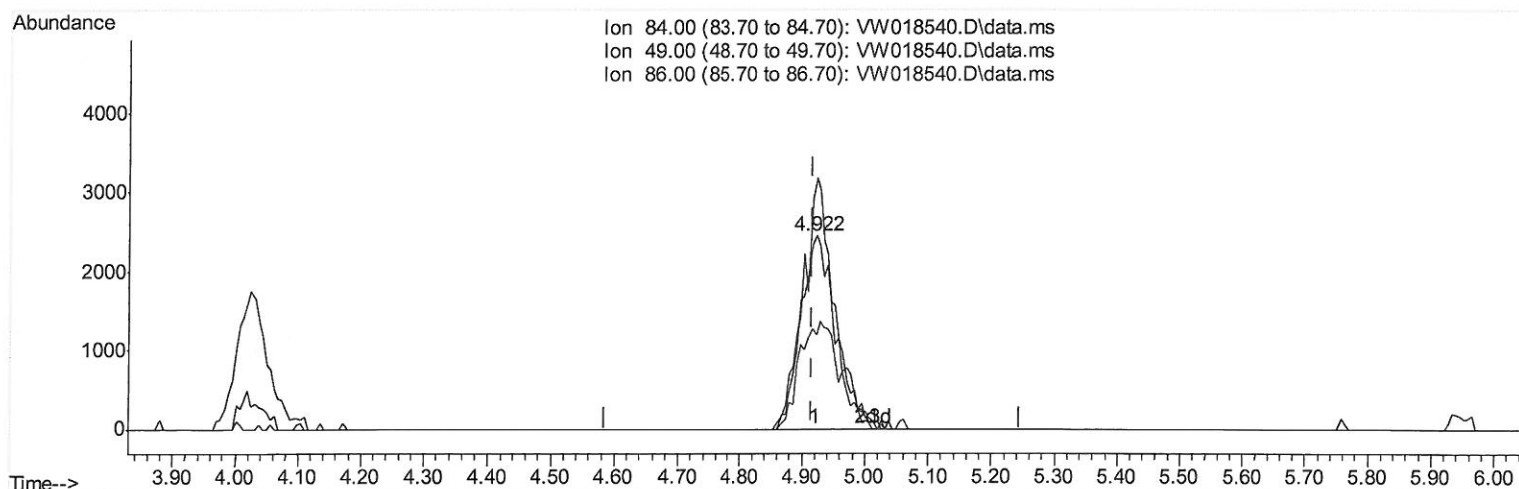

TIC: VW018540.D\data.ms

(16) Methylene chloride (T)

4.922min (+ 0.006) 1.39 ug/L m

response 9553

Ion	Exp%	Act%
84.00	100.00	100.00
49.00	106.30	130.19
86.00	65.90	48.50
0.00	0.00	0.00

7m0
4/9/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040121\
 Data File : VW018540.D
 Acq On : 01 Apr 2021 16:57
 Operator : SY/VA
 Sample : M1896-07
 Misc : 5.66G/10ML/MSVOA_W/SOIL
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG583

Manual Integrations
 APPROVED

MMDadoda
 4/6/2021 1:05:41 PM

Quant Time: Apr 02 03:33:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 02 03:28:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	417675	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	363409	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	141179	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	162084	27.89	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 111.56%			
7) Chloroethane-d5	2.891	69	127631	25.09	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 100.36%			
10) 1,1-Dichloroethene-d2	4.025	63	168950	16.83	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 67.32%			
20) 2-Butanone-d5	7.074	46	88989	68.77	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 137.54%#			
24) Chloroform-d	7.653	84	250396	23.54	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 94.16%			
26) 1,2-Dichloroethane-d4	8.305	65	165291	26.62	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 106.48%			
29) Benzene-d6	8.275	84	487001	25.21	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 100.84%			
33) 1,2-Dichloropropane-d6	9.274	67	145780	26.16	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 104.64%			
37) Toluene-d8	10.323	98	454215	24.42	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 97.68%			
38) trans-1,3-Dichloroprop...	10.579	79	63230	22.00	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 88.00%			
39) 2-Hexanone-d5	10.927	63	71281	65.36	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 130.72%			
48) 1,1,2,2-Tetrachloroeth...	12.695	84	145171	29.12	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 116.48%			
61) 1,2-Dichlorobenzene-d4	13.853	152	116521	23.22	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 92.88%			
Target Compounds						
13) Acetone	4.129	43	8746m	9.41	ug/L	
16) Methylene chloride	4.922	84	9553m	1.39	ug/L	
44) Toluene	10.390	91	7030	0.29	ug/L	

Qvalue

MD
 92 4/9/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed