

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040219\
Quantitation Report (QT Reviewed)


Data File : VW009648.D
Acq On : 02 Apr 2019 11:00
Operator : SY/VA
Sample : VW0402SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
VBLK20

Manual Integrations
APPROVED

MMDadoda
4/9/2019 5:12:30 PM

Quant Time: Apr 03 04:18:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 03 04:08:07 2019
Response via : Initial Calibration

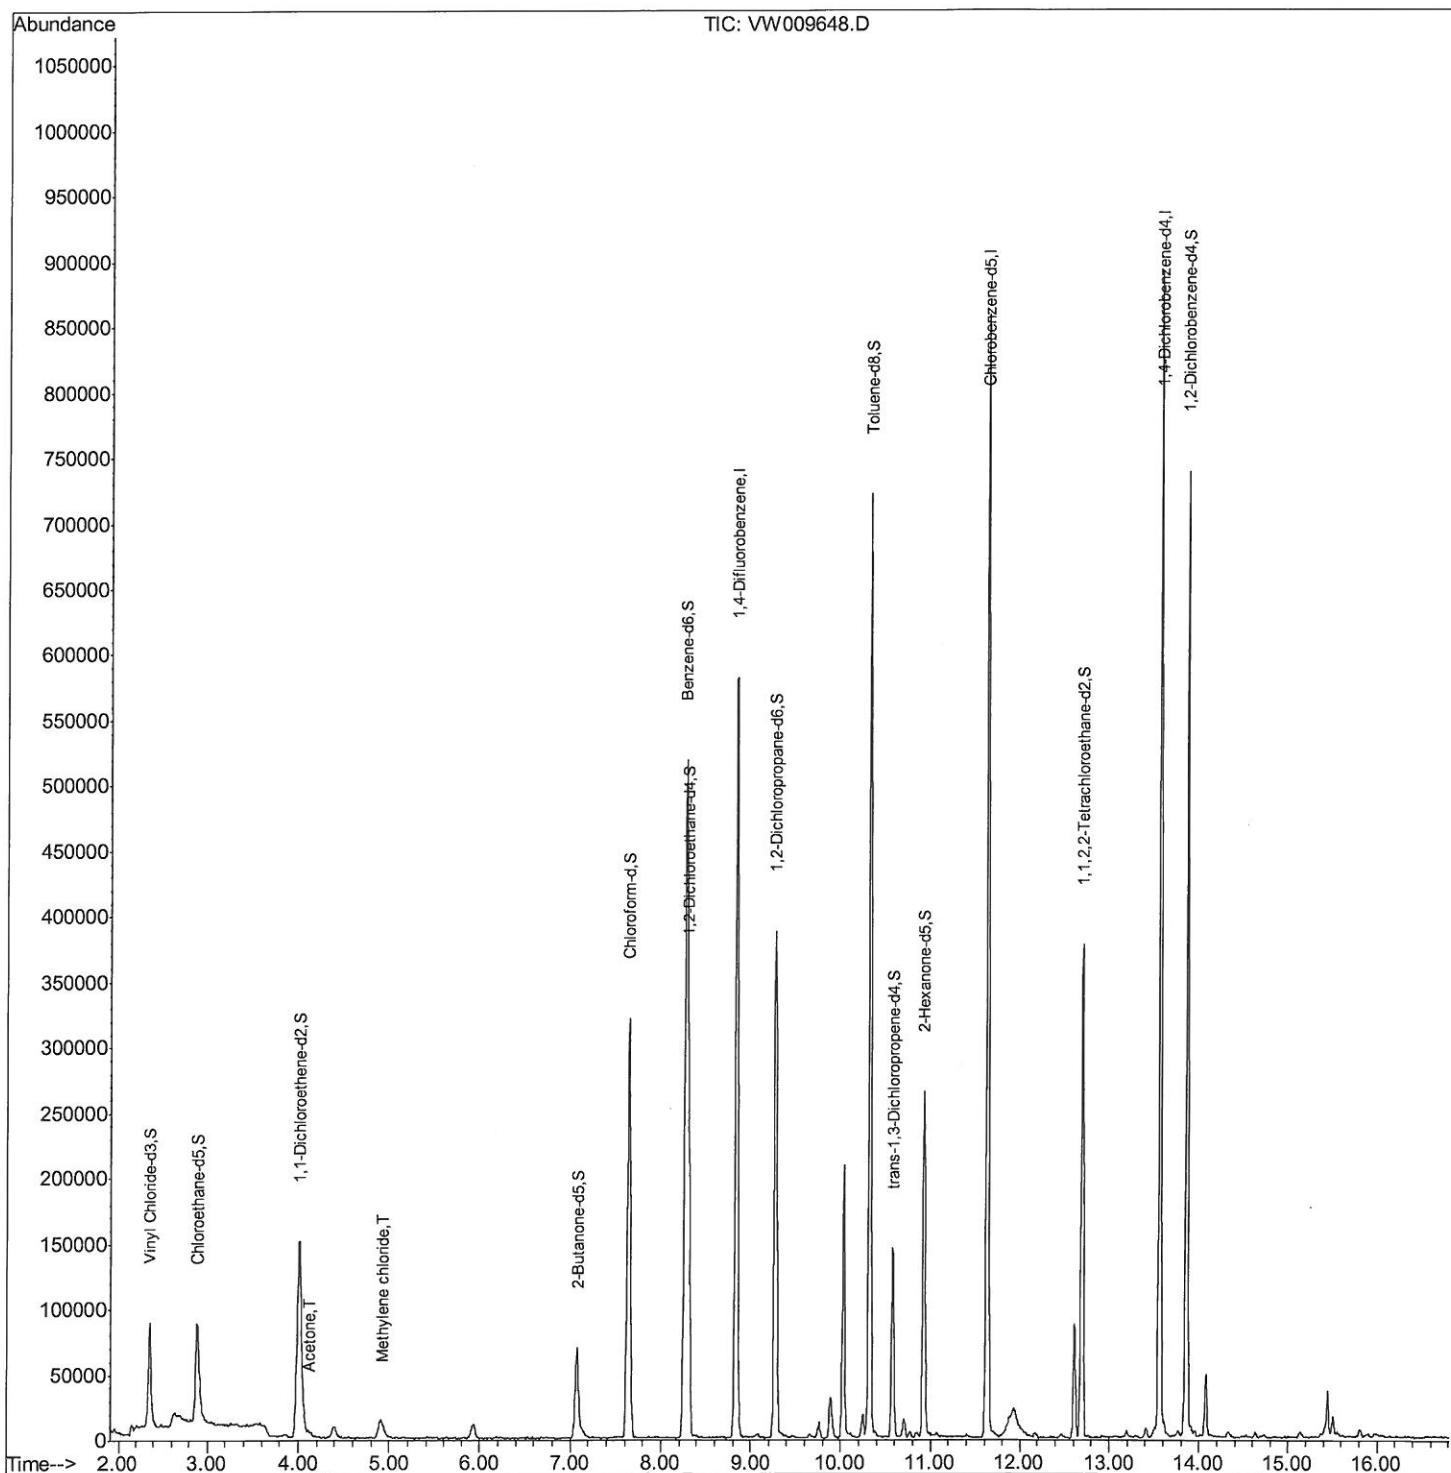

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040219\
Quantitation Report (Qedit)




Data File : VW009648.D
Acq On : 02 Apr 2019 11:00
Operator : SY/VA
Sample : VW0402SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK20

Manual Integrations
APPROVED

MMDadoda
4/9/2019 5:12:30 PM

Quant Time: Apr 03 04:10:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 03 04:08:07 2019
Response via : Initial Calibration

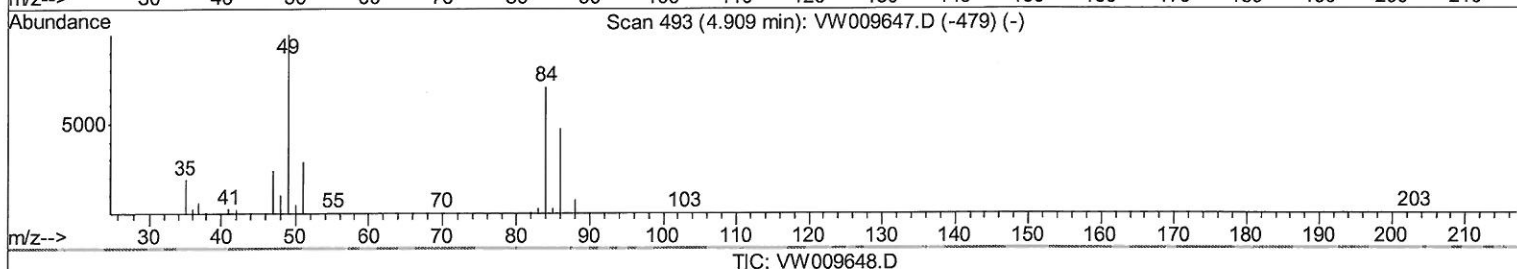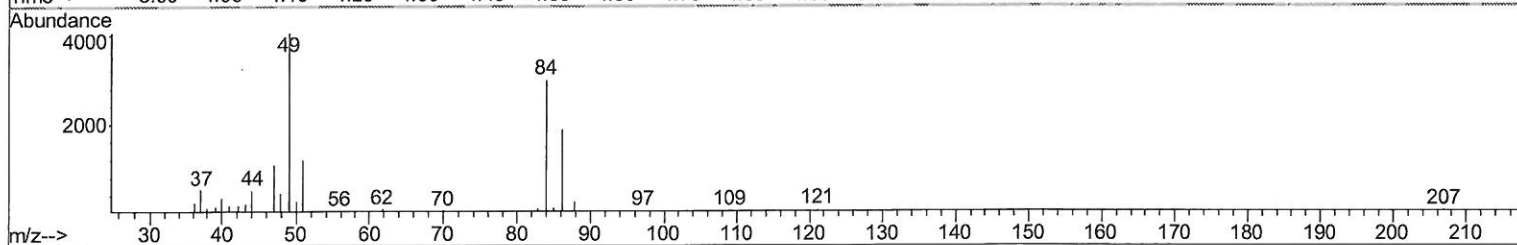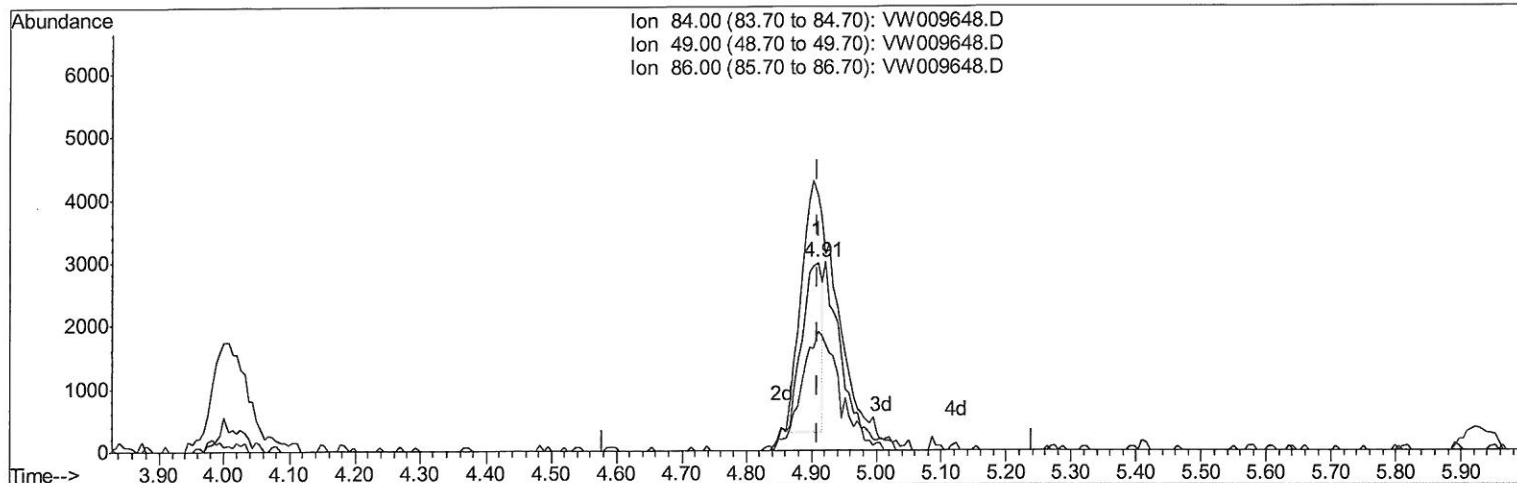

(16) Methylene chloride (T)

4.909min (+0.000) 0.86ug/L

response 5713

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	135.36
86.00	63.50	63.43
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040219\
Quantitation Report (Qedit)




Data File : VW009648.D
Acq On : 02 Apr 2019 11:00
Operator : SY/VA
Sample : VW0402SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
VBLK20

Manual Integrations
APPROVED

MMDadoda
4/9/2019 5:12:30 PM

Quant Time: Apr 03 04:10:55 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 03 04:08:07 2019
Response via : Initial Calibration

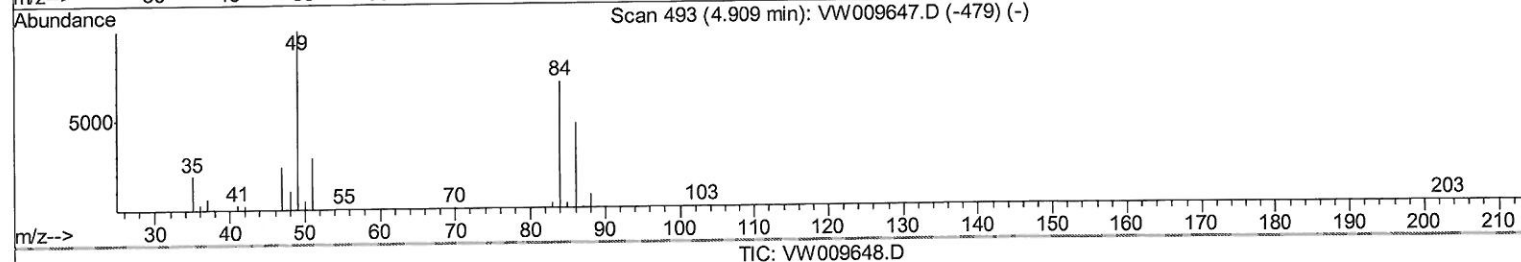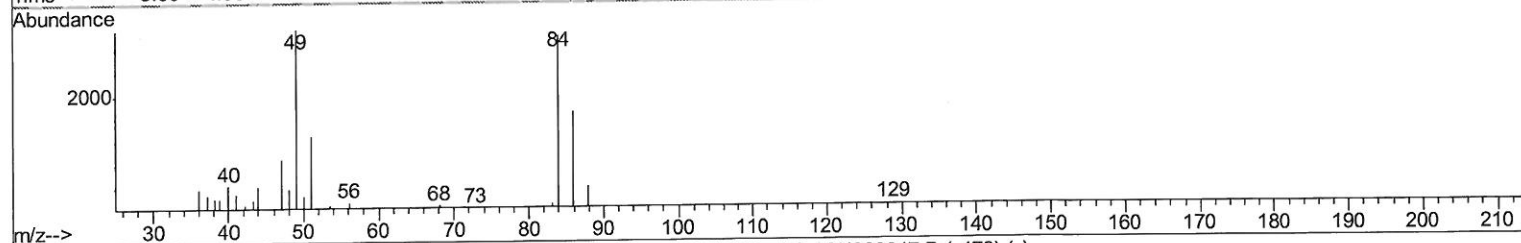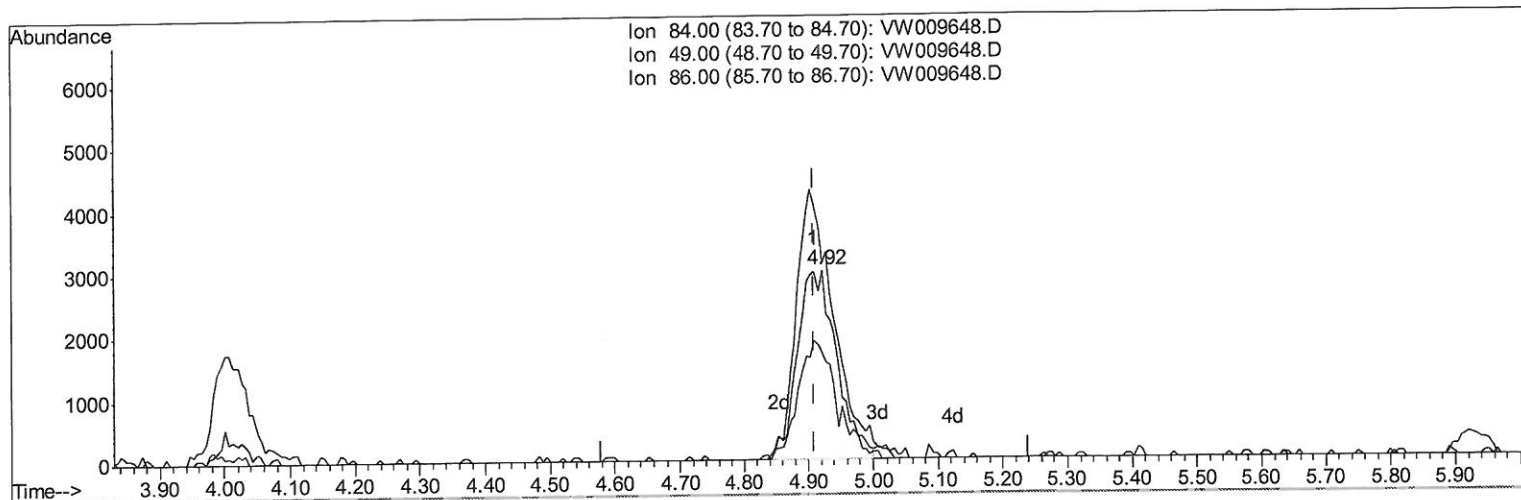

(16) Methylene chloride (T)

4.922min (+0.012) 1.90ug/L m

response 12645

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	103.89
86.00	63.50	56.01
0.00	0.00	0.00

7 MO
4/13/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040219\
Quantitation Report (QT Reviewed)

Data File : VW009648.D
Acq On : 02 Apr 2019 11:00
Operator : SY/VA
Sample : VW0402SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
VBLK20

Quant Time: Apr 03 04:18:05 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 03 04:08:07 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
4/9/2019 5:12:30 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	456523	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	434490	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	206359	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	99951	18.32	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	73.28%
7) Chloroethane-d5	2.89	69	109468	17.15	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.60%
10) 1,1-Dichloroethene-d2	4.01	63	184469	15.64	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.56%
20) 2-Butanone-d5	7.07	46	116963	51.84	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.68%
24) Chloroform-d	7.64	84	286805	23.02	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.08%
26) 1,2-Dichloroethane-d4	8.30	65	179085	23.86	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.44%
29) Benzene-d6	8.27	84	506960	21.16	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.64%
33) 1,2-Dichloropropane-d6	9.27	67	164736	22.89	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.56%
37) Toluene-d8	10.32	98	454722	20.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.08%
38) trans-1,3-Dichloropropene-	10.57	79	72133	19.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.84%
39) 2-Hexanone-d5	10.92	63	83147	47.70	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.40%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	166947	23.55	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.20%
61) 1,2-Dichlorobenzene-d4	13.85	152	177566	22.44	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.76%

Target Compounds

					Qvalue
13) Acetone	4.12	43	4530	2.448	ug/L
16) Methylene chloride	4.92	84	12645m	1.899	ug/L

90
7m0
4/13/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed