

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040219\
Quantitation Report (QT/LSC Reviewed)


Data File : VW009651.D
Acq On : 02 Apr 2019 12:43
Operator : SY/VA
Sample : K2119-11
Misc : 5.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5A5

Quant Time: Apr 03 04:33:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 03 04:08:07 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
4/9/2019 5:12:35 PM

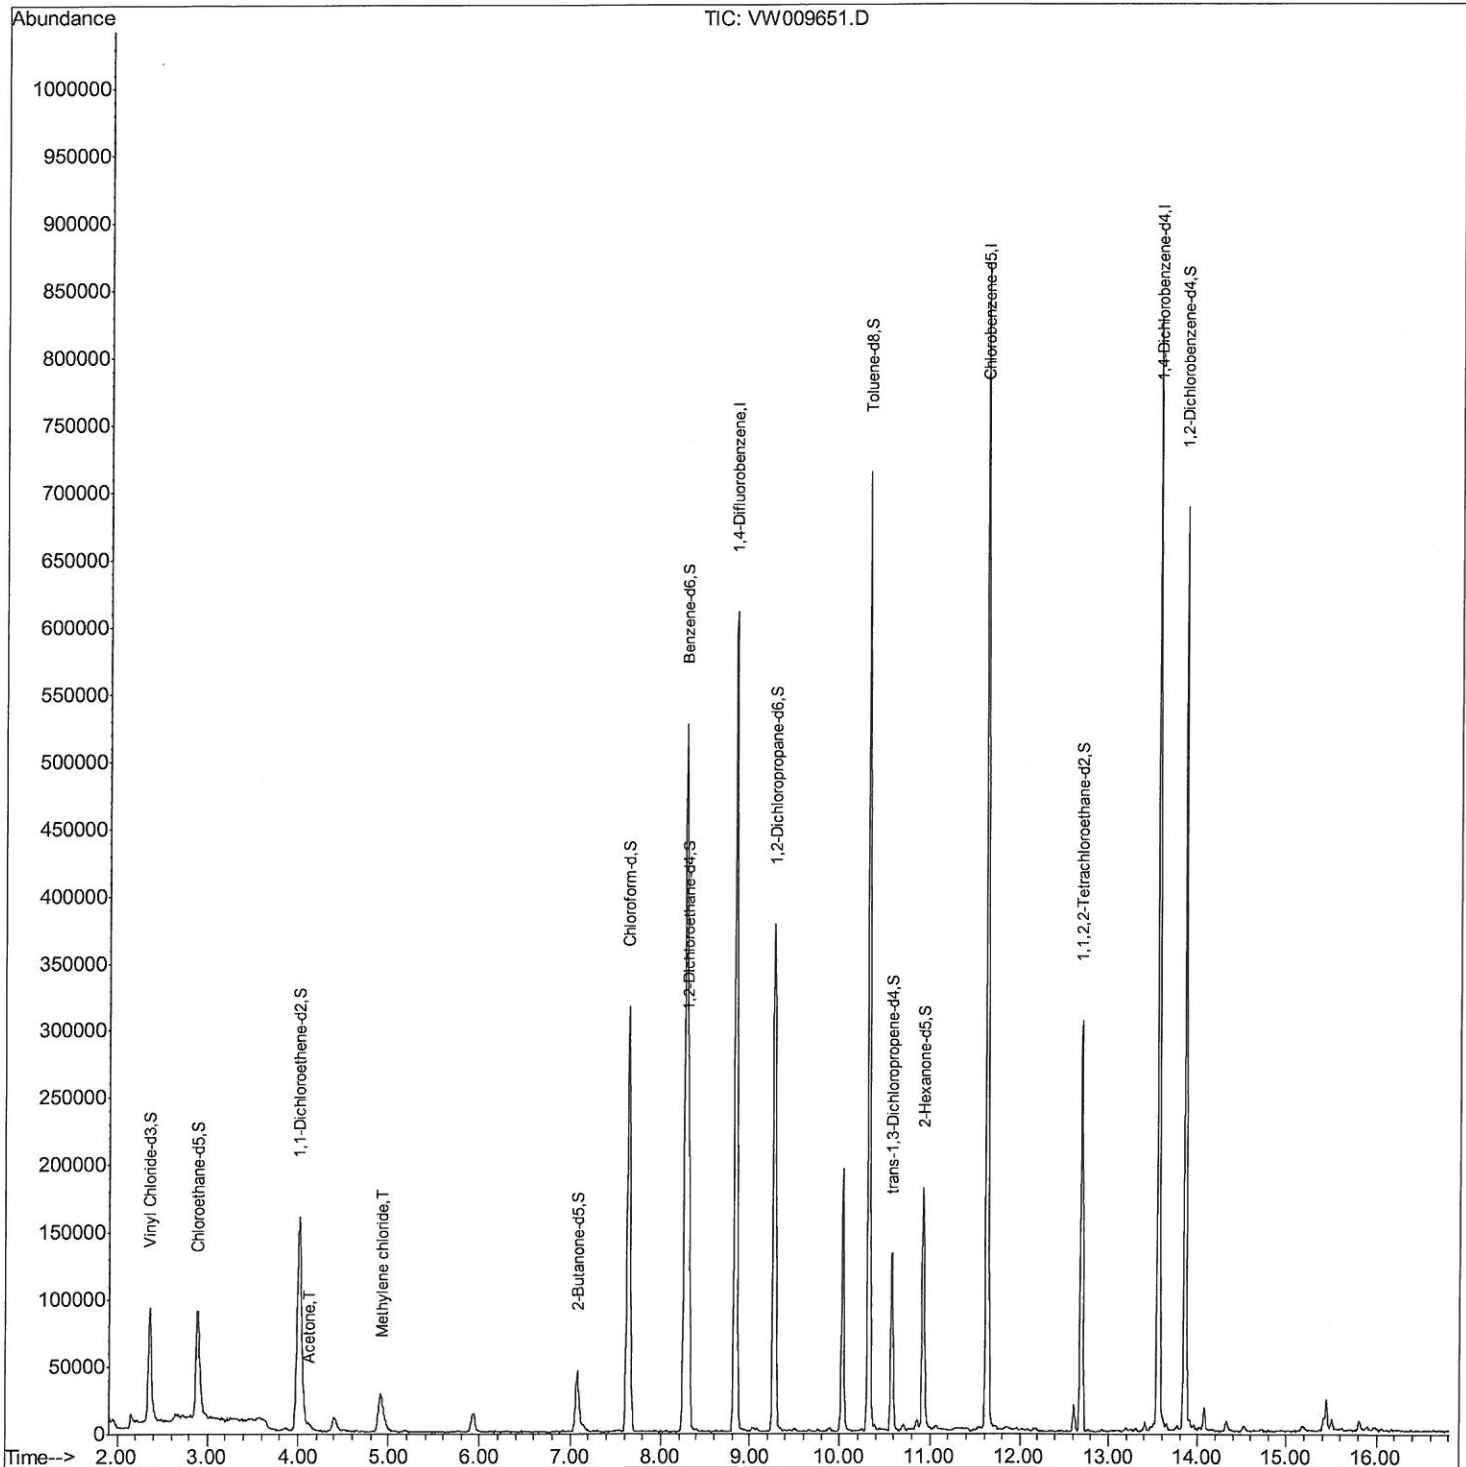

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040219\
Quantitation Report (Qedit)




Data File : VW009651.D
Acq On : 02 Apr 2019 12:43
Operator : SY/VA
Sample : K2119-11
Misc : 5.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5A5

Manual Integrations
APPROVED

MMDadoda
4/9/2019 5:12:35 PM

Quant Time: Apr 03 04:11:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 03 04:08:07 2019
Response via : Initial Calibration

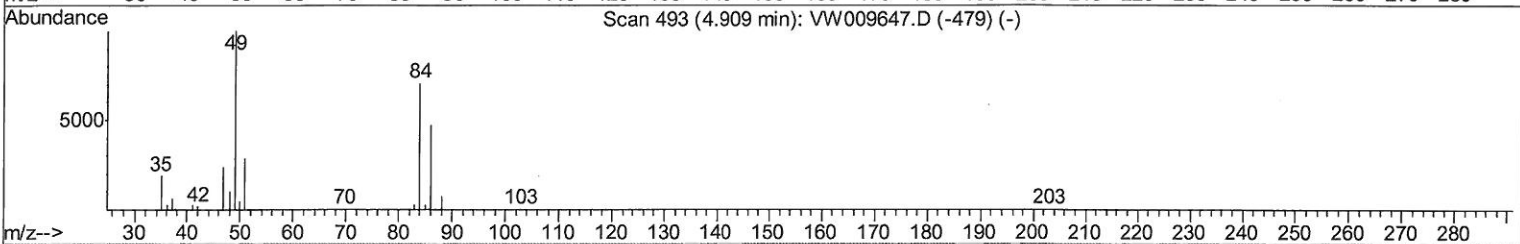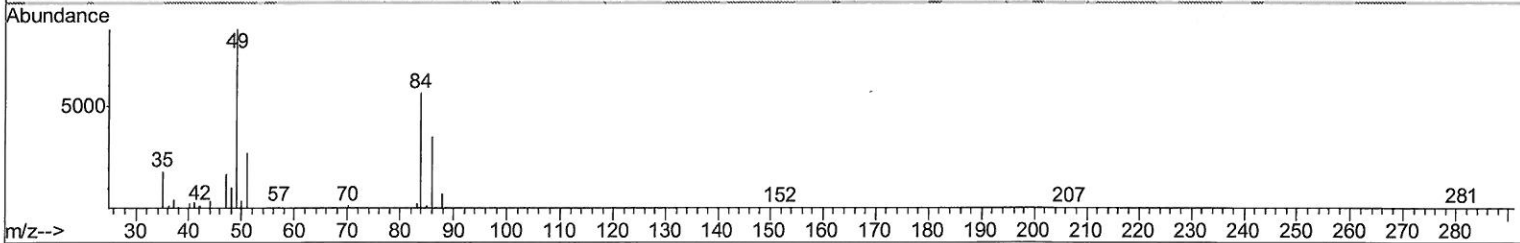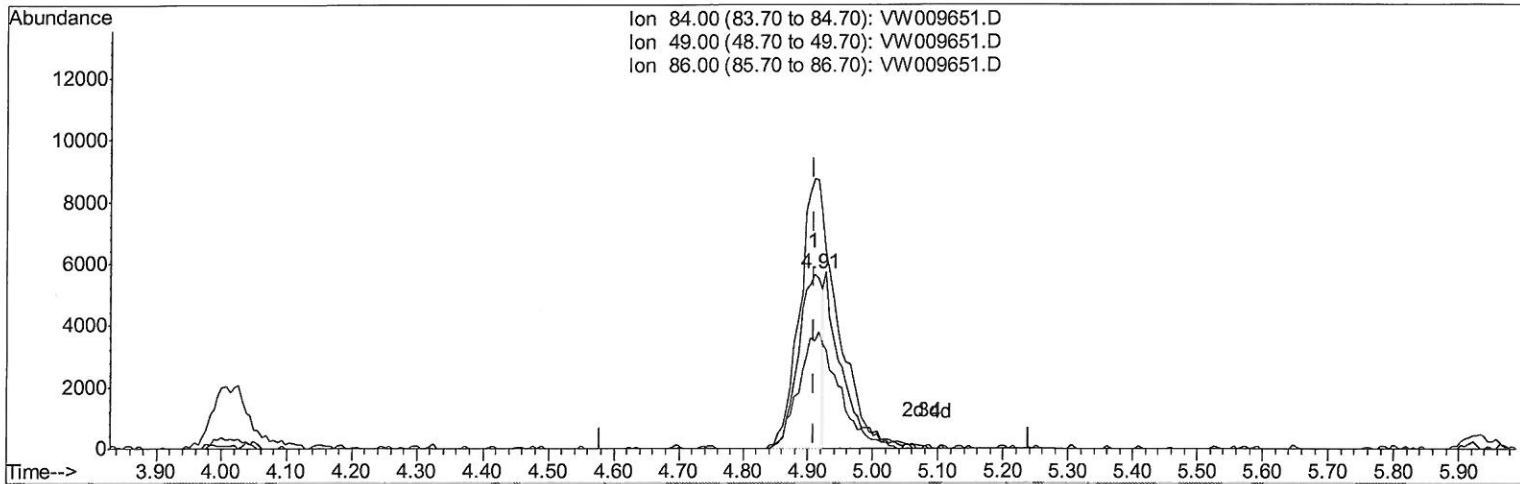

TIC: VW009651.D

(16) Methylene chloride (T)

4.910min (+0.000) 2.10ug/L

response 14473

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	154.81
86.00	63.50	61.93
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040219\
Quantitation Report (Qedit)




Data File : VW009651.D
Acq On : 02 Apr 2019 12:43
Operator : SY/VA
Sample : K2119-11
Misc : 5.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BF5A5

Manual Integrations
APPROVED

MMDadoda
4/9/2019 5:12:35 PM

Quant Time: Apr 03 04:11:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 03 04:08:07 2019
Response via : Initial Calibration

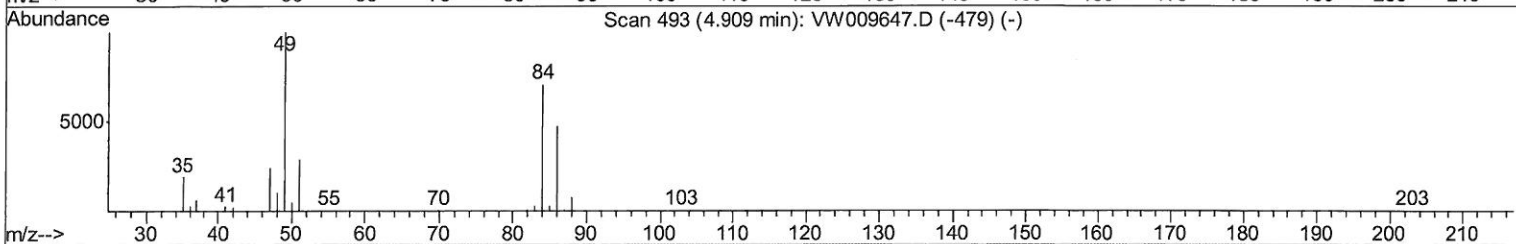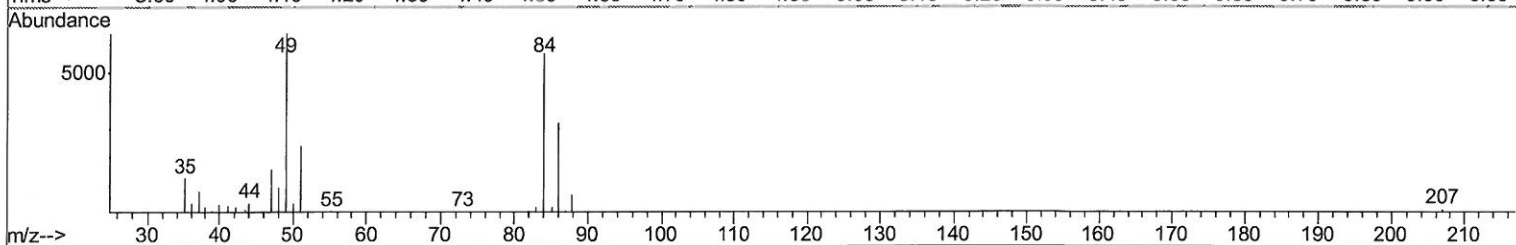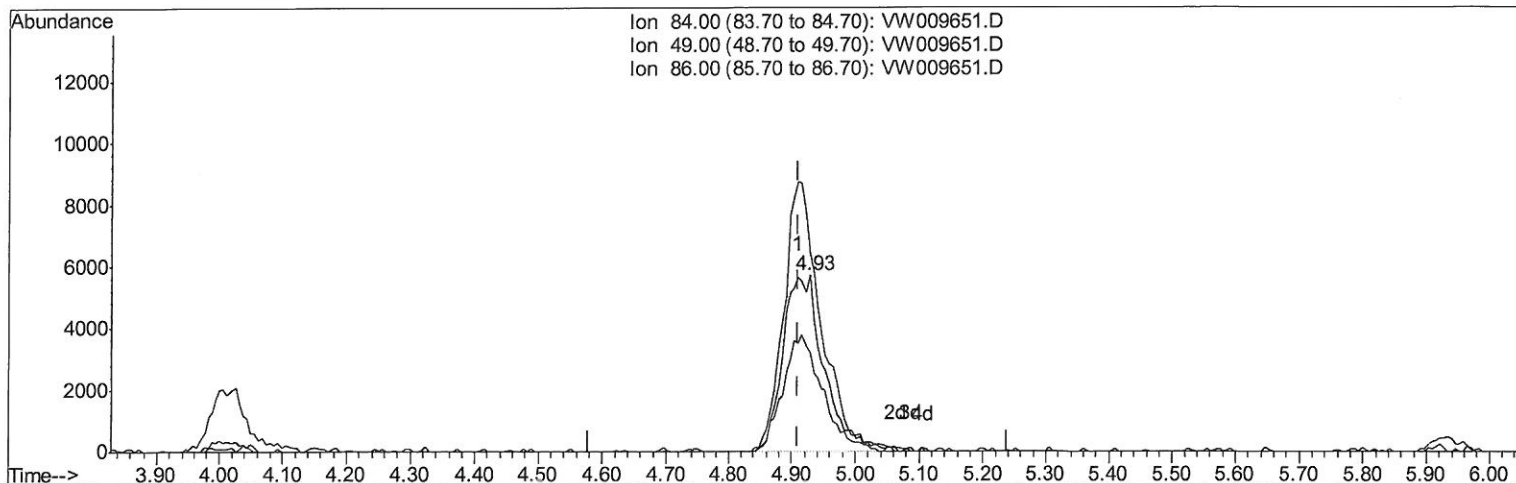

TIC: VW009651.D

(16) Methylene chloride (T)

4.928min (+0.019) 3.63ug/L m

response 25035

Ion	Exp%	Act%
84.00	100	100
49.00	137.10	111.77
86.00	63.50	56.71
0.00	0.00	0.00

7 M2
4/13/19

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040219\
Quantitation Report (QT/LSC Reviewed)

Data File : VW009651.D
Acq On : 02 Apr 2019 12:43
Operator : SY/VA
Sample : K2119-11
Misc : 5.70G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
BF5A5

Manual Integrations
APPROVED

MMDadoda
4/9/2019 5:12:35 PM

Quant Time: Apr 03 04:33:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM031419S.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 03 04:08:07 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	473360	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	446893	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	198008	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	123554	21.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.36%
7) Chloroethane-d5	2.89	69	118228	17.86	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.44%
10) 1,1-Dichloroethene-d2	4.01	63	197738	16.17	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.68%
20) 2-Butanone-d5	7.07	46	78689	33.64	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	67.28%
24) Chloroform-d	7.64	84	283138	21.92	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.68%
26) 1,2-Dichloroethane-d4	8.31	65	164963	21.20	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.80%
29) Benzene-d6	8.27	84	501578	20.35	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.40%
33) 1,2-Dichloropropane-d6	9.27	67	161291	21.79	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.16%
37) Toluene-d8	10.32	98	436520	19.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.64%
38) trans-1,3-Dichloropropene-	10.58	79	66640	17.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.72%
39) 2-Hexanone-d5	10.93	63	52360	29.21	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	58.42%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	133608	18.33	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	73.32%
61) 1,2-Dichlorobenzene-d4	13.85	152	166736	21.96	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.84%

Target Compounds

				Qvalue	
13) Acetone	4.12	43	4457	2.323 ug/L	890
16) Methylene chloride	4.93	84	25035m	3.627 ug/L	7713/119

(#) = qualifier out of range (m) = manual integration (+) = signals summed