

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040320\
 Data File : VW015153.D
 Acq On : 03 Apr 2020 18:11
 Operator : SY/VA
 Sample : L2045-05
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 VHBLK02

Manual Integrations
APPROVED

MMDadoda
 4/7/2020 9:19:22 AM

Quant Time: Apr 03 23:43:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 03 23:41:26 2020
 Response via : Initial Calibration

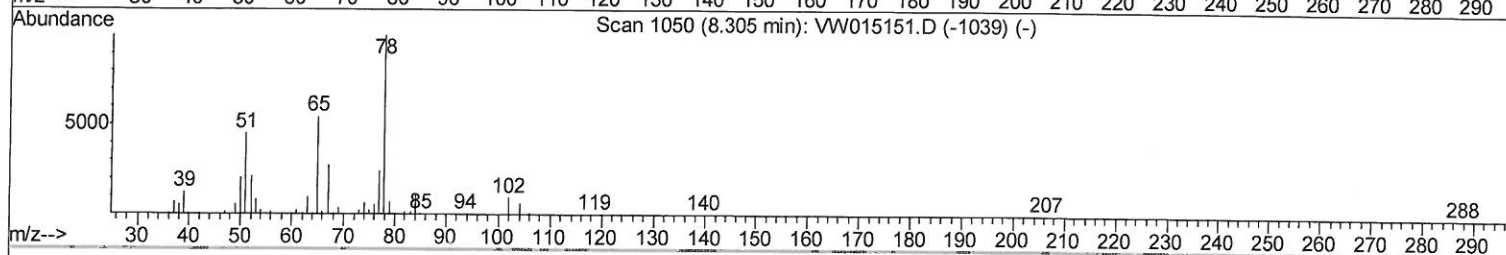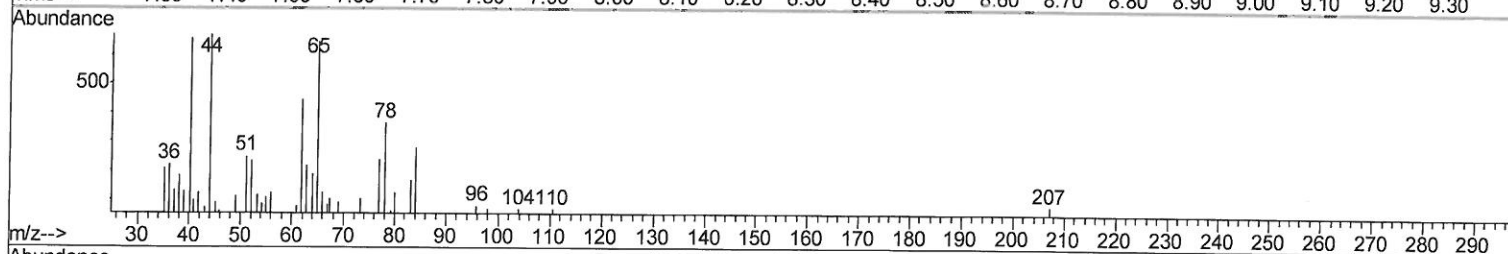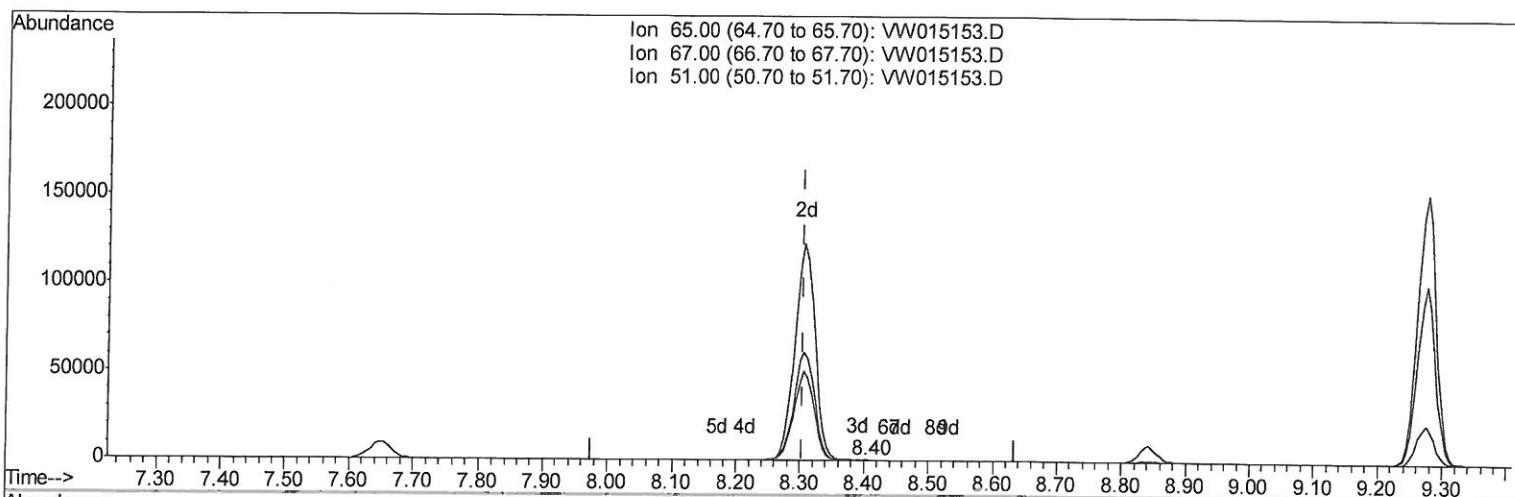

TIC: VW015153.D

(26) 1,2-Dichloroethane-d4 (S)

8.403min (+0.098) 0.03ug/L

response 336

Ion	Exp%	Act%
65.00	100	100
67.00	52.70	38.99
51.00	140.40	132.44
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040320\
 Data File : VW015153.D
 Acq On : 03 Apr 2020 18:11.
 Operator : SY/VA
 Sample : L2045-05
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 VHBLK02

Manual Integrations
APPROVED

MMDadoda
 4/7/2020 9:19:22 AM

Quant Time: Apr 03 23:43:26 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 03 23:41:26 2020
 Response via : Initial Calibration

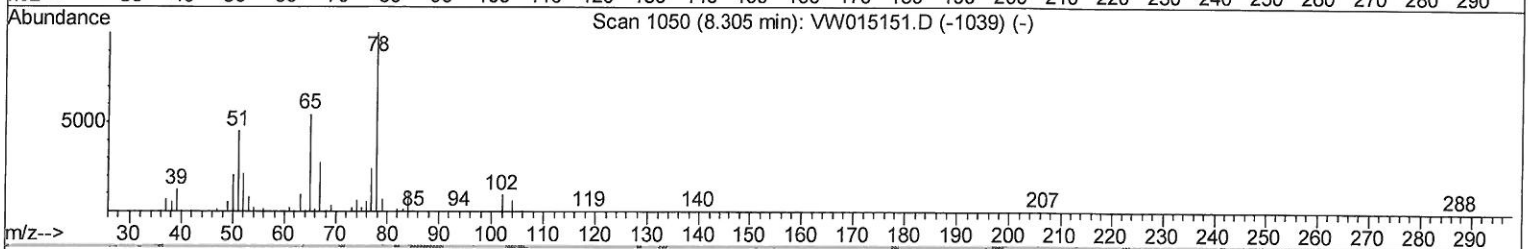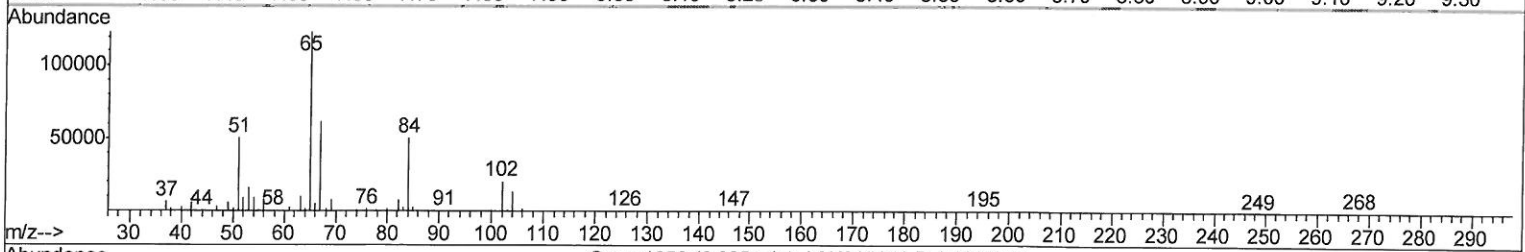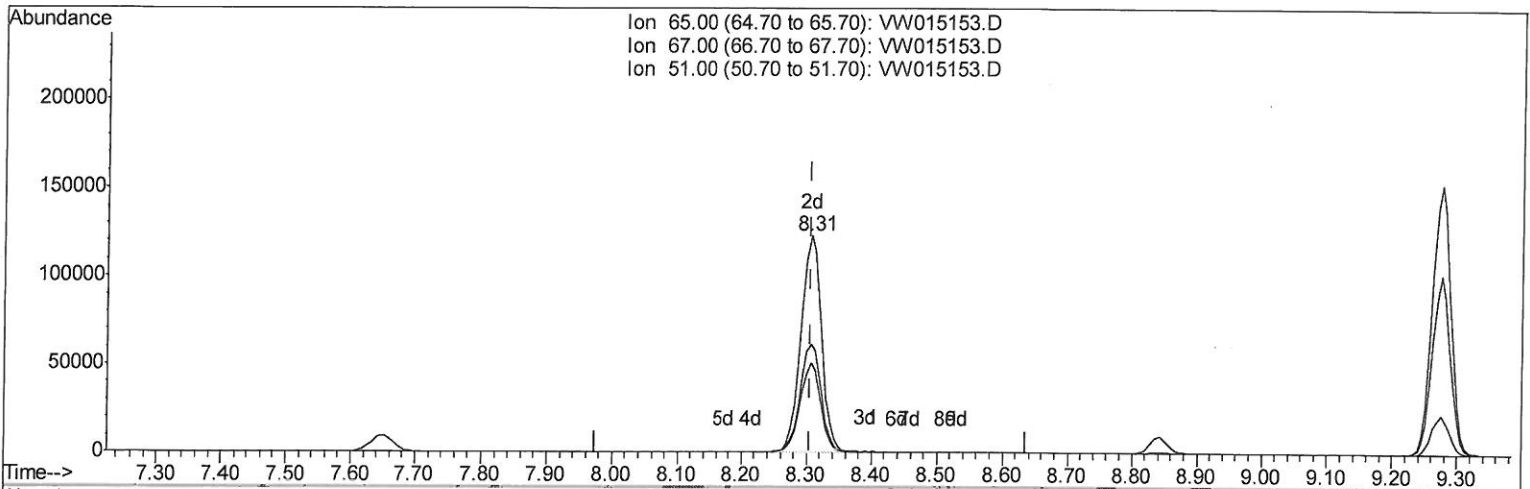

TIC: VW015153.D

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.000) 24.96ug/L m

response 270668

Ion	Exp%	Act%
65.00	100	100
67.00	52.70	0.05#
51.00	140.40	0.16#
0.00	0.00	0.00

204/08/22 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040320\
 Data File : VW015153.D
 Acq On : 03 Apr 2020 18:11
 Operator : SY/VA
 Sample : L2045-05
 Misc : 5.02G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK02

Manual Integrations
 APPROVED

MMDadoda
 4/7/2020 9:19:22 AM

Quant Time: Apr 03 23:50:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 03 23:41:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	626668	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	572300	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	203554	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	255624	23.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.48%
7) Chloroethane-d5	2.90	69	213128	23.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.52%
10) 1,1-Dichloroethene-d2	4.02	63	402052	18.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.92%
20) 2-Butanone-d5	7.08	46	115520	46.89	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.78%
24) Chloroform-d	7.65	84	465806	24.88	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.52%
26) 1,2-Dichloroethane-d4	8.31	65	270668m	24.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.84%
29) Benzene-d6	8.27	84	923002	25.20	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.80%
33) 1,2-Dichloropropane-d6	9.27	67	303360	24.93	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.72%
37) Toluene-d8	10.32	98	779620	24.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.88%
38) trans-1,3-Dichloropropene-	10.58	79	106381	22.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.36%
39) 2-Hexanone-d5	10.93	63	72904	40.57	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.14%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	181266	21.78	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.12%
61) 1,2-Dichlorobenzene-d4	13.85	152	195387	27.58	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.32%

04/08/2020

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW040320\
Data File : VW015153.D
Acq On : 03 Apr 2020 18:11
Operator : SY/VA
Sample : L2045-05
Misc : 5.02G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK02

Manual Integrations
APPROVED

MMDadoda
4/7/2020 9:19:22 AM

Quant Time: Apr 03 23:50:09 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM032520S.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 03 23:41:26 2020
Response via : Initial Calibration

