

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040424\
 Data File : VW028305.D
 Acq On : 04 Apr 2024 10:45
 Operator : SY/MD
 Sample : VW0404SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Apr 05 01:00:22 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 05 00:59:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	231627	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	214024	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	105538	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	43002	15.867	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	63.480%
7) Chloroethane-d5	2.905	69	37477	19.793	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.160%
11) 1,1-Dichloroethene-d2	4.027	65	27943	16.259	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.040%
21) 2-Butanone-d5	7.087	46	38095	47.659	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.320%
24) Chloroform-d	7.648	84	147504	21.596	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.400%
26) 1,2-Dichloroethane-d4	8.307	65	78783	20.931	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.720%
32) Benzene-d6	8.276	84	284376	21.763	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.040%
36) 1,2-Dichloropropane-d6	9.276	67	90429	24.048	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.200%
41) Toluene-d8	10.325	98	249148	20.672	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.680%
43) trans-1,3-Dichloroprop...	10.575	79	33905	19.852	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.400%
47) 2-Hexanone-d5	10.922	63	28656	46.102	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.200%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	67472	24.290	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.160%
66) 1,2-Dichlorobenzene-d4	13.848	152	90564	23.556	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	94.240%
Target Compounds						
					Qvalue	
35) Methylcyclohexane	9.276	83	21476	3.458	ug/L	# 18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040424\
Data File : VW028305.D
Acq On : 04 Apr 2024 10:45
Operator : SY/MD
Sample : VW0404SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Apr 05 01:00:22 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 05 00:59:55 2024
Response via : Initial Calibration

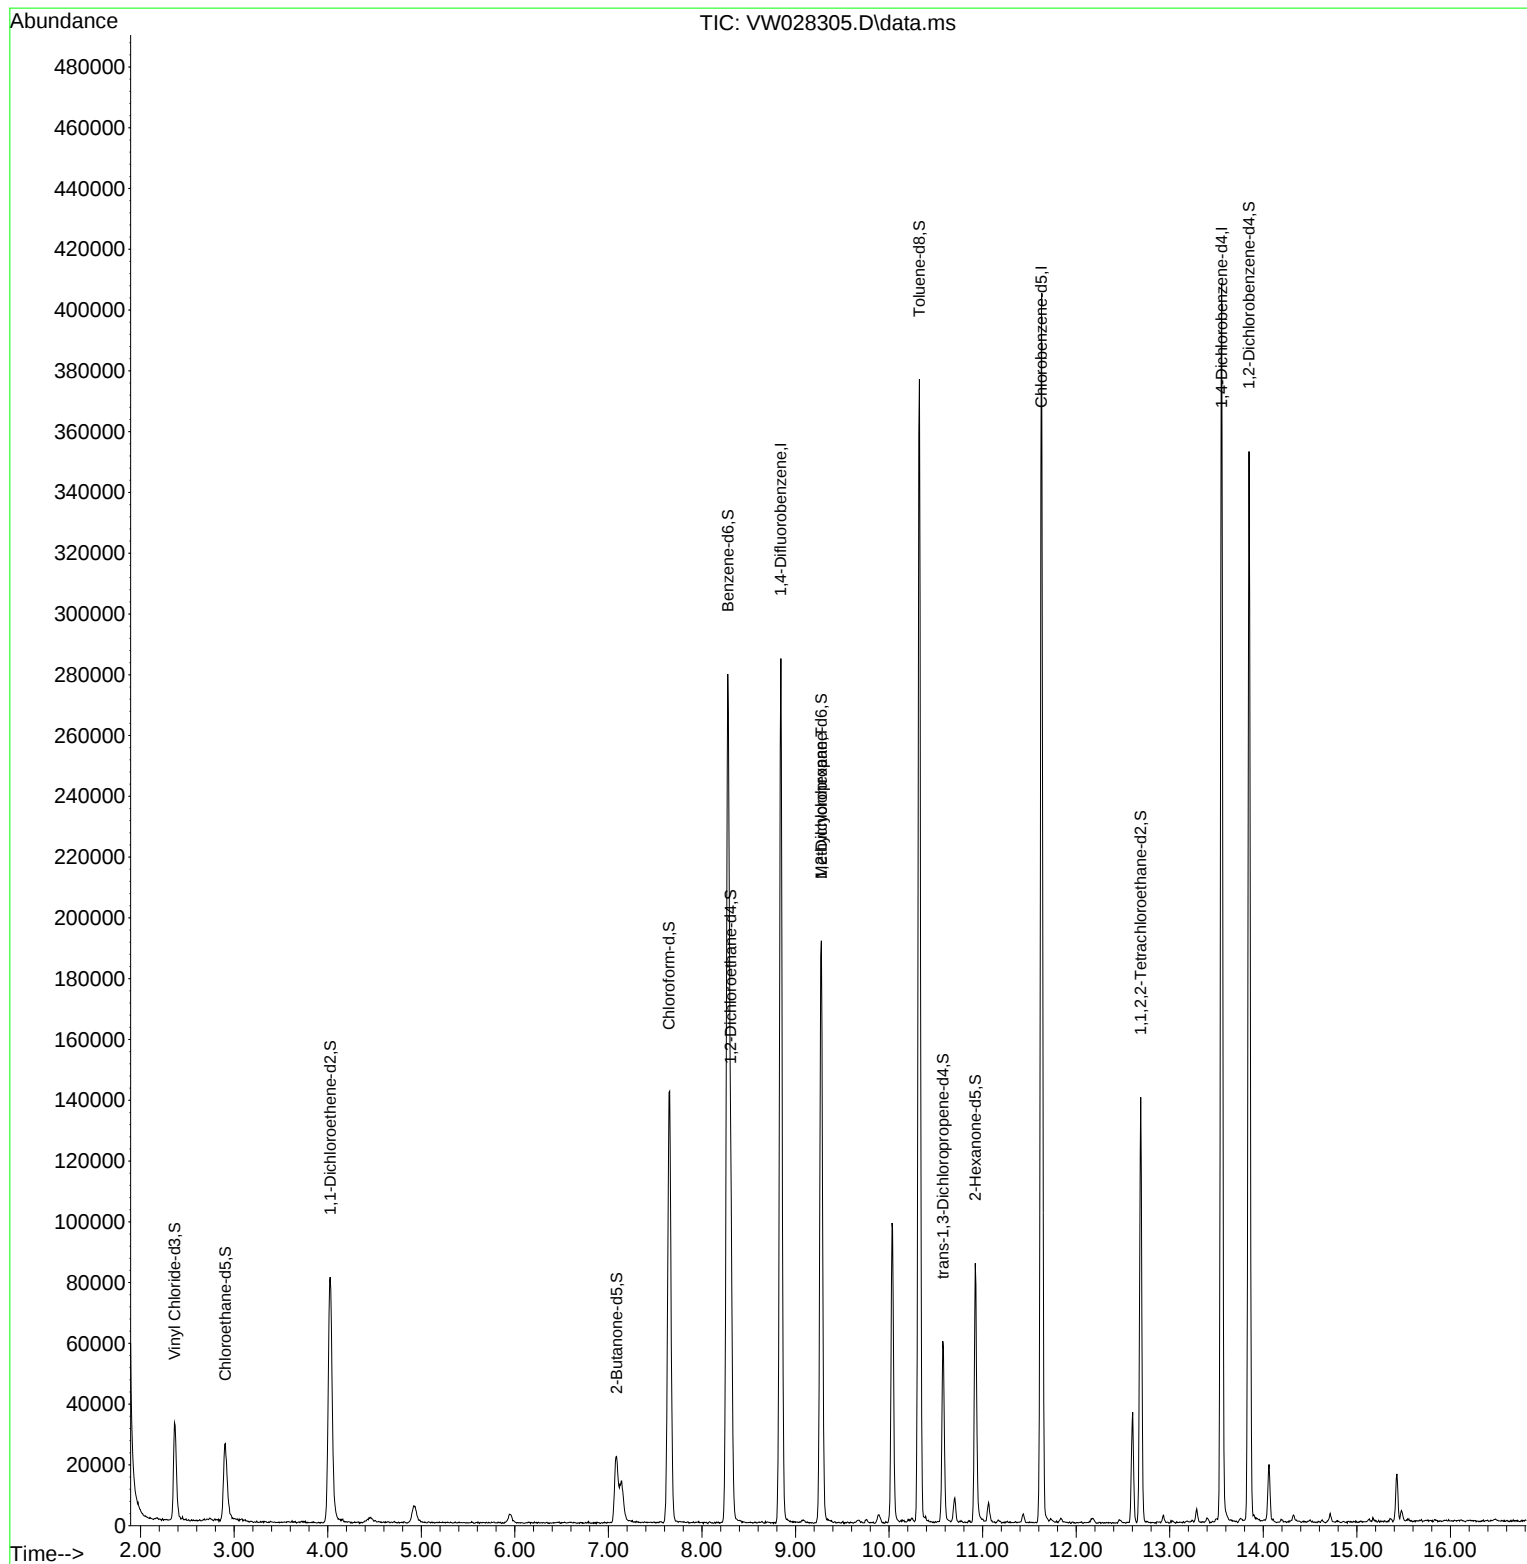

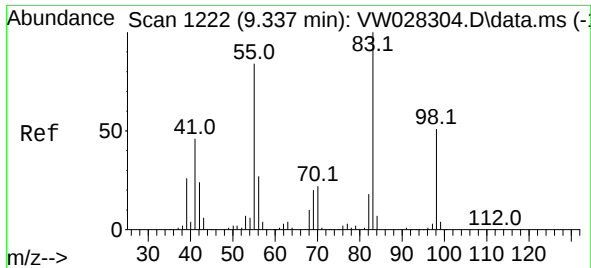

#35
Methylcyclohexane
Concen: 3.458 ug/L
RT: 9.276 min Scan# 11
Delta R.T. -0.061 min
Lab File: VW028305.D
Acq: 04 Apr 2024 10:45

Instrument :
MSVOA_W
ClientSampleId :

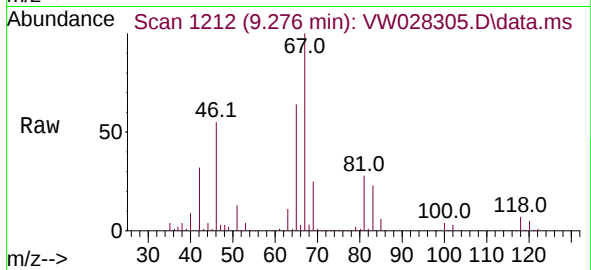

Tgt Ion:	83	Resp:	21476
Ion	Ratio	Lower	Upper
83	100		
55	0.8	64.2	96.4#
98	1.0	38.3	57.5#

