

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040424\
 Data File : VW028314.D
 Acq On : 04 Apr 2024 15:04
 Operator : SY/MD
 Sample : P1988-03
 Misc : 4.92g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E07S9

Quant Time: Apr 05 01:02:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 05 00:59:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	189685	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	183819	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	87612	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	33238	14.976	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.920%
7) Chloroethane-d5	2.899	69	27403	17.673	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.680%
11) 1,1-Dichloroethene-d2	4.027	65	21602	15.349	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.400%
21) 2-Butanone-d5	7.081	46	29817	45.551	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	91.100%
24) Chloroform-d	7.648	84	107093	19.147	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	76.600%
26) 1,2-Dichloroethane-d4	8.307	65	63048	20.454	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	81.800%
32) Benzene-d6	8.276	84	207007	18.445	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.800%
36) 1,2-Dichloropropane-d6	9.276	67	66822	20.690	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	82.760%
41) Toluene-d8	10.325	98	180861	17.472	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	69.880%
43) trans-1,3-Dichloroprop...	10.575	79	26853	18.306	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.240%
47) 2-Hexanone-d5	10.922	63	24907	46.655	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.320%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	55238	23.153	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	92.600%
66) 1,2-Dichlorobenzene-d4	13.848	152	66627	20.876	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.520%
Target Compounds						
13) Acetone	4.131	43	3756	5.168	ug/L	Qvalue 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040424\
Data File : VW028314.D
Acq On : 04 Apr 2024 15:04
Operator : SY/MD
Sample : P1988-03
Misc : 4.92g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E07S9

Quant Time: Apr 05 01:02:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 05 00:59:55 2024
Response via : Initial Calibration

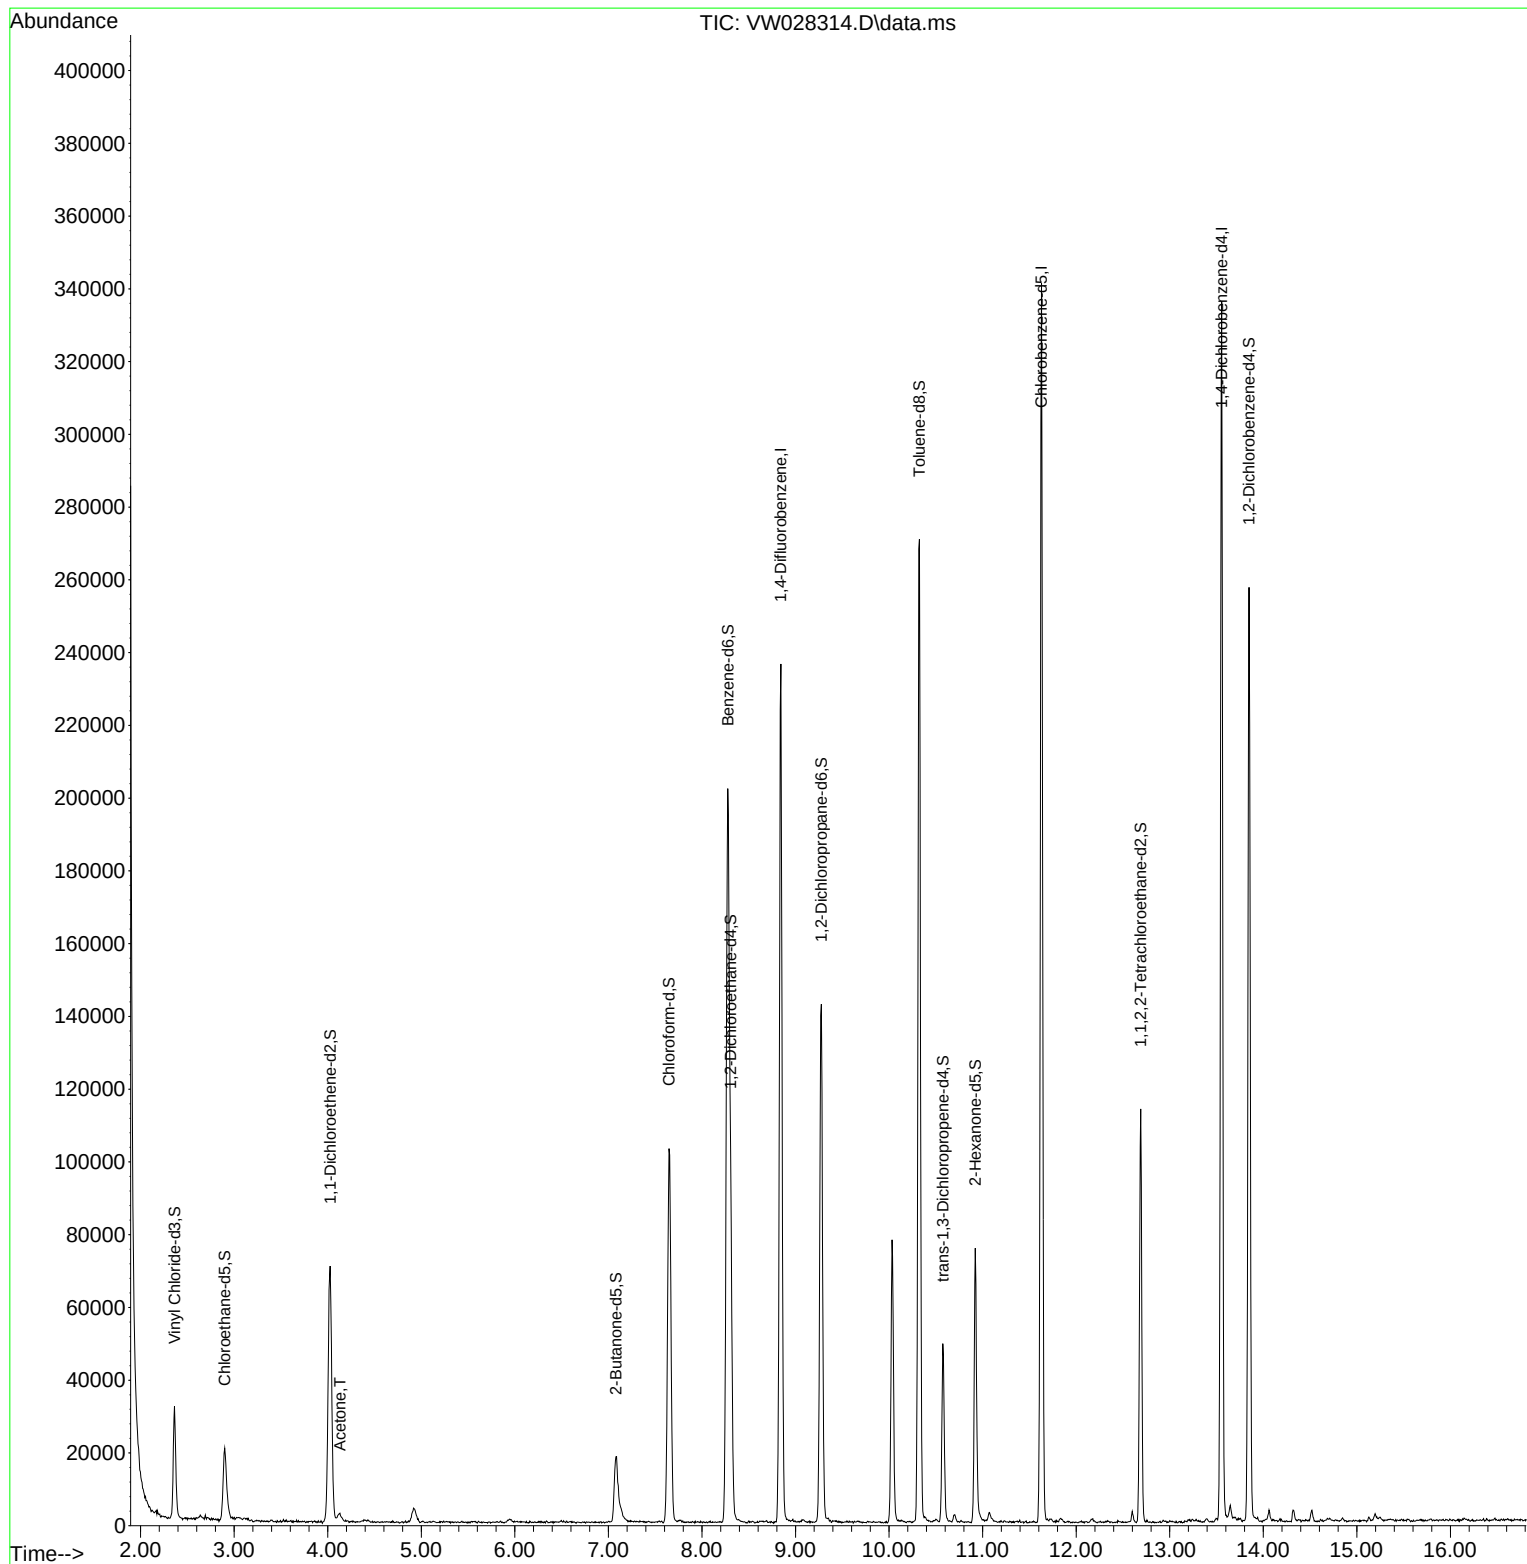

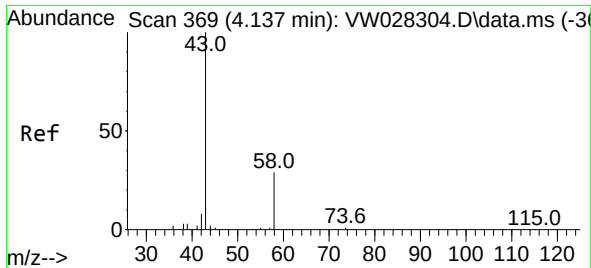

#13
 Acetone
 Concen: 5.168 ug/L
 RT: 4.131 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW028314.D
 Acq: 04 Apr 2024 15:04

Instrument :
 MSVOA_W
 ClientSampleId :
 E07S9

Tgt Ion: 43 Resp: 3756
 Ion Ratio Lower Upper
 43 100
 58 12.6 0.0 57.8

