

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040424\
 Data File : VW028325.D
 Acq On : 04 Apr 2024 19:26
 Operator : SY/MD
 Sample : P1993-12
 Misc : 4.62g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH2L3

Quant Time: Apr 05 01:05:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 05 00:59:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	358108	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	330185	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	162171	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	60091	14.341	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	57.360%
7) Chloroethane-d5	2.899	69	47956	16.382	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.520%
11) 1,1-Dichloroethene-d2	4.027	65	39296	14.789	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.160%
21) 2-Butanone-d5	7.081	46	54128	43.800	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.600%
24) Chloroform-d	7.648	84	189255	17.922	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	71.680%
26) 1,2-Dichloroethane-d4	8.307	65	102871	17.678	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	70.720%
32) Benzene-d6	8.276	84	367991	18.254	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	73.000%
36) 1,2-Dichloropropane-d6	9.270	67	114660	19.764	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	79.040%
41) Toluene-d8	10.318	98	325355	17.498	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.000%
43) trans-1,3-Dichloroprop...	10.575	79	45308	17.195	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	68.800%
47) 2-Hexanone-d5	10.922	63	43027	44.870	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.740%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	91417	21.332	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.320%
66) 1,2-Dichlorobenzene-d4	13.848	152	115742	19.592	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.360%
Target Compounds						
16) Methylene chloride	4.917	84	14801	2.716	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040424\
Data File : VW028325.D
Acq On : 04 Apr 2024 19:26
Operator : SY/MD
Sample : P1993-12
Misc : 4.62g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH2L3


Quant Time: Apr 05 01:05:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 05 00:59:55 2024
Response via : Initial Calibration

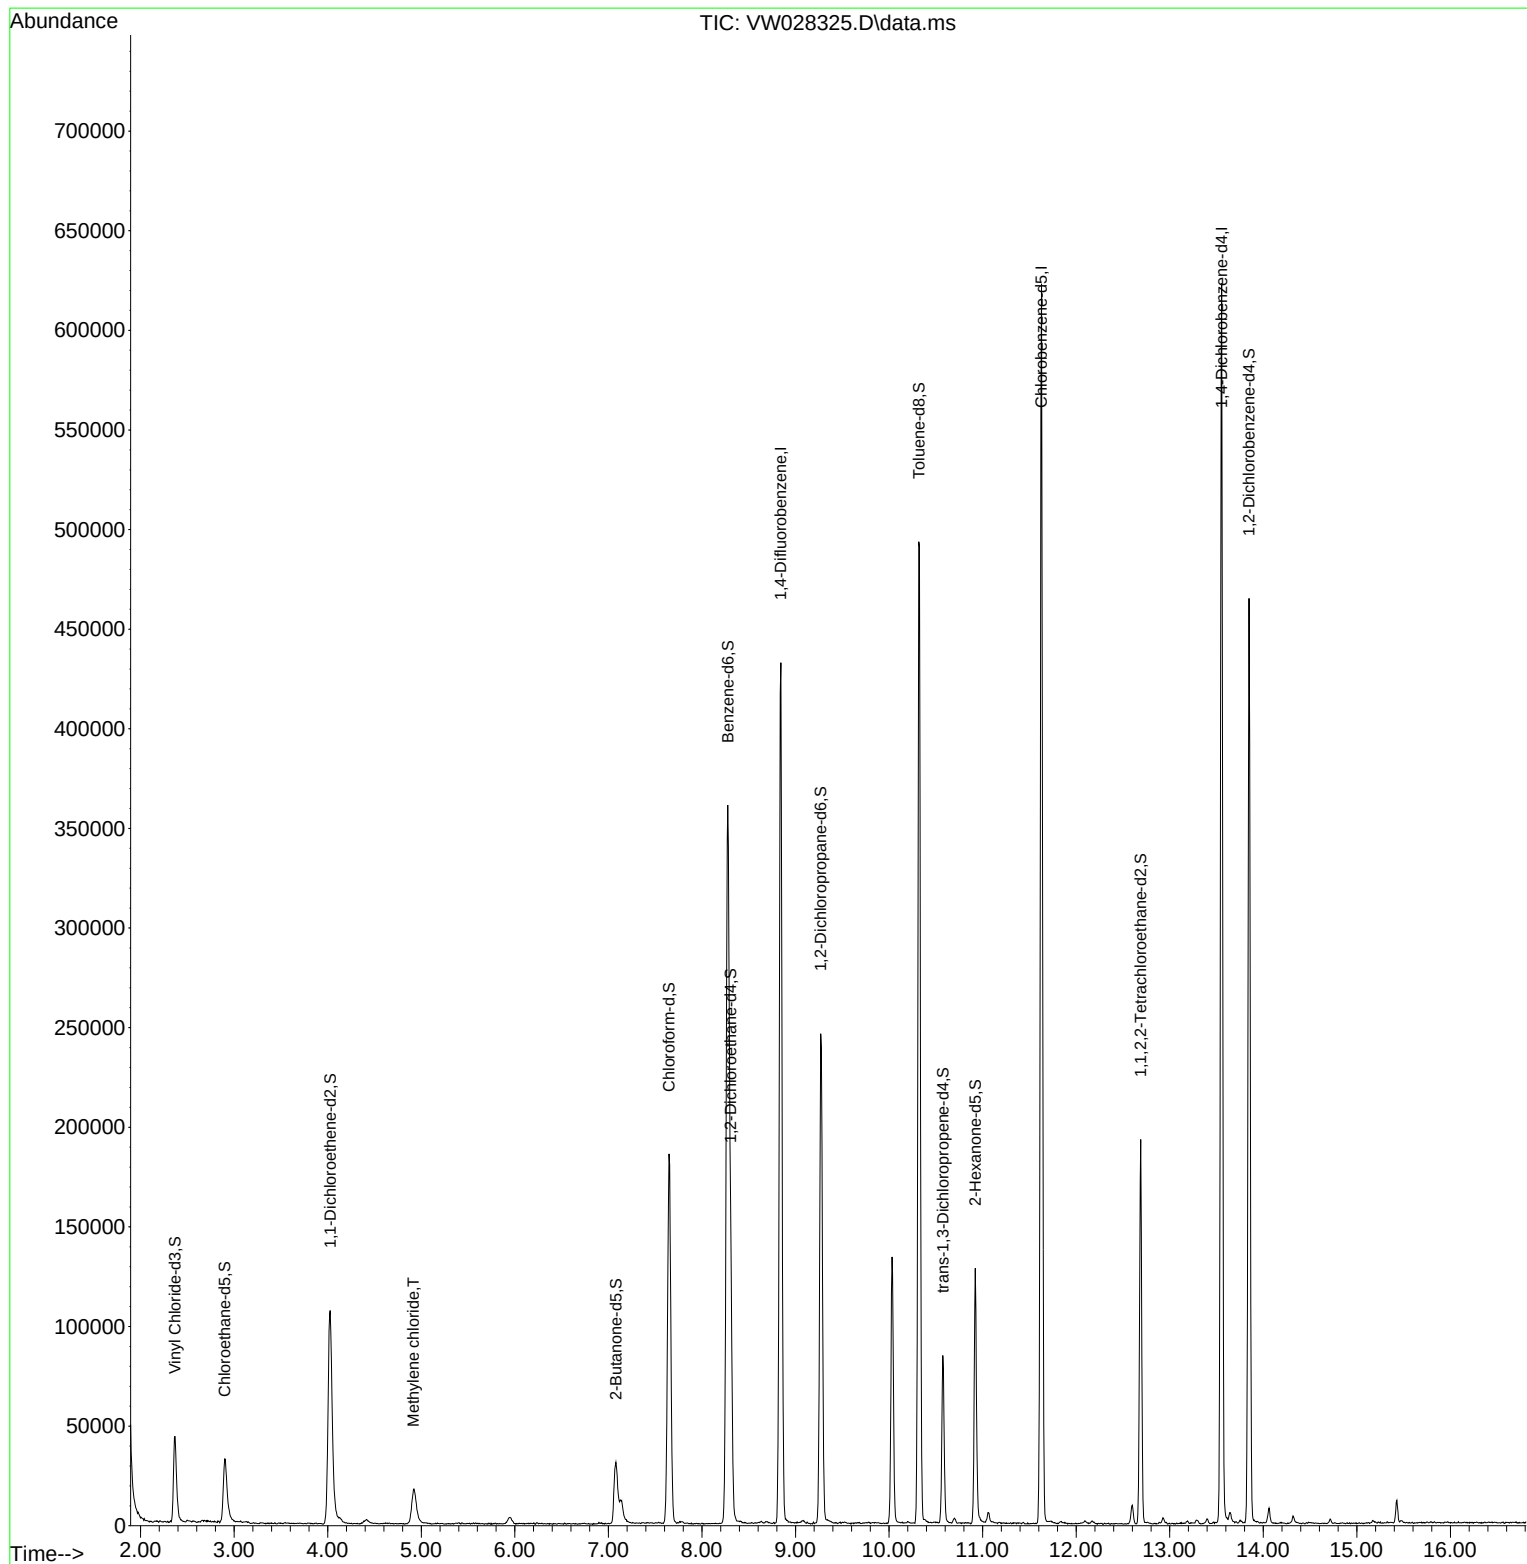

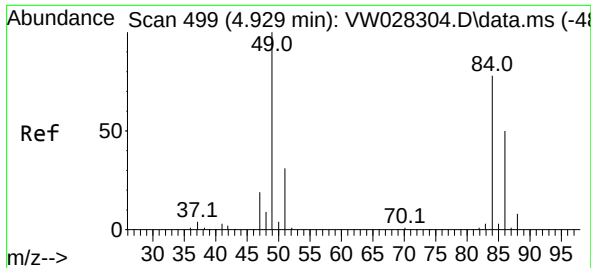

#16
Methylene chloride
Concen: 2.716 ug/L
RT: 4.917 min Scan# 49
Delta R.T. -0.012 min
Lab File: VW028325.D
Acq: 04 Apr 2024 19:26

Instrument :
MSVOA_W
ClientSampleId :
BH2L3

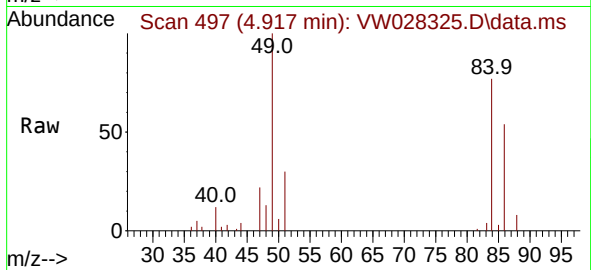

Tgt Ion:	84	Resp:	14801
Ion	Ratio	Lower	Upper
84	100		
86	70.2	43.1	80.1
49	130.5	89.4	166.0

