

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040521\
 Data File : VW018554.D
 Acq On : 05 Apr 2021 13:29
 Operator : SY/VA
 Sample : M1896-09
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 4/6/2021 9:36:30 AM

Quant Time: Apr 06 01:18:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 06 01:17:41 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	473665	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	440489	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.554	152	211108	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	192987	29.28	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 117.12%			
7) Chloroethane-d5	2.891	69	150821	26.14	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 104.56%			
10) 1,1-Dichloroethene-d2	4.013	63	211539	18.59	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 74.36%			
20) 2-Butanone-d5	7.074	46	76418	52.08	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 104.16%			
24) Chloroform-d	7.647	84	320263	26.55	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 106.20%			
26) 1,2-Dichloroethane-d4	8.305	65	190887m	27.10	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 108.40%			
29) Benzene-d6	8.275	84	623989	26.65	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 106.60%			
33) 1,2-Dichloropropane-d6	9.268	67	180578	26.73	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 106.92%			
37) Toluene-d8	10.323	98	602690	26.73	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 106.92%			
38) trans-1,3-Dichloroprop...	10.579	79	81923	23.52	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 94.08%			
39) 2-Hexanone-d5	10.920	63	62084	46.97	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 93.94%			
48) 1,1,2,2-Tetrachloroeth...	12.688	84	153953	25.48	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 101.92%			
61) 1,2-Dichlorobenzene-d4	13.853	152	201920	26.90	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 107.60%			
Target Compounds					Qvalue	
13) Acetone	4.123	43	3337m	3.17	ug/L	
16) Methylene chloride	4.922	84	13734	1.77	ug/L	95
44) Toluene	10.384	91	10300	0.36	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040521\
Data File : VW018554.D
Acq On : 05 Apr 2021 13:29
Operator : SY/VA
Sample : M1896-09
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

MMDadoda
4/6/2021 9:36:30 AM

Quant Time: Apr 06 01:18:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM031921S.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 06 01:17:41 2021
Response via : Initial Calibration

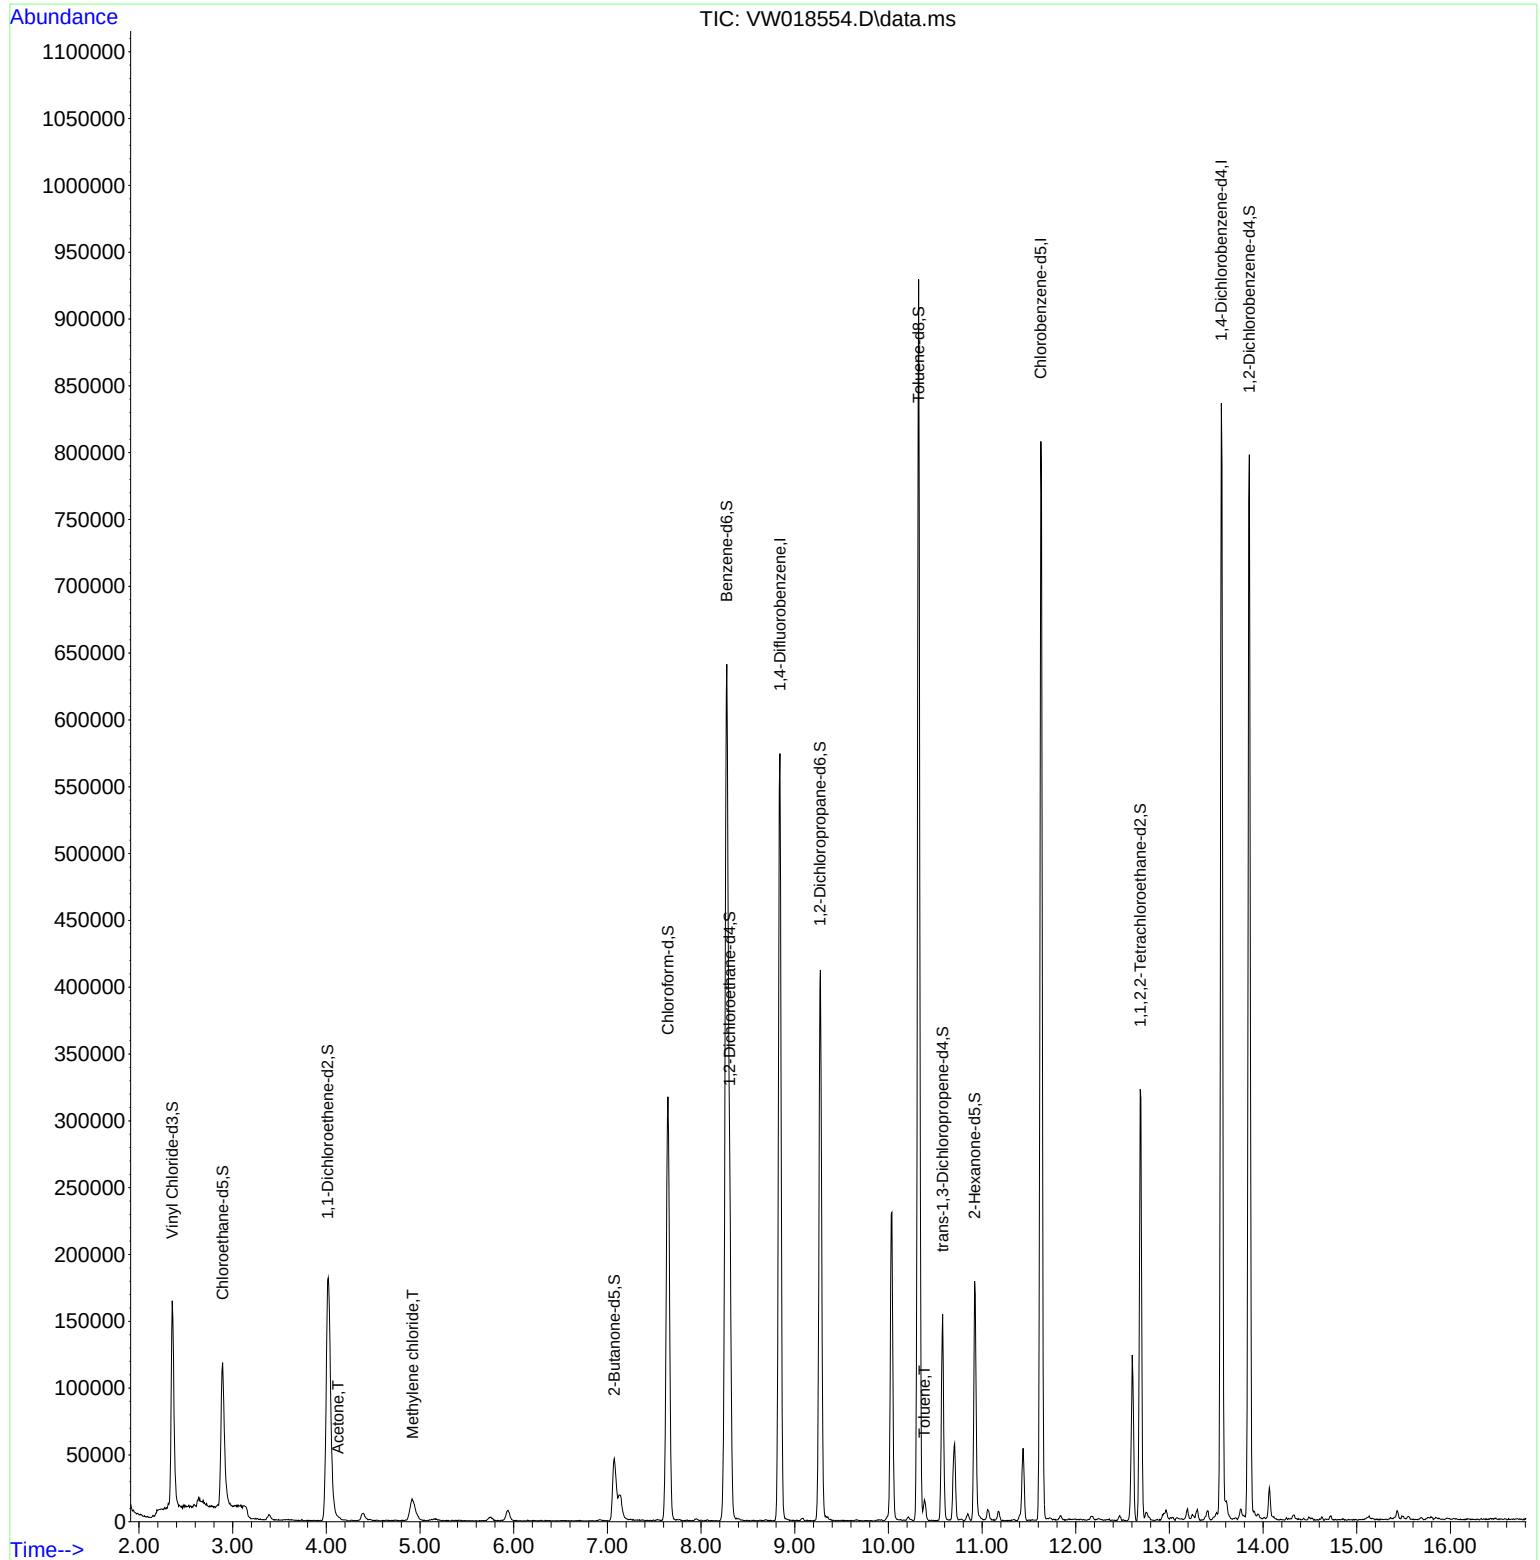

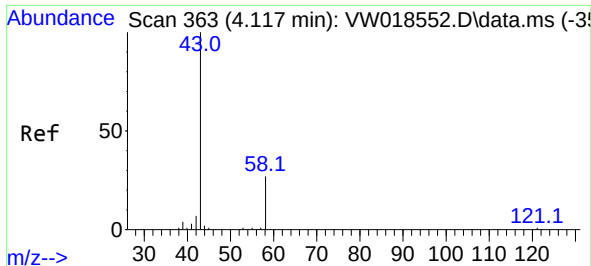





#13
Acetone
Concen: 3.17 ug/L m
RT: 4.123 min Scan# 364
Delta R.T. 0.006 min
Lab File: VW018554.D
Acq: 05 Apr 2021 13:29

Tgt Ion: 43 Resp: 3337
Ion Ratio Lower Upper
43 100
58 11.4 0.0 62.2

Instrument :
MSVOA_W
ClientSampled :
VHBLK01




Manual Integrations
APPROVED


MMDadoda
4/6/2021 9:36:30 AM

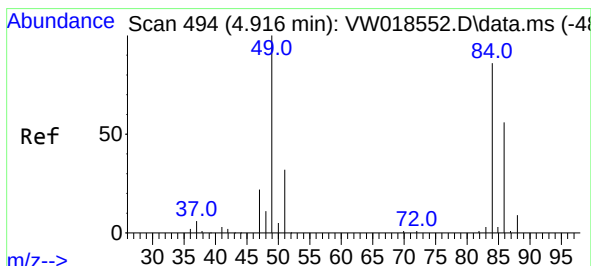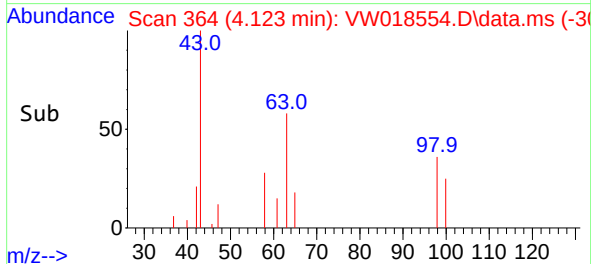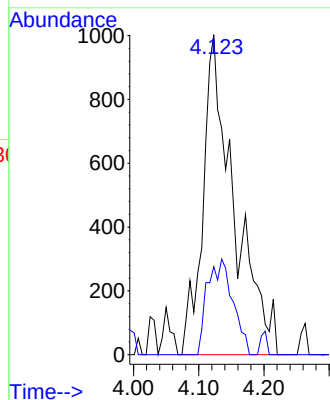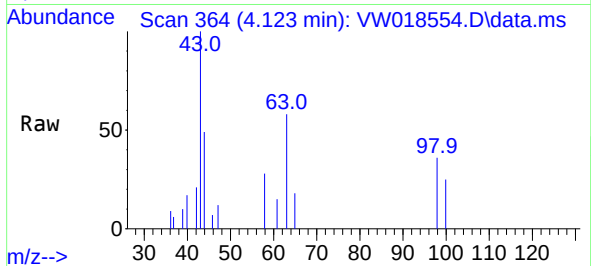

#16
Methylene chloride
Concen: 1.77 ug/L
RT: 4.922 min Scan# 495
Delta R.T. 0.006 min
Lab File: VW018554.D
Acq: 05 Apr 2021 13:29


Tgt Ion: 84 Resp: 13734
Ion Ratio Lower Upper
84 100
49 99.9 74.4 138.2
86 63.0 46.1 85.7

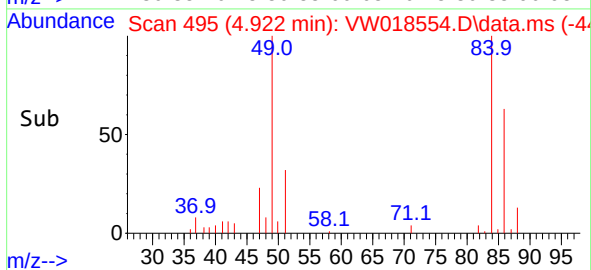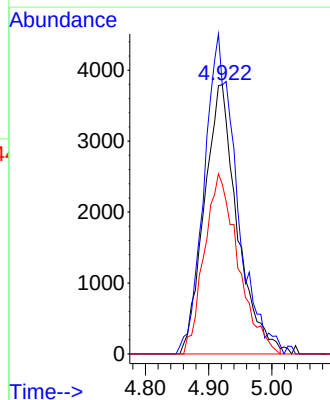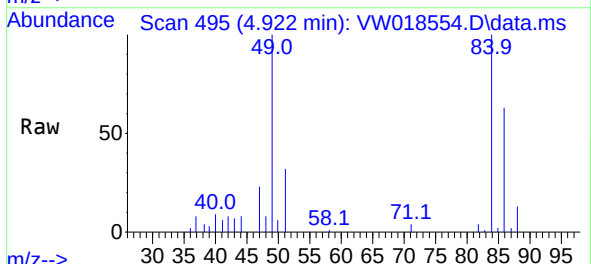

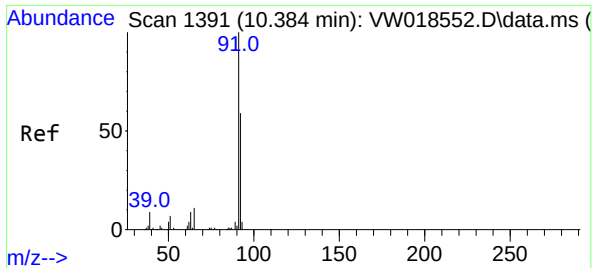

#44
Toluene
Concen: 0.36 ug/L
RT: 10.384 min Scan# 1391
Delta R.T. -0.000 min
Lab File: VW018554.D
Acq: 05 Apr 2021 13:29

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

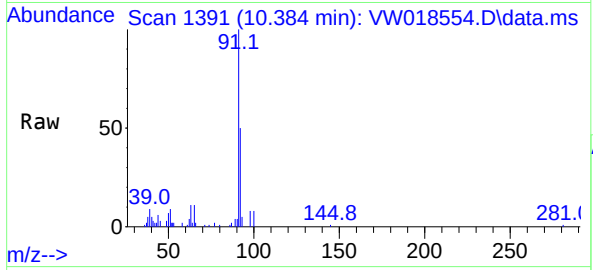

Tgt Ion: 91 Resp: 10300
Ion Ratio Lower Upper
91 100
92 49.9 42.3 78.5

Manual Integrations
APPROVED

MMDadoda
4/6/2021 9:36:30 AM

