

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040524\
 Data File : VW028331.D
 Acq On : 05 Apr 2024 11:47
 Operator : SY/MD
 Sample : P1988-10
 Misc : 5.04g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Quant Time: Apr 05 23:43:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 05 23:38:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	217740	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	197694	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	97520	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	41644	16.346	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.400%
7) Chloroethane-d5	3.040	69	63	0.035	ug/L	0.14
Spiked Amount	25.000	Range	30 - 150	Recovery	=	0.160%#
11) 1,1-Dichloroethene-d2	4.027	65	26966	16.691	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.760%
21) 2-Butanone-d5	7.075	46	39799	52.966	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.940%
24) Chloroform-d	7.648	84	145474	22.657	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.640%
26) 1,2-Dichloroethane-d4	8.307	65	78207	22.103	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.400%
32) Benzene-d6	8.276	84	273520	22.661	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.640%
36) 1,2-Dichloropropane-d6	9.270	67	87538	25.202	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.800%
41) Toluene-d8	10.325	98	238904	21.459	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	85.840%
43) trans-1,3-Dichloroprop...	10.575	79	32591	20.659	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.640%
47) 2-Hexanone-d5	10.922	63	28716	50.015	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.040%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	65551	25.548	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.200%
66) 1,2-Dichlorobenzene-d4	13.849	152	88934	25.034	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.120%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	2522	0.506	ug/L	# 71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040524\
Data File : VW028331.D
Acq On : 05 Apr 2024 11:47
Operator : SY/MD
Sample : P1988-10
Misc : 5.04g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK002

Quant Time: Apr 05 23:43:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 05 23:38:30 2024
Response via : Initial Calibration

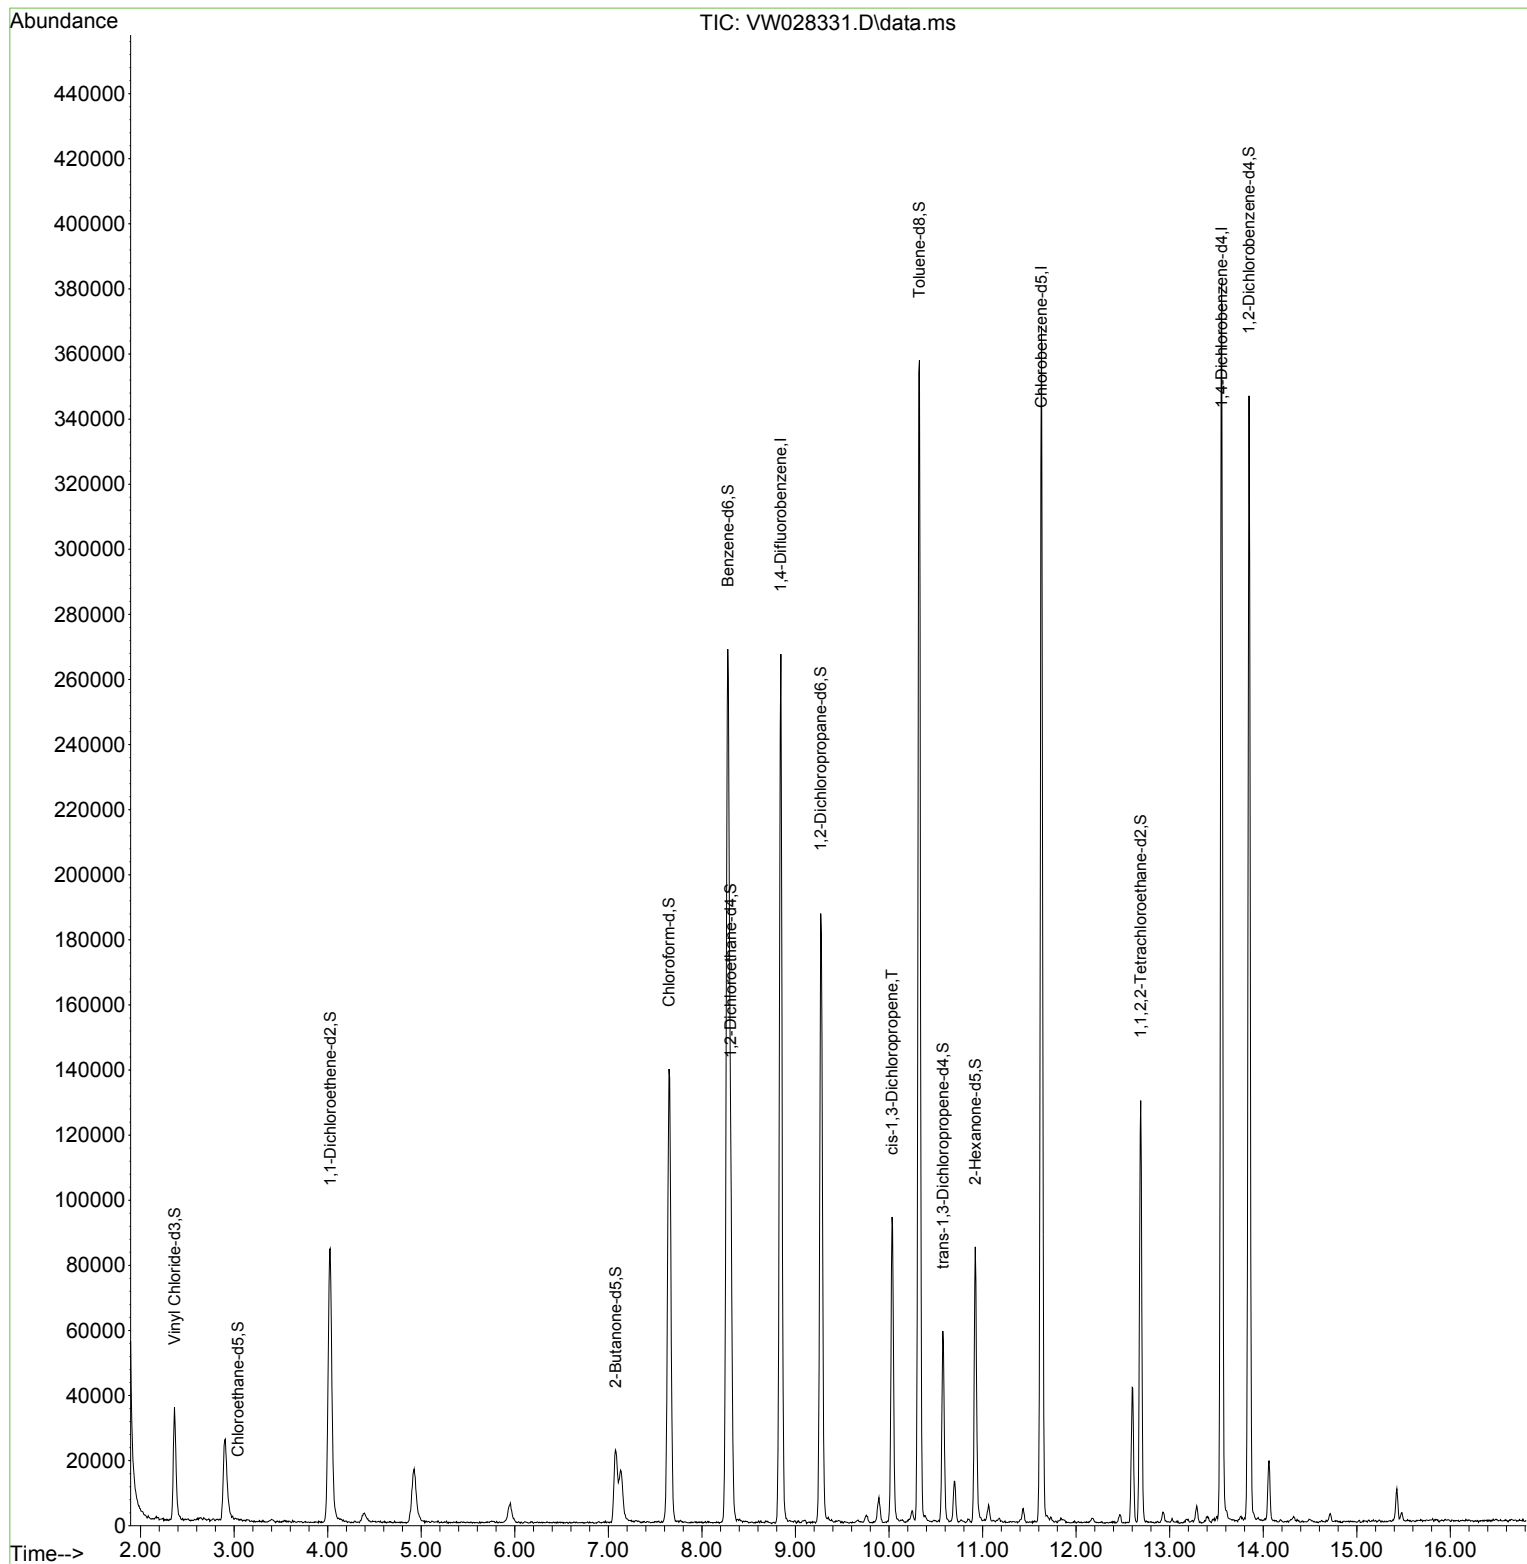

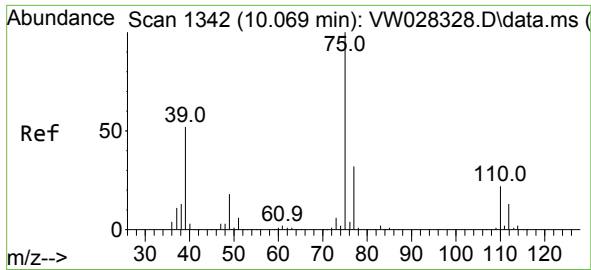

#39
 cis-1,3-Dichloropropene
 Concen: 0.506 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW028331.D
 Acq: 05 Apr 2024 11:47

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK002

Tgt Ion: 75 Resp: 2522
 Ion Ratio Lower Upper
 75 100
 77 48.0 22.5 41.7#

