

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040524\
 Data File : VW028342.D
 Acq On : 05 Apr 2024 17:42
 Operator : SY/MD
 Sample : P2018-01
 Misc : 4.25g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH5E8

Quant Time: Apr 05 23:46:07 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 05 23:38:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	288326	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	237264	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	91836	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	48945	14.508	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.040%
7) Chloroethane-d5	2.899	69	38728	16.432	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.720%
11) 1,1-Dichloroethene-d2	4.021	65	30820	14.407	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.640%
21) 2-Butanone-d5	7.075	46	29985	30.136	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	60.280%
24) Chloroform-d	7.648	84	142059	16.709	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	66.840%
26) 1,2-Dichloroethane-d4	8.307	65	76600	16.349	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	65.400%#
32) Benzene-d6	8.276	84	270747	18.690	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.760%
36) 1,2-Dichloropropane-d6	9.270	67	84442	20.256	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.040%
41) Toluene-d8	10.318	98	227041	16.992	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	67.960%
43) trans-1,3-Dichloroprop...	10.575	79	28407	15.003	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	60.000%
47) 2-Hexanone-d5	10.922	63	22907	33.243	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.480%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	60466	19.636	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	78.560%
66) 1,2-Dichlorobenzene-d4	13.848	152	59684	17.840	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	71.360%#
Target Compounds						
					Qvalue	
13) Acetone	4.131	43	8117	7.347	ug/L	100
15) Methyl Acetate	4.691	43	1073	0.631	ug/L #	90
34) Trichloroethene	8.843	95	8709	2.138	ug/L #	5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040524\
Data File : VW028342.D
Acq On : 05 Apr 2024 17:42
Operator : SY/MD
Sample : P2018-01
Misc : 4.25g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH5E8

Quant Time: Apr 05 23:46:07 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 05 23:38:30 2024
Response via : Initial Calibration




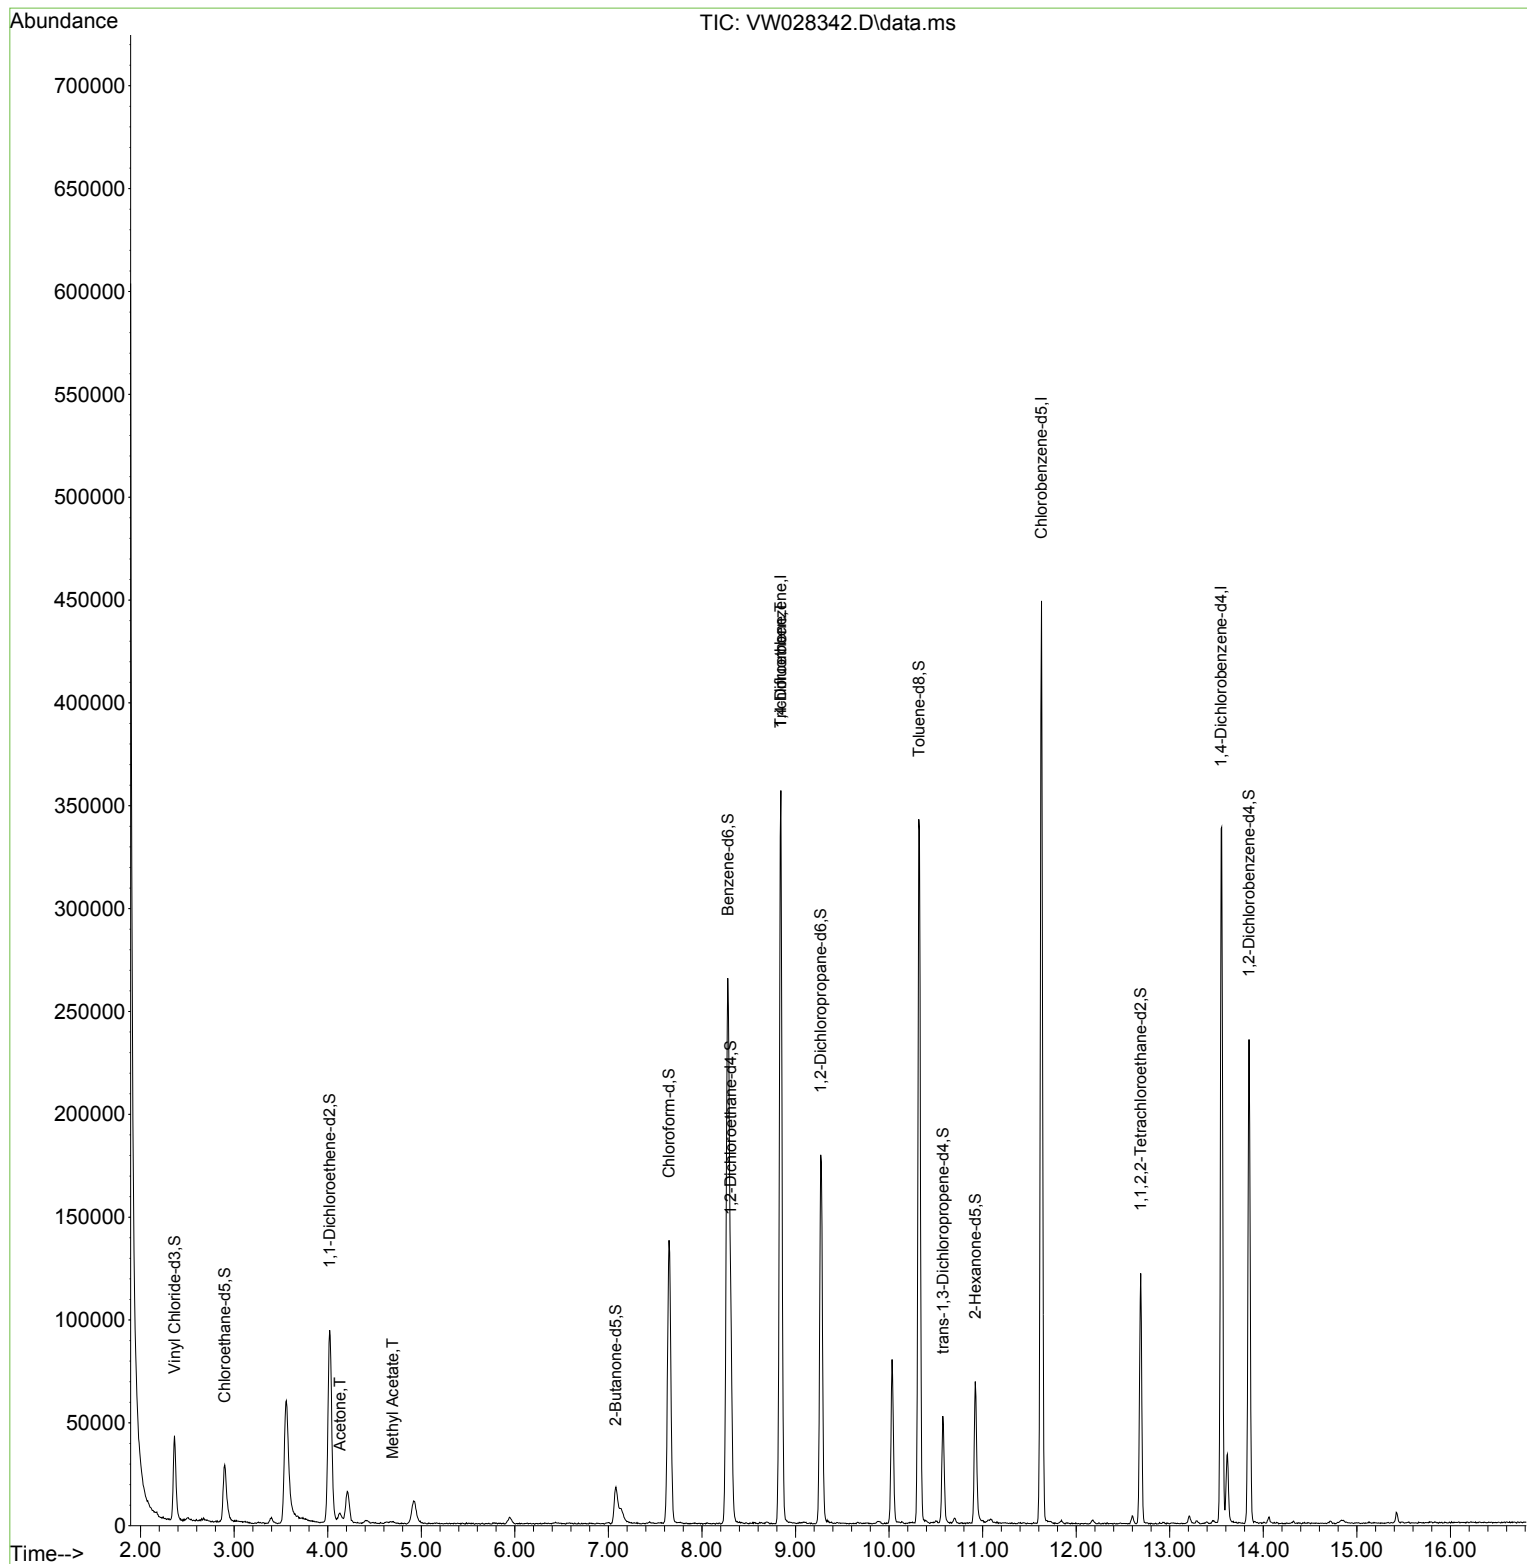


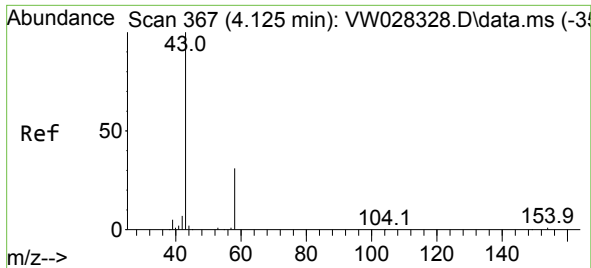

#13
Acetone
Concen: 7.347 ug/L
RT: 4.131 min Scan# 368
Delta R.T. 0.006 min
Lab File: VW028342.D
Acq: 05 Apr 2024 17:42




Instrument :
MSVOA_W
ClientSampleId :
BH5E8


Tgt Ion: 43 Resp: 8117
Ion Ratio Lower Upper
43 100
58 28.8 0.0 57.8

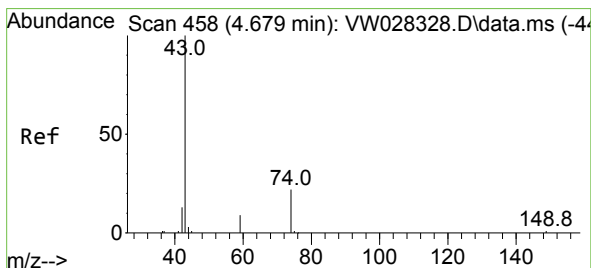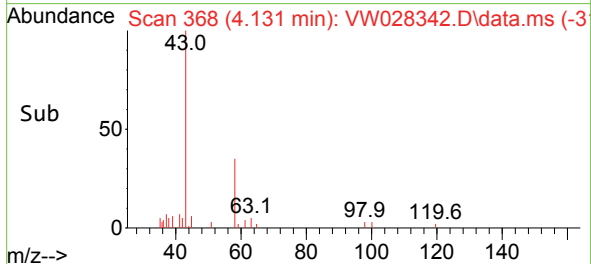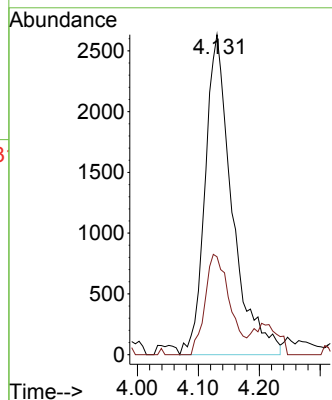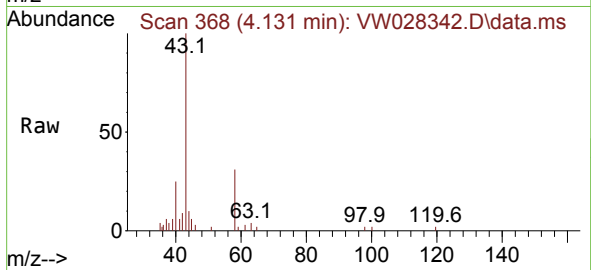

#15
Methyl Acetate
Concen: 0.631 ug/L
RT: 4.691 min Scan# 460
Delta R.T. 0.012 min
Lab File: VW028342.D
Acq: 05 Apr 2024 17:42


Tgt Ion: 43 Resp: 1073
Ion Ratio Lower Upper
43 100
74 27.4 18.2 27.2#

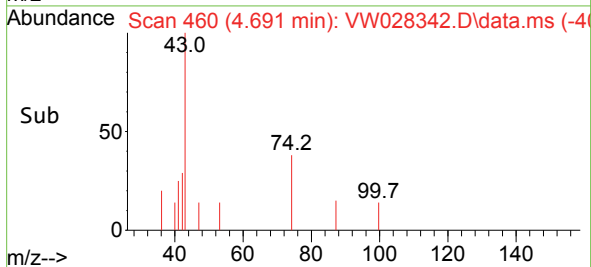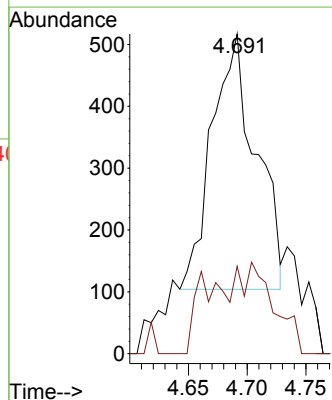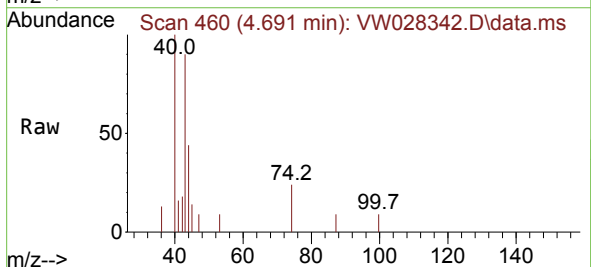

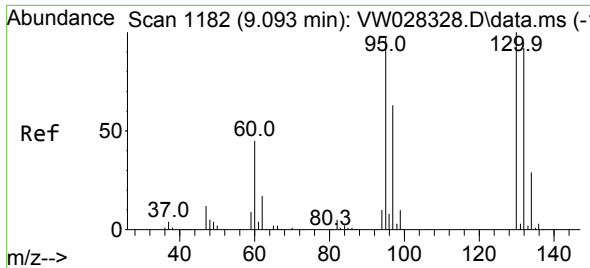

#34
 Trichloroethene
 Concen: 2.138 ug/L
 RT: 8.843 min Scan# 11
 Delta R.T. -0.250 min
 Lab File: VW028342.D
 Acq: 05 Apr 2024 17:42

Instrument :
 MSVOA_W
 ClientSampleId :
 BH5E8

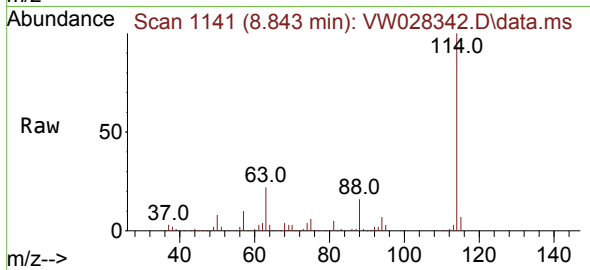

Tgt Ion: 95 Resp: 8709

Ion	Ratio	Lower	Upper
95	100		
97	0.0	42.4	78.6#
132	0.0	69.4	128.8#
130	0.0	69.7	129.4#

