

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040524\
 Data File : VW028344.D
 Acq On : 05 Apr 2024 18:29
 Operator : SY/MD
 Sample : P2018-03
 Misc : 5.15g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH5E5

Quant Time: Apr 05 23:46:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 05 23:38:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	39245	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	32602	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	11439	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	8034	17.496	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.000%
7) Chloroethane-d5	2.887	69	7468	23.279	ug/L	-0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.120%
11) 1,1-Dichloroethene-d2	4.027	65	5032	17.281	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.120%
21) 2-Butanone-d5	7.093	46	4216	31.130	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.260%
24) Chloroform-d	7.648	84	23437	20.253	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	81.000%
26) 1,2-Dichloroethane-d4	8.307	65	12576	19.720	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	78.880%
32) Benzene-d6	8.270	84	42023	21.112	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	84.440%
36) 1,2-Dichloropropane-d6	9.276	67	13552	23.659	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.640%
41) Toluene-d8	10.325	98	33487	18.239	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.960%
43) trans-1,3-Dichloroprop...	10.575	79	4345	16.701	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	66.800%
47) 2-Hexanone-d5	10.928	63	3201	33.807	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	67.620%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	9461	22.359	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.440%
66) 1,2-Dichlorobenzene-d4	13.848	152	8387	20.127	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	80.520%
Target Compounds						
					Qvalue	
13) Acetone	4.137	43	686	4.562	ug/L	92
34) Trichloroethene	8.843	95	1310	2.340	ug/L #	5
35) Methylcyclohexane	9.276	83	3431	3.627	ug/L #	17
37) 1,2-Dichloropropane	9.276	63	1698	3.309	ug/L #	85
39) cis-1,3-Dichloropropene	10.044	75	392	0.477	ug/L #	54
61) 1,2,3-Trichloropropane	13.556	75	1478	6.770	ug/L #	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040524\
Data File : VW028344.D
Acq On : 05 Apr 2024 18:29
Operator : SY/MD
Sample : P2018-03
Misc : 5.15g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH5E5

Quant Time: Apr 05 23:46:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 05 23:38:30 2024
Response via : Initial Calibration

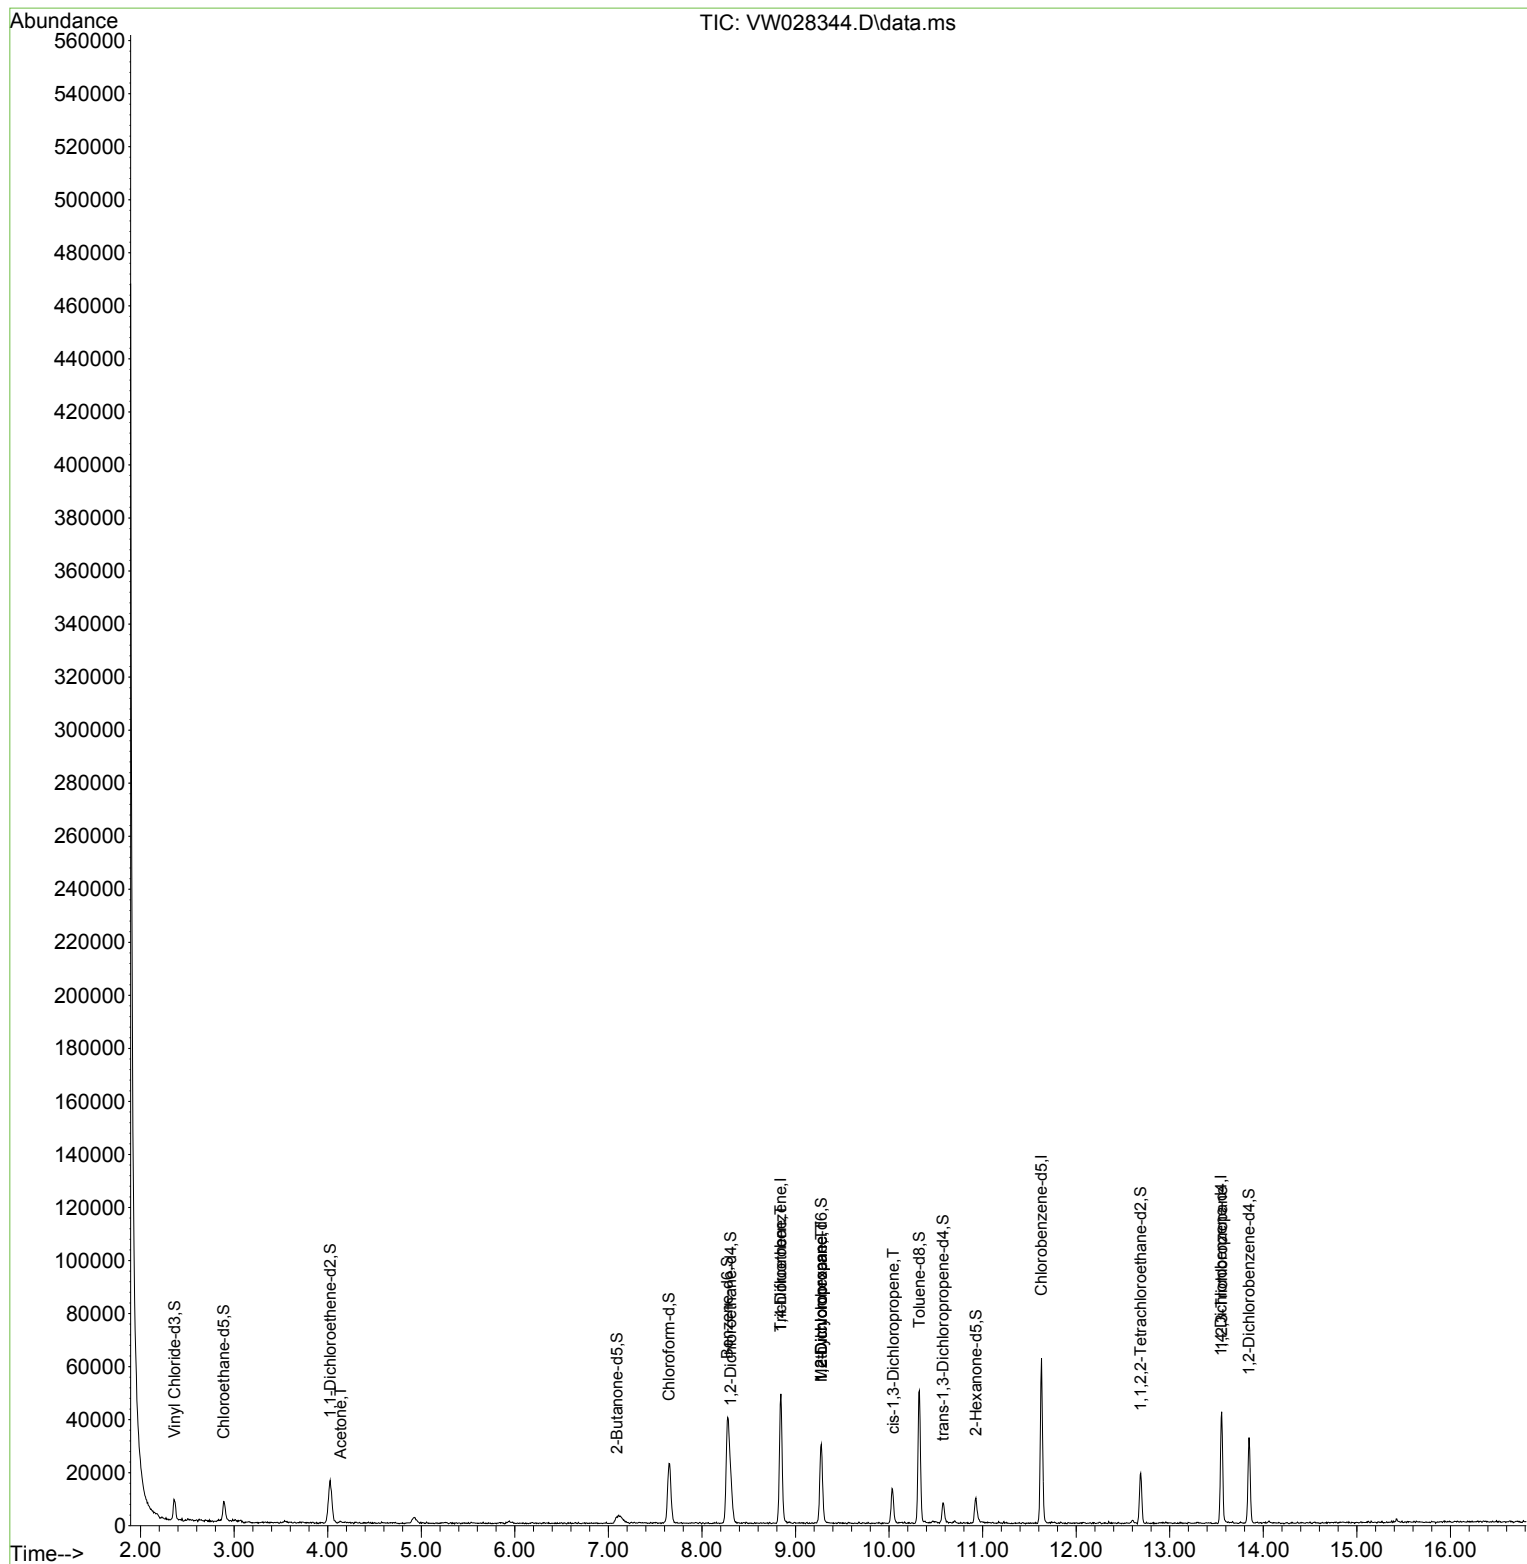

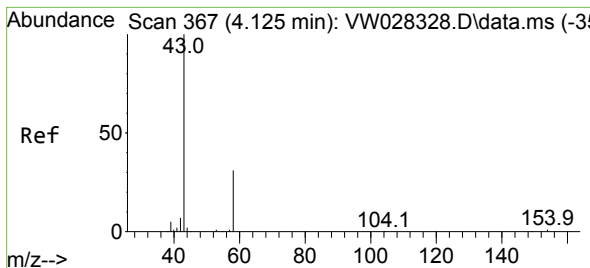

#13

Acetone

Concen: 4.562 ug/L

RT: 4.137 min Scan# 3

Delta R.T. 0.012 min

Lab File: VW028344.D

Acq: 05 Apr 2024 18:29

Instrument :

MSVOA_W

ClientSampleId :





BH5E5

Tgt Ion: 43 Resp: 686

Ion Ratio Lower Upper

43 100

58 24.5 0.0 57.8

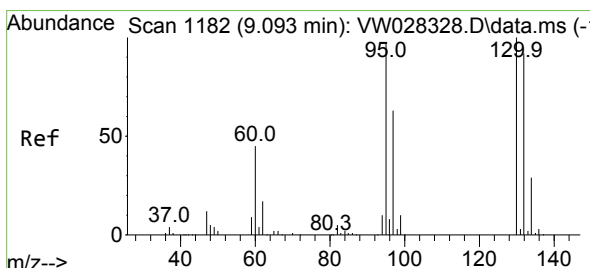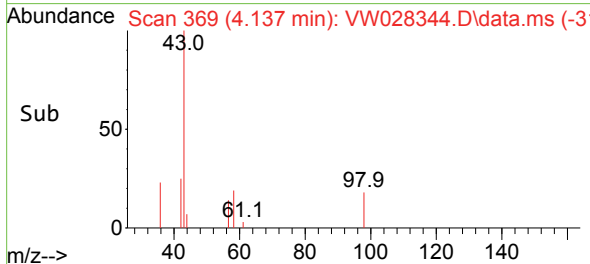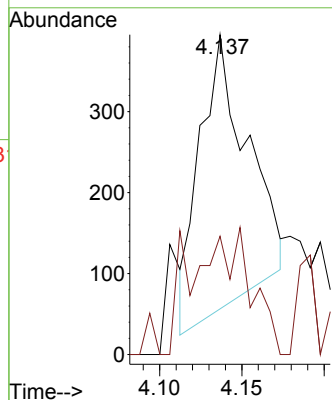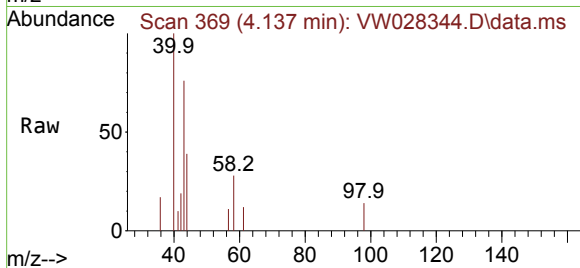

#34

Trichloroethene

Concen: 2.340 ug/L

RT: 8.843 min Scan# 1141

Delta R.T. -0.250 min

Lab File: VW028344.D

Acq: 05 Apr 2024 18:29

Tgt Ion: 95 Resp: 1310




Ion Ratio Lower Upper


95 100

97 0.0 42.4 78.6#

132 0.0 69.4 128.8#

130 0.0 69.7 129.4#


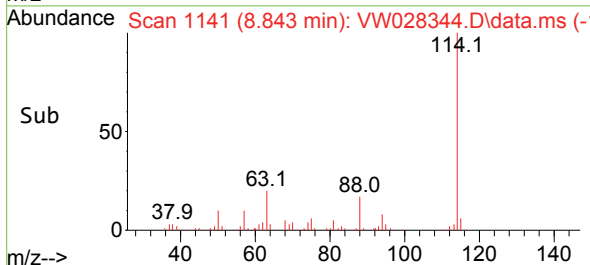
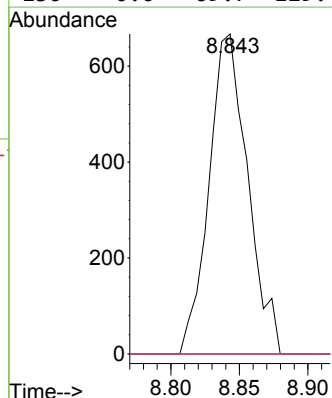
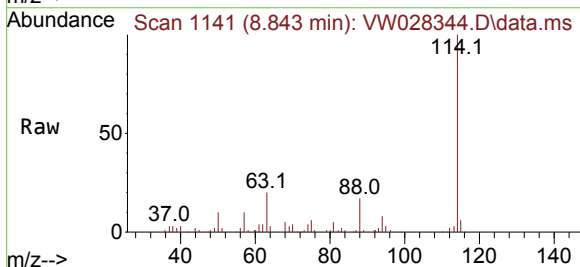


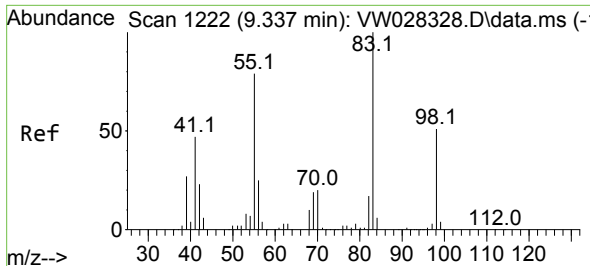

#35
Methylcyclohexane
Concen: 3.627 ug/L
RT: 9.276 min Scan# 11
Delta R.T. -0.061 min
Lab File: VW028344.D
Acq: 05 Apr 2024 18:29




Instrument :
MSVOA_W
ClientSampleId :
BH5E5


Tgt Ion: 83 Resp: 3431
Ion Ratio Lower Upper
83 100
55 1.2 64.2 96.4#
98 0.0 38.3 57.5#

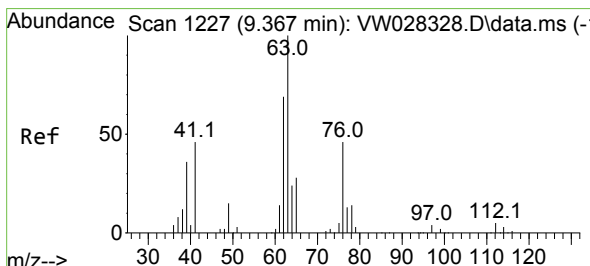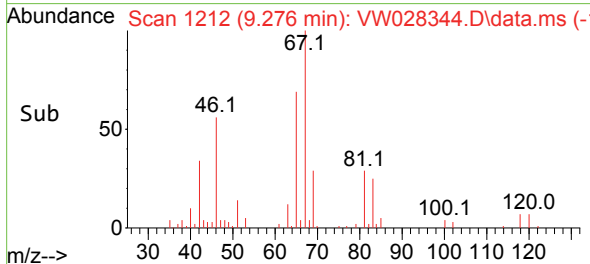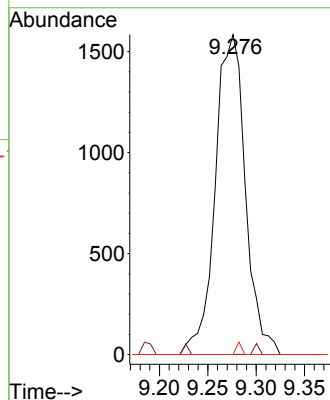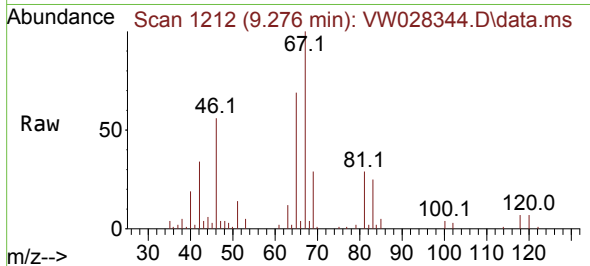

#37
1,2-Dichloropropane
Concen: 3.309 ug/L
RT: 9.276 min Scan# 1212
Delta R.T. -0.091 min
Lab File: VW028344.D
Acq: 05 Apr 2024 18:29

Tgt Ion: 63 Resp: 1698
Ion Ratio Lower Upper
63 100
112 0.0 3.8 5.8#


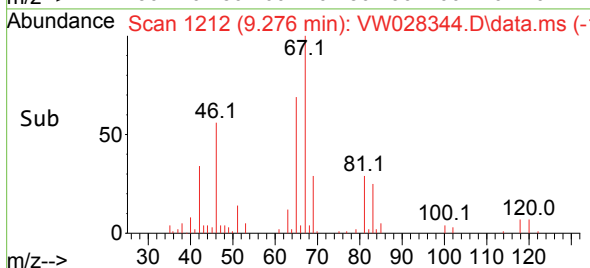
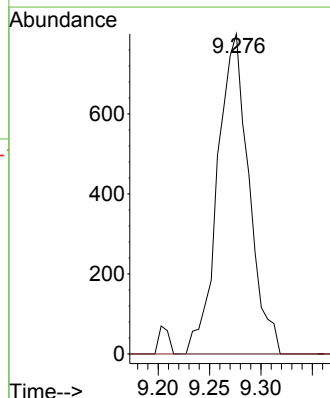
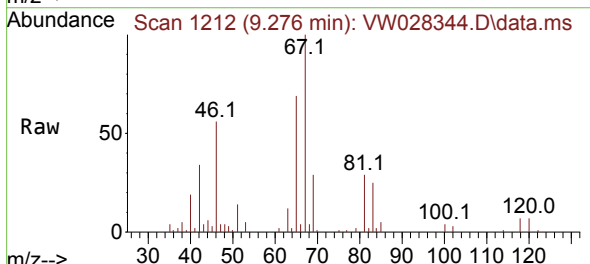


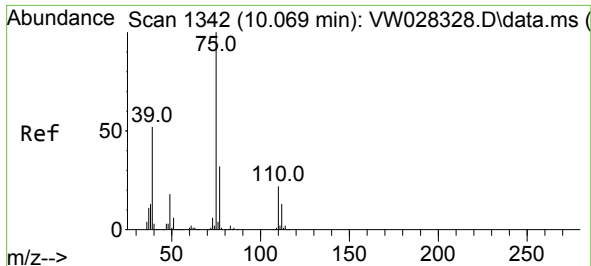

#39
cis-1,3-Dichloropropene
Concen: 0.477 ug/L
RT: 10.044 min Scan# 11
Delta R.T. -0.024 min
Lab File: VW028344.D
Acq: 05 Apr 2024 18:29

Instrument :
MSVOA_W
ClientSampleId :
BH5E5

Tgt Ion: 75 Resp: 392
Ion Ratio Lower Upper
75 100
77 57.8 22.5 41.7#

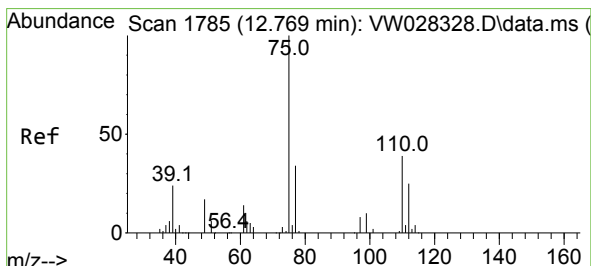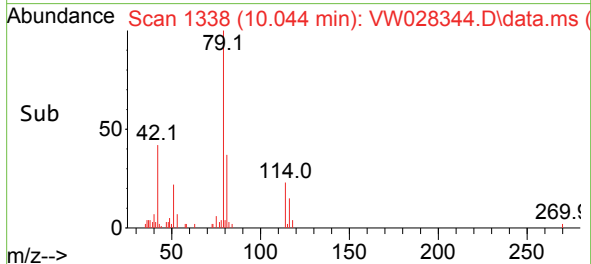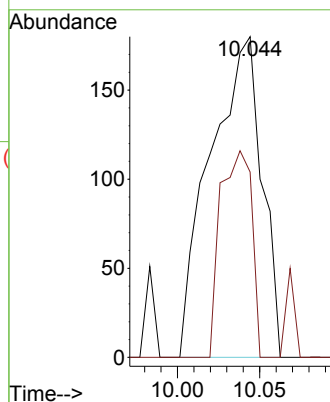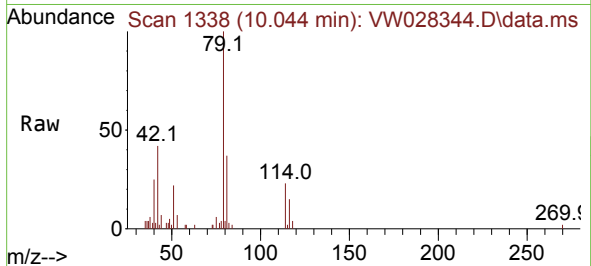

#61
1,2,3-Trichloropropane
Concen: 6.770 ug/L
RT: 13.556 min Scan# 1914
Delta R.T. 0.786 min
Lab File: VW028344.D
Acq: 05 Apr 2024 18:29

Tgt Ion: 75 Resp: 1478
Ion Ratio Lower Upper
75 100
77 42.1 26.0 39.0#
110 0.0 32.2 48.2#

