

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040524\
 Data File : VW028345.D
 Acq On : 05 Apr 2024 18:53
 Operator : SY/MD
 Sample : P2018-04
 Misc : 4.76g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH5E6

Quant Time: Apr 05 23:46:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 05 23:38:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	355956	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	288156	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	100281	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	62744	15.065	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.280%
7) Chloroethane-d5	2.899	69	50578	17.382	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.520%
11) 1,1-Dichloroethene-d2	4.021	65	38754	14.673	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.680%
21) 2-Butanone-d5	7.081	46	45465	37.012	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.020%
24) Chloroform-d	7.648	84	190215	18.122	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	72.480%
26) 1,2-Dichloroethane-d4	8.307	65	99874	17.266	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	69.080%#
32) Benzene-d6	8.276	84	356812	20.281	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.120%
36) 1,2-Dichloropropane-d6	9.270	67	112042	22.130	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.520%
41) Toluene-d8	10.319	98	297168	18.313	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.240%
43) trans-1,3-Dichloroprop...	10.581	79	38947	16.937	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.760%
47) 2-Hexanone-d5	10.922	63	31417	37.541	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.080%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	76020	20.327	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	81.320%
66) 1,2-Dichlorobenzene-d4	13.848	152	68269	18.688	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	74.760%#
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.038	75	2915	0.401	ug/L #	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040524\
Data File : VW028345.D
Acq On : 05 Apr 2024 18:53
Operator : SY/MD
Sample : P2018-04
Misc : 4.76g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH5E6


Quant Time: Apr 05 23:46:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 05 23:38:30 2024
Response via : Initial Calibration

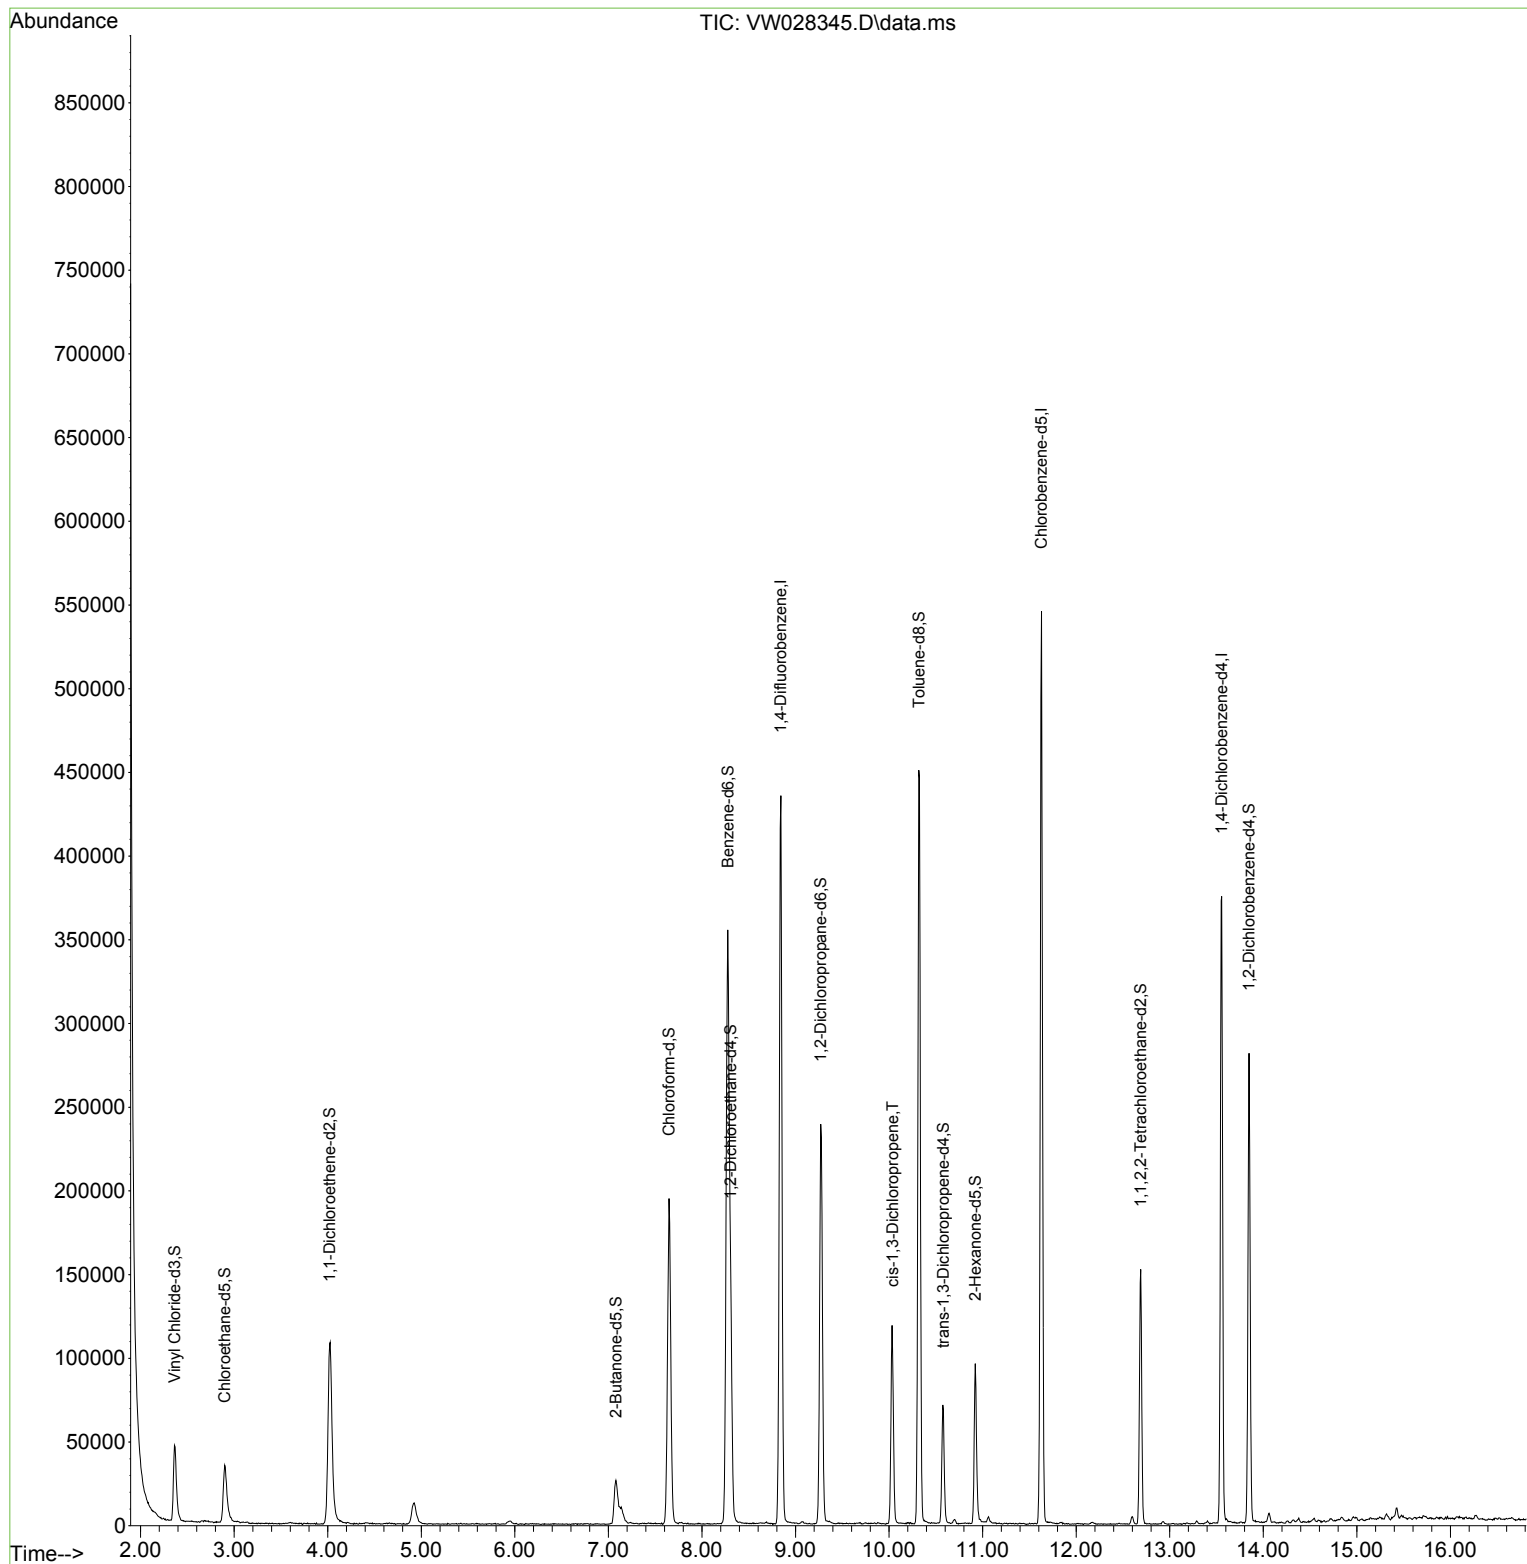

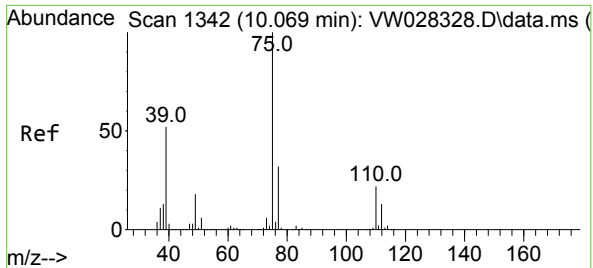

#39
cis-1,3-Dichloropropene
Concen: 0.401 ug/L
RT: 10.038 min Scan# 11
Delta R.T. -0.030 min
Lab File: VW028345.D
Acq: 05 Apr 2024 18:53

Instrument :
MSVOA_W
ClientSampleId :
BH5E6

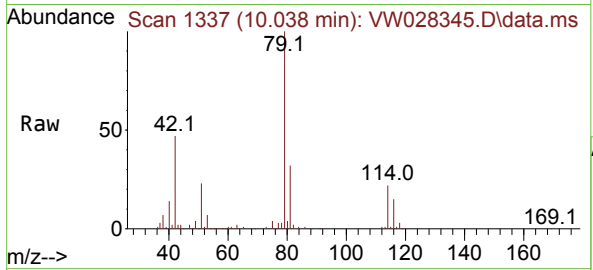

Tgt Ion: 75 Resp: 2915
Ion Ratio Lower Upper
75 100
77 59.1 22.5 41.7#

