

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040524\
 Data File : VW028346.D
 Acq On : 05 Apr 2024 19:17
 Operator : SY/MD
 Sample : P2018-06
 Misc : 5.64g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH5E7

Quant Time: Apr 05 23:47:01 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Apr 05 23:38:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	394782	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	323069	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	128950	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	64871	14.044	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.160%
7) Chloroethane-d5	2.899	69	52202	16.176	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.720%
11) 1,1-Dichloroethene-d2	4.027	65	41556	14.187	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	56.760%
21) 2-Butanone-d5	7.075	46	37433	27.476	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.960%
24) Chloroform-d	7.648	84	204205	17.542	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	70.160%
26) 1,2-Dichloroethane-d4	8.301	65	108937	16.981	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	67.920%#
32) Benzene-d6	8.276	84	389488	19.746	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.000%
36) 1,2-Dichloropropane-d6	9.270	67	120883	21.296	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.200%
41) Toluene-d8	10.319	98	332632	18.283	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.120%
43) trans-1,3-Dichloroprop...	10.575	79	38256	14.839	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	59.360%
47) 2-Hexanone-d5	10.922	63	28104	29.953	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.900%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	84330	20.112	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.440%
66) 1,2-Dichlorobenzene-d4	13.849	152	88069	18.748	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	75.000%
Target Compounds					Qvalue	
13) Acetone	4.137	43	8506	5.623	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW040524\
Data File : VW028346.D
Acq On : 05 Apr 2024 19:17
Operator : SY/MD
Sample : P2018-06
Misc : 5.64g/10mL/MSVOA_W/SOIL/A
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH5E7

Quant Time: Apr 05 23:47:01 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM031424SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Apr 05 23:38:30 2024
Response via : Initial Calibration

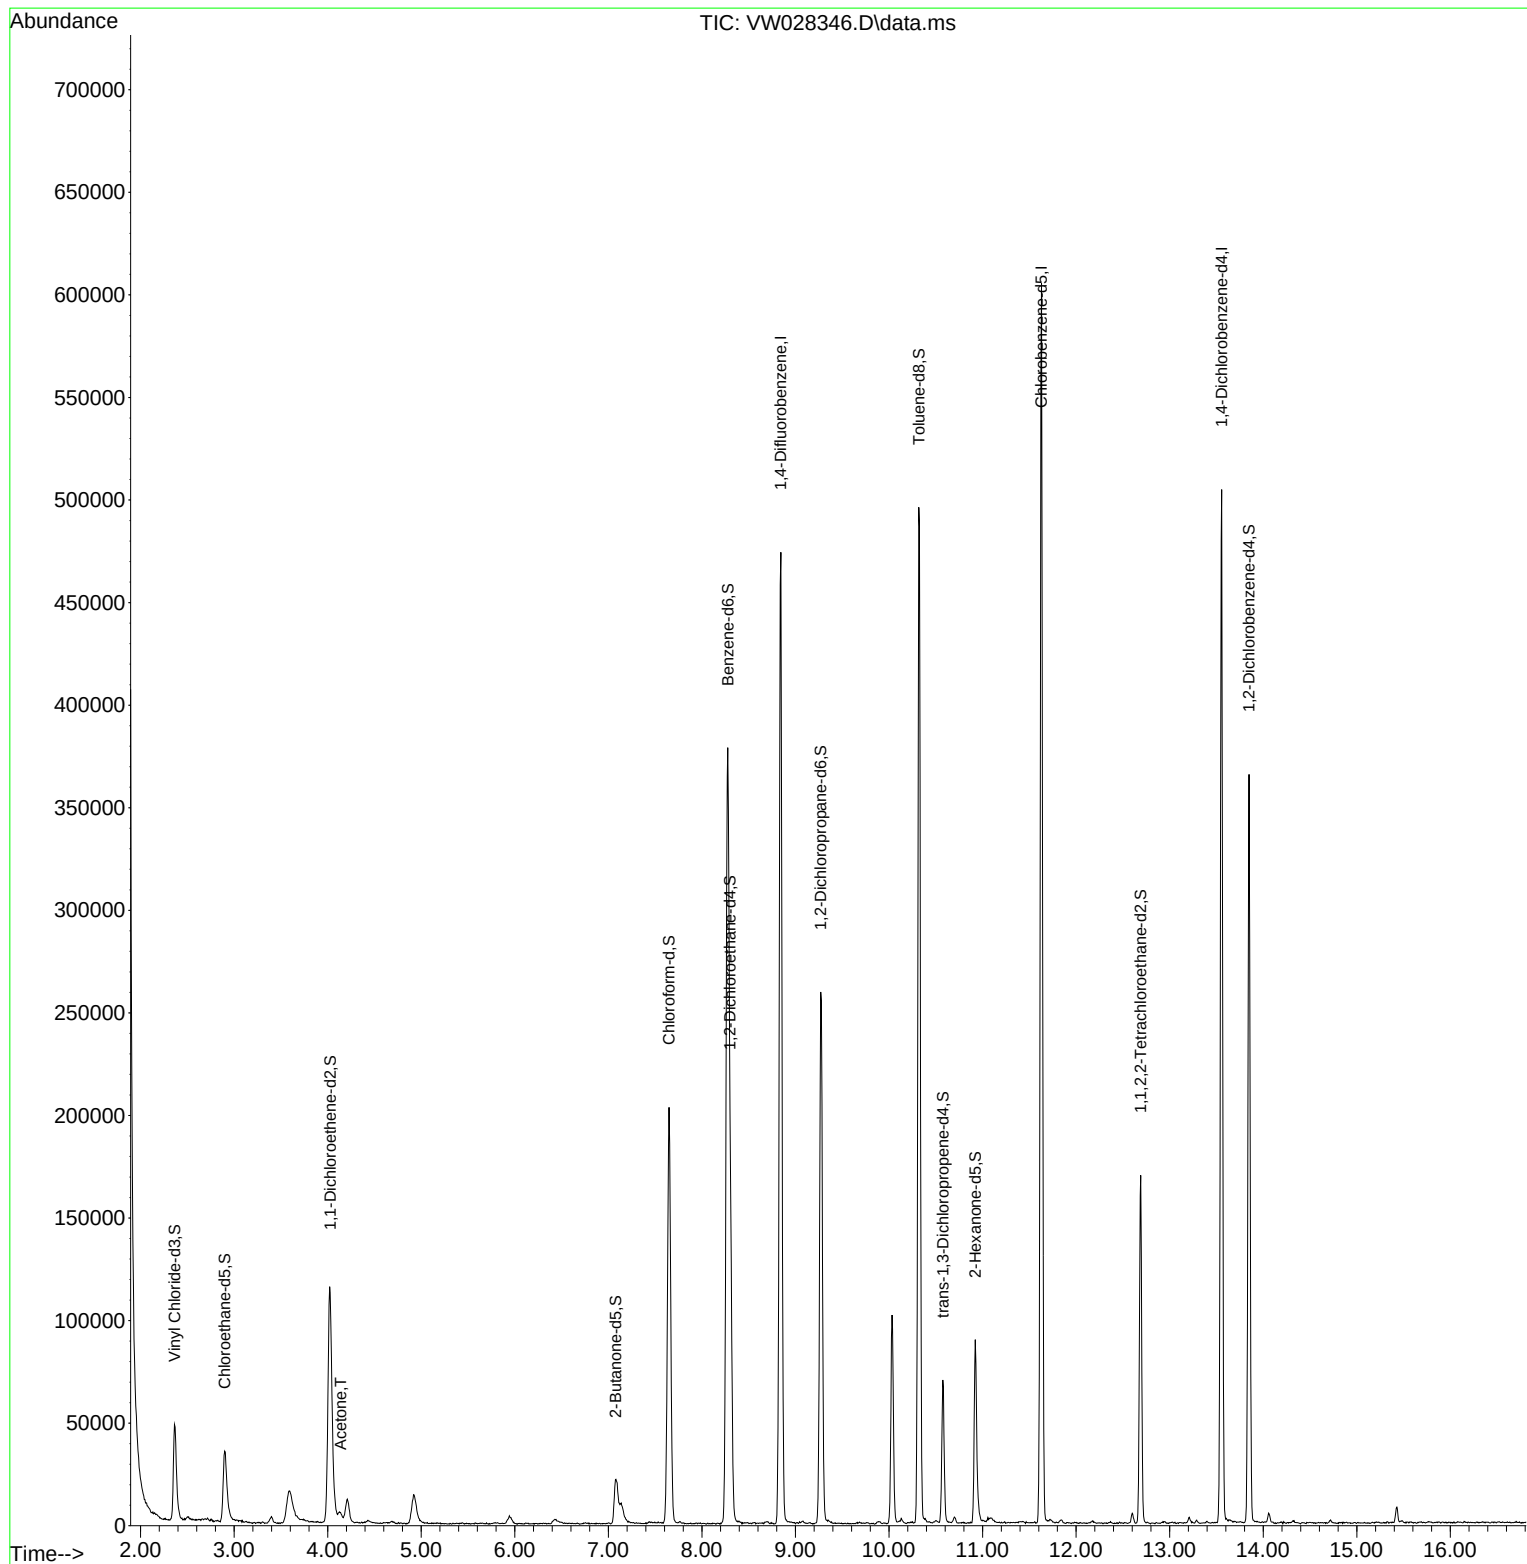

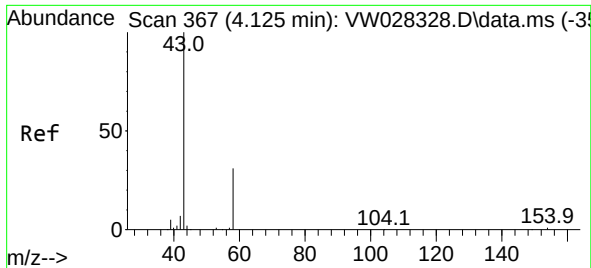

#13

Acetone

Concen: 5.623 ug/L

RT: 4.137 min Scan# 30

Delta R.T. 0.012 min

Lab File: VW028346.D


Acq: 05 Apr 2024 19:17

Instrument :

MSVOA_W

ClientSampleId :

BH5E7

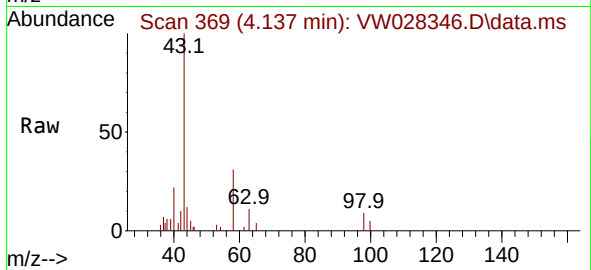

Tgt Ion: 43 Resp: 8506

Ion Ratio Lower Upper

43 100

58 30.9 0.0 57.8

