


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009762.D
Acq On : 06 Apr 2019 10:17
Operator : SY/VA
Sample : VW0406SBL02
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK25

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:42:58 AM

Quant Time: Apr 07 04:09:39 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

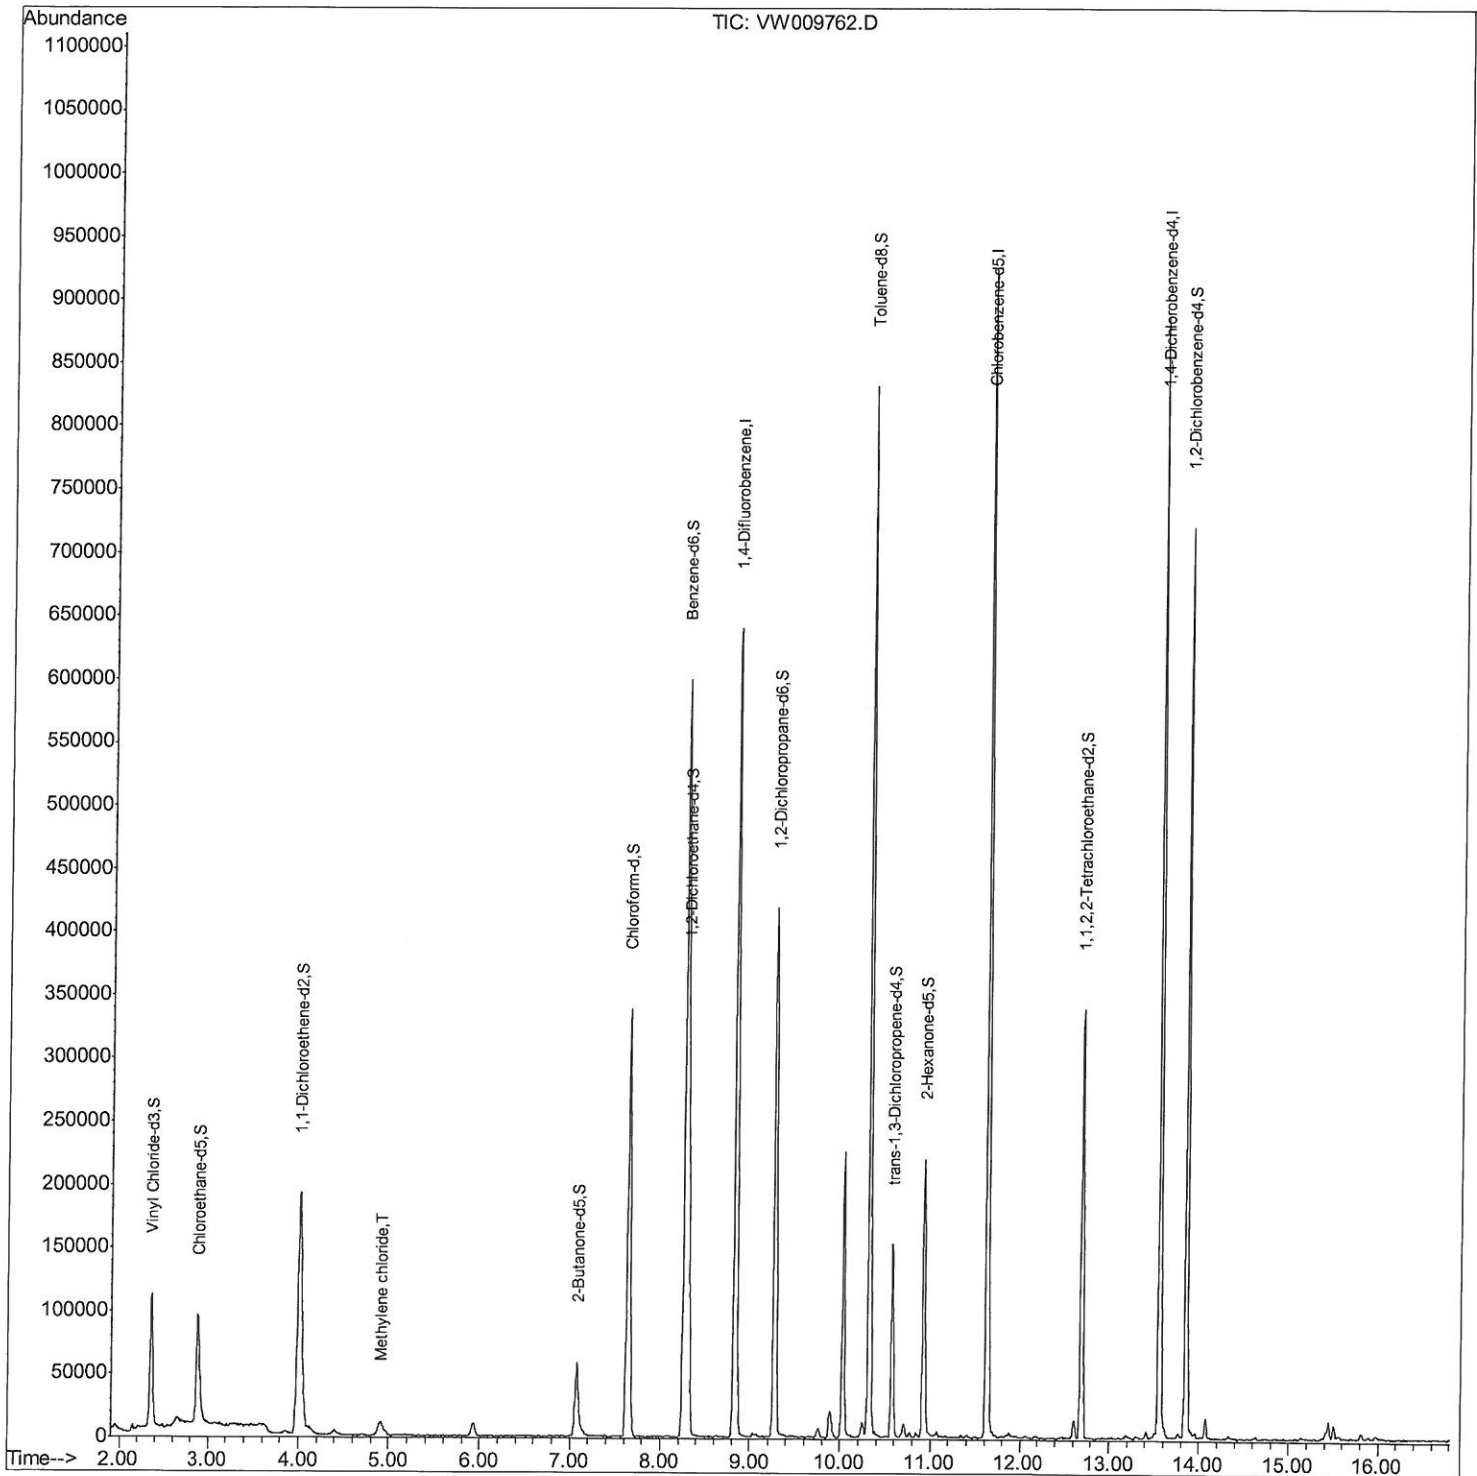

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009762.D
 Acq On : 06 Apr 2019 10:17
 Operator : SY/VA
 Sample : VW0406SBL02
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK25

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:42:58 AM

Quant Time: Apr 07 03:59:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 03:56:20 2019
 Response via : Initial Calibration

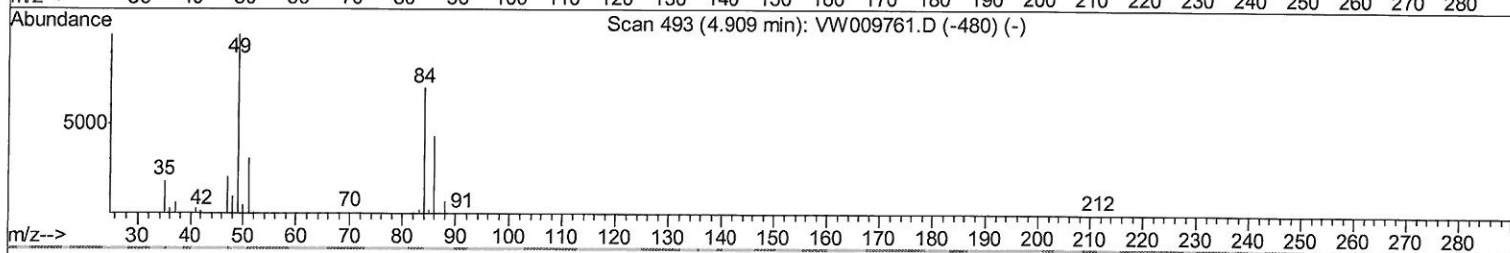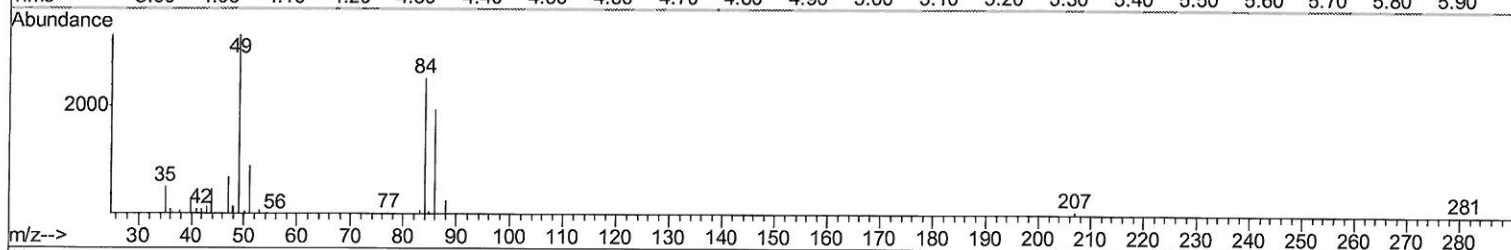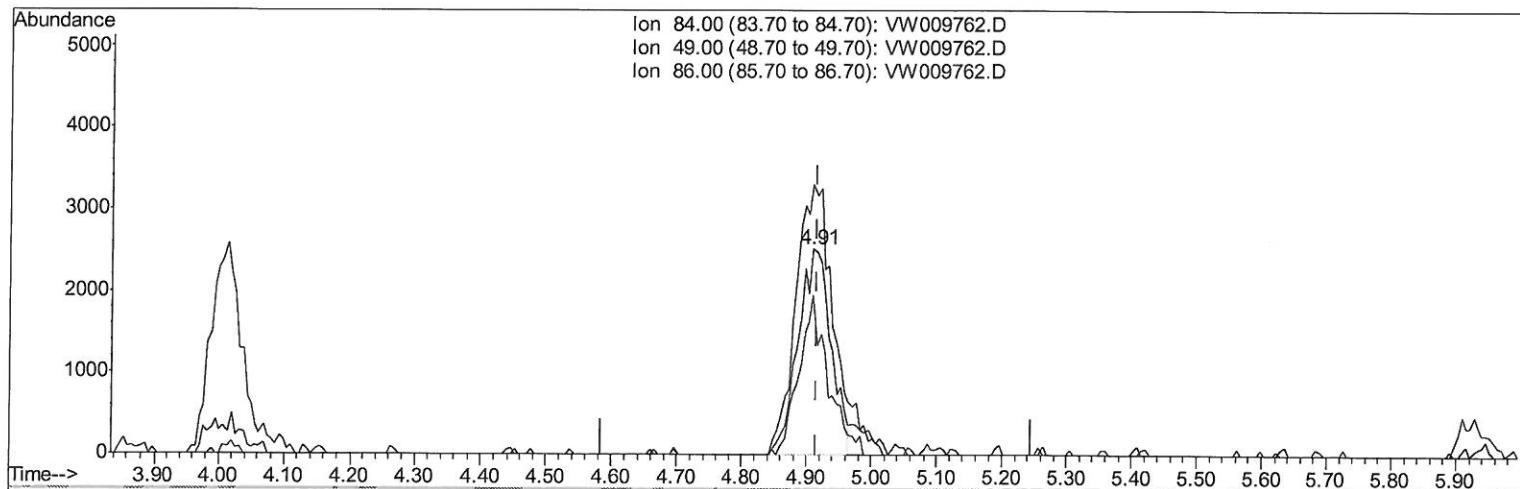

TIC: VW009762.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.02ug/L

response 8856

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	131.20
86.00	66.30	77.34
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009762.D
 Acq On : 06 Apr 2019 10:17
 Operator : SY/VA
 Sample : VW0406SBL02
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK25

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:42:58 AM

Quant Time: Apr 07 03:59:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 03:56:20 2019
 Response via : Initial Calibration

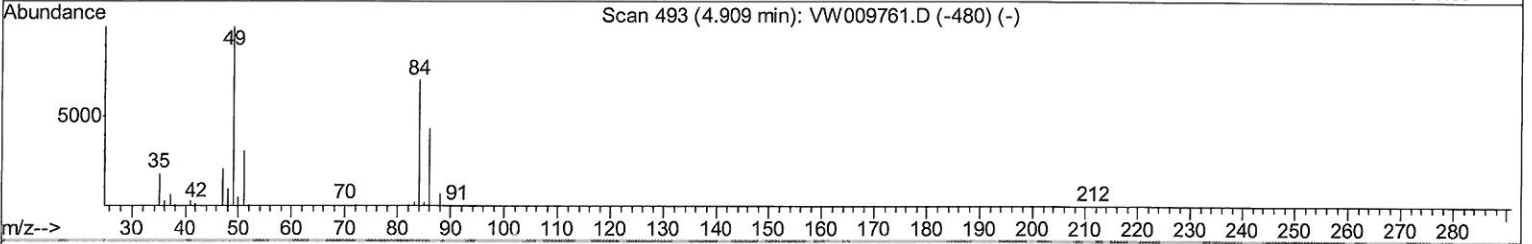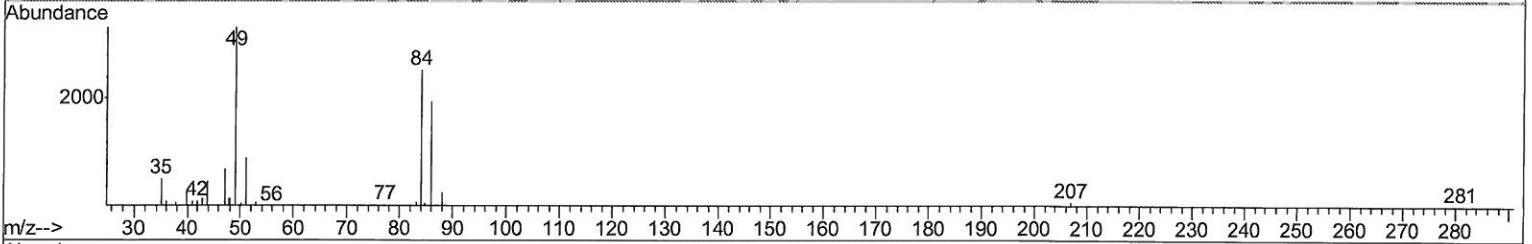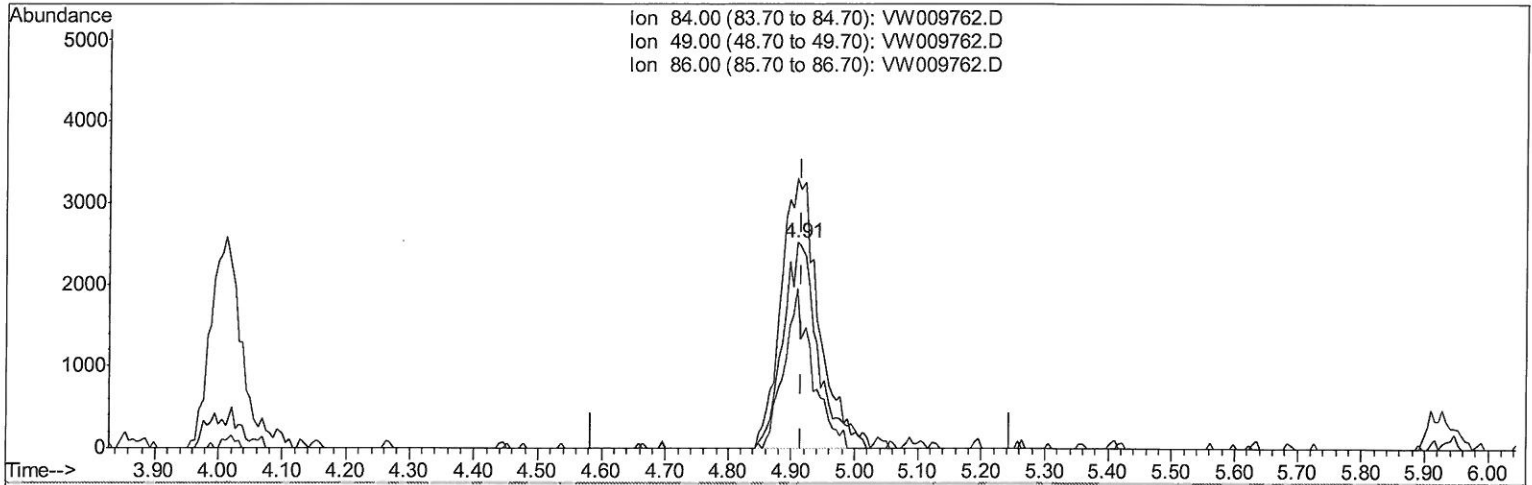

TIC: VW009762.D

(16) Methylene chloride (T)

4.909min (-0.006) 1.10ug/L m

response 9587

Ion	Exp%	Act%
84.00	100	100
49.00	140.40	131.20
86.00	66.30	77.34
0.00	0.00	0.00

7 MO
 4/9/19




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
Data File : VW009762.D
Acq On : 06 Apr 2019 10:17
Operator : SY/VA
Sample : VW0406SBL02
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK25

Manual Integrations
APPROVED

MMDadoda
4/11/2019 11:42:58 AM

Quant Time: Apr 07 03:59:38 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
Quant Title : VOC Analysis
QLast Update : Sun Apr 07 03:56:20 2019
Response via : Initial Calibration

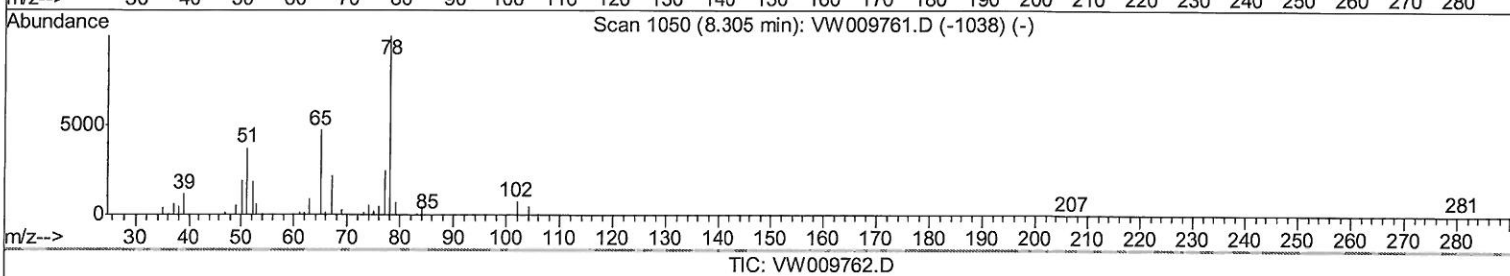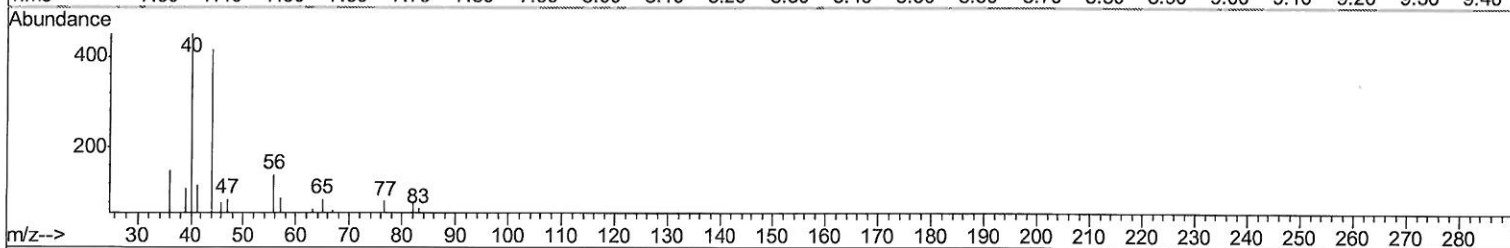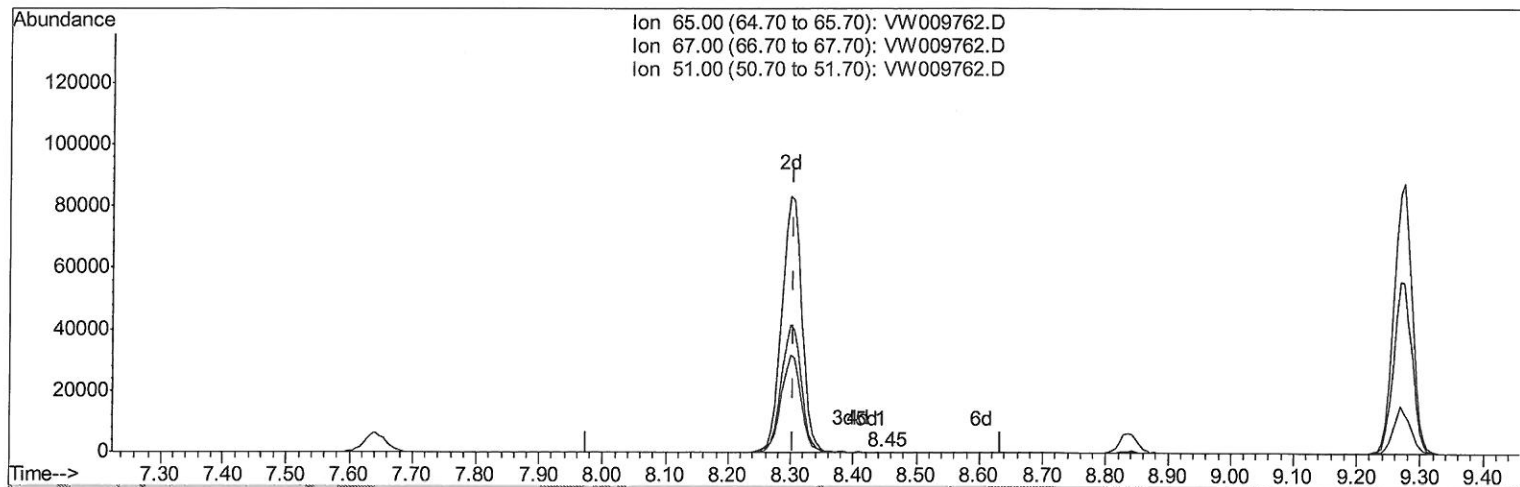

(26) 1,2-Dichloroethane-d4 (S)

8.445min (+0.140) 0.01ug/L

response 55

Ion	Exp%	Act%
65.00	100	100
67.00	50.90	40.00
51.00	109.90	100.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009762.D
 Acq On : 06 Apr 2019 10:17
 Operator : SY/VA
 Sample : VW0406SBL02
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 VBLK25

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:42:58 AM

Quant Time: Apr 07 03:59:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 03:56:20 2019
 Response via : Initial Calibration

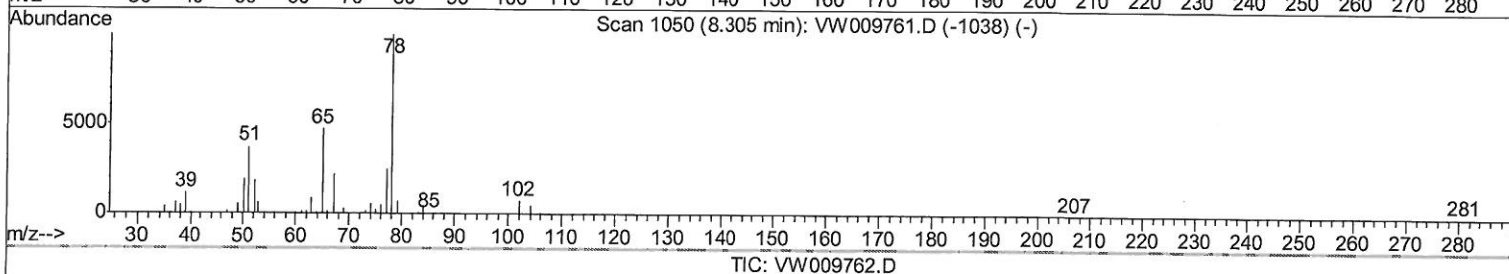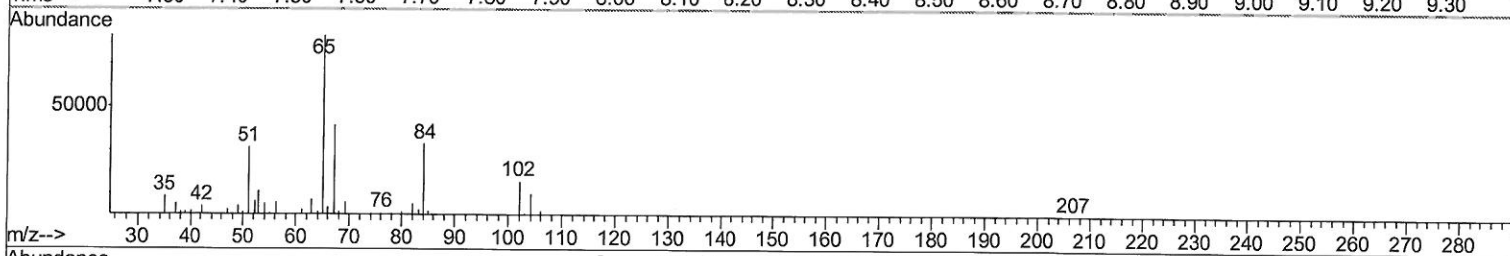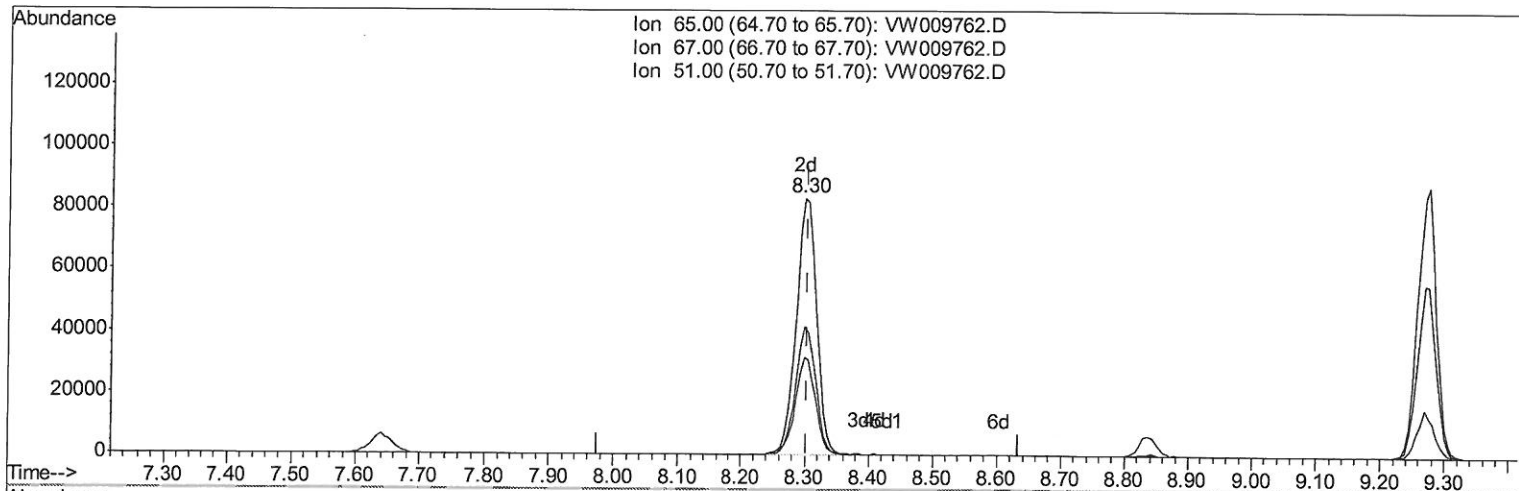

(26) 1,2-Dichloroethane-d4 (S)

8.299min (-0.006) 22.44ug/L m

response 185551

Ion	Exp%	Act%
65.00	100	100
67.00	50.90	0.01#
51.00	109.90	0.03#
0.00	0.00	0.00

7 M Q
 4/11/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW040619\
 Data File : VW009762.D
 Acq On : 06 Apr 2019 10:17
 Operator : SY/VA
 Sample : VW0406SBL02
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK25

Manual Integrations
 APPROVED

MMDadoda
 4/11/2019 11:42:58 AM

Quant Time: Apr 07 04:09:39 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM040319S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Apr 07 03:56:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	8.84	114	493518	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	468904	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	208133	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	128621	19.92	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.68%		
7) Chloroethane-d5	2.89	69	122220	20.66	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.64%		
10) 1,1-Dichloroethene-d2	4.01	63	234461	16.88	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.52%		
20) 2-Butanone-d5	7.07	46	98088	46.78	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.56%		
24) Chloroform-d	7.64	84	303807	22.56	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.24%		
26) 1,2-Dichloroethane-d4	8.30	65	185551m	22.44	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	89.76%		
29) Benzene-d6	8.27	84	566763	23.03	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.12%		
33) 1,2-Dichloropropane-d6	9.27	67	174880	23.00	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	92.00%		
37) Toluene-d8	10.32	98	512962	22.54	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	90.16%		
38) trans-1,3-Dichloropropene-	10.57	79	77459	21.36	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.44%		
39) 2-Hexanone-d5	10.93	63	67001	46.76	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.52%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	150539	21.30	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.20%		
61) 1,2-Dichlorobenzene-d4	13.85	152	177144	24.25	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	97.00%		

7 mbe
 4/9/19

Target Compounds

16) Methylene chloride	4.91	84	9587m	1.101	ug/L	Qvalue
------------------------	------	----	-------	-------	------	--------

7 mbe
 4/9/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed